

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072320\
 Data File : PL060147.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2020 17:21
 Operator : DD\AJ
 Sample : L3379-02
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ETGI-361

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 02:29:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.012	41266038	54337201	21.335	20.503
28)	SA Decachlor...	8.223	9.100	25503983	33083798	15.503	15.819
Target Compounds							
4)	MA Heptachlor	0.000	5.198	0	1415618	N.D.	0.421 #
6)	B beta-BHC	4.438	0.000	1781299	0	1.744	N.D. #
8)	B Heptachlo...	0.000	5.871f	0	3914518	N.D.	1.453 #
11)	B alpha-Chl...	5.452f	0.000	1213398	0	0.673	N.D. #
15)	B Endosulfa...	0.000	6.942	0	4677007	N.D.	1.862 #
18)	B Endrin al...	0.000	7.072	0	856658	N.D.	0.394 #
20)	A Methoxychlor	0.000	7.629f	0	2087328	N.D.	1.839 #
26)	Chlordane-4	5.452f	0.000	1213398	0	8.697	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072320\
Data File : PL060147.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jul 2020 17:21
Operator : DD\AJ
Sample : L3379-02
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ETGI-361

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 02:29:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

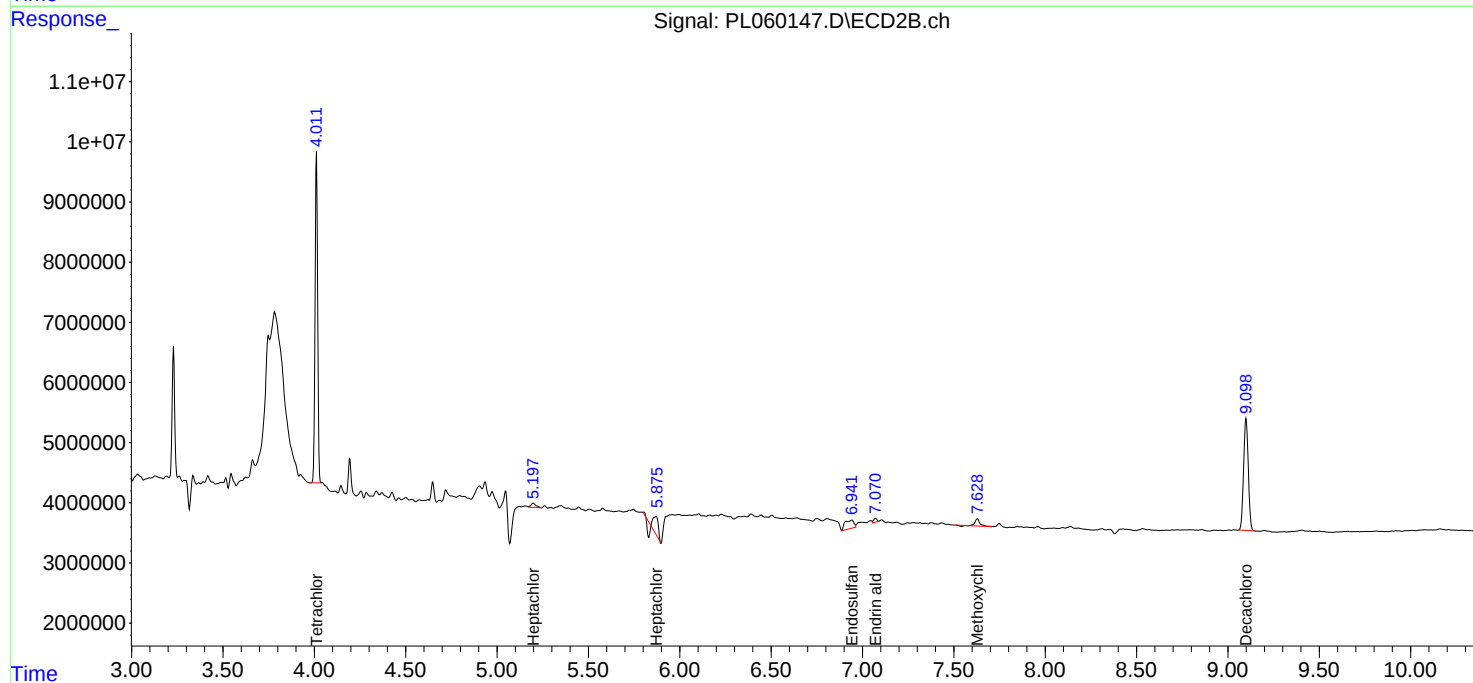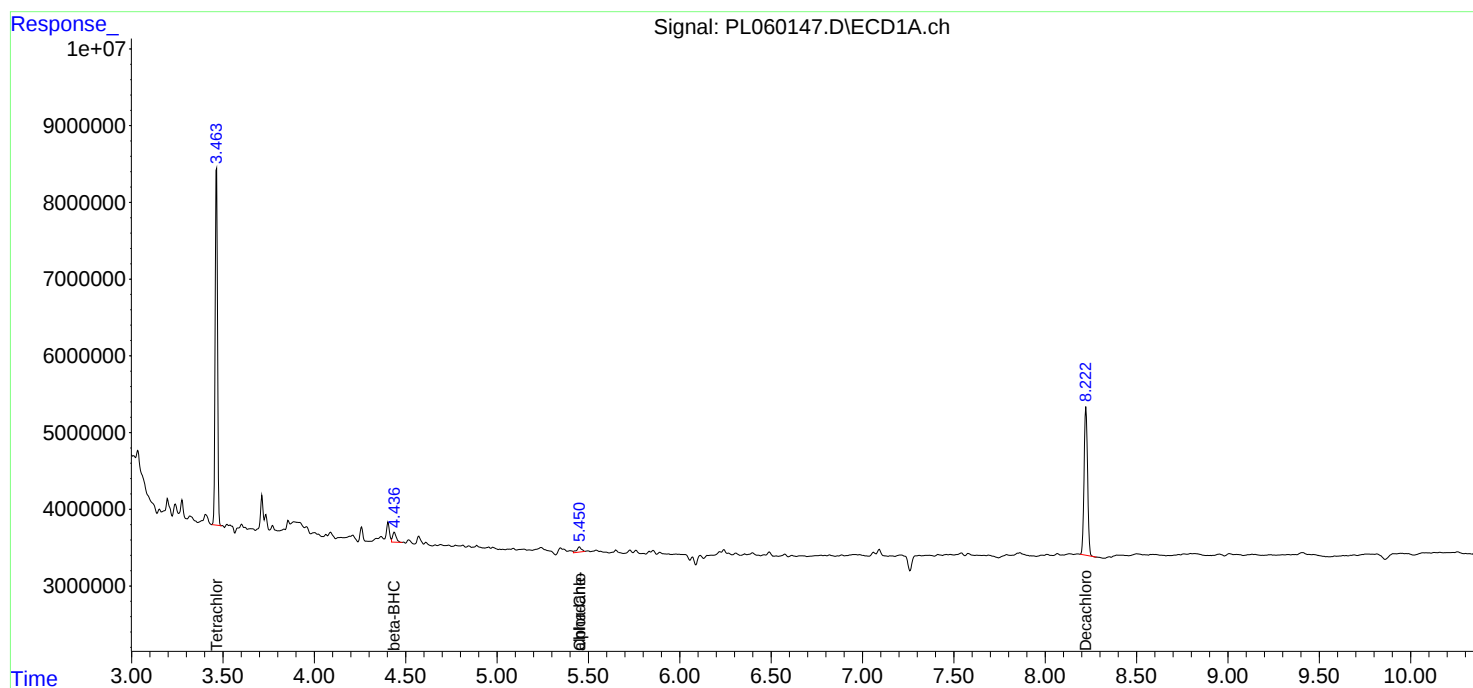


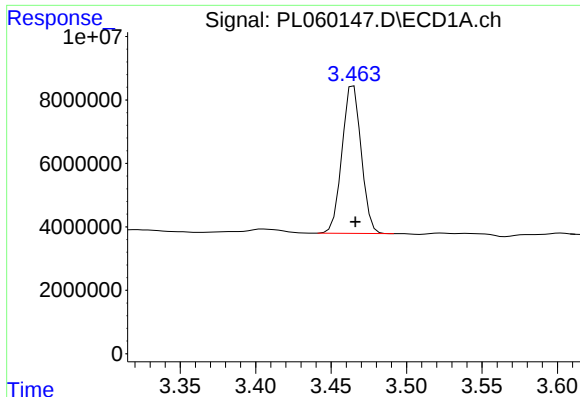

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: -0.001 min
Response: 41266038
Conc: 21.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
ETGI-361

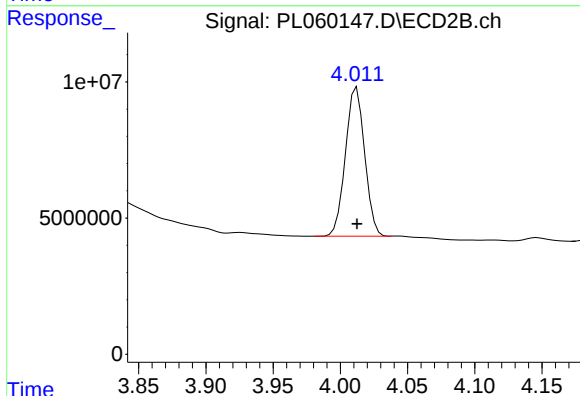


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 54337201
Conc: 20.50 ng/ml

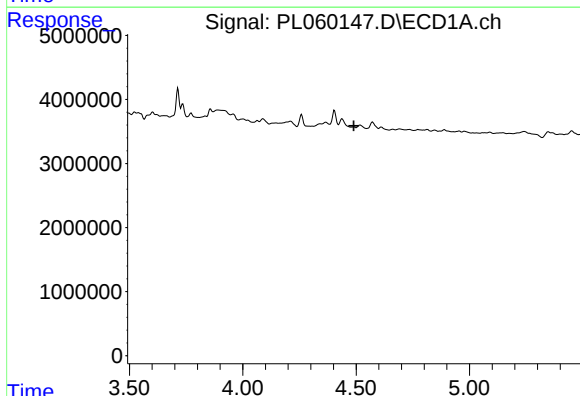


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.490 min
Response: 0
Conc: N.D.

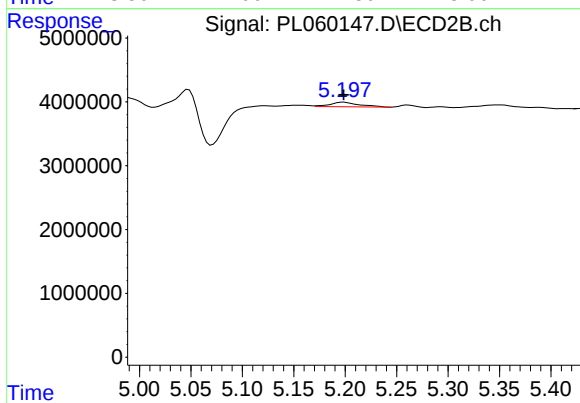

#4 Heptachlor


R.T.: 5.198 min
Delta R.T.: 0.000 min
Response: 1415618
Conc: 0.42 ng/ml

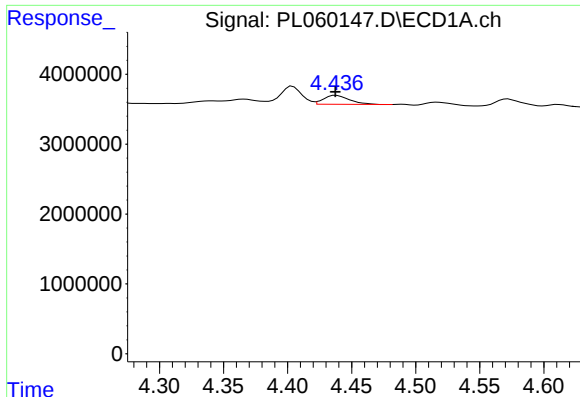

#6 beta-BHC


R.T.: 4.438 min
Delta R.T.: 0.000 min
Response: 1781299
Conc: 1.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
ETGI-361

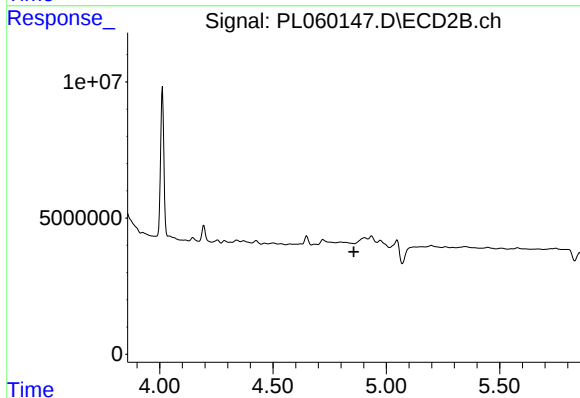


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.857 min
Response: 0
Conc: N.D.

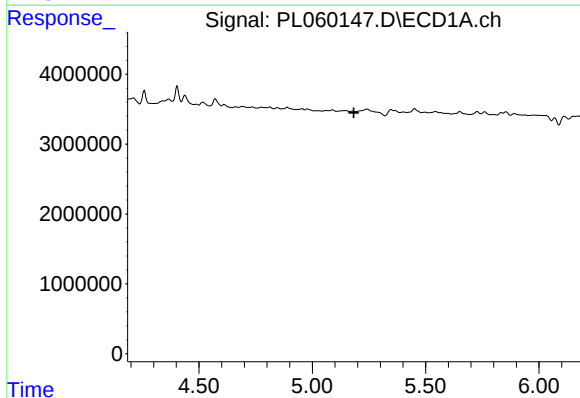


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.183 min
Response: 0
Conc: N.D.

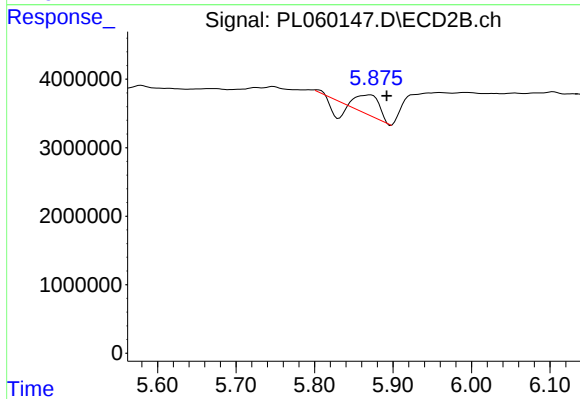

#8 Heptachlor epoxide


R.T.: 5.871 min
Delta R.T.: -0.021 min
Response: 3914518
Conc: 1.45 ng/ml

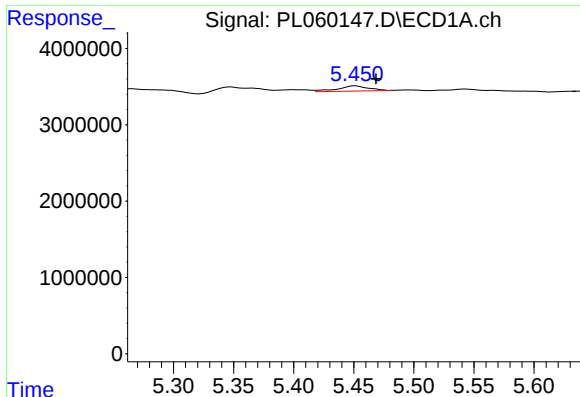

#11 alpha-Chlordane


R.T.: 5.452 min
Delta R.T.: -0.017 min
Response: 1213398
Conc: 0.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
ETGI-361

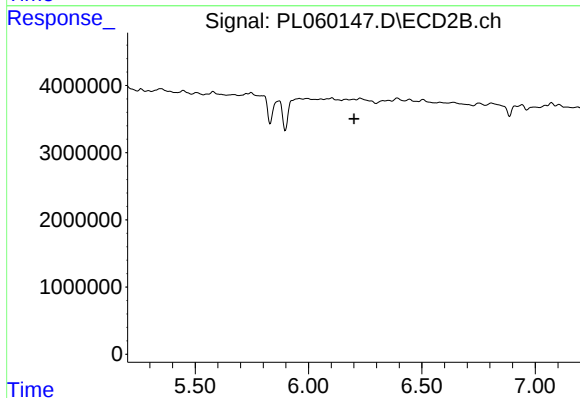


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.201 min
Response: 0
Conc: N.D.

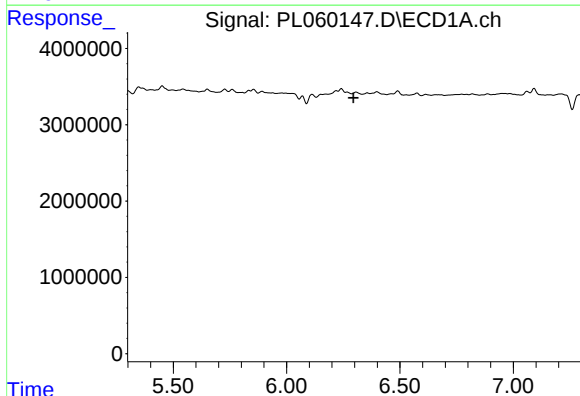


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.296 min
Response: 0
Conc: N.D.

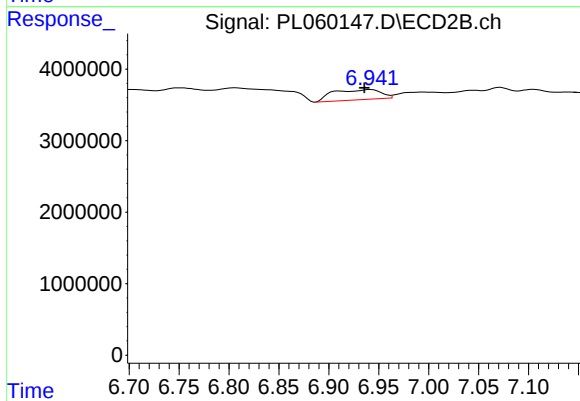

#15 Endosulfan II


R.T.: 6.942 min
Delta R.T.: 0.006 min
Response: 4677007
Conc: 1.86 ng/ml

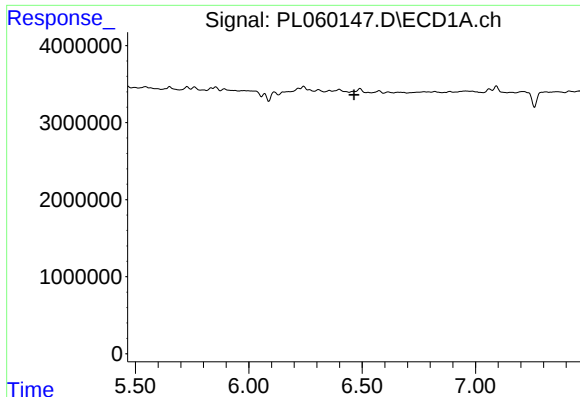

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.464 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
ETGI-361

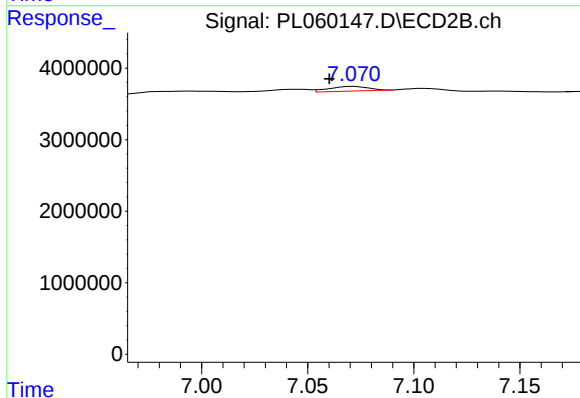


#18 Endrin aldehyde

R.T.: 7.072 min
Delta R.T.: 0.012 min
Response: 856658
Conc: 0.39 ng/ml

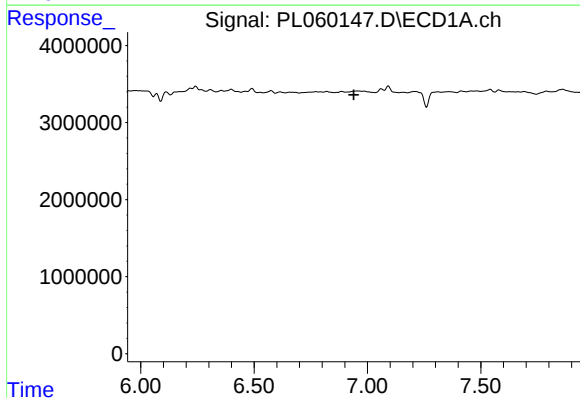


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.939 min
Response: 0
Conc: N.D.

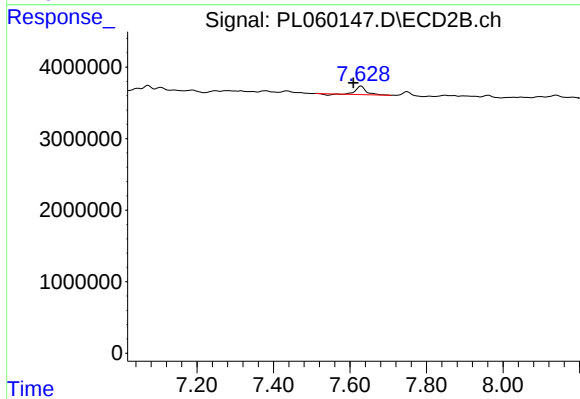

#20 Methoxychlor


R.T.: 7.629 min
Delta R.T.: 0.021 min
Response: 2087328
Conc: 1.84 ng/ml

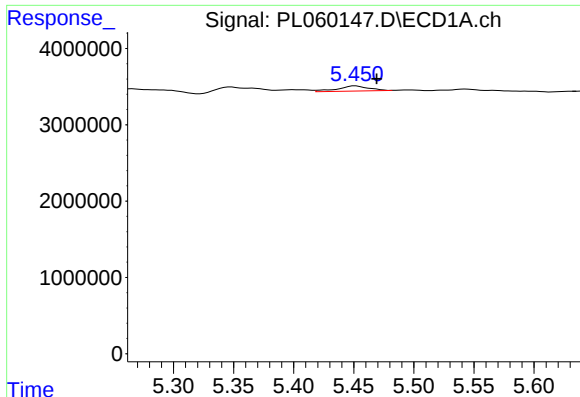

#26 Chlordane-4


R.T.: 5.452 min
Delta R.T.: -0.017 min
Response: 1213398
Conc: 8.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
ETGI-361

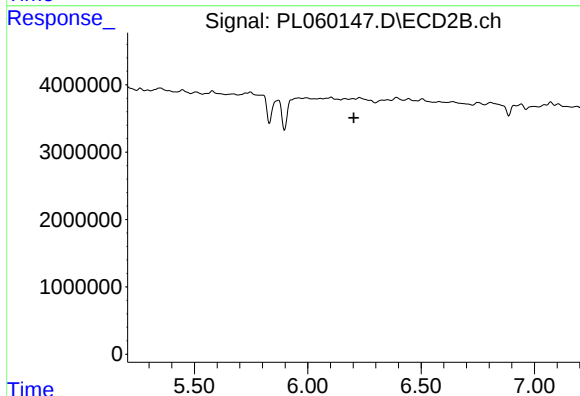


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.203 min
Response: 0
Conc: N.D.

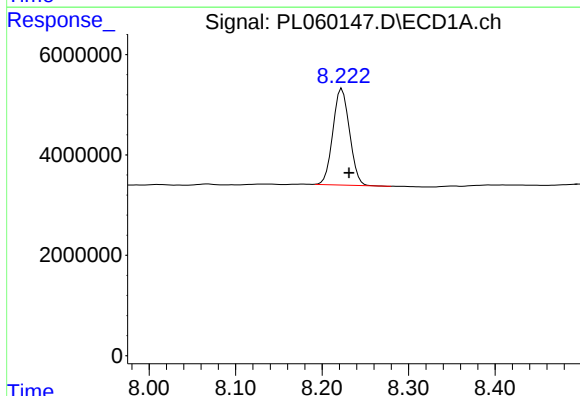

#28 Decachlorobiphenyl

R.T.: 8.223 min
Delta R.T.: -0.008 min
Response: 25503983
Conc: 15.50 ng/ml

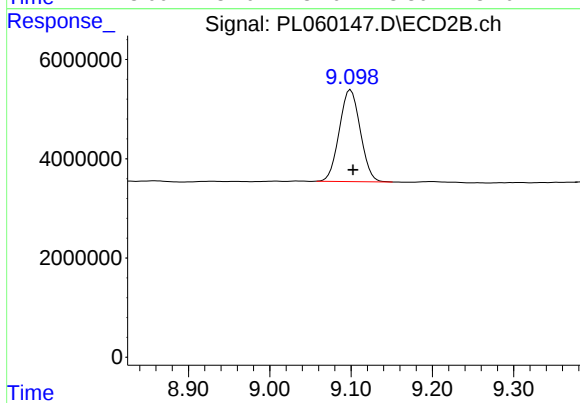

#28 Decachlorobiphenyl

R.T.: 9.100 min
Delta R.T.: -0.003 min
Response: 33083798
Conc: 15.82 ng/ml