

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072321\
 Data File : PL068436.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2021 17:21
 Operator : AR\AJ
 Sample : M3150-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 04:56:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:44:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.642	5.569	6802809	15117598	15.851	14.815
28)	SA Decachlor...	10.417	11.490	7628677	12880443	13.564	14.440
Target Compounds							
10)	B gamma-Chl...	0.000	8.301	0	261123	N.D.	0.232 #
11)	B alpha-Chl...	0.000	8.384	0	703828	N.D.	0.626 #
23)	Chlordane-1	0.000	6.978f	0	340212	N.D.	8.398 #
25)	Chlordane-3	0.000	8.301	0	261123	N.D.	1.686 #
26)	Chlordane-4	0.000	8.384	0	703828	N.D.	3.754 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072321\
Data File : PL068436.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jul 2021 17:21
Operator : AR\AJ
Sample : M3150-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 04:56:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:44:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

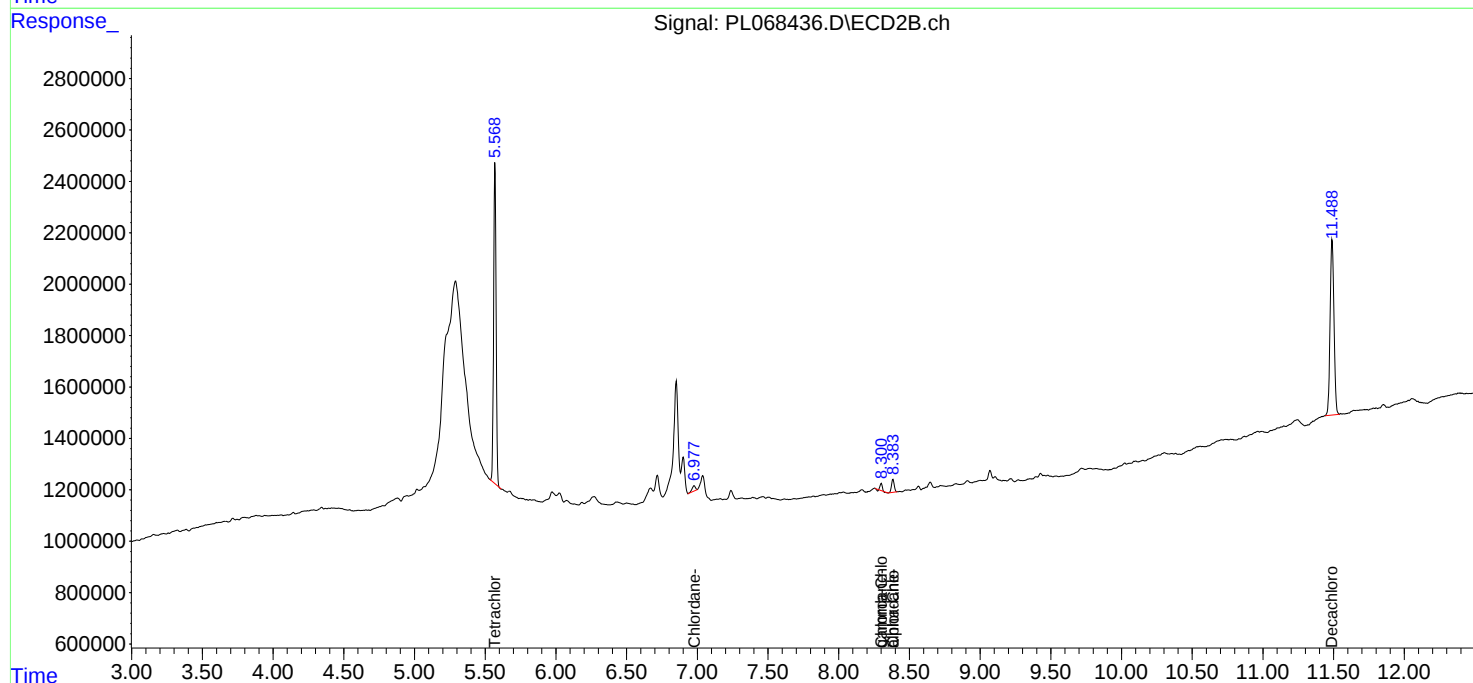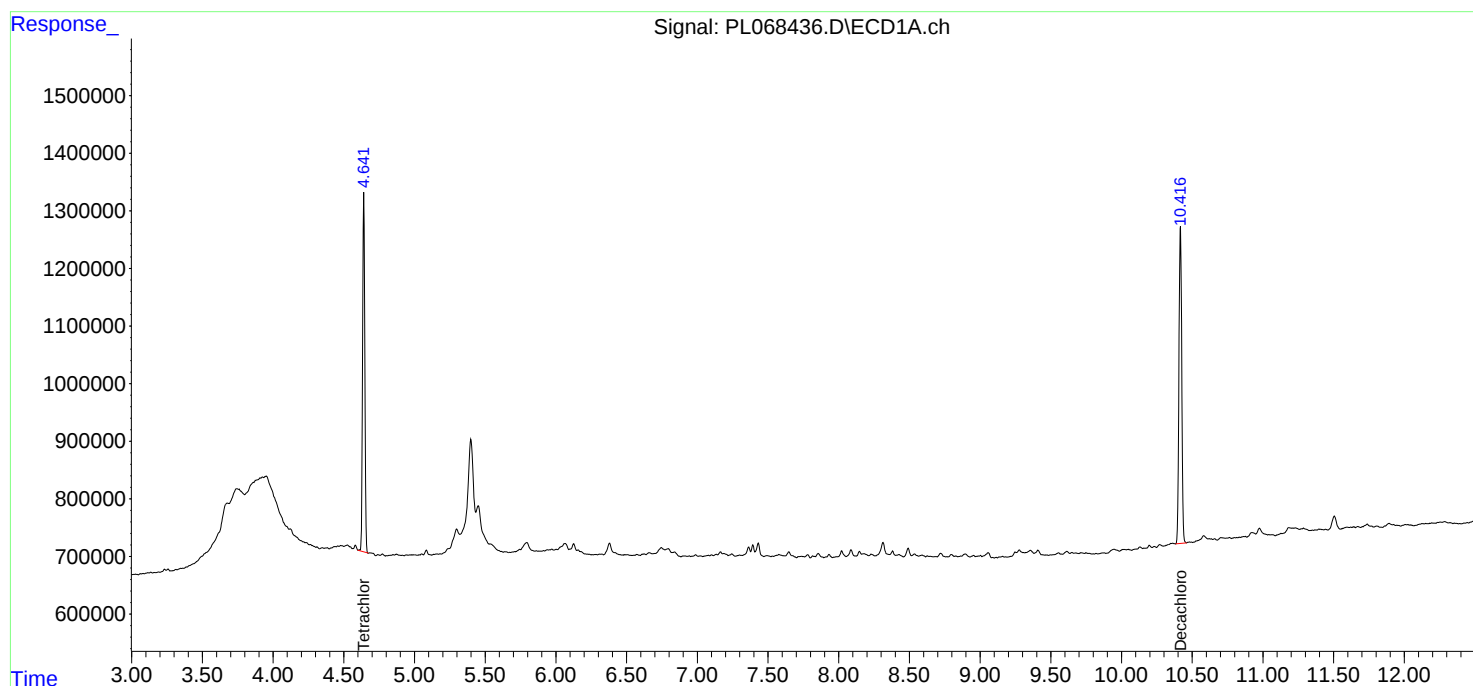


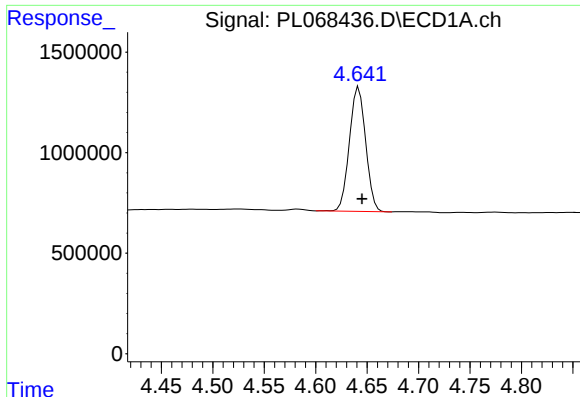

#1 Tetrachloro-m-xylene


R.T.: 4.642 min
Delta R.T.: -0.003 min
Response: 6802809
Conc: 15.85 ng/ml

Instrument :
ECD_L
ClientSampleId :

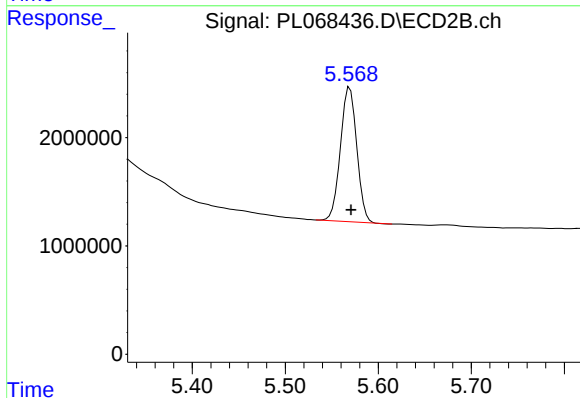


#1 Tetrachloro-m-xylene

R.T.: 5.569 min
Delta R.T.: -0.001 min
Response: 15117598
Conc: 14.81 ng/ml

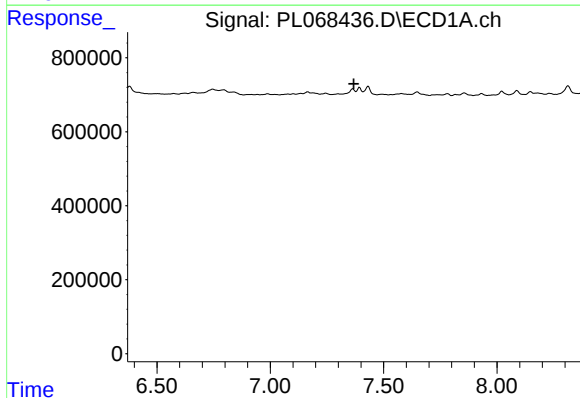


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.369 min
Response: 0
Conc: N.D.

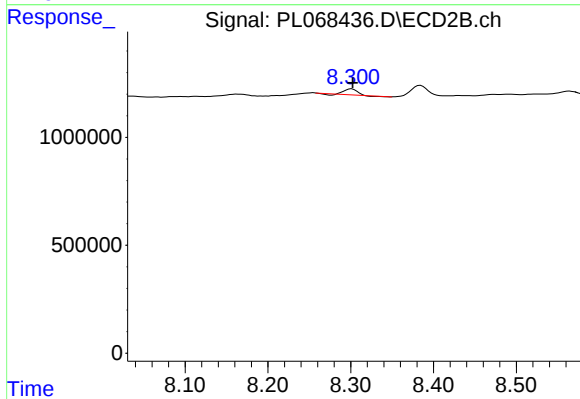

#10 gamma-Chlordane


R.T.: 8.301 min
Delta R.T.: -0.001 min
Response: 261123
Conc: 0.23 ng/ml

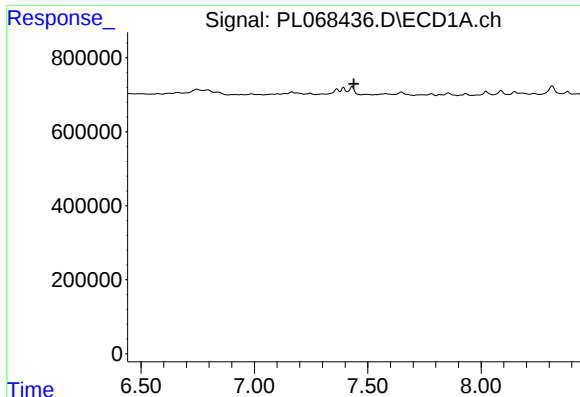

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.438 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

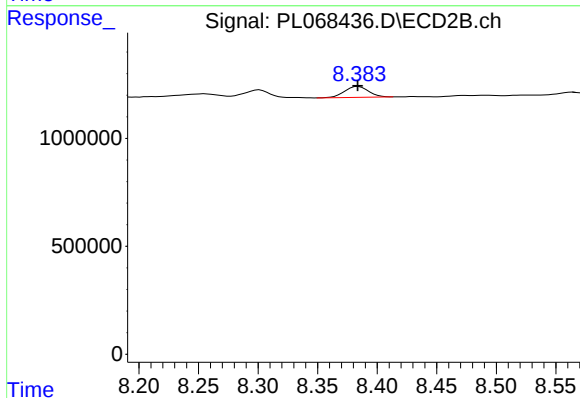


#11 alpha-Chlordane

R.T.: 8.384 min
Delta R.T.: 0.000 min
Response: 703828
Conc: 0.63 ng/ml

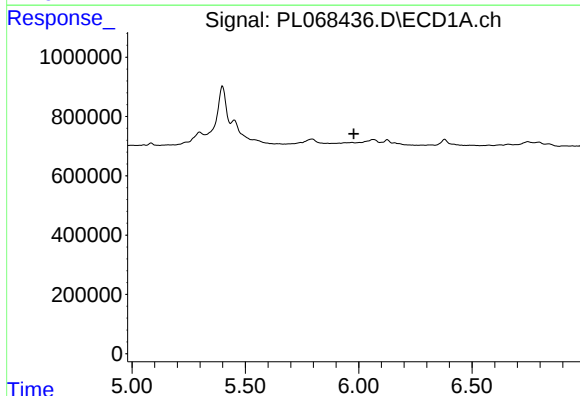


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.978 min
Response: 0
Conc: N.D.

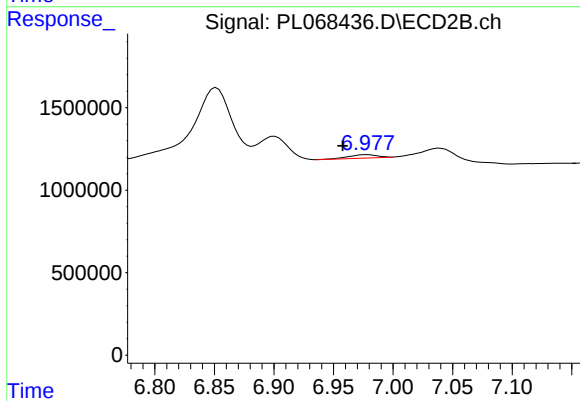

#23 Chlordane-1


R.T.: 6.978 min
Delta R.T.: 0.020 min
Response: 340212
Conc: 8.40 ng/ml

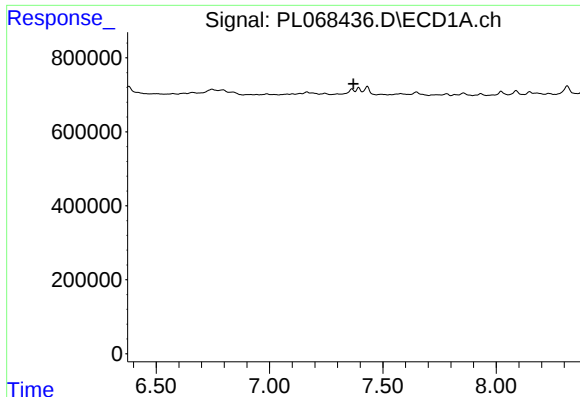

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 7.371 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

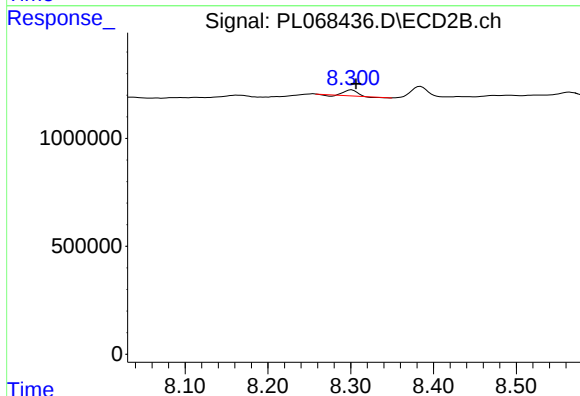


#25 Chlordane-3

R.T.: 8.301 min
Delta R.T.: -0.005 min
Response: 261123
Conc: 1.69 ng/ml

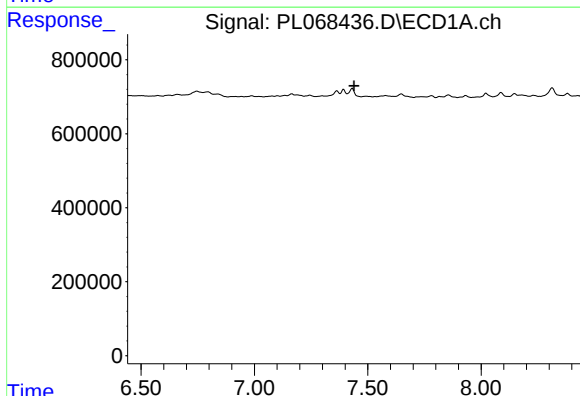


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 7.440 min
Response: 0
Conc: N.D.

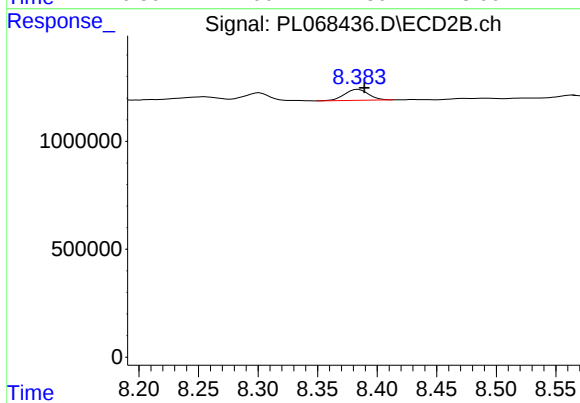

#26 Chlordane-4


R.T.: 8.384 min
Delta R.T.: -0.005 min
Response: 703828
Conc: 3.75 ng/ml

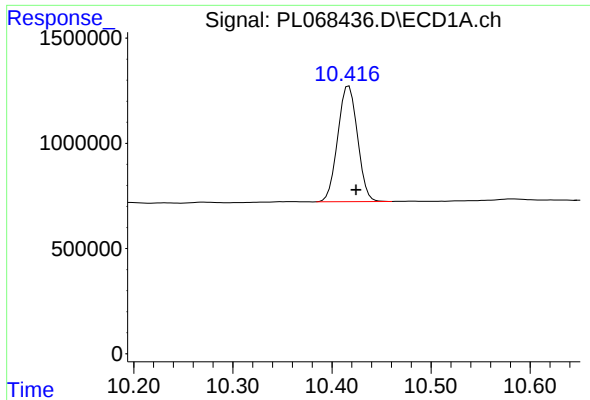

#28 Decachlorobiphenyl

R.T.: 10.417 min
Delta R.T.: -0.007 min
Response: 7628677
Conc: 13.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

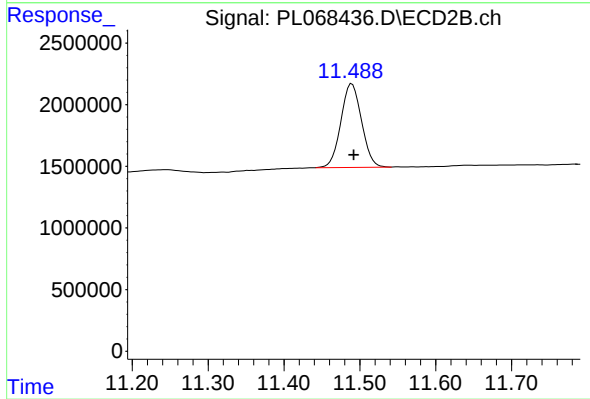

#28 Decachlorobiphenyl

R.T.: 11.490 min
Delta R.T.: -0.003 min
Response: 12880443
Conc: 14.44 ng/ml