

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072321\
 Data File : PL068447.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2021 20:23
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 04:58:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:44:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.642	5.569	10039868	22604662	23.393	22.152
28)	SA Decachlor...	10.417	11.489	12902785	20658953	22.942	23.160
Target Compounds							
4)	MA Heptachlor	6.161f	0.000	621187	0	1.019	N.D. #
6)	B beta-BHC	6.161	0.000	621187	0	2.123	N.D. #
8)	B Heptachlo...	0.000	8.036	0	1144266	N.D.	1.012 #
14)	MA Endrin	8.088f	0.000	762551	0	1.525	N.D. #
15)	B Endosulfa...	0.000	9.217f	0	2077286	N.D.	2.292 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072321\
Data File : PL068447.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jul 2021 20:23
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 04:58:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:44:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

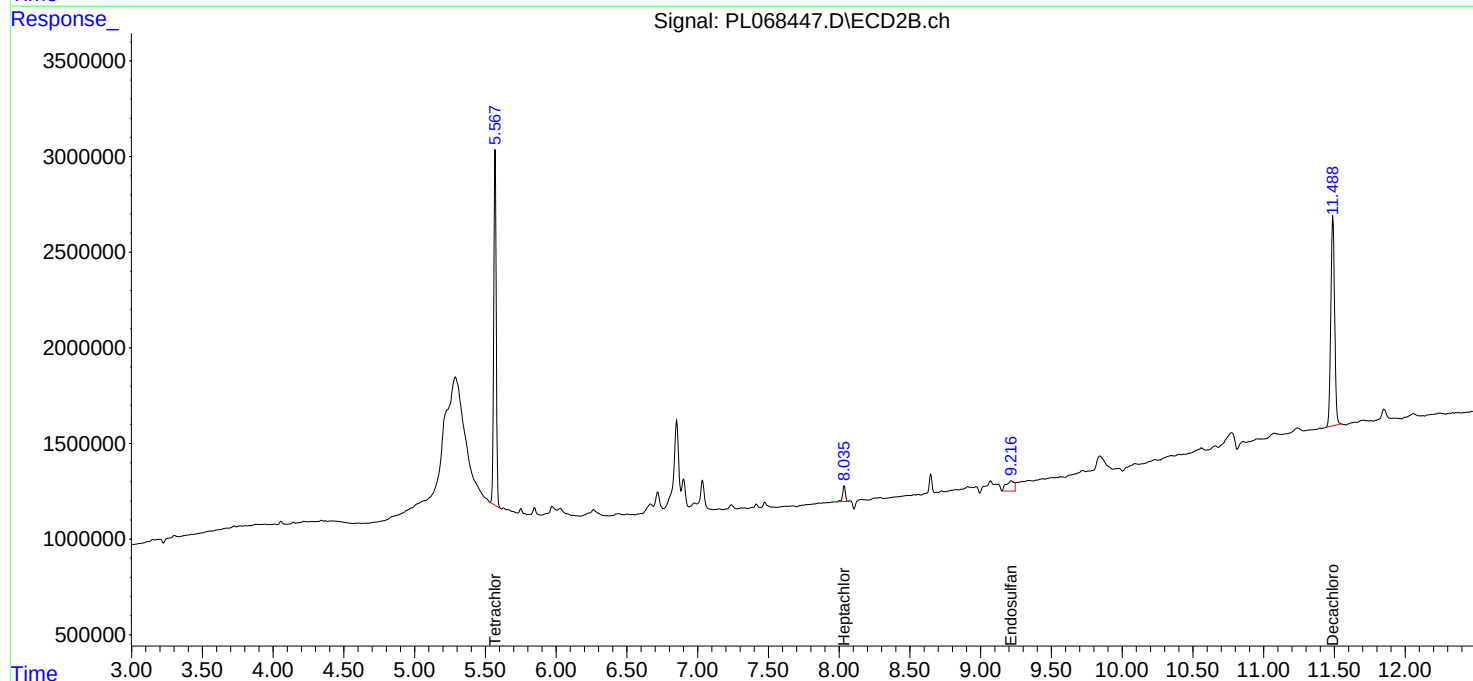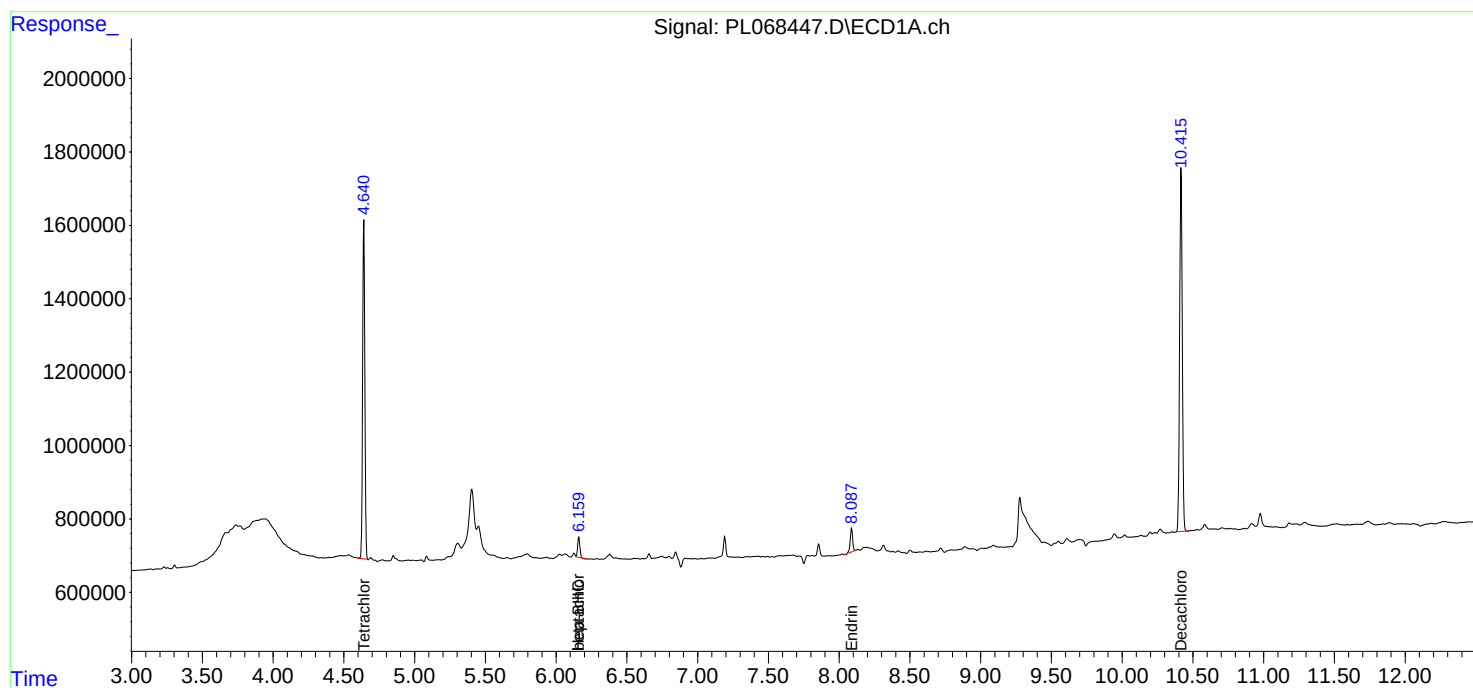


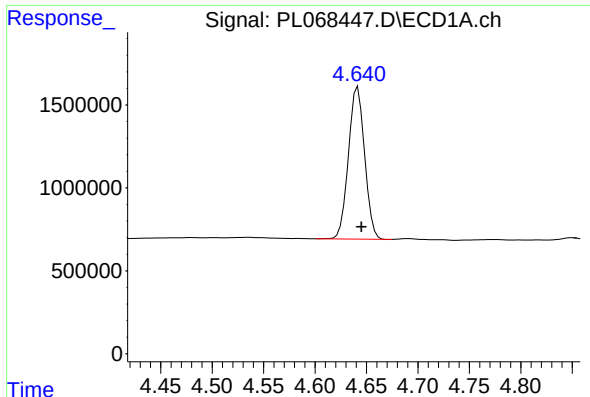

#1 Tetrachloro-m-xylene


R.T.: 4.642 min
Delta R.T.: -0.003 min
Response: 10039868
Conc: 23.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

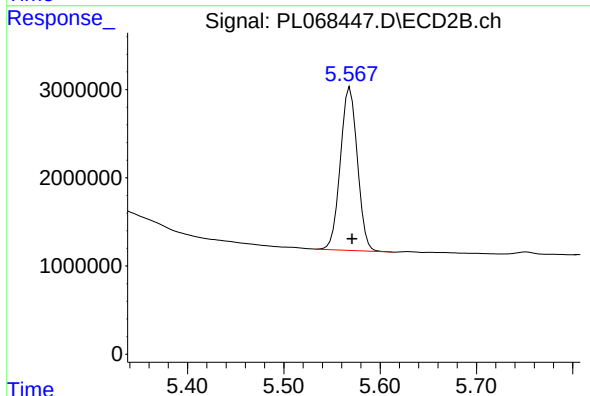


#1 Tetrachloro-m-xylene

R.T.: 5.569 min
Delta R.T.: -0.002 min
Response: 22604662
Conc: 22.15 ng/ml

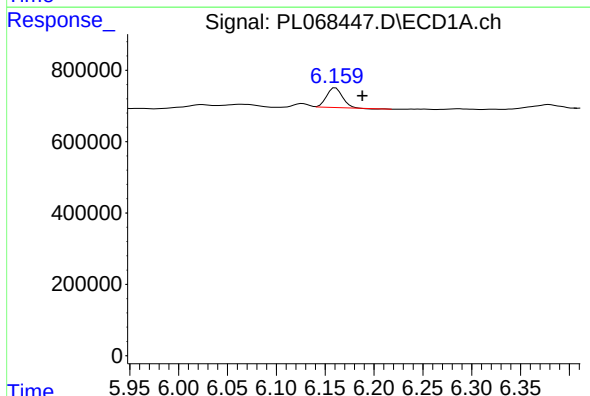


#4 Heptachlor

R.T.: 6.161 min
Delta R.T.: -0.028 min
Response: 621187
Conc: 1.02 ng/ml

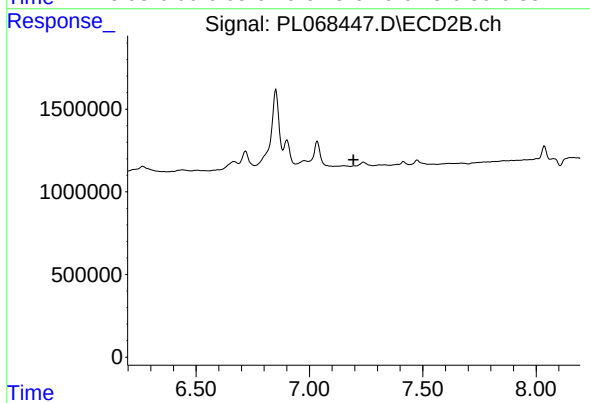

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 7.195 min
Response: 0
Conc: N.D.

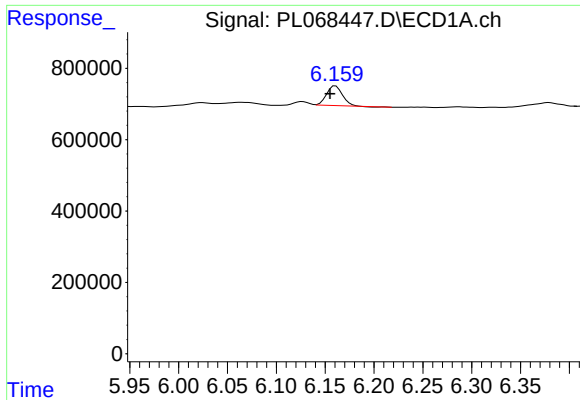

#6 beta-BHC


R.T.: 6.161 min
Delta R.T.: 0.006 min
Response: 621187
Conc: 2.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

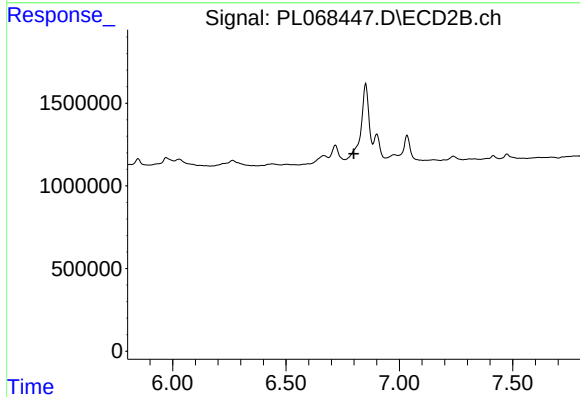


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.799 min
Response: 0
Conc: N.D.

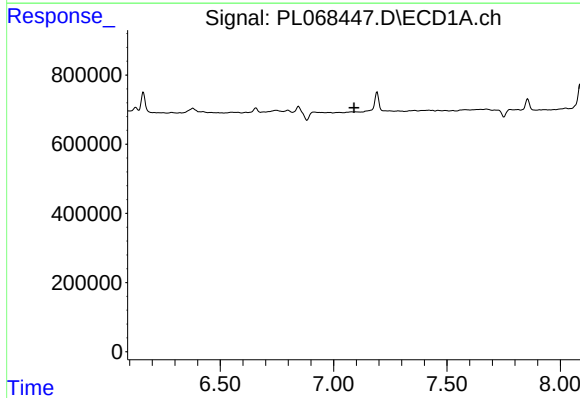


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.091 min
Response: 0
Conc: N.D.

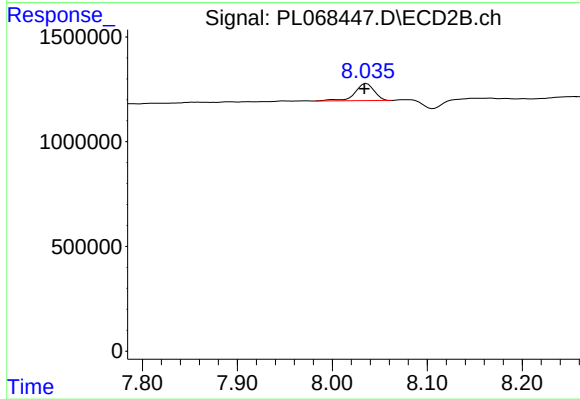

#8 Heptachlor epoxide


R.T.: 8.036 min
Delta R.T.: 0.002 min
Response: 1144266
Conc: 1.01 ng/ml

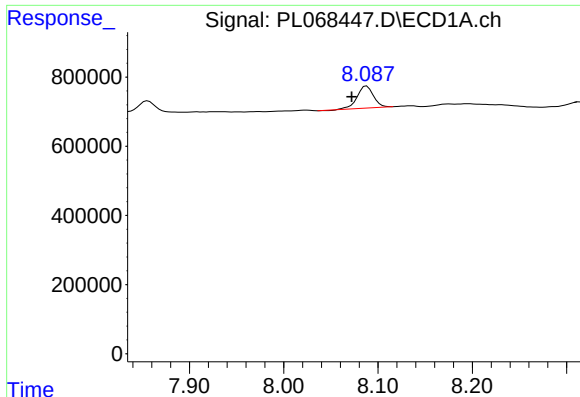

#14 Endrin


R.T.: 8.088 min
Delta R.T.: 0.016 min
Response: 762551
Conc: 1.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

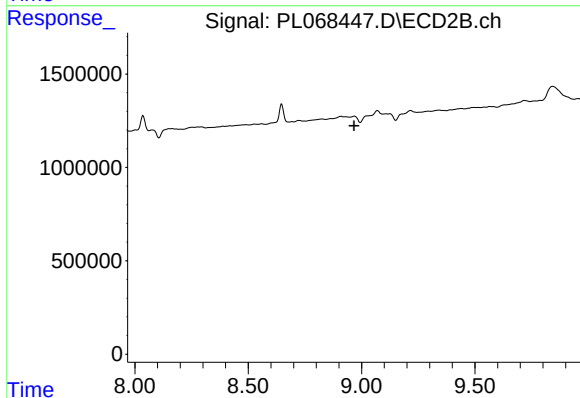


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.966 min
Response: 0
Conc: N.D.

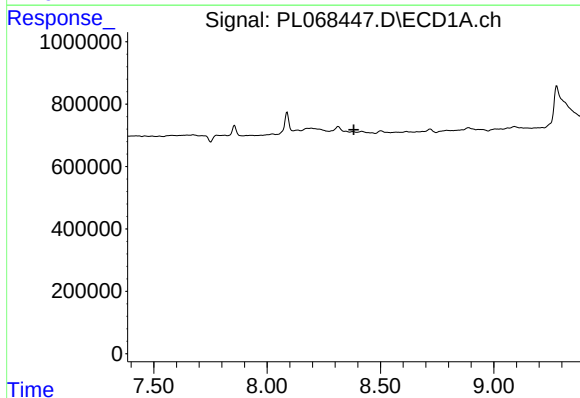


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.382 min
Response: 0
Conc: N.D.

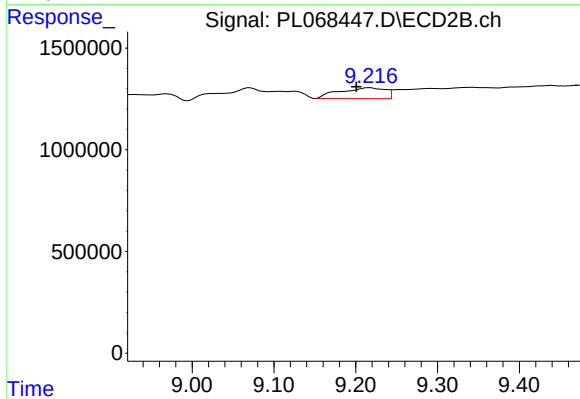

#15 Endosulfan II


R.T.: 9.217 min
Delta R.T.: 0.016 min
Response: 2077286
Conc: 2.29 ng/ml

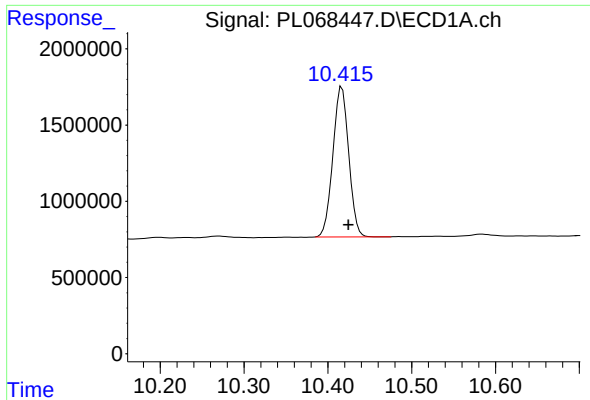

#28 Decachlorobiphenyl

R.T.: 10.417 min
Delta R.T.: -0.008 min
Response: 12902785
Conc: 22.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

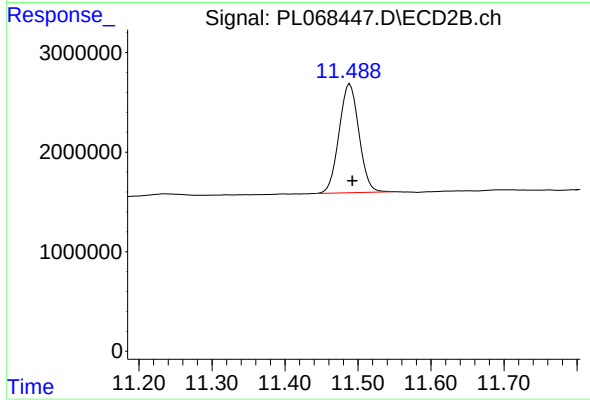

#28 Decachlorobiphenyl

R.T.: 11.489 min
Delta R.T.: -0.003 min
Response: 20658953
Conc: 23.16 ng/ml