

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072323\
 Data File : PL084136.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2023 00:49
 Operator : AR\AJ
 Sample : 03706-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 B-P9A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 03:56:32 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 00:03:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.475	2.687	16270173	7944675	8.136	7.154
28)	SA Decachlor...	9.025	7.871	14330572	11341555	11.010	10.207
Target Compounds							
12)	B 4,4'-DDE	6.147	5.166	871640	384014	0.433	0.313 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072323\
Data File : PL084136.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jul 2023 00:49
Operator : AR\AJ
Sample : 03706-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
B-P9A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 03:56:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 00:03:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

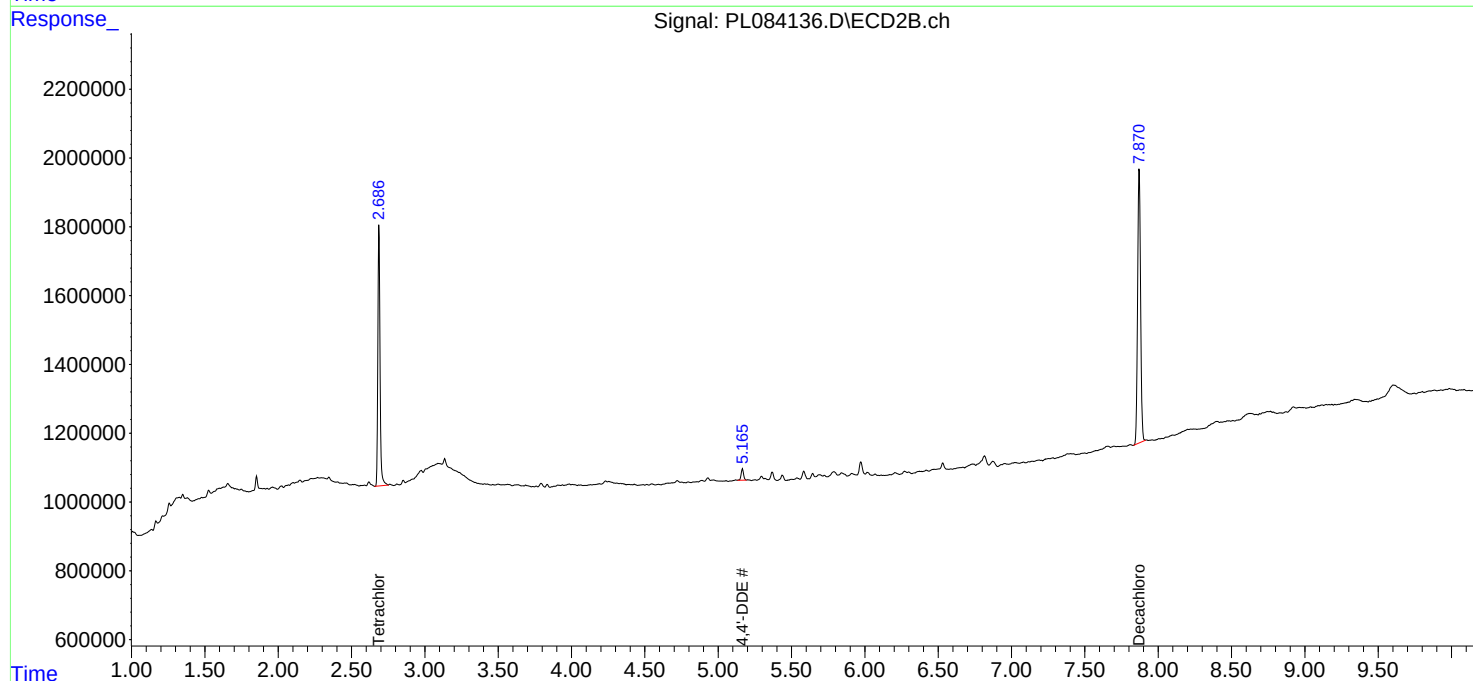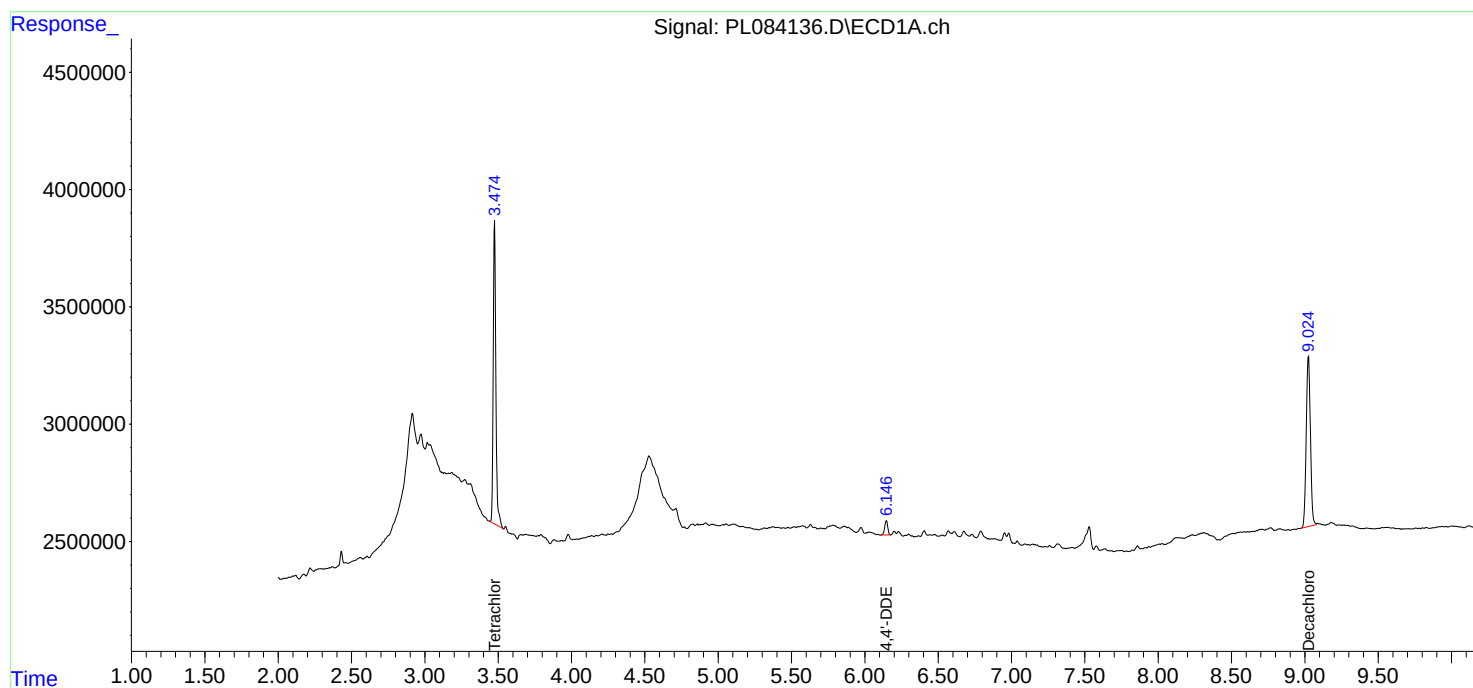


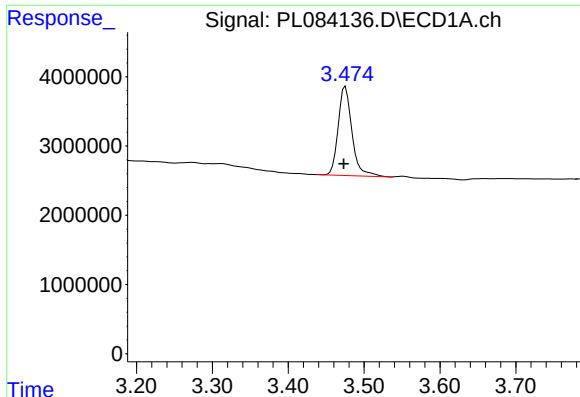

#1 Tetrachloro-m-xylene


R.T.: 3.475 min
Delta R.T.: 0.002 min
Response: 16270173
Conc: 8.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
B-P9A

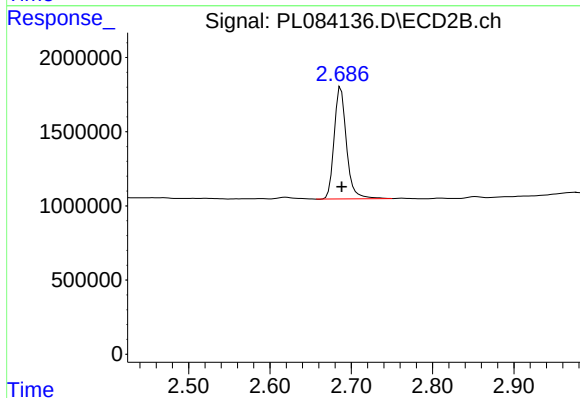


#1 Tetrachloro-m-xylene

R.T.: 2.687 min
Delta R.T.: -0.001 min
Response: 7944675
Conc: 7.15 ng/ml

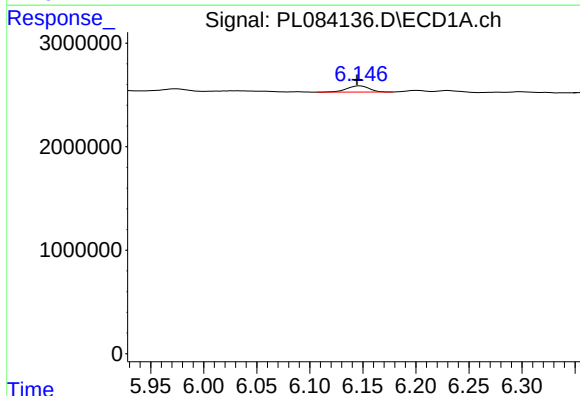


#12 4,4'-DDE

R.T.: 6.147 min
Delta R.T.: 0.003 min
Response: 871640
Conc: 0.43 ng/ml

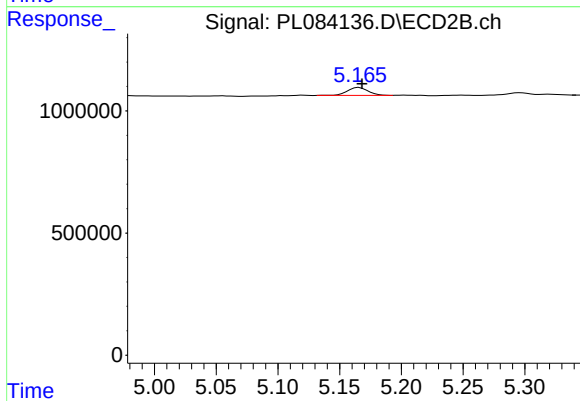

#12 4,4'-DDE


R.T.: 5.166 min
Delta R.T.: -0.002 min
Response: 384014
Conc: 0.31 ng/ml

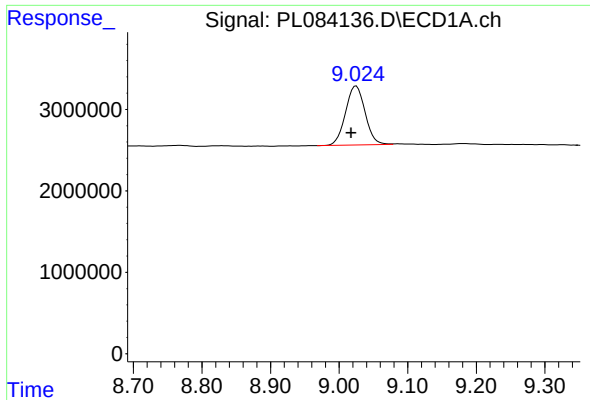

#28 Decachlorobiphenyl

R.T.: 9.025 min
Delta R.T.: 0.007 min
Response: 14330572
Conc: 11.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
B-P9A

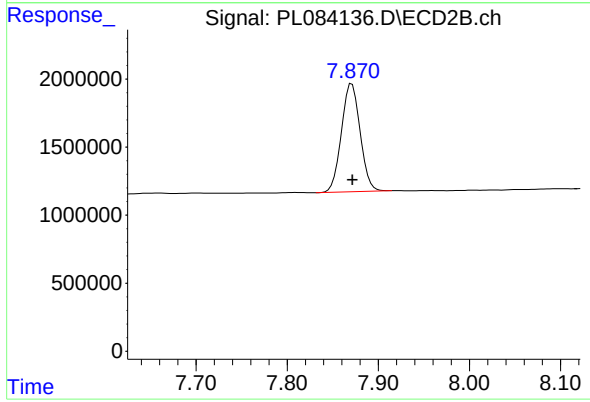

#28 Decachlorobiphenyl

R.T.: 7.871 min
Delta R.T.: 0.000 min
Response: 11341555
Conc: 10.21 ng/ml