

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072325\
 Data File : PL096536.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 15:35
 Operator : AR\AJ
 Sample : Q2668-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 05:09:10 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 07 15:22:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	2.827	52627650	83408709	14.423	14.453
28)	SA Decachlor...	9.016	7.991	38512891	53621134	13.691	10.753
Target Compounds							
10)	B gamma-Chl...	5.915	0.000	2360294	0	0.533	N.D. #
11)	B alpha-Chl...	5.999	0.000	6489988	0	1.482	N.D. #
25)	Chlordane-3	5.915	0.000	2360294	0	3.204	N.D. #
26)	Chlordane-4	5.999	0.000	6489988	0	7.233	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072325\
Data File : PL096536.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jul 2025 15:35
Operator : AR\AJ
Sample : Q2668-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 05:09:10 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
Quant Title : GC Extractables
QLast Update : Mon Jul 07 15:22:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

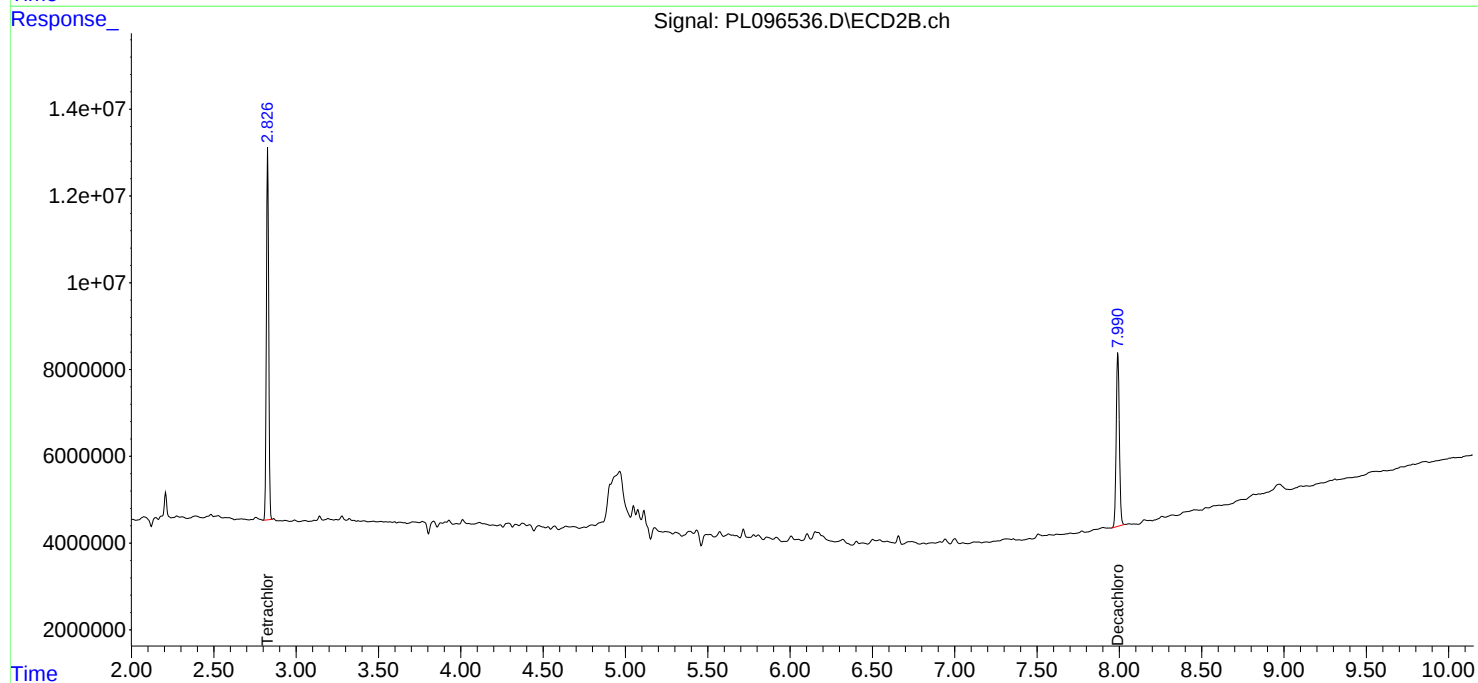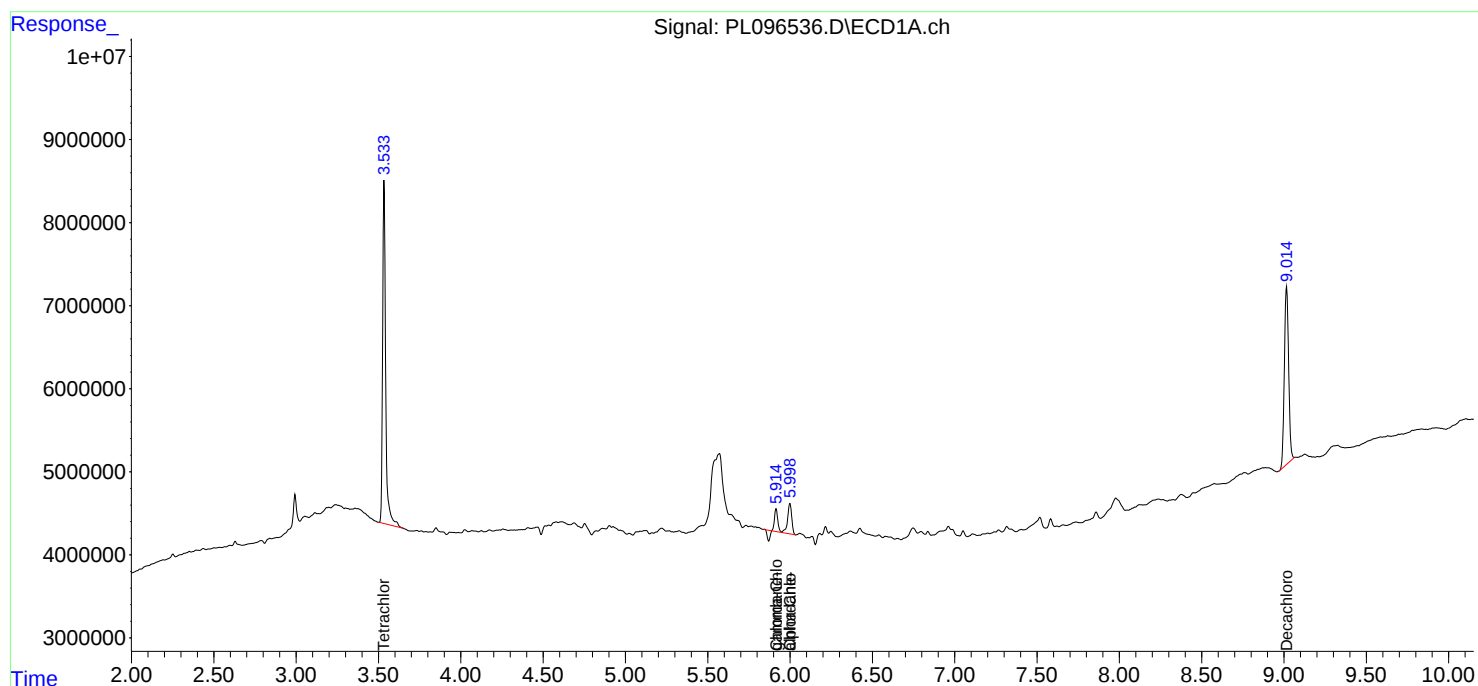


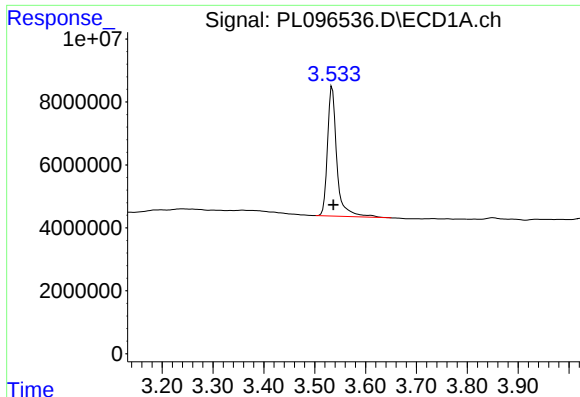

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: -0.002 min
Response: 52627650
Conc: 14.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3

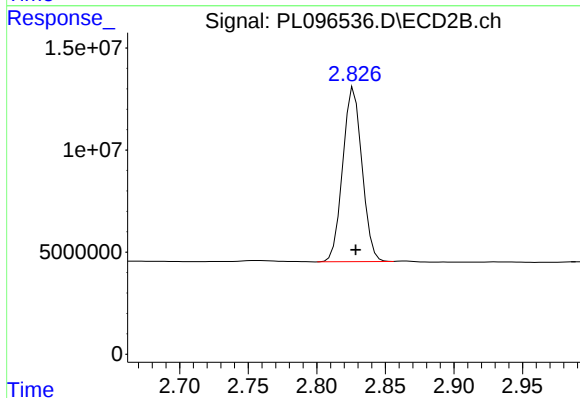


#1 Tetrachloro-m-xylene

R.T.: 2.827 min
Delta R.T.: -0.001 min
Response: 83408709
Conc: 14.45 ng/ml

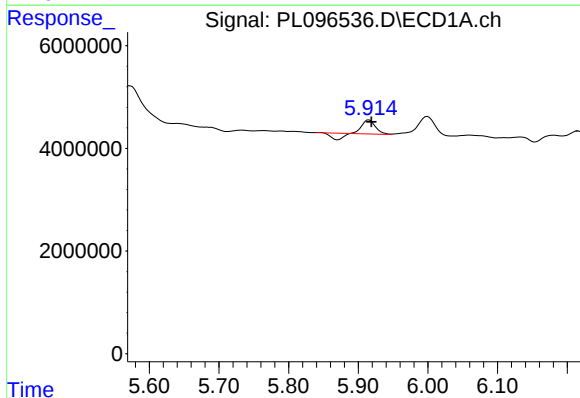


#10 gamma-Chlordane

R.T.: 5.915 min
Delta R.T.: -0.003 min
Response: 2360294
Conc: 0.53 ng/ml

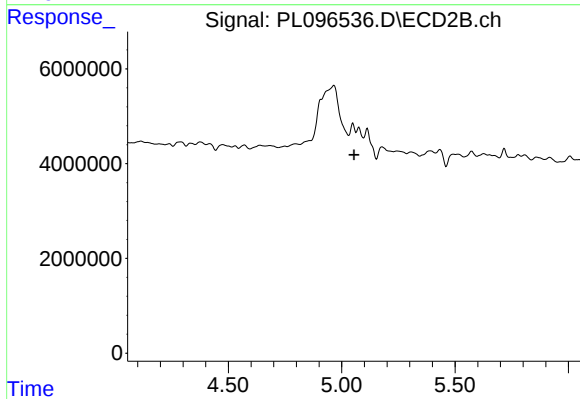

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.054 min
Response: 0
Conc: N.D.

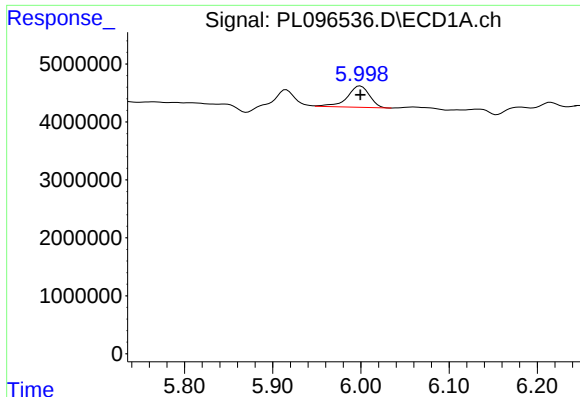

#11 alpha-Chlordane


R.T.: 5.999 min
Delta R.T.: 0.000 min
Response: 6489988
Conc: 1.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3

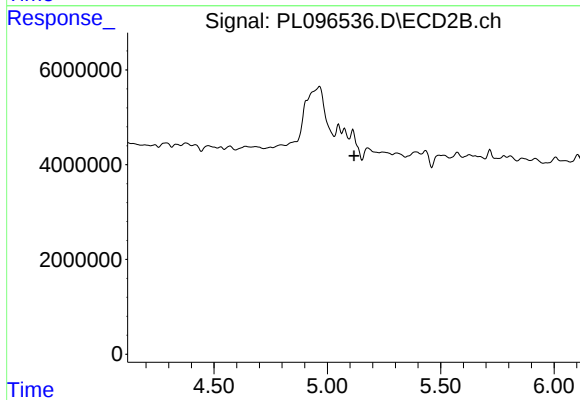


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.119 min
Response: 0
Conc: N.D.

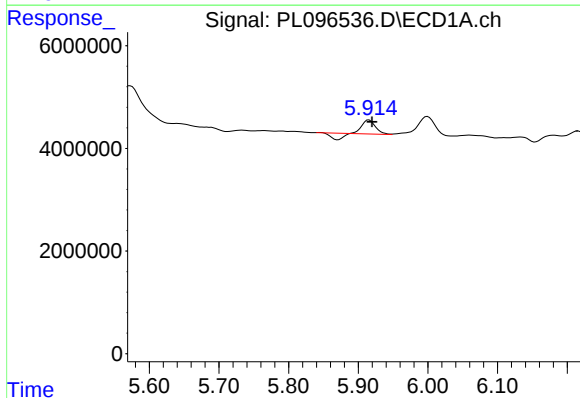


#25 Chlordane-3

R.T.: 5.915 min
Delta R.T.: -0.004 min
Response: 2360294
Conc: 3.20 ng/ml

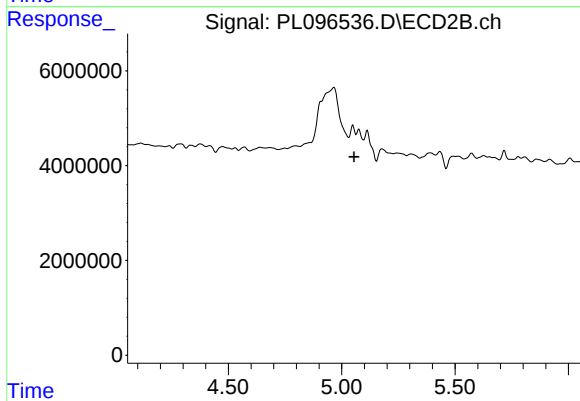

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.055 min
Response: 0
Conc: N.D.

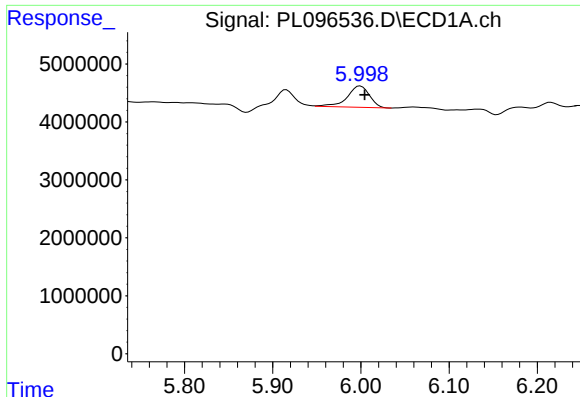

#26 Chlordane-4


R.T.: 5.999 min
Delta R.T.: -0.005 min
Response: 6489988
Conc: 7.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3

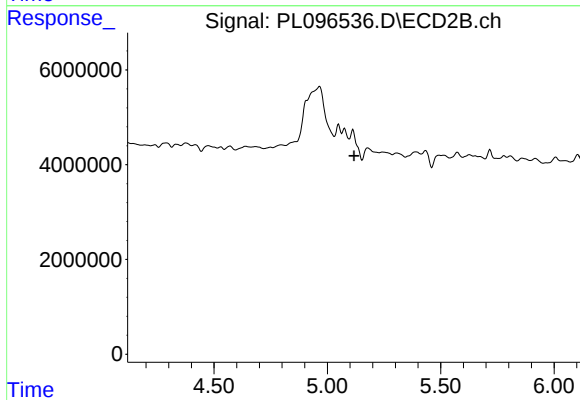


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.118 min
Response: 0
Conc: N.D.

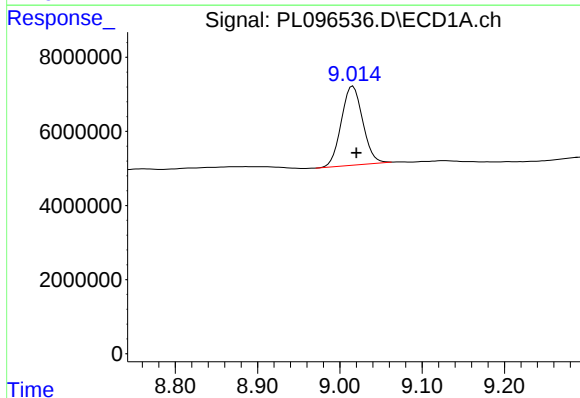

#28 Decachlorobiphenyl

R.T.: 9.016 min
Delta R.T.: -0.004 min
Response: 38512891
Conc: 13.69 ng/ml

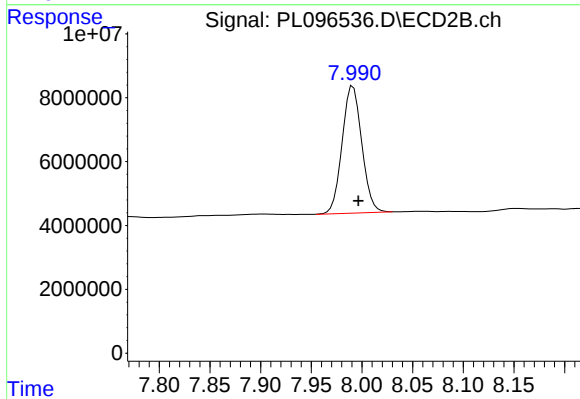

#28 Decachlorobiphenyl

R.T.: 7.991 min
Delta R.T.: -0.005 min
Response: 53621134
Conc: 10.75 ng/ml