

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072325\
 Data File : PL096535.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 15:21
 Operator : AR\AJ
 Sample : Q2668-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-2

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/24/2025
 Supervised By :mohammad ahmed 07/25/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 05:09:02 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 07 15:22:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.533	2.825	44578999	65857126	12.217m	11.411
28) SA Decachlor...	9.020	7.993	32790414	47865038	11.656	9.599

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072325\
Data File : PL096535.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jul 2025 15:21
Operator : AR\AJ
Sample : Q2668-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-2


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/24/2025
Supervised By : mohammad ahmed 07/25/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 05:09:02 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
Quant Title : GC Extractables
QLast Update : Mon Jul 07 15:22:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

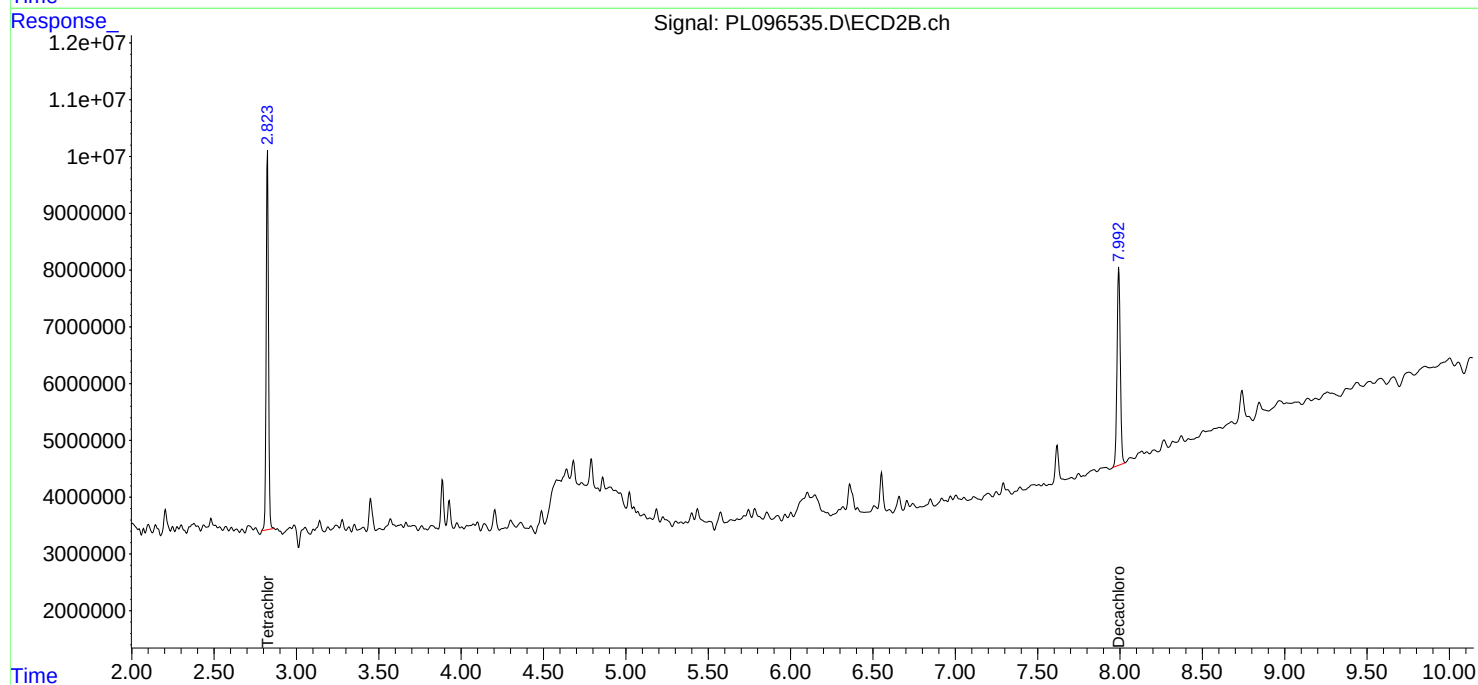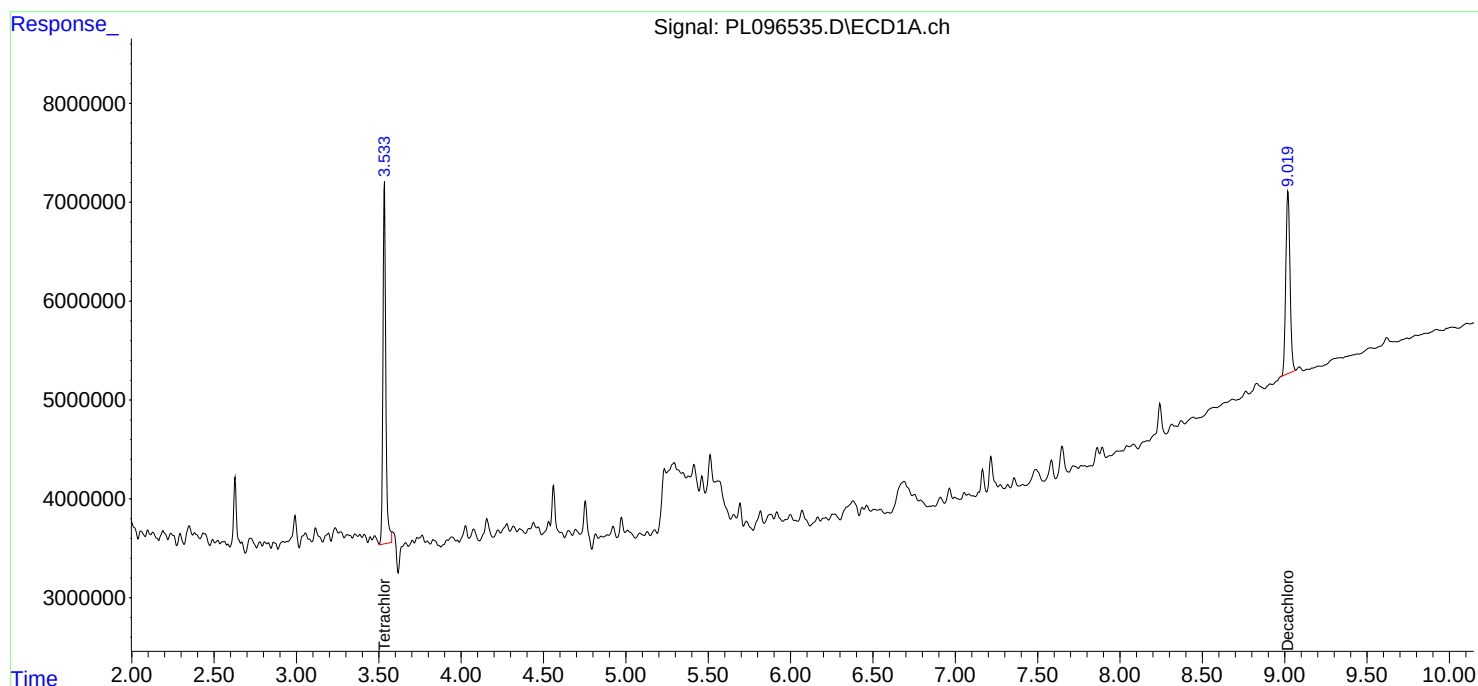

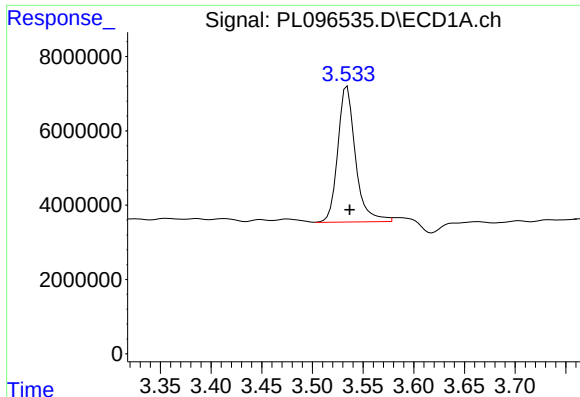


#1 Tetrachloro-m-xylene

R.T.: 3.533 min
Delta R.T.: -0.004 min
Response: 44578999
Conc: 12.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/24/2025
Supervised By :mohammad ahmed 07/25/2025

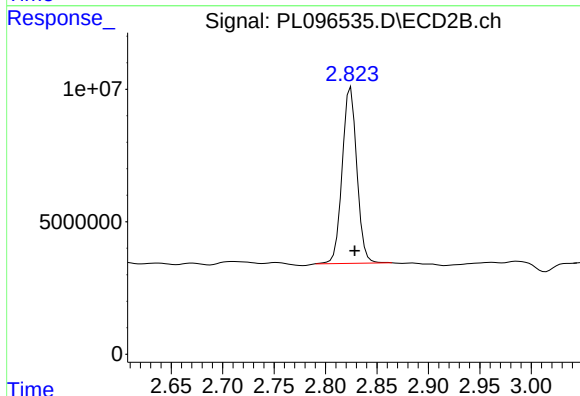


#1 Tetrachloro-m-xylene

R.T.: 2.825 min
Delta R.T.: -0.004 min
Response: 65857126
Conc: 11.41 ng/ml

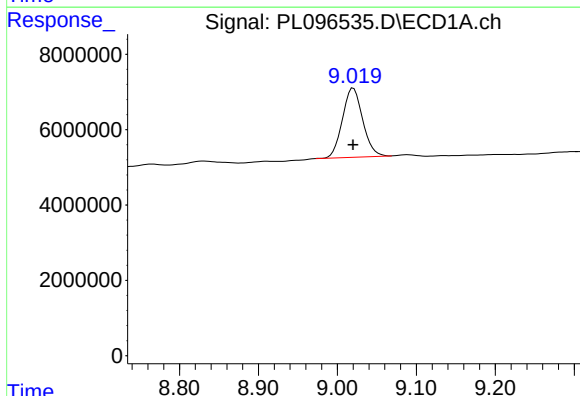

#28 Decachlorobiphenyl

R.T.: 9.020 min
Delta R.T.: 0.000 min
Response: 32790414
Conc: 11.66 ng/ml

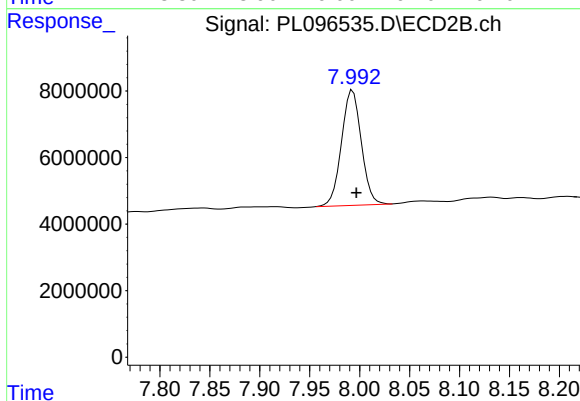

#28 Decachlorobiphenyl

R.T.: 7.993 min
Delta R.T.: -0.003 min
Response: 47865038
Conc: 9.60 ng/ml