

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072420\
 Data File : PL060192.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jul 2020 17:45
 Operator : DD\AJ
 Sample : L3383-29
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 04:30:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.012	35715005	49563096	18.465	18.702
28)	SA Decachlor...	8.222	9.097	29291190	36836003	17.805	17.613
Target Compounds							
3)	MA gamma-BHC...	4.190	0.000	2042863	0	0.827	N.D. #
9)	A Endosulfan I	5.538f	0.000	3224183	0	1.917	N.D. #
10)	B gamma-Chl...	0.000	6.127	0	2647314	N.D.	0.924 #
15)	B Endosulfa...	6.309	6.949	872184	2289389	0.522	0.912 #
17)	MA 4,4'-DDT	6.385	0.000	929245	0	0.715	N.D. #
20)	A Methoxychlor	6.969f	0.000	1526648	0	2.041	N.D. #
23)	Chlordane-1	4.335	0.000	1712829	0	27.957	N.D. #
25)	Chlordane-3	0.000	6.127	0	2647314	N.D.	6.842 #
27)	Chlordane-5	6.309	0.000	872184	0	15.371	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072420\
Data File : PL060192.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2020 17:45
Operator : DD\AJ
Sample : L3383-29
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 04:30:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

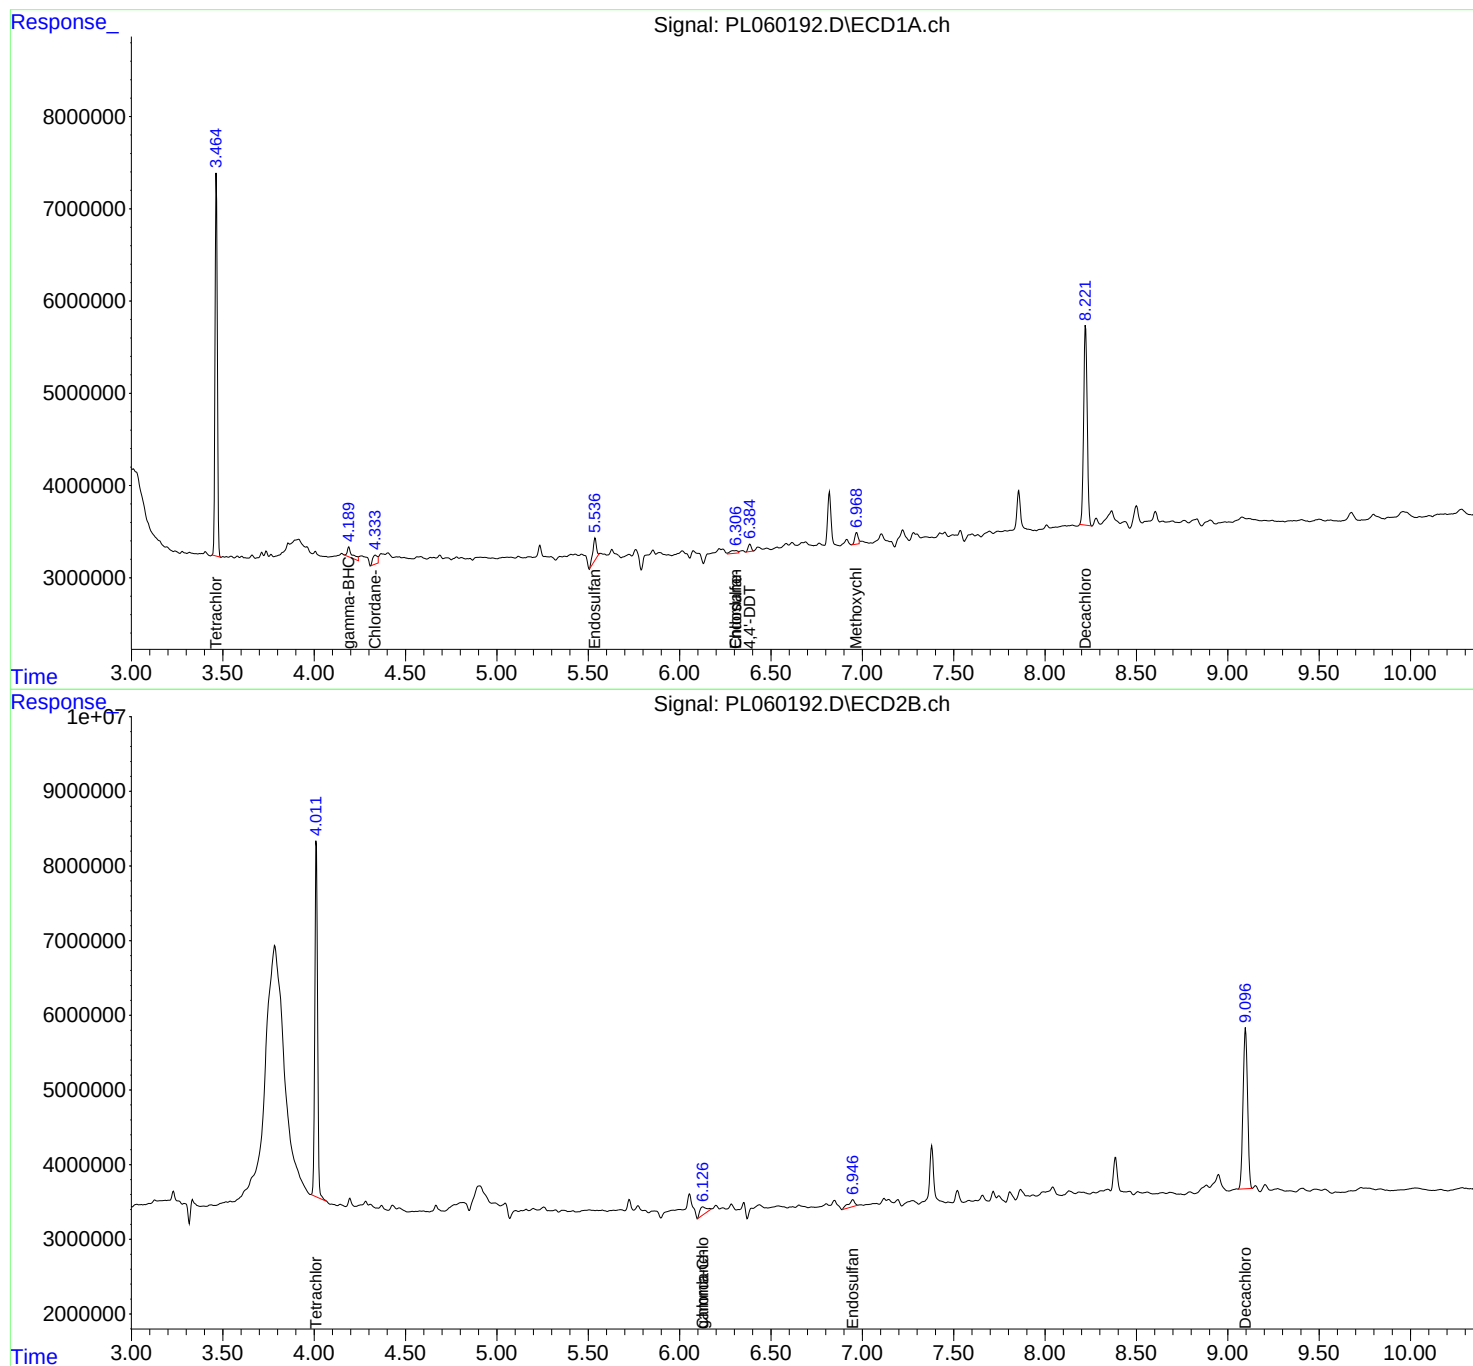


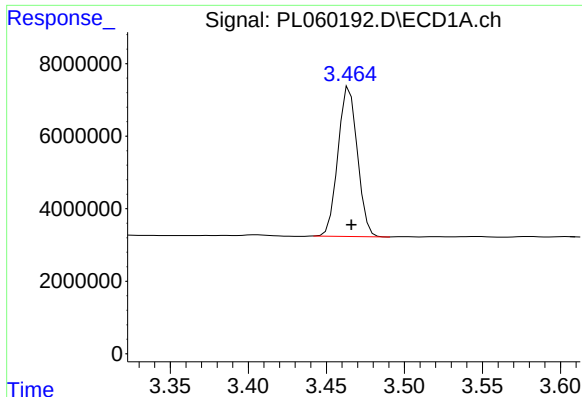

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: -0.001 min
Response: 35715005
Conc: 18.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

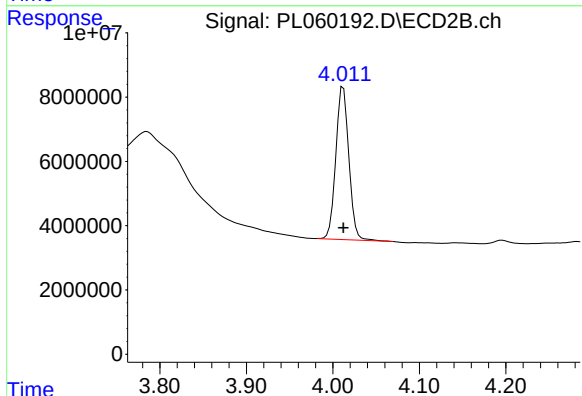


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 49563096
Conc: 18.70 ng/ml

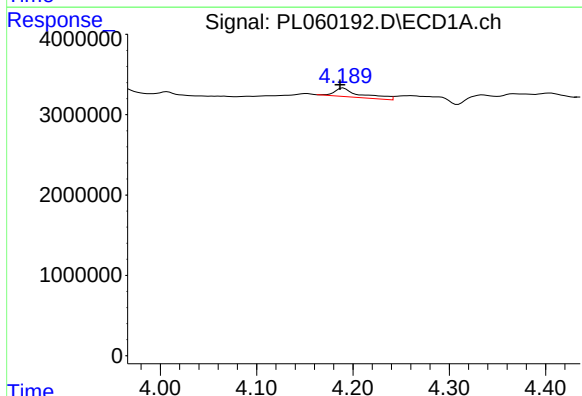


#3 gamma-BHC (Lindane)

R.T.: 4.190 min
Delta R.T.: 0.004 min
Response: 2042863
Conc: 0.83 ng/ml

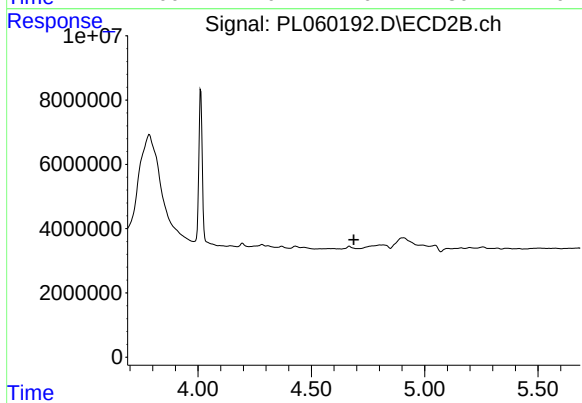

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.687 min
Response: 0
Conc: N.D.

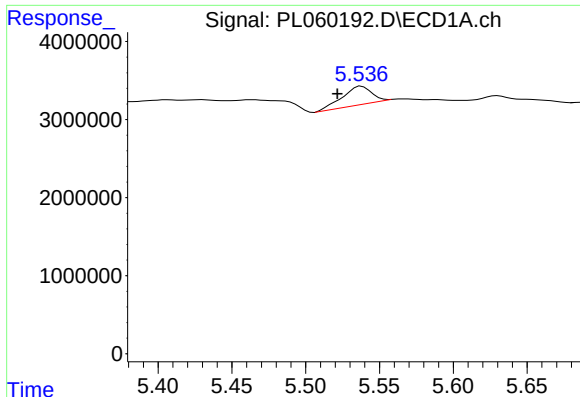

#9 Endosulfan I


R.T.: 5.538 min
Delta R.T.: 0.016 min
Response: 3224183
Conc: 1.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

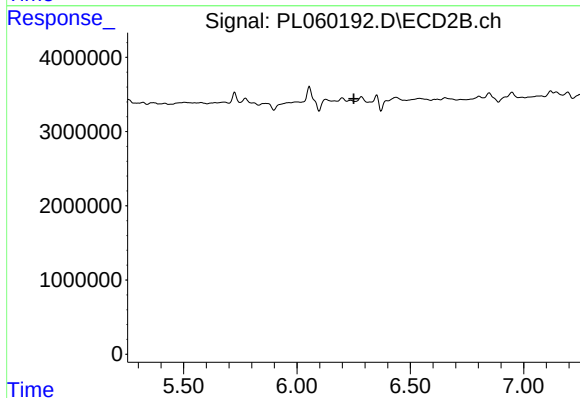


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.250 min
Response: 0
Conc: N.D.

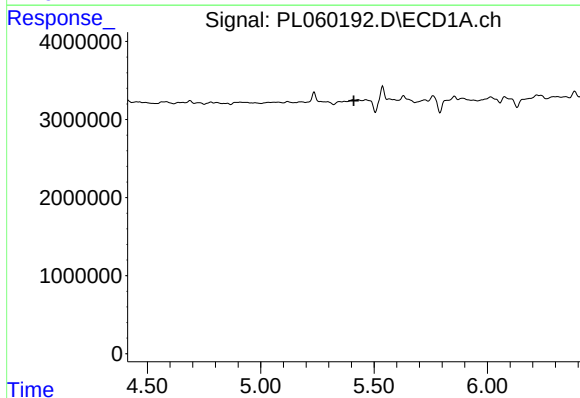


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.410 min
Response: 0
Conc: N.D.

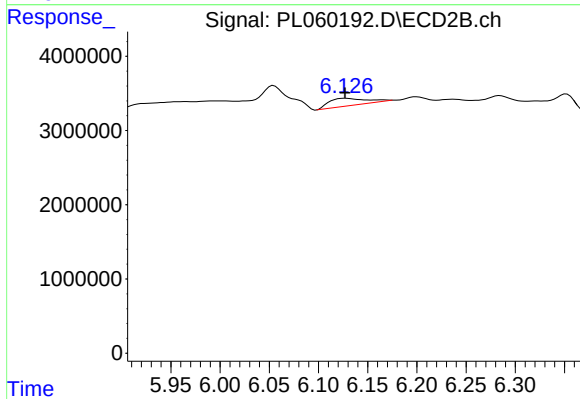

#10 gamma-Chlordane


R.T.: 6.127 min
Delta R.T.: 0.000 min
Response: 2647314
Conc: 0.92 ng/ml

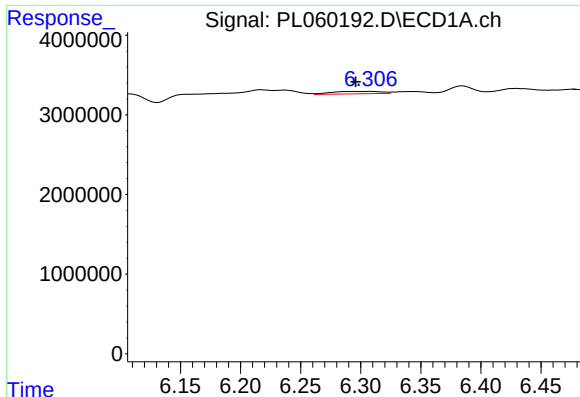

#15 Endosulfan II


R.T.: 6.309 min
Delta R.T.: 0.013 min
Response: 872184
Conc: 0.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

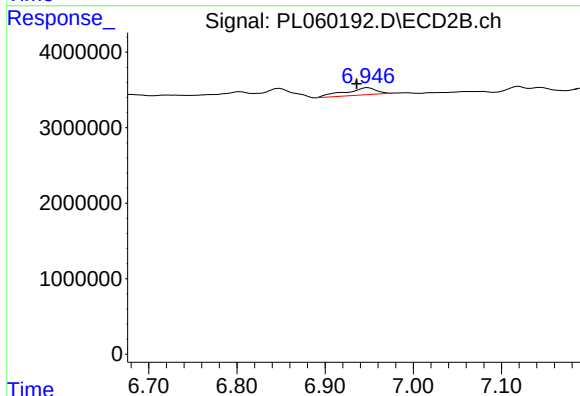


#15 Endosulfan II

R.T.: 6.949 min
Delta R.T.: 0.013 min
Response: 2289389
Conc: 0.91 ng/ml

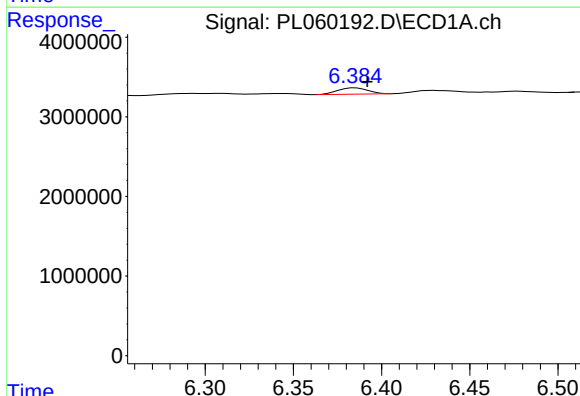


#17 4,4'-DDT

R.T.: 6.385 min
Delta R.T.: -0.007 min
Response: 929245
Conc: 0.71 ng/ml

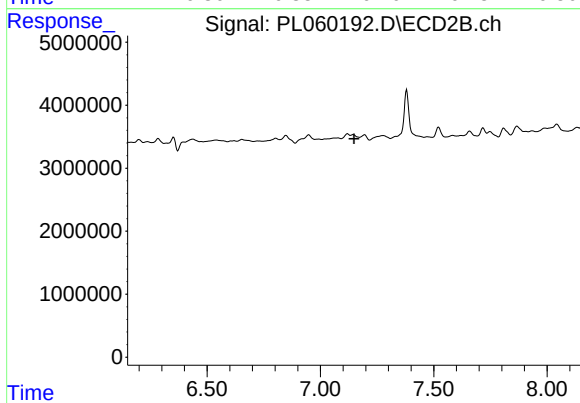

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.149 min
Response: 0
Conc: N.D.

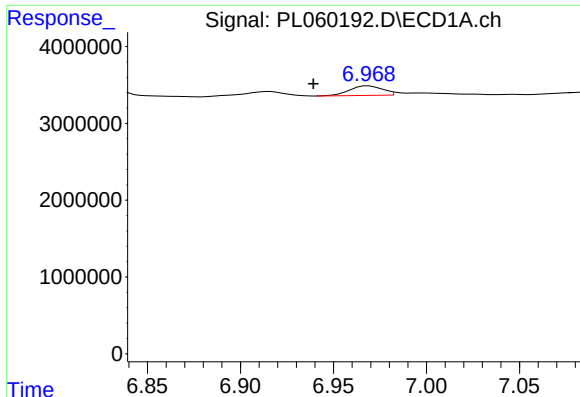

#20 Methoxychlor


R.T.: 6.969 min
Delta R.T.: 0.030 min
Response: 1526648
Conc: 2.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

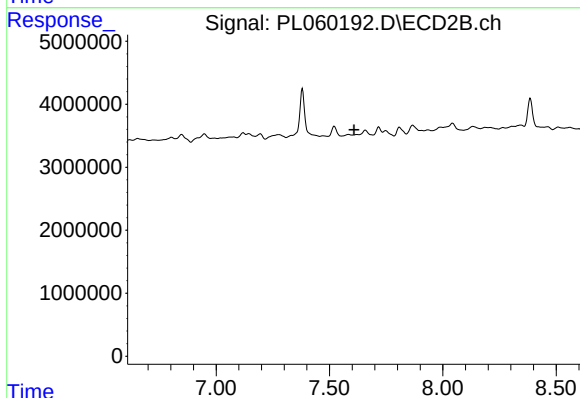


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.609 min
Response: 0
Conc: N.D.

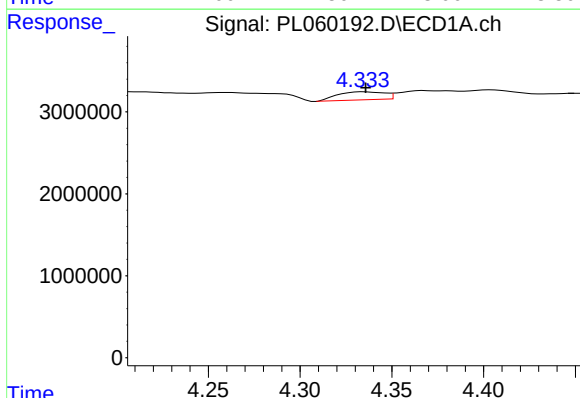


#23 Chlordane-1

R.T.: 4.335 min
Delta R.T.: 0.000 min
Response: 1712829
Conc: 27.96 ng/ml

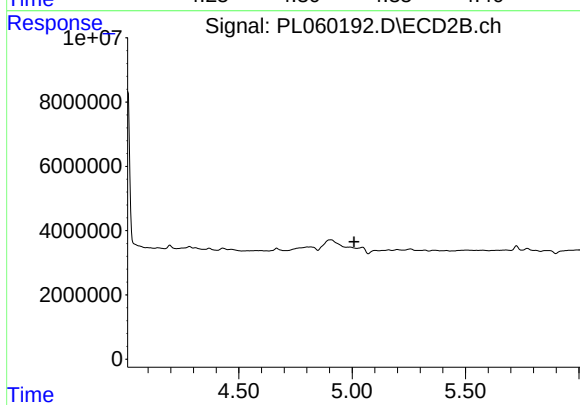

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.009 min
Response: 0
Conc: N.D.

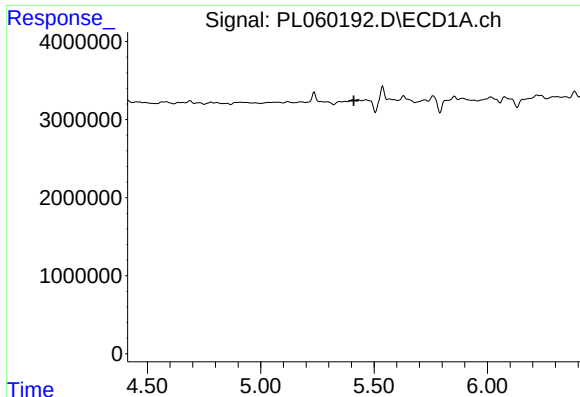

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.411 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

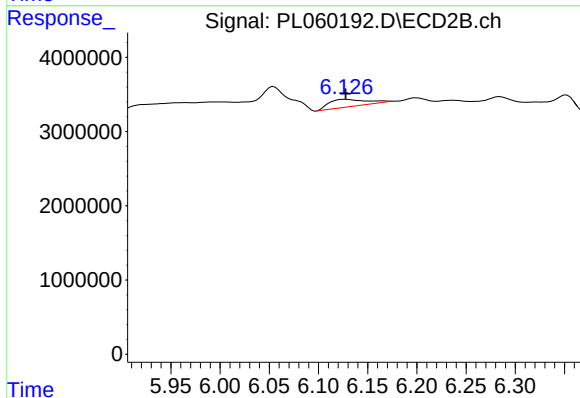


#25 Chlordane-3

R.T.: 6.127 min
Delta R.T.: 0.000 min
Response: 2647314
Conc: 6.84 ng/ml

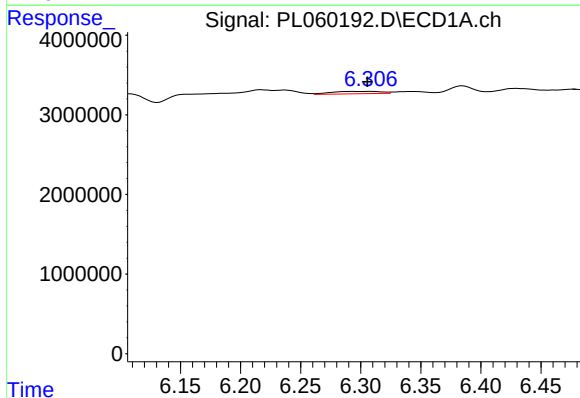


#27 Chlordane-5

R.T.: 6.309 min
Delta R.T.: 0.003 min
Response: 872184
Conc: 15.37 ng/ml

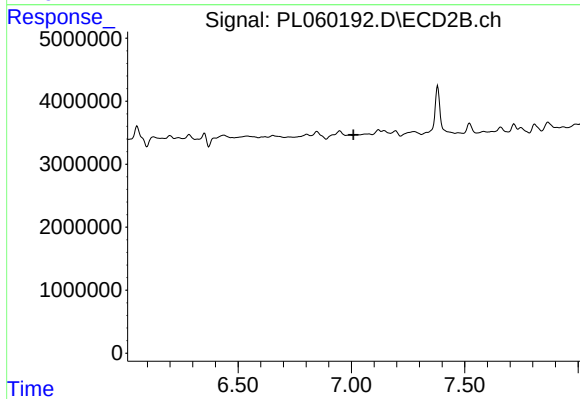

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 7.010 min
Response: 0
Conc: N.D.

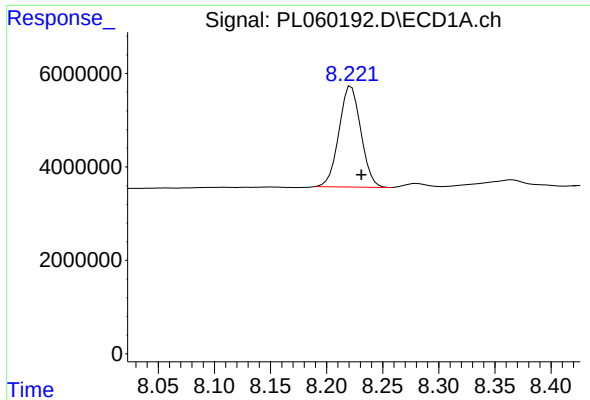

#28 Decachlorobiphenyl

R.T.: 8.222 min
Delta R.T.: -0.009 min
Response: 29291190
Conc: 17.81 ng/ml

Instrument :
ECD_L
ClientSampleId :

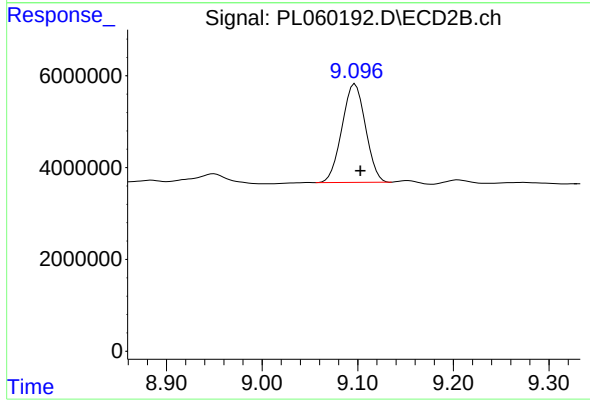

#28 Decachlorobiphenyl

R.T.: 9.097 min
Delta R.T.: -0.005 min
Response: 36836003
Conc: 17.61 ng/ml