

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072420\
 Data File : PL060193.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jul 2020 17:59
 Operator : DD\AJ
 Sample : L3408-02
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 04:30:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.012	25236547	30515038	13.047	11.514
28)	SA Decachlor...	8.224	9.098	23519415	31363753	14.297	14.997
Target Compounds							
10)	B gamma-Chl...	5.426f	0.000	178919	0	0.099	N.D. #
13)	MA Dieldrin	5.755	0.000	2339860	0	1.326	N.D. #
14)	MA Endrin	0.000	6.716	0	2297794	N.D.	1.080 #
17)	MA 4,4'-DDT	6.384	7.119f	1611779	3358394	1.240	1.706 #
19)	B Endosulfa...	6.693	0.000	2070614	0	1.260	N.D. #
25)	Chlordane-3	5.426f	0.000	178919	0	1.058	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072420\
Data File : PL060193.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2020 17:59
Operator : DD\AJ
Sample : L3408-02
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 04:30:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

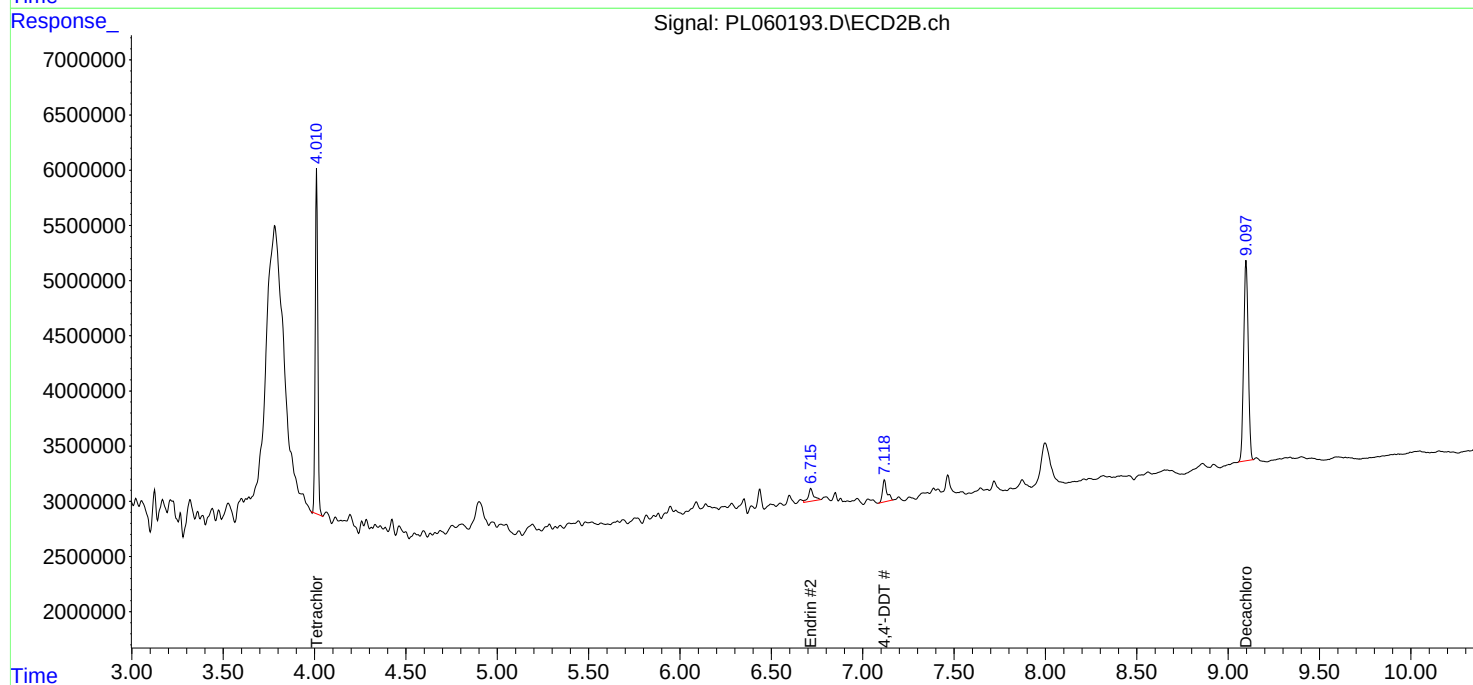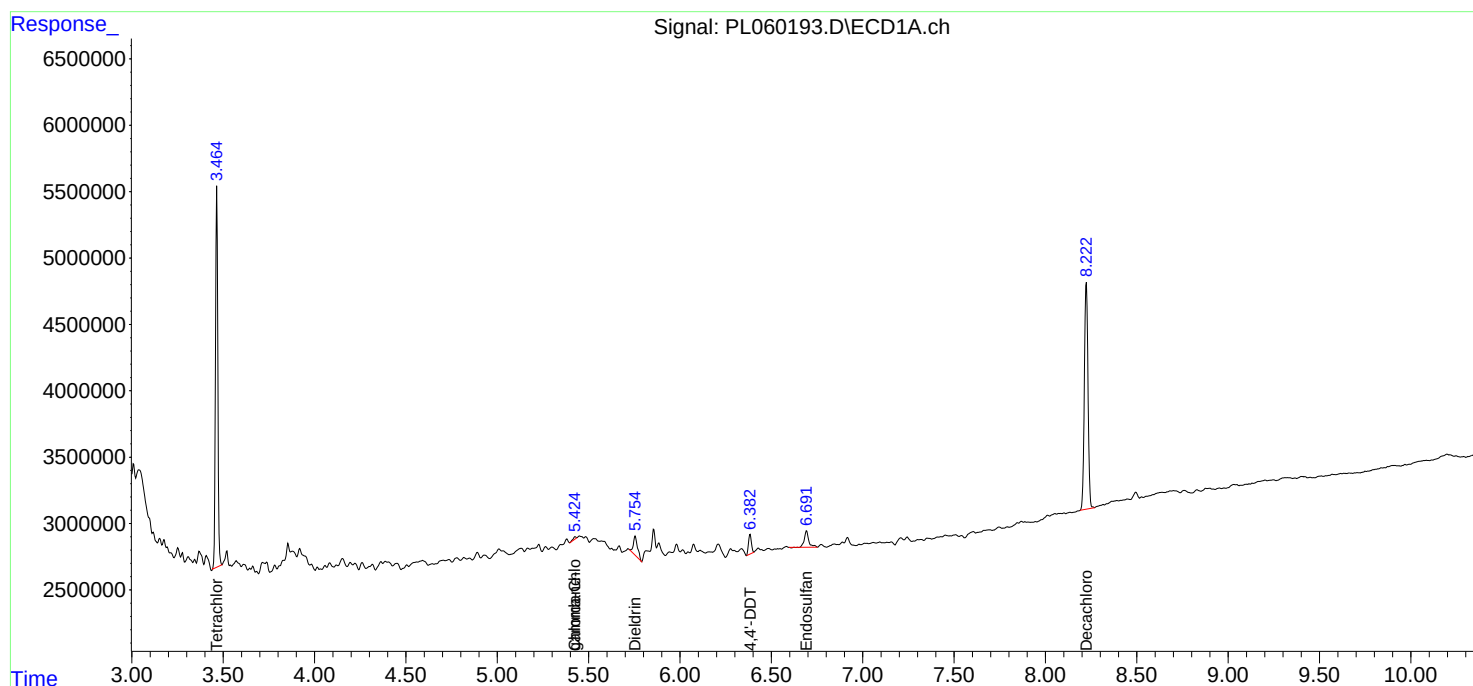


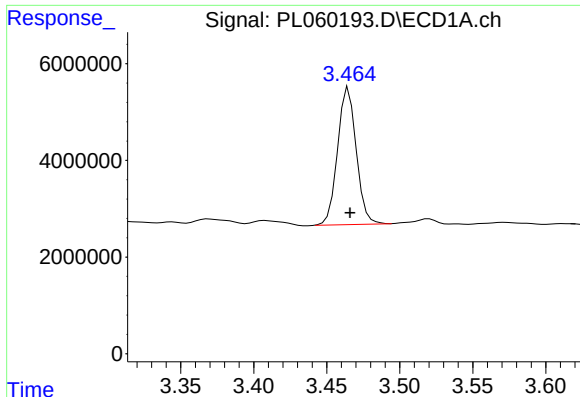

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: -0.001 min
Response: 25236547
Conc: 13.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

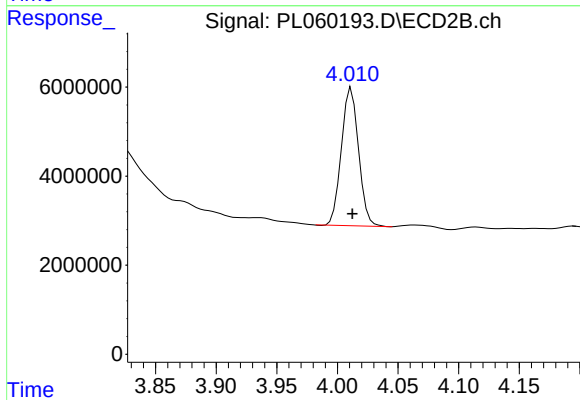


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 30515038
Conc: 11.51 ng/ml

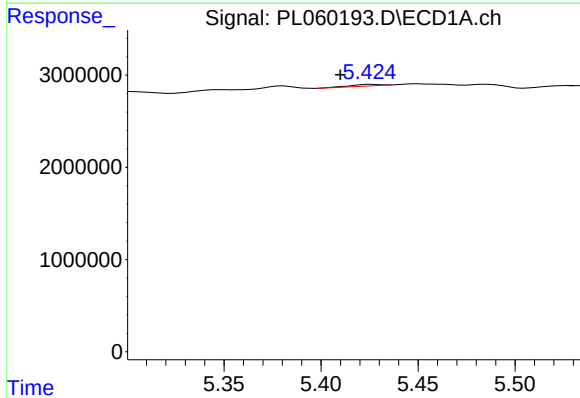


#10 gamma-Chlordane

R.T.: 5.426 min
Delta R.T.: 0.016 min
Response: 178919
Conc: 0.10 ng/ml

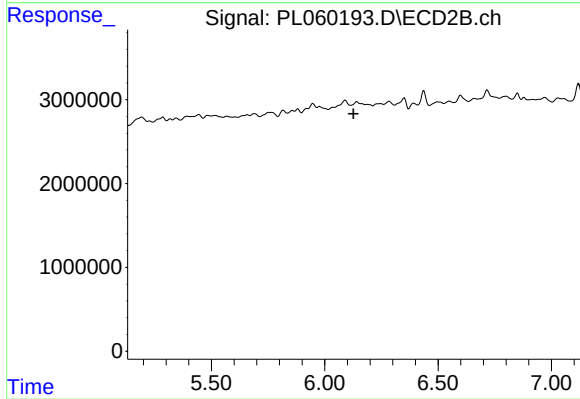

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.127 min
Response: 0
Conc: N.D.

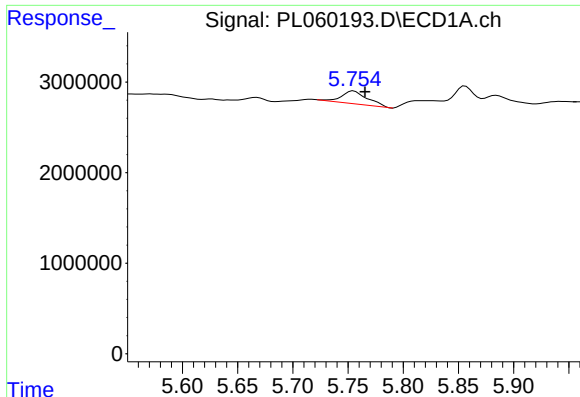

#13 Dieldrin


R.T.: 5.755 min
Delta R.T.: -0.010 min
Response: 2339860
Conc: 1.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

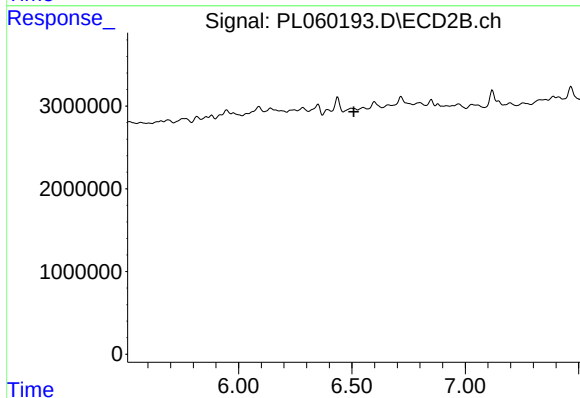


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.508 min
Response: 0
Conc: N.D.

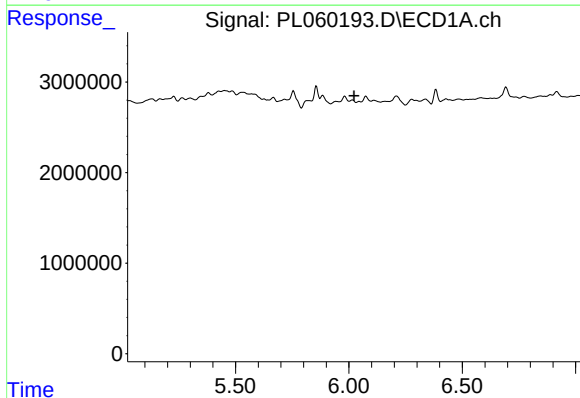


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

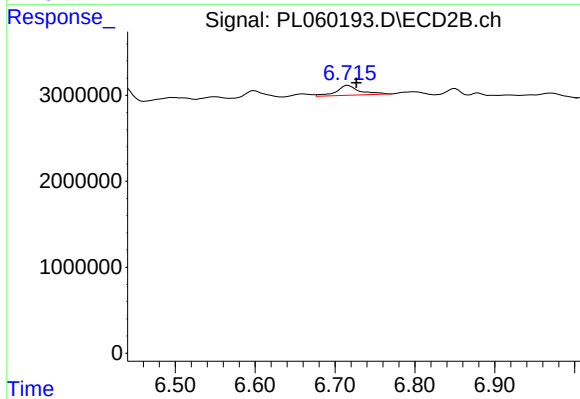

#14 Endrin


R.T.: 6.716 min
Delta R.T.: -0.010 min
Response: 2297794
Conc: 1.08 ng/ml

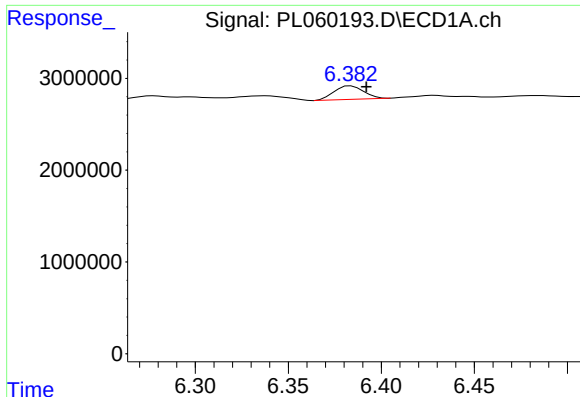

#17 4,4'-DDT


R.T.: 6.384 min
Delta R.T.: -0.008 min
Response: 1611779
Conc: 1.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

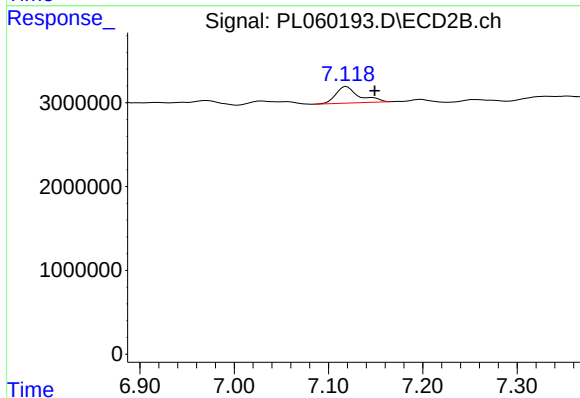


#17 4,4'-DDT

R.T.: 7.119 min
Delta R.T.: -0.030 min
Response: 3358394
Conc: 1.71 ng/ml

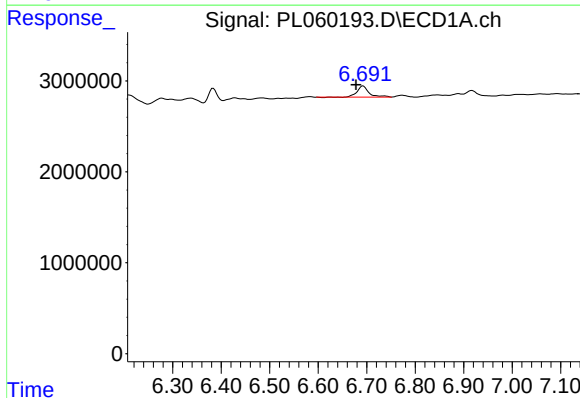


#19 Endosulfan Sulfate

R.T.: 6.693 min
Delta R.T.: 0.015 min
Response: 2070614
Conc: 1.26 ng/ml

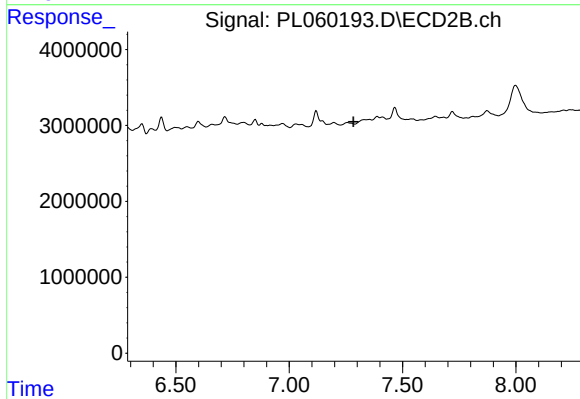

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.284 min
Response: 0
Conc: N.D.

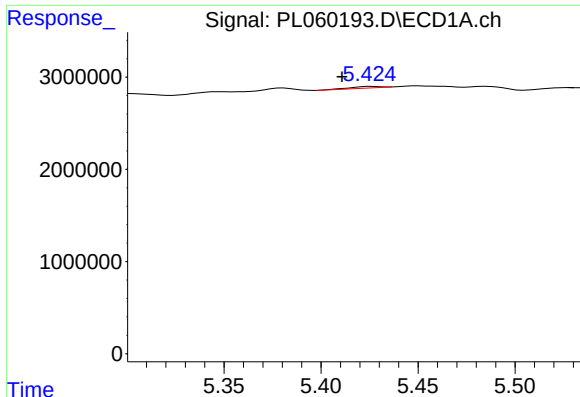

#25 Chlordane-3


R.T.: 5.426 min
Delta R.T.: 0.015 min
Response: 178919
Conc: 1.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

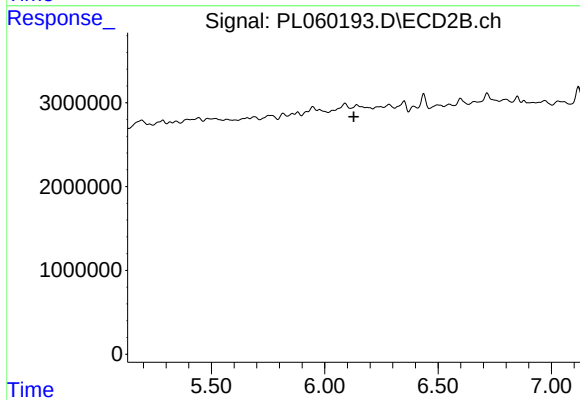


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.128 min
Response: 0
Conc: N.D.

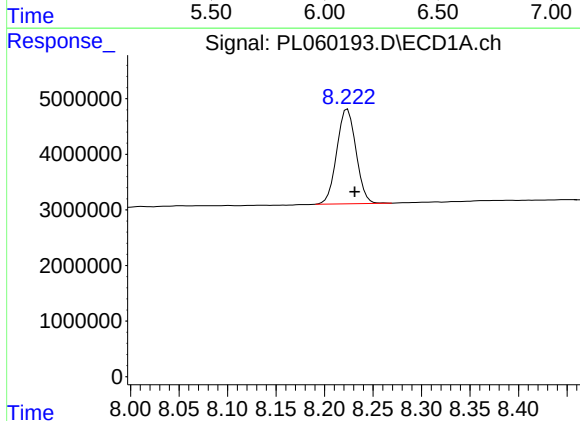

#28 Decachlorobiphenyl

R.T.: 8.224 min
Delta R.T.: -0.007 min
Response: 23519415
Conc: 14.30 ng/ml

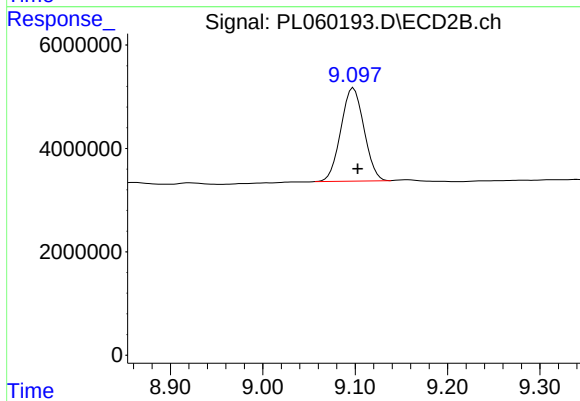

#28 Decachlorobiphenyl

R.T.: 9.098 min
Delta R.T.: -0.005 min
Response: 31363753
Conc: 15.00 ng/ml