

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072420\
 Data File : PL060211.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jul 2020 22:14
 Operator : DD\AJ
 Sample : L3383-07
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 04:34:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.466	4.012	38974875	53432509	20.150	20.162
28)	SA Decachlor...	8.223	9.096	28735897	37571611	17.468	17.965
Target Compounds							
10)	B gamma-Chl...	0.000	6.105f	0	1049293	N.D.	0.366 #
25)	Chlordane-3	0.000	6.105f	0	1049293	N.D.	2.712 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072420\
Data File : PL060211.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2020 22:14
Operator : DD\AJ
Sample : L3383-07
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 04:34:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

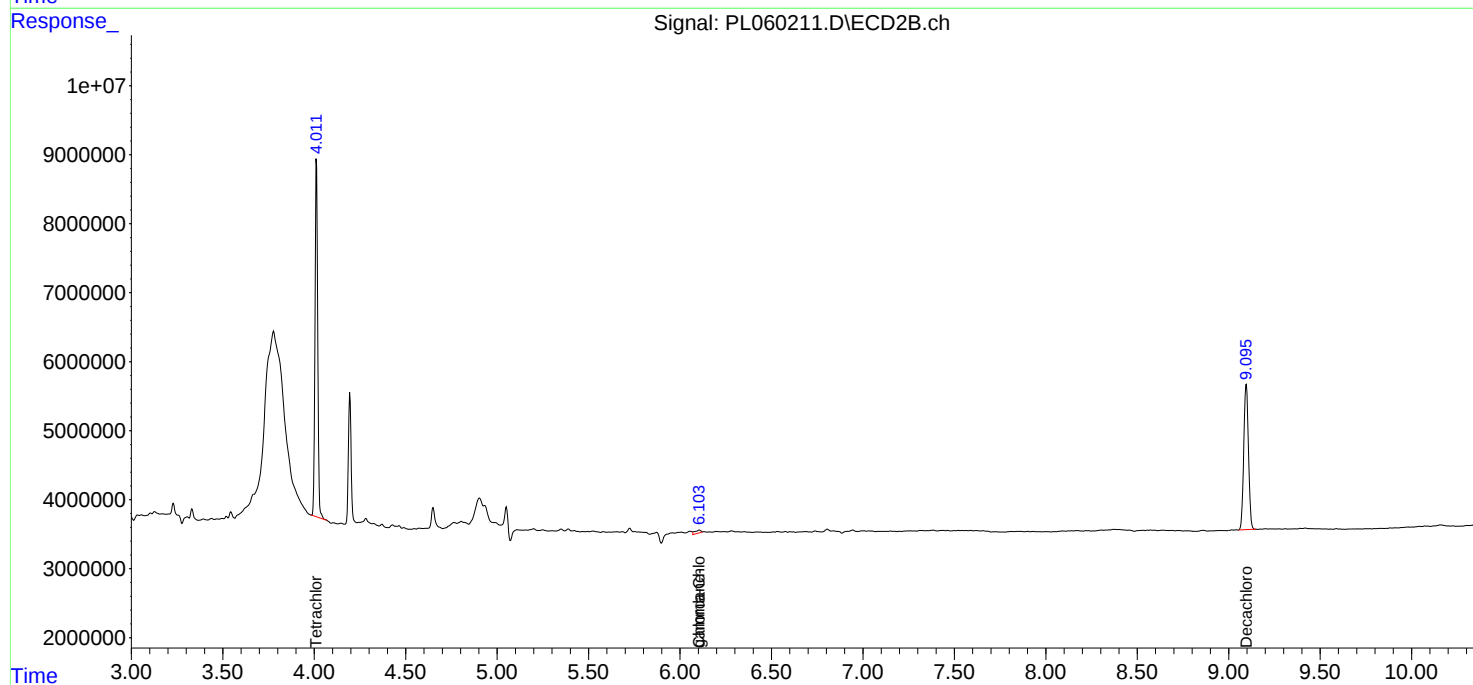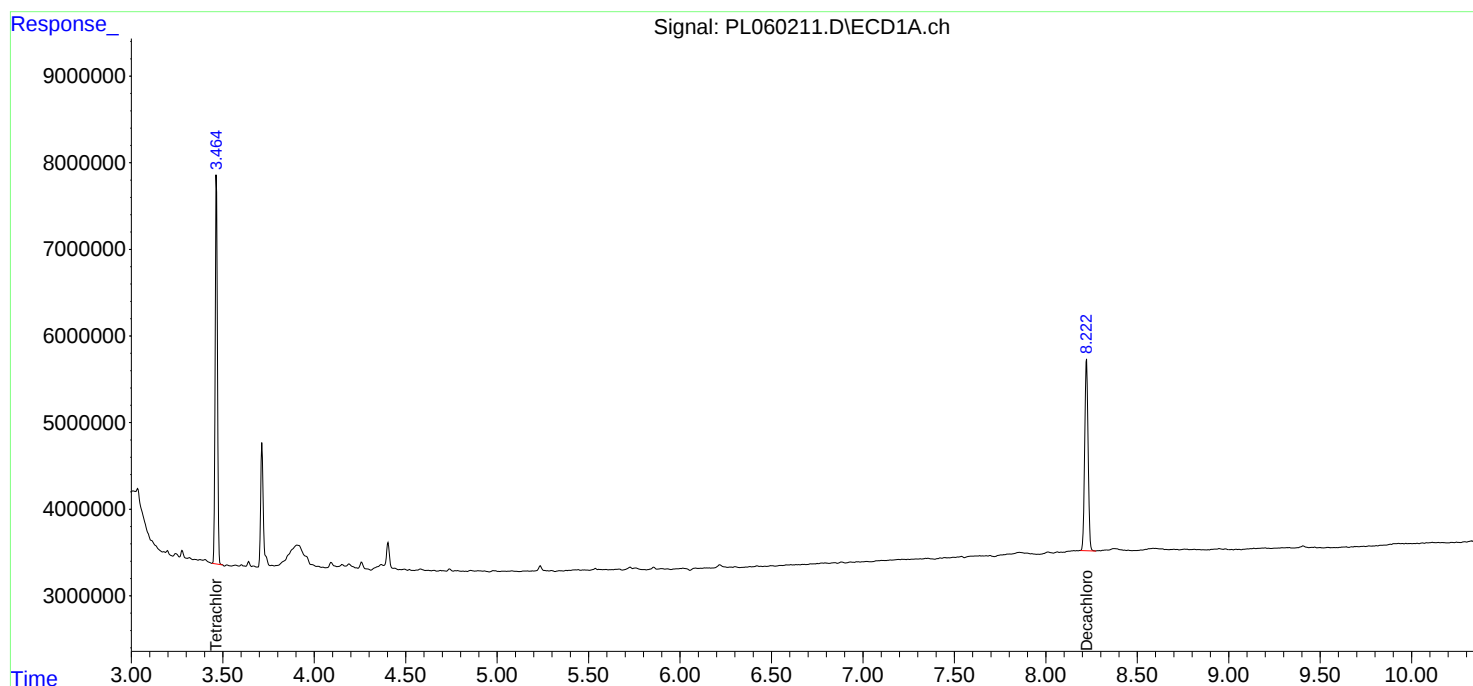


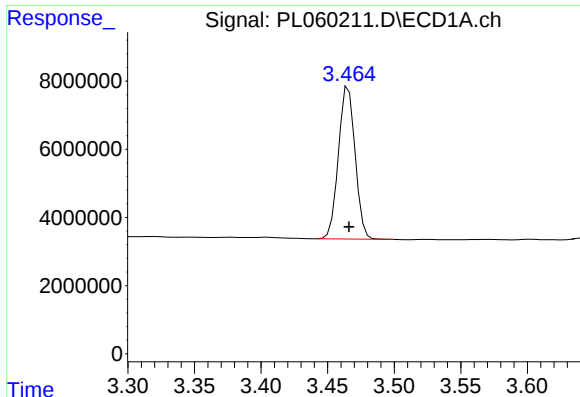

#1 Tetrachloro-m-xylene


R.T.: 3.466 min
Delta R.T.: 0.000 min
Response: 38974875
Conc: 20.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

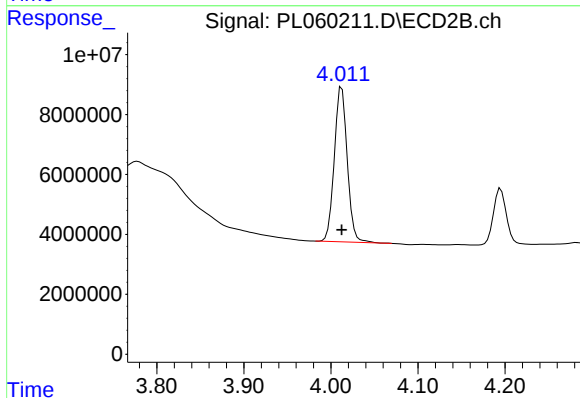


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 53432509
Conc: 20.16 ng/ml

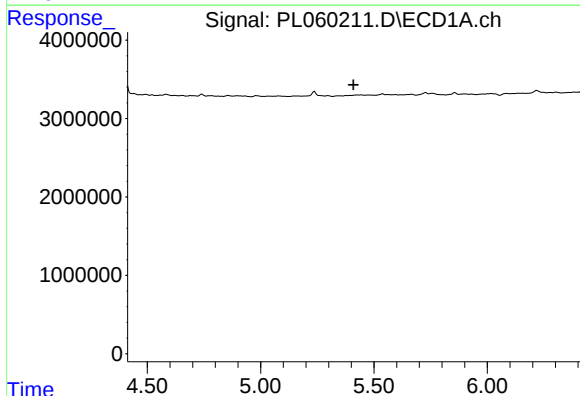


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.410 min
Response: 0
Conc: N.D.

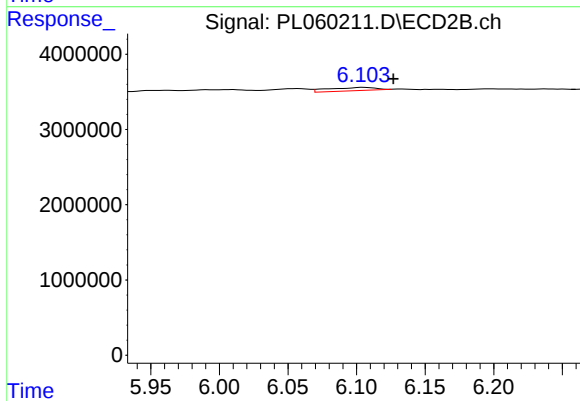

#10 gamma-Chlordane


R.T.: 6.105 min
Delta R.T.: -0.022 min
Response: 1049293
Conc: 0.37 ng/ml

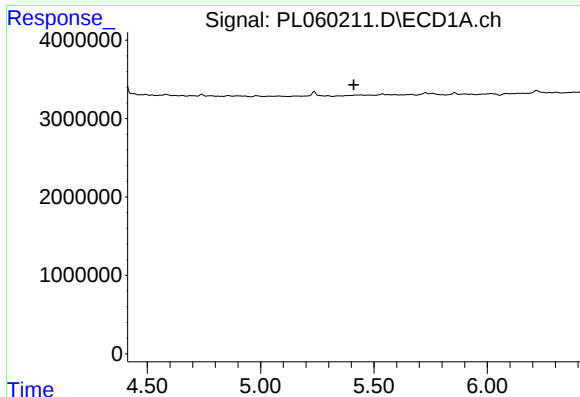

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.411 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

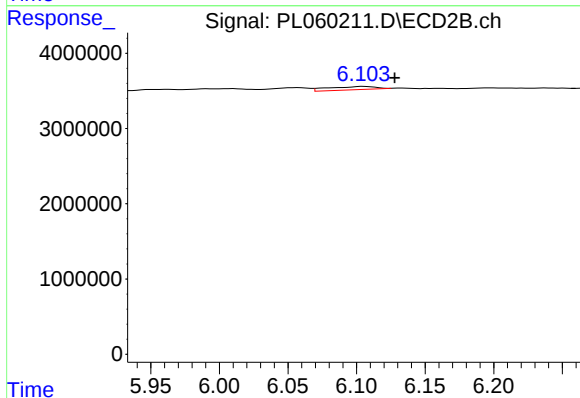


#25 Chlordane-3

R.T.: 6.105 min
Delta R.T.: -0.023 min
Response: 1049293
Conc: 2.71 ng/ml

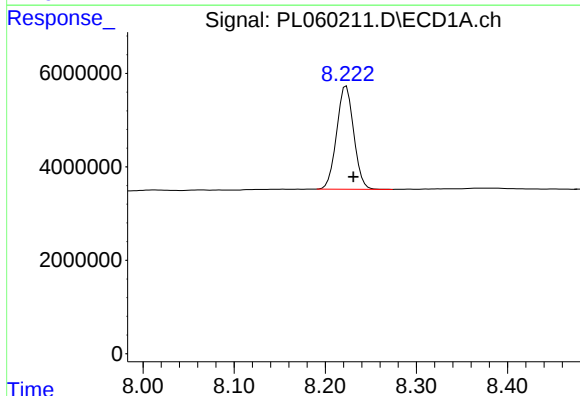

#28 Decachlorobiphenyl

R.T.: 8.223 min
Delta R.T.: -0.008 min
Response: 28735897
Conc: 17.47 ng/ml

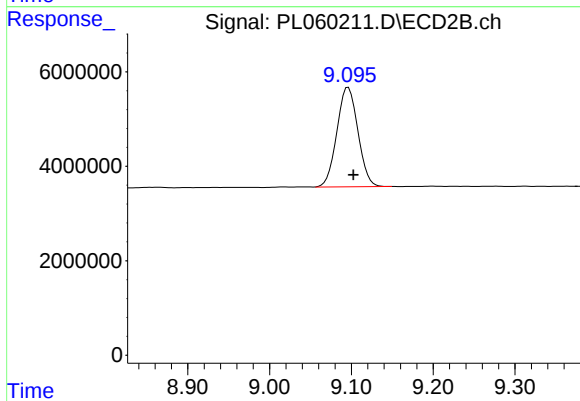

#28 Decachlorobiphenyl

R.T.: 9.096 min
Delta R.T.: -0.006 min
Response: 37571611
Conc: 17.96 ng/ml