

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072420\
 Data File : PL060213.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jul 2020 22:42
 Operator : DD\AJ
 Sample : L3383-15
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 04:35:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.013	39854527	58667640	20.605	22.137
28)	SA Decachlor...	8.223	9.096	27426531	35782952	16.672	17.110
Target Compounds							
3)	MA gamma-BHC...	0.000	4.685	0	4688299	N.D.	1.293 #
4)	MA Heptachlor	0.000	5.206	0	227442	N.D.	0.068 #
8)	B Heptachlo...	5.157f	0.000	2566696	0	1.398	N.D. #
10)	B gamma-Chl...	0.000	6.125	0	332526	N.D.	0.116 #
25)	Chlordane-3	0.000	6.125	0	332526	N.D.	0.859 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072420\
Data File : PL060213.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2020 22:42
Operator : DD\AJ
Sample : L3383-15
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 04:35:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

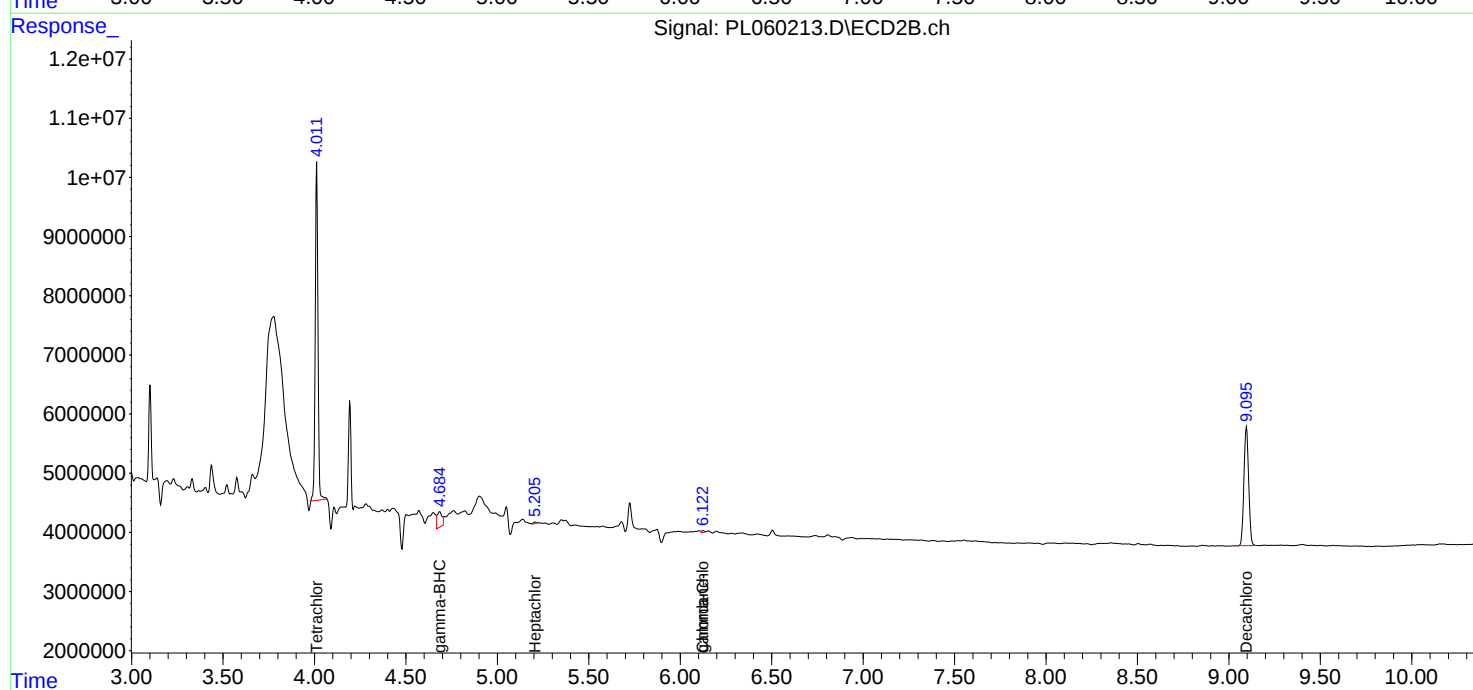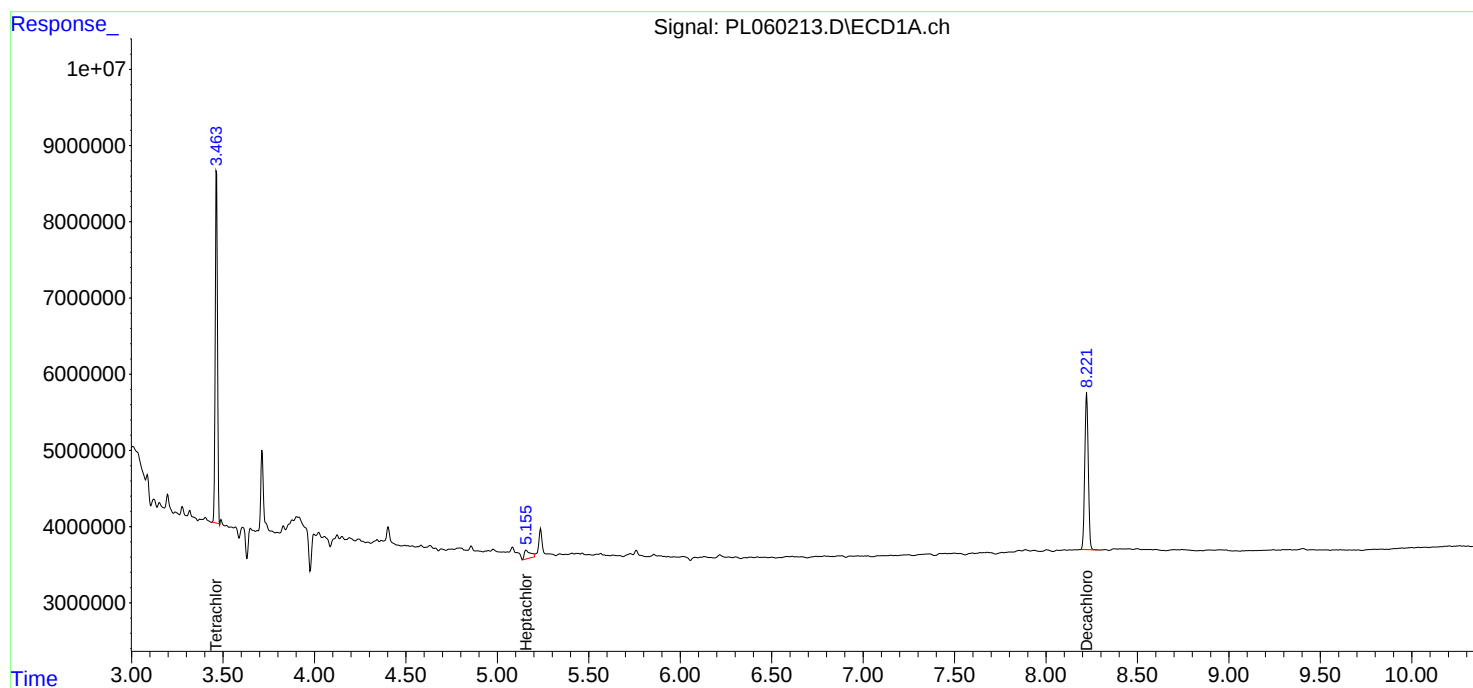


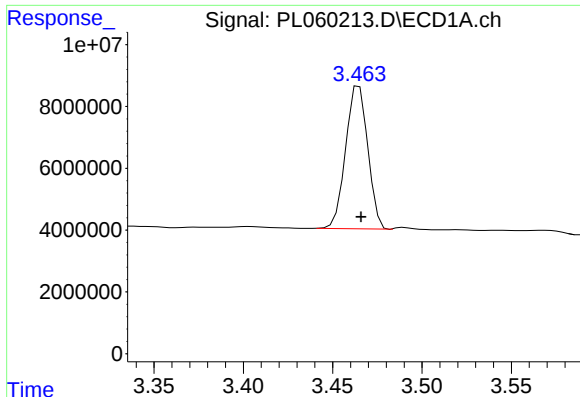

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: -0.001 min
Response: 39854527
Conc: 20.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

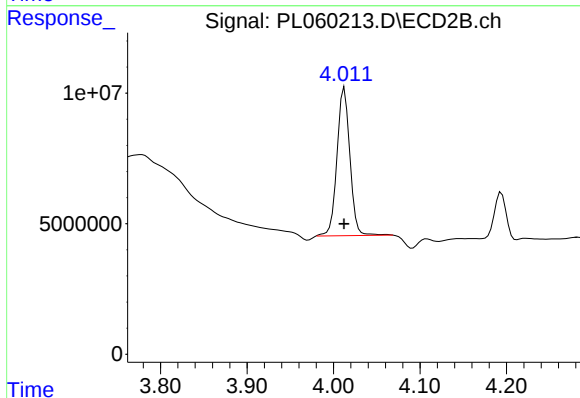


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 58667640
Conc: 22.14 ng/ml

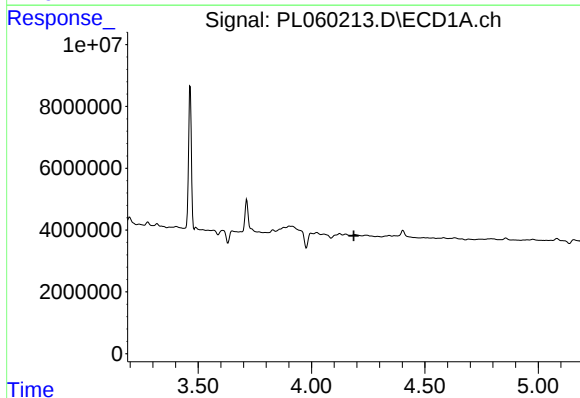


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.187 min
Response: 0
Conc: N.D.

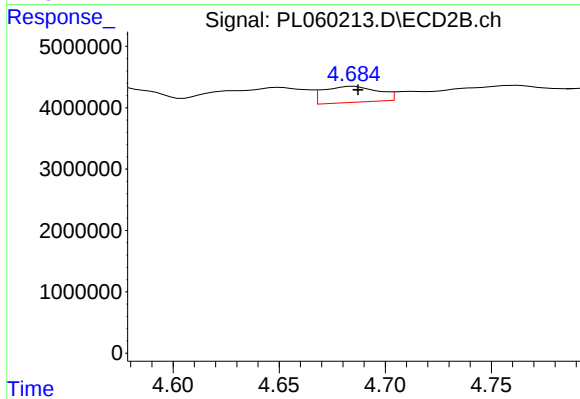

#3 gamma-BHC (Lindane)


R.T.: 4.685 min
Delta R.T.: -0.002 min
Response: 4688299
Conc: 1.29 ng/ml

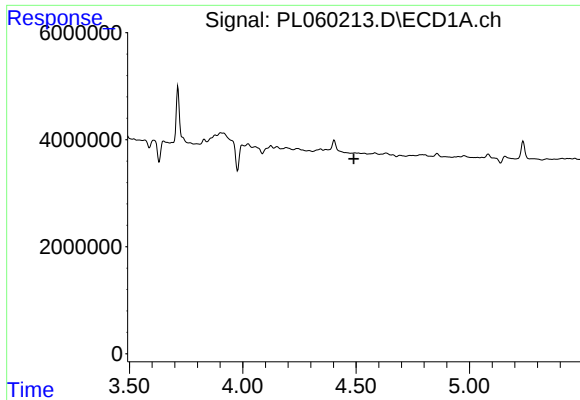

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.490 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

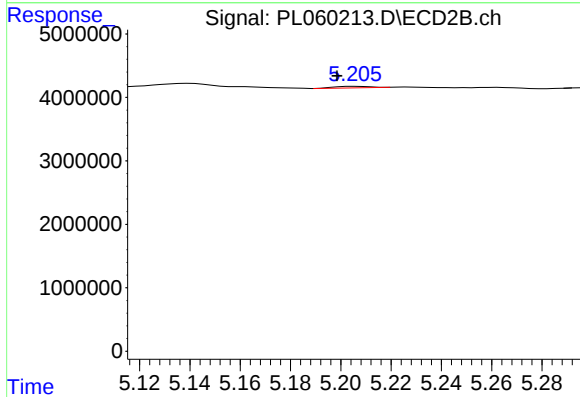


#4 Heptachlor

R.T.: 5.206 min
Delta R.T.: 0.007 min
Response: 227442
Conc: 0.07 ng/ml

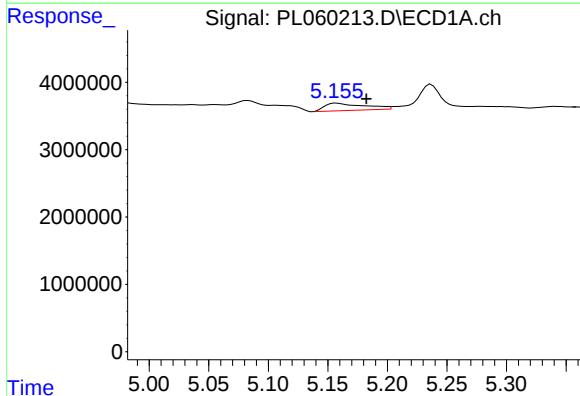


#8 Heptachlor epoxide

R.T.: 5.157 min
Delta R.T.: -0.025 min
Response: 2566696
Conc: 1.40 ng/ml

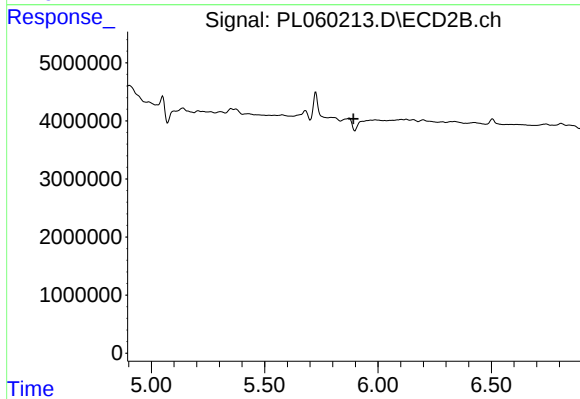

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.892 min
Response: 0
Conc: N.D.

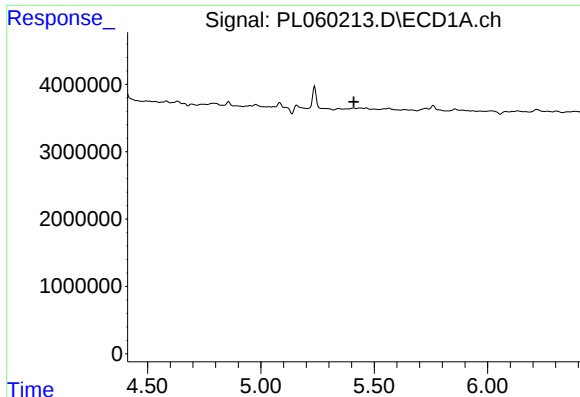

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.410 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

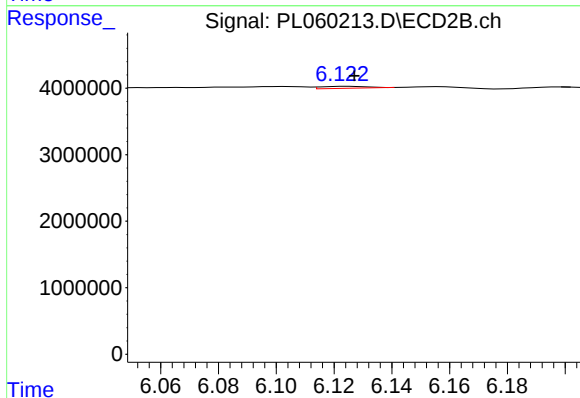


#10 gamma-Chlordane

R.T.: 6.125 min
Delta R.T.: -0.002 min
Response: 332526
Conc: 0.12 ng/ml

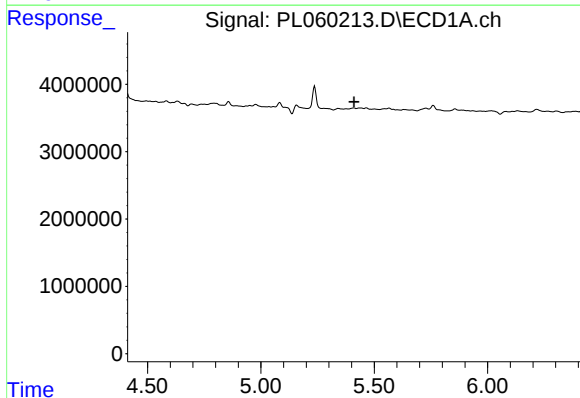


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.411 min
Response: 0
Conc: N.D.

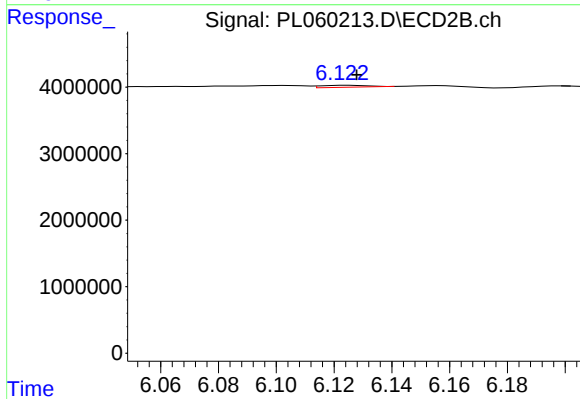

#25 Chlordane-3


R.T.: 6.125 min
Delta R.T.: -0.003 min
Response: 332526
Conc: 0.86 ng/ml

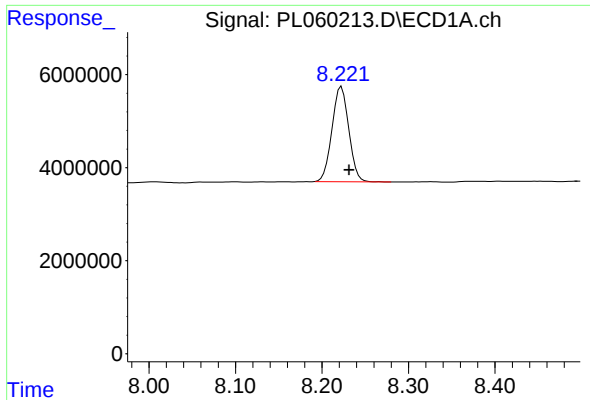

#28 Decachlorobiphenyl

R.T.: 8.223 min
Delta R.T.: -0.008 min
Response: 27426531
Conc: 16.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

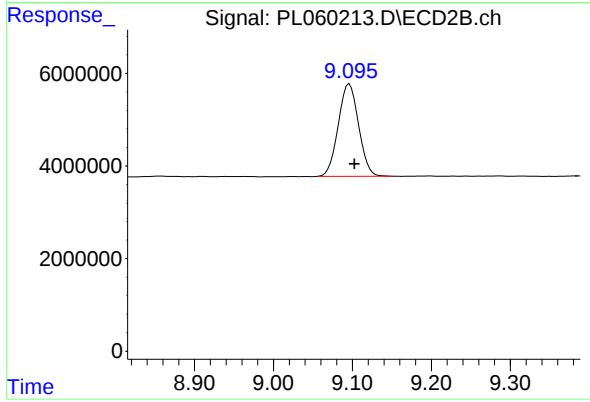

#28 Decachlorobiphenyl

R.T.: 9.096 min
Delta R.T.: -0.007 min
Response: 35782952
Conc: 17.11 ng/ml