

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072420\
 Data File : PL060218.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jul 2020 23:53
 Operator : DD\AJ
 Sample : L3414-04
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 04:35:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.012	38933897	53473387	20.129	20.177
28)	SA Decachlor...	8.222	9.096	32742795	42070172	19.903	20.116
Target Compounds							
10)	B gamma-Chl...	0.000	6.108f	0	1712194	N.D.	0.598 #
25)	Chlordane-3	0.000	6.108f	0	1712194	N.D.	4.425 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072420\
Data File : PL060218.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2020 23:53
Operator : DD\AJ
Sample : L3414-04
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 04:35:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

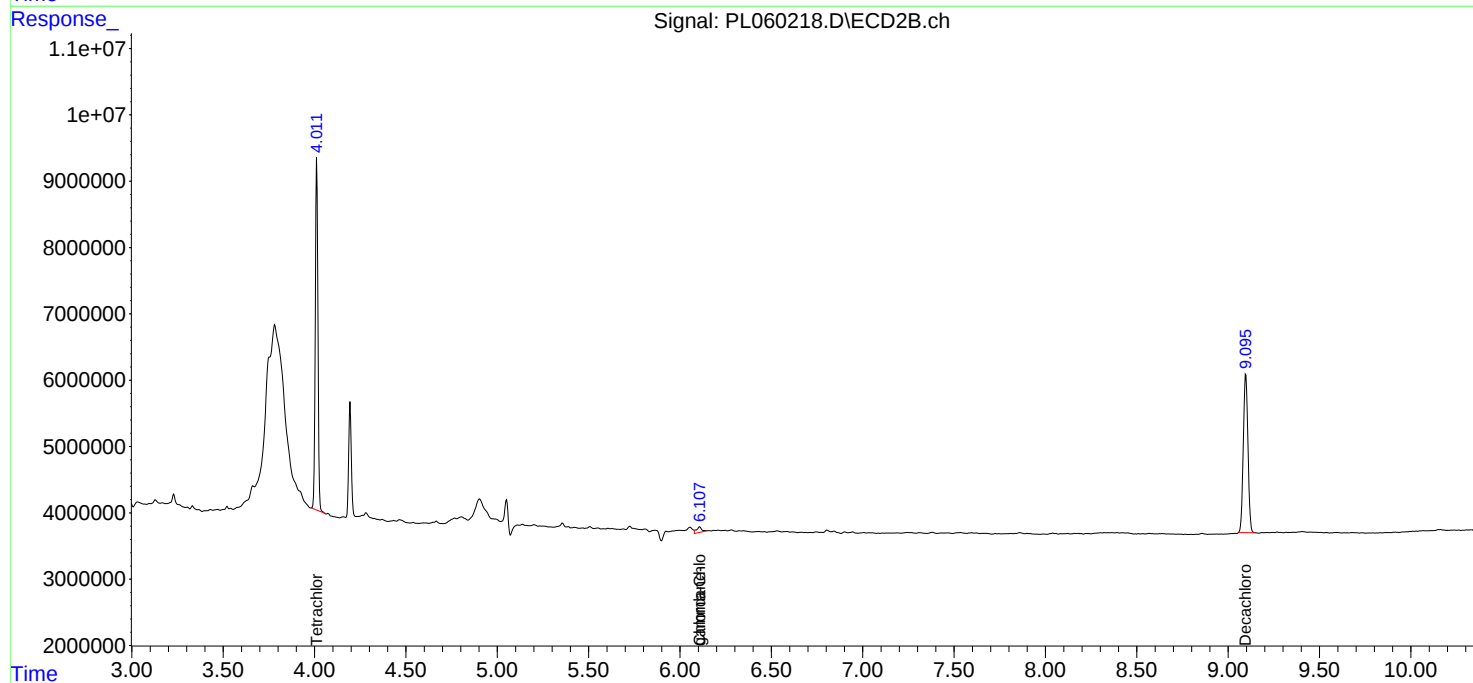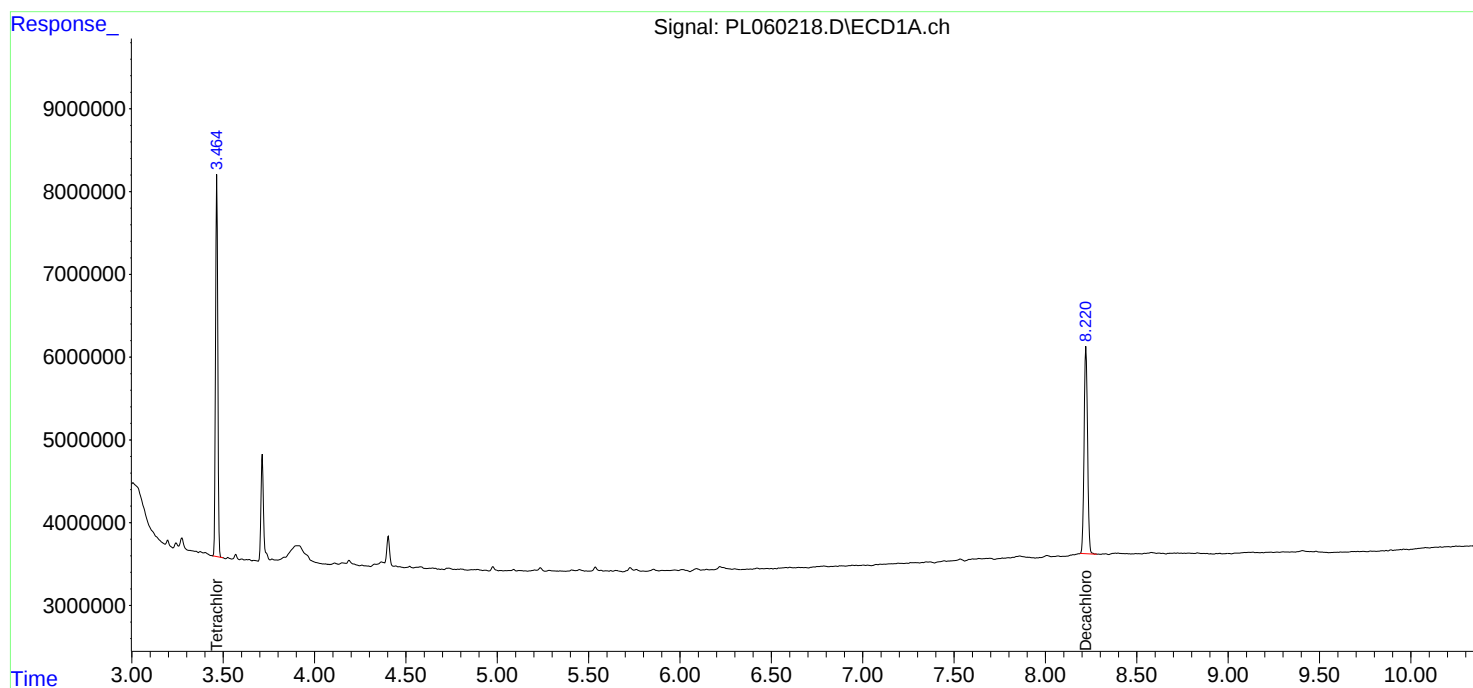


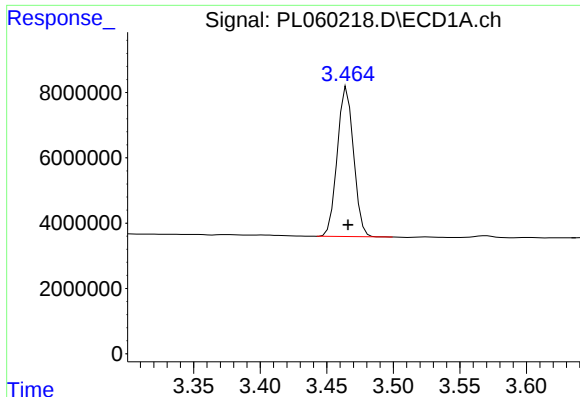

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: 0.000 min
Response: 38933897
Conc: 20.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

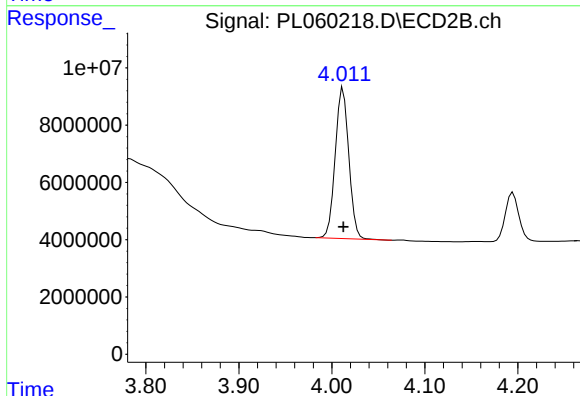


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 53473387
Conc: 20.18 ng/ml

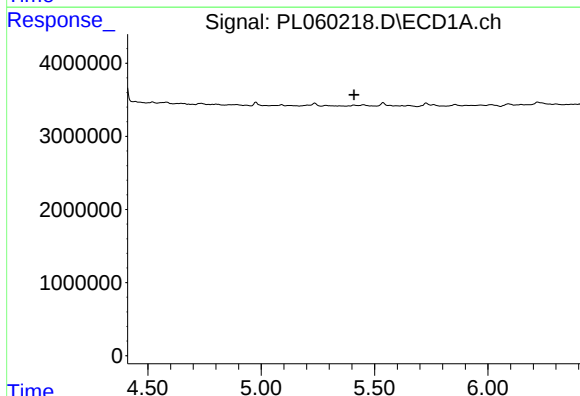


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.410 min
Response: 0
Conc: N.D.

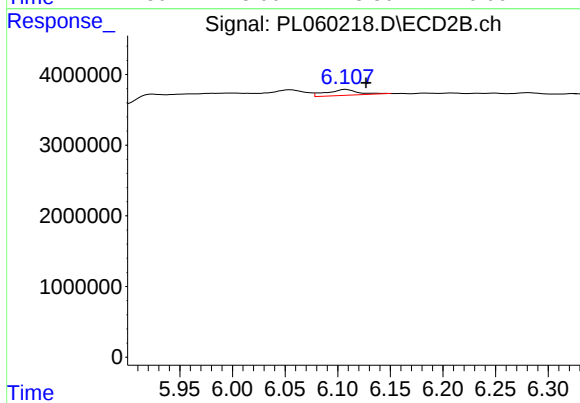

#10 gamma-Chlordane


R.T.: 6.108 min
Delta R.T.: -0.019 min
Response: 1712194
Conc: 0.60 ng/ml

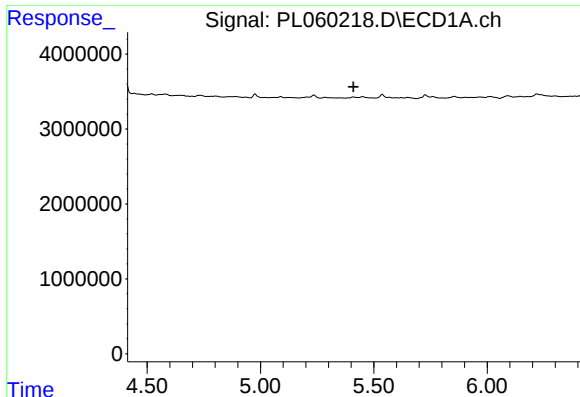

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.411 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

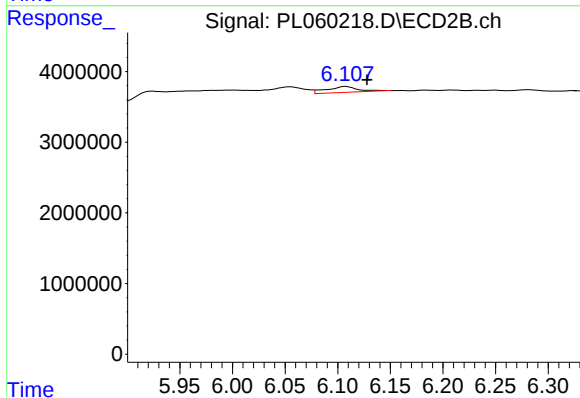


#25 Chlordane-3

R.T.: 6.108 min
Delta R.T.: -0.020 min
Response: 1712194
Conc: 4.43 ng/ml

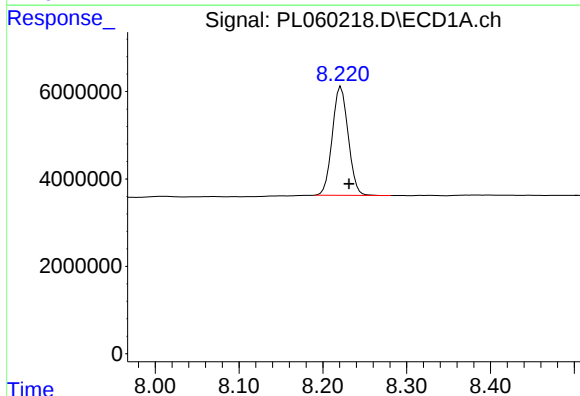

#28 Decachlorobiphenyl

R.T.: 8.222 min
Delta R.T.: -0.009 min
Response: 32742795
Conc: 19.90 ng/ml

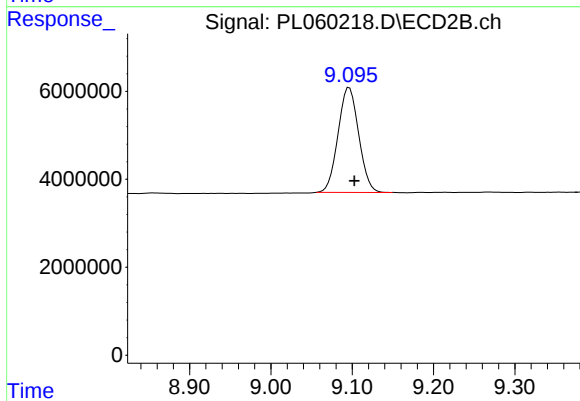

#28 Decachlorobiphenyl

R.T.: 9.096 min
Delta R.T.: -0.006 min
Response: 42070172
Conc: 20.12 ng/ml