

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072420\
 Data File : PL060175.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jul 2020 12:56
 Operator : DD\AJ
 Sample : L3382-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CTR-020

Manual Integrations
 APPROVED

Ankita
 7/27/2020 12:27:06 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 04:25:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.464	4.011	47039791	63971725	24.320	24.138
28) SA Decachlor...	8.220	9.095	37687747	46833780	22.909m	22.394m
Target Compounds						
12) B 4,4'-DDE	5.628	6.351	830540	1905187	0.499m	0.712m#
17) MA 4,4'-DDT	6.385	7.143	1828517	3325289	1.406	1.689m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072420\
Data File : PL060175.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2020 12:56
Operator : DD\AJ
Sample : L3382-05
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
CTR-020


Manual Integrations
APPROVED

Ankita
7/27/2020 12:27:06 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 04:25:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

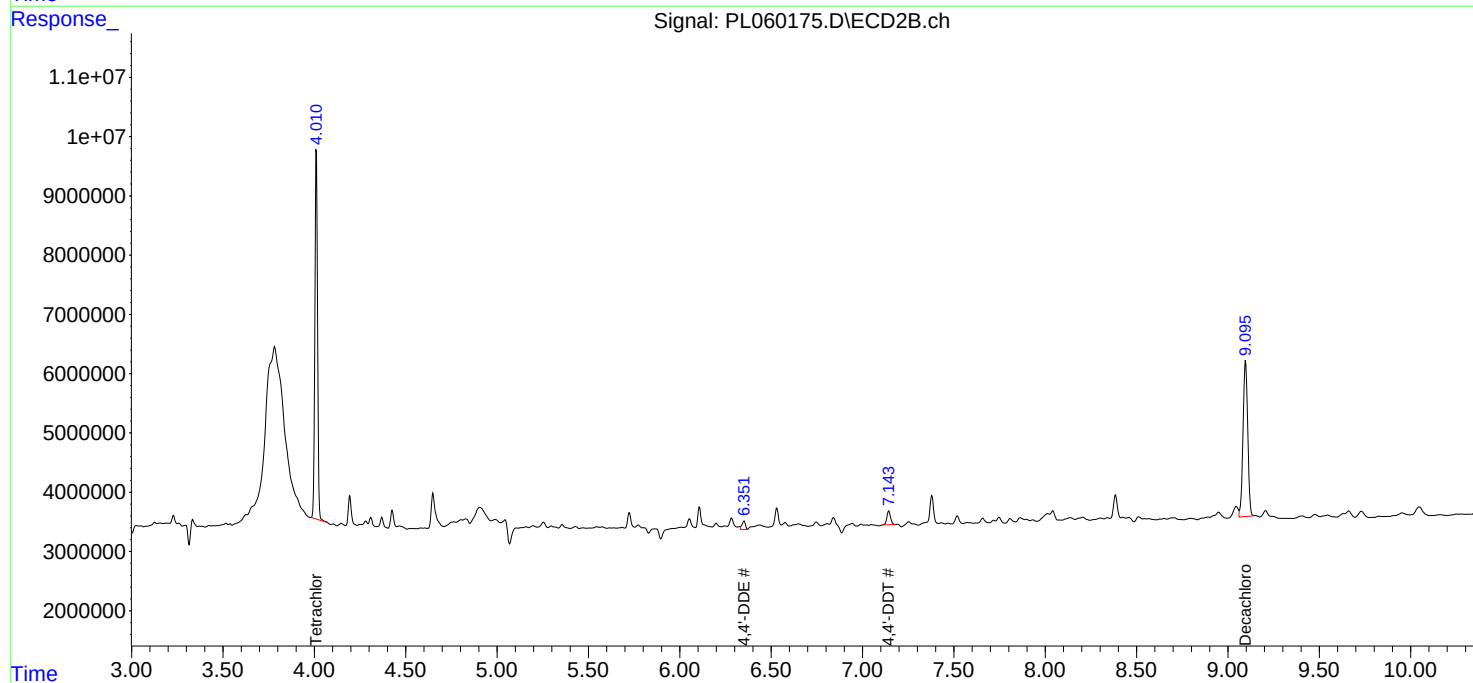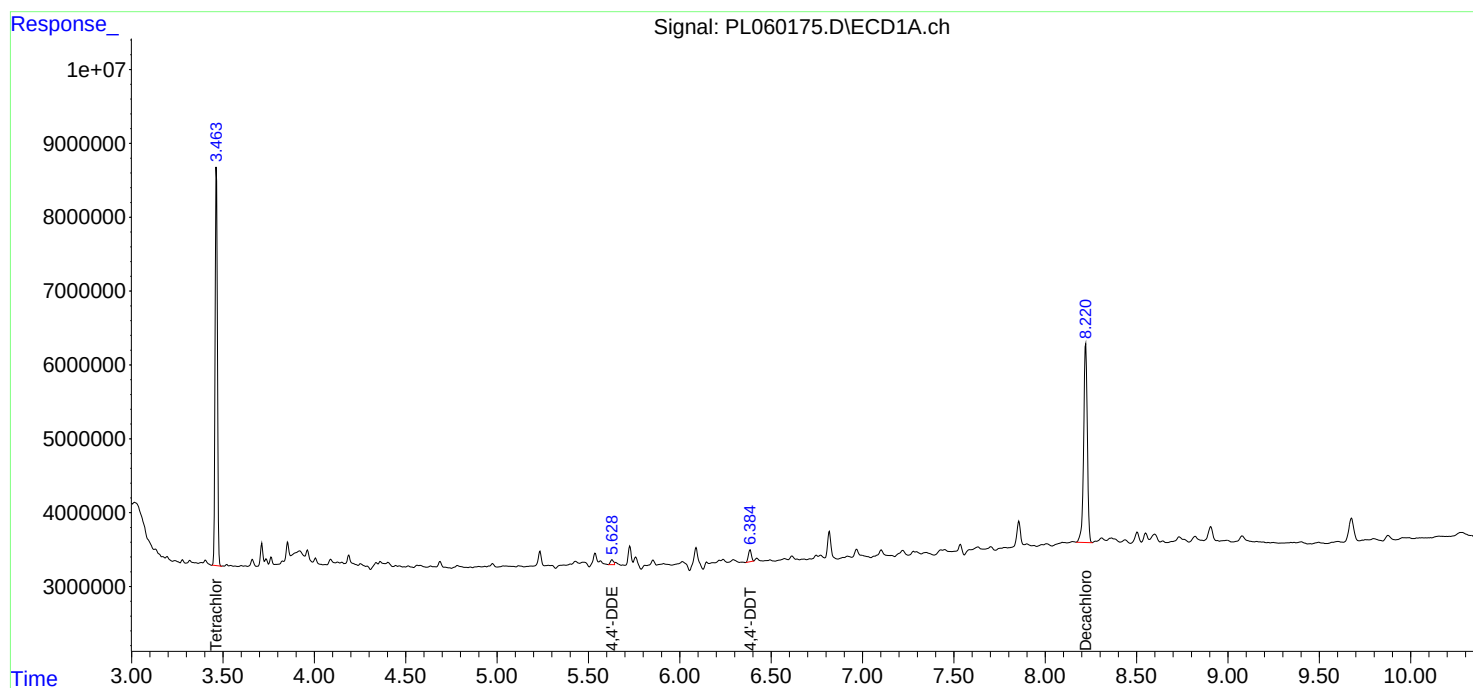

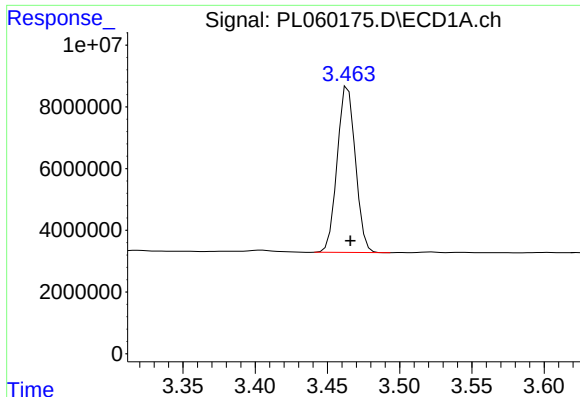


#1 Tetrachloro-m-xylene

R.T.: 3.464 min
Delta R.T.: -0.002 min
Response: 47039791
Conc: 24.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
CTR-020


Manual Integrations
APPROVED

Ankita
7/27/2020 12:27:06 PM

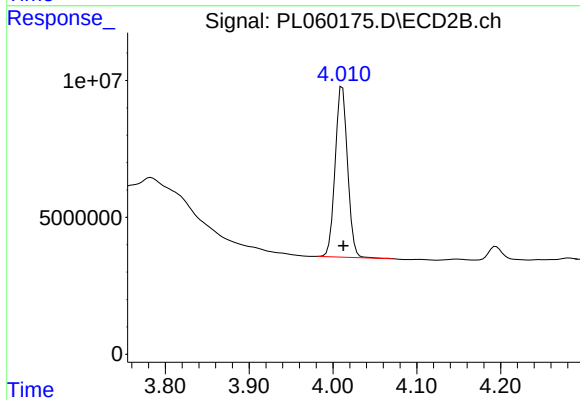


#1 Tetrachloro-m-xylene

R.T.: 4.011 min
Delta R.T.: -0.001 min
Response: 63971725
Conc: 24.14 ng/ml

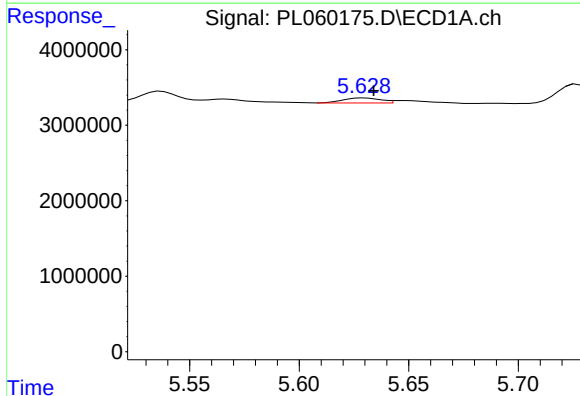


#12 4,4'-DDE

R.T.: 5.628 min
Delta R.T.: -0.006 min
Response: 830540
Conc: 0.50 ng/ml m

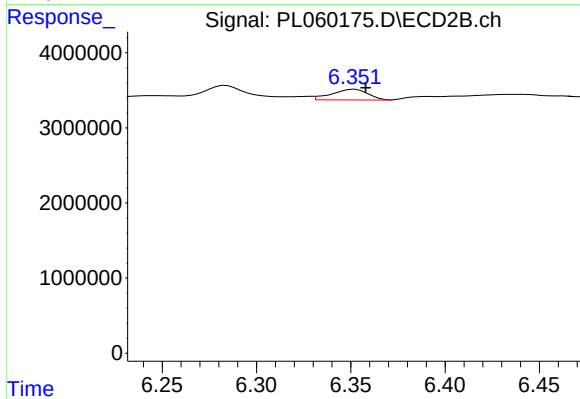

#12 4,4'-DDE

R.T.: 6.351 min
Delta R.T.: -0.007 min
Response: 1905187
Conc: 0.71 ng/ml m

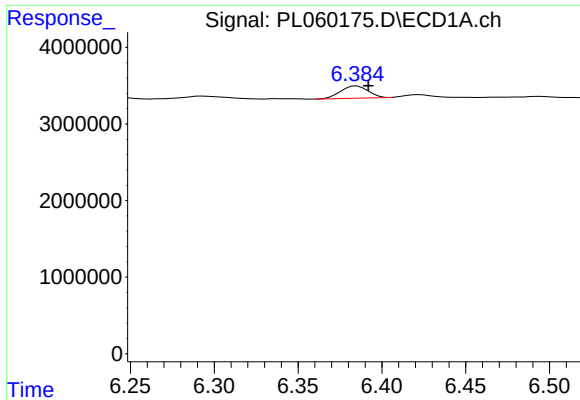


#17 4,4'-DDT

R.T.: 6.385 min
Delta R.T.: -0.007 min
Response: 1828517
Conc: 1.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
CTR-020


Manual Integrations
APPROVED

Ankita
7/27/2020 12:27:06 PM

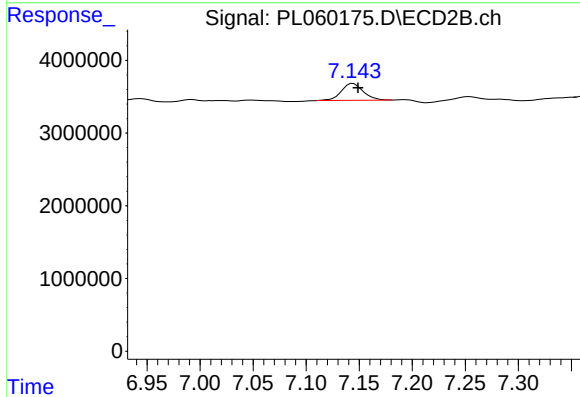


#17 4,4'-DDT

R.T.: 7.143 min
Delta R.T.: -0.006 min
Response: 3325289
Conc: 1.69 ng/ml m

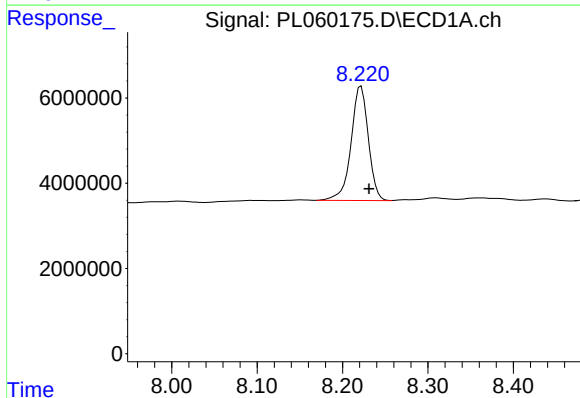

#28 Decachlorobiphenyl

R.T.: 8.220 min
Delta R.T.: -0.011 min
Response: 37687747
Conc: 22.91 ng/ml m

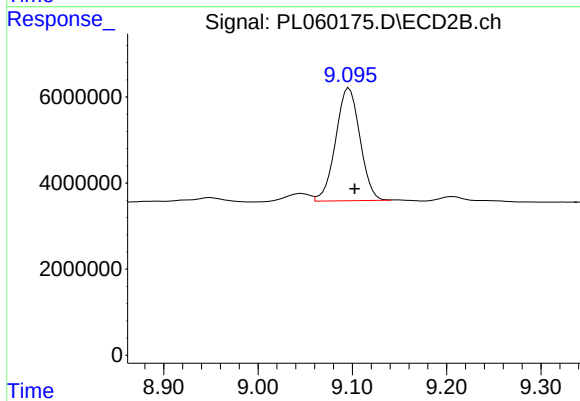

#28 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: -0.008 min
Response: 46833780
Conc: 22.39 ng/ml m