

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072420\
 Data File : PL060190.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jul 2020 17:17
 Operator : DD\AJ
 Sample : L3383-21
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CRT-015

Manual Integrations
 APPROVED

Ankita
 7/27/2020 12:27:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 04:29:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.012	39793434	54717547	20.573	20.647
28)	SA Decachlor...	8.221	9.097	31026710	37628115	18.860m	17.992
Target Compounds							
10)	B gamma-Chl...	5.405	6.119	3718729	12603928	2.050m	4.401m#
11)	B alpha-Chl...	5.464	6.198	2747050	5831261	1.523m	2.039m#
12)	B 4,4'-DDE	5.628	6.350	1211200	1582894	0.727m	0.591m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072420\
Data File : PL060190.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2020 17:17
Operator : DD\AJ
Sample : L3383-21
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CRT-015


Manual Integrations
APPROVED

Ankita
7/27/2020 12:27:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 04:29:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

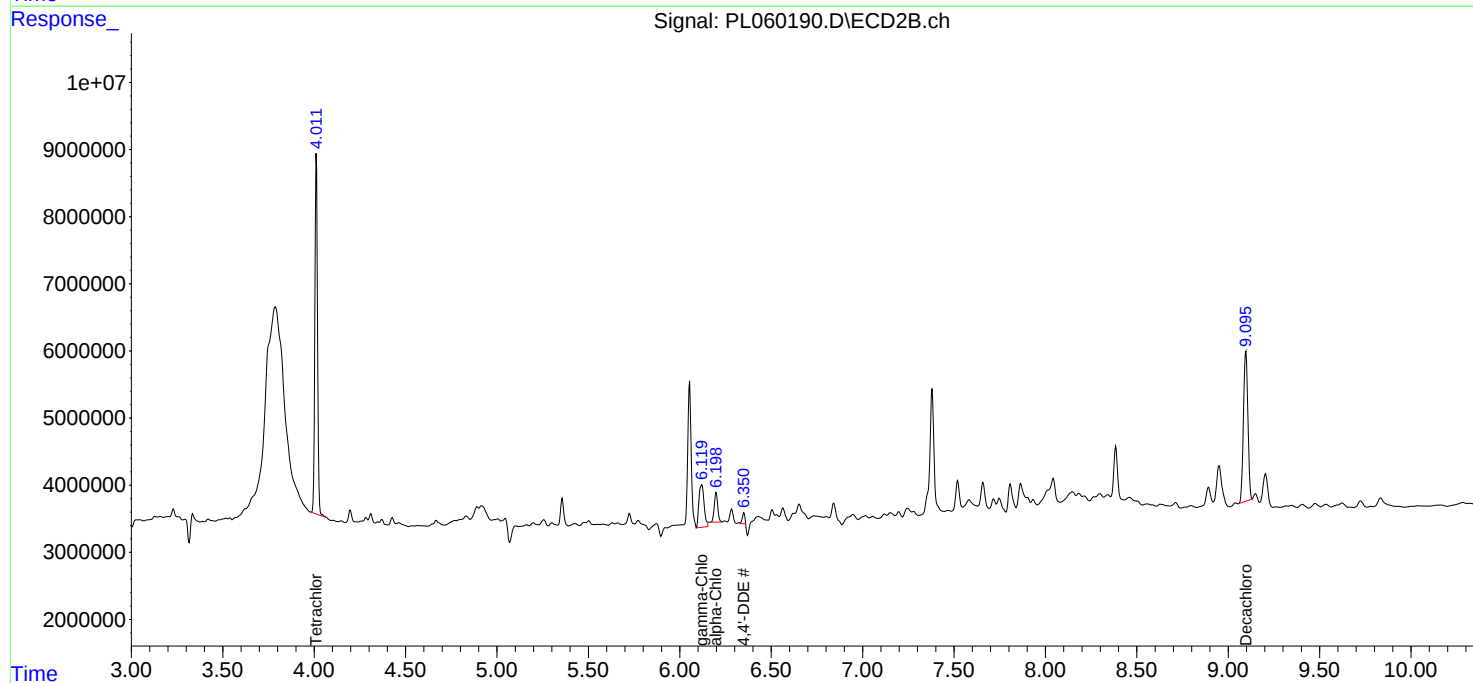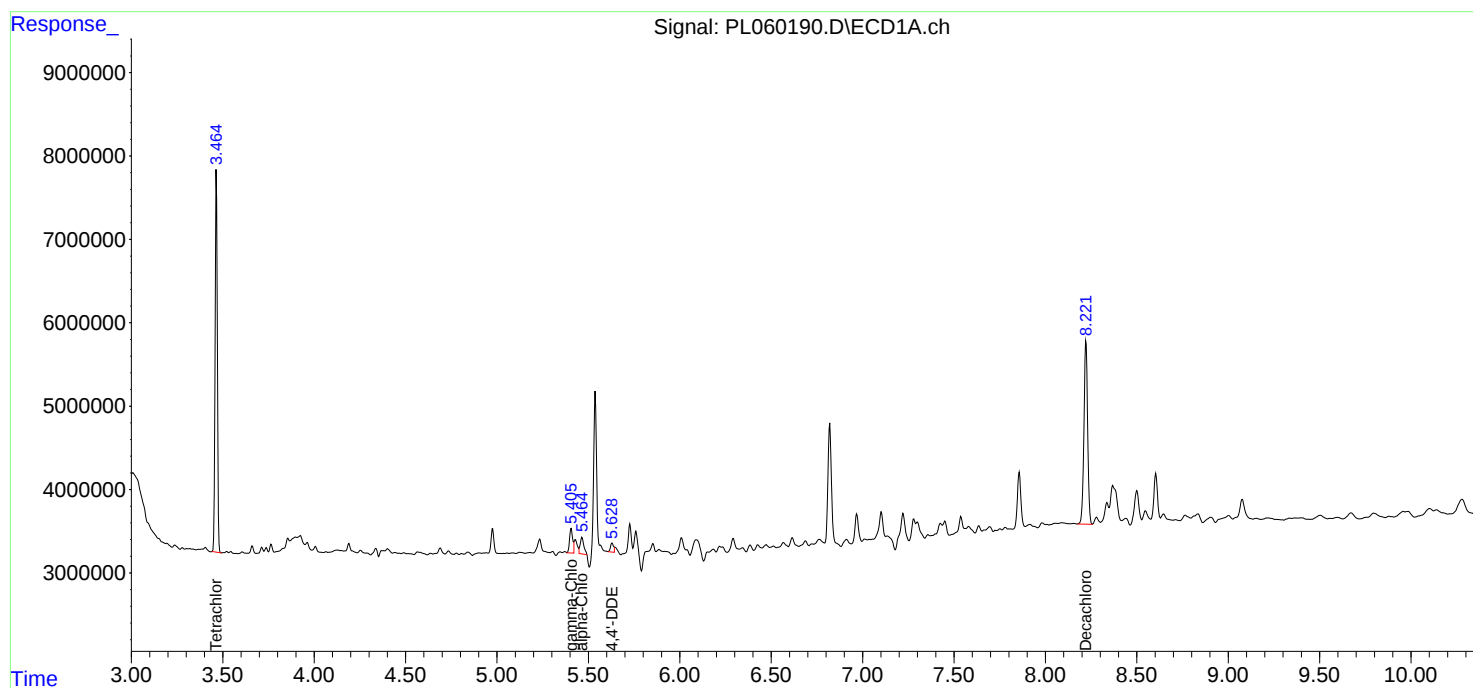

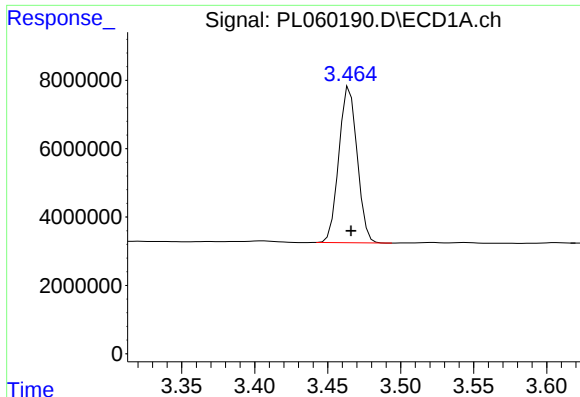


#1 Tetrachloro-m-xylene

R.T.: 3.465 min
Delta R.T.: 0.000 min
Response: 39793434
Conc: 20.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
CRT-015


Manual Integrations
APPROVED

Ankita
7/27/2020 12:27:42 PM

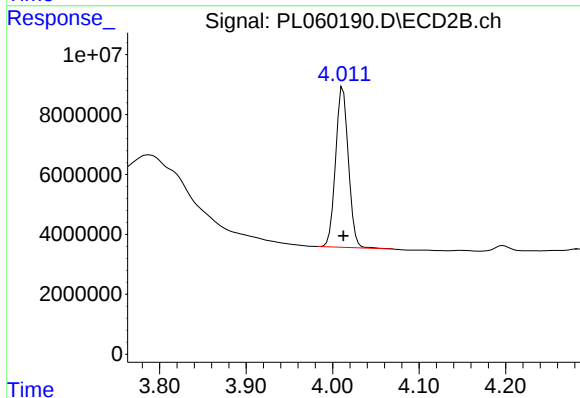


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 54717547
Conc: 20.65 ng/ml

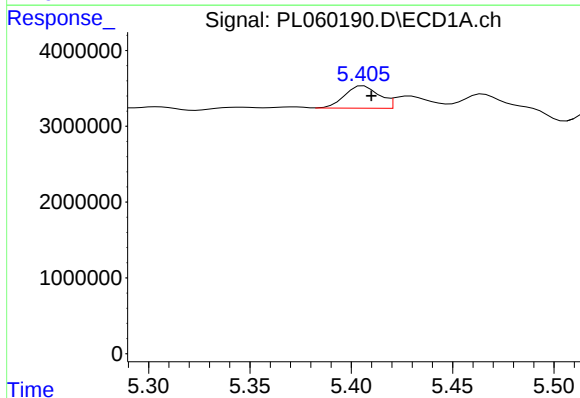


#10 gamma-Chlordane

R.T.: 5.405 min
Delta R.T.: -0.005 min
Response: 3718729
Conc: 2.05 ng/ml m

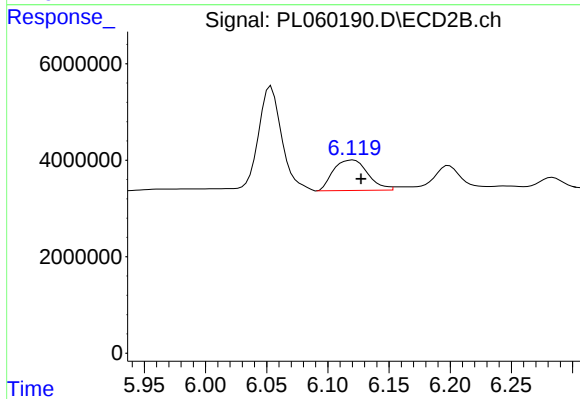

#10 gamma-Chlordane

R.T.: 6.119 min
Delta R.T.: -0.008 min
Response: 12603928
Conc: 4.40 ng/ml m

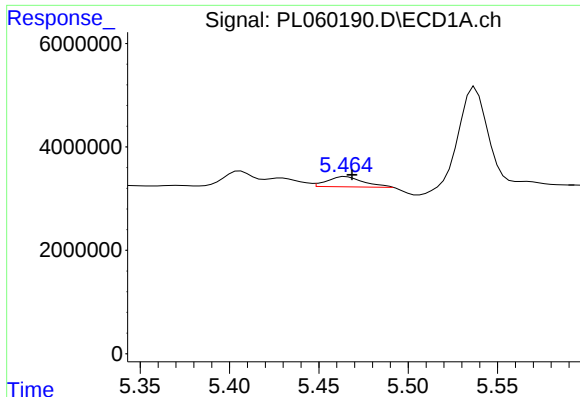


#11 alpha-Chlordane

R.T.: 5.464 min
Delta R.T.: -0.005 min
Response: 2747050
Conc: 1.52 ng/ml m

Instrument :
ECD_L
ClientSampleId :
CRT-015


Manual Integrations
APPROVED

Ankita
7/27/2020 12:27:42 PM

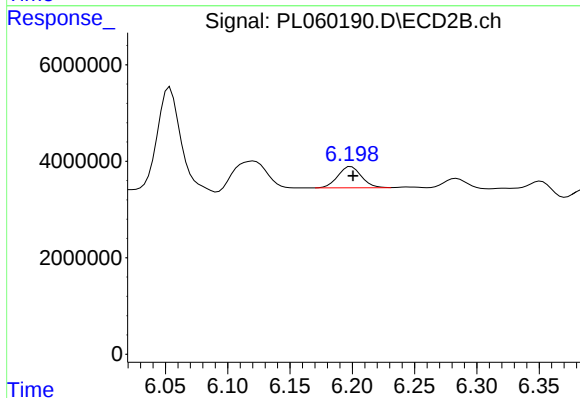


#11 alpha-Chlordane

R.T.: 6.198 min
Delta R.T.: -0.003 min
Response: 5831261
Conc: 2.04 ng/ml m

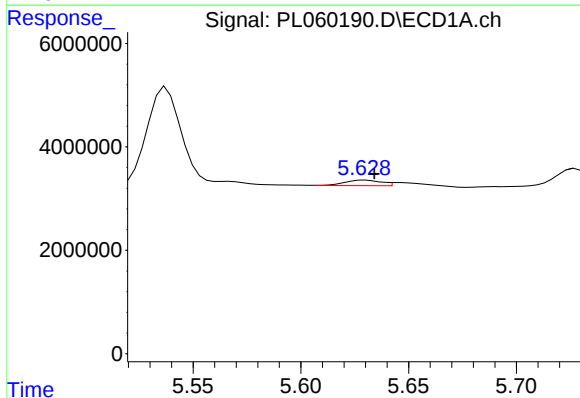


#12 4,4'-DDE

R.T.: 5.628 min
Delta R.T.: -0.006 min
Response: 1211200
Conc: 0.73 ng/ml m

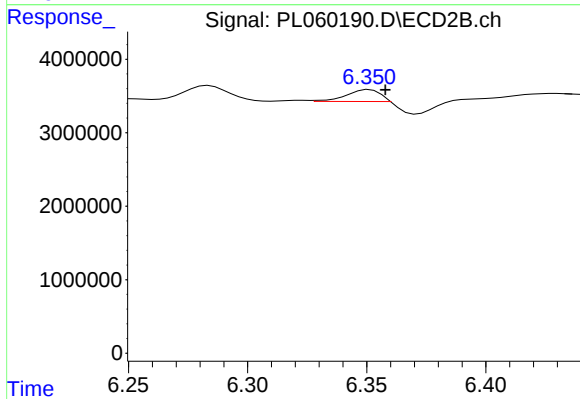

#12 4,4'-DDE

R.T.: 6.350 min
Delta R.T.: -0.008 min
Response: 1582894
Conc: 0.59 ng/ml m

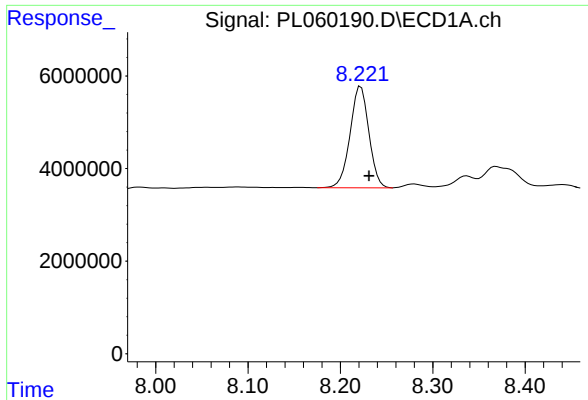


#28 Decachlorobiphenyl

R.T.: 8.221 min
Delta R.T.: -0.010 min
Response: 31026710
Conc: 18.86 ng/ml m

Instrument :
ECD_L
ClientSampleId :
CRT-015

Manual Integrations
APPROVED

Ankita
7/27/2020 12:27:42 PM

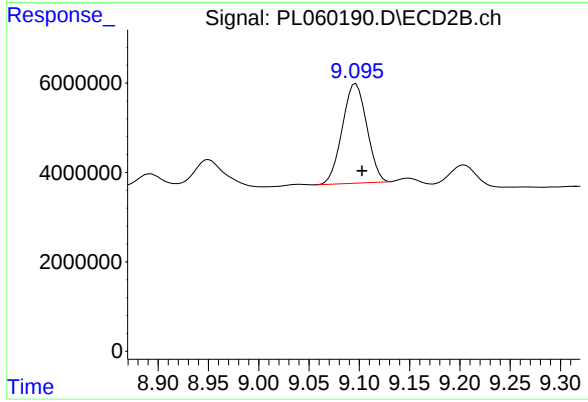

#28 Decachlorobiphenyl

R.T.: 9.097 min
Delta R.T.: -0.006 min
Response: 37628115
Conc: 17.99 ng/ml