

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072420\
 Data File : PL060195.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jul 2020 18:28
 Operator : DD\AJ
 Sample : L3412-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 DUCK-BANK

Manual Integrations
 APPROVED

Ankita
 7/27/2020 12:27:57 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 04:31:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.012	43038789	58506505	22.251	22.076
28)	SA Decachlor...	8.222	9.097	31052403	37900608	18.876	18.122
Target Compounds							
11)	B alpha-Chl...	5.466	6.200	1392538	3533958	0.772m	1.236 #
12)	B 4,4'-DDE	5.628	6.352	782352	1445292	0.470m	0.540m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072420\
Data File : PL060195.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2020 18:28
Operator : DD\AJ
Sample : L3412-01
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
DUCK-BANK


Manual Integrations
APPROVED

Ankita
7/27/2020 12:27:57 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 04:31:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

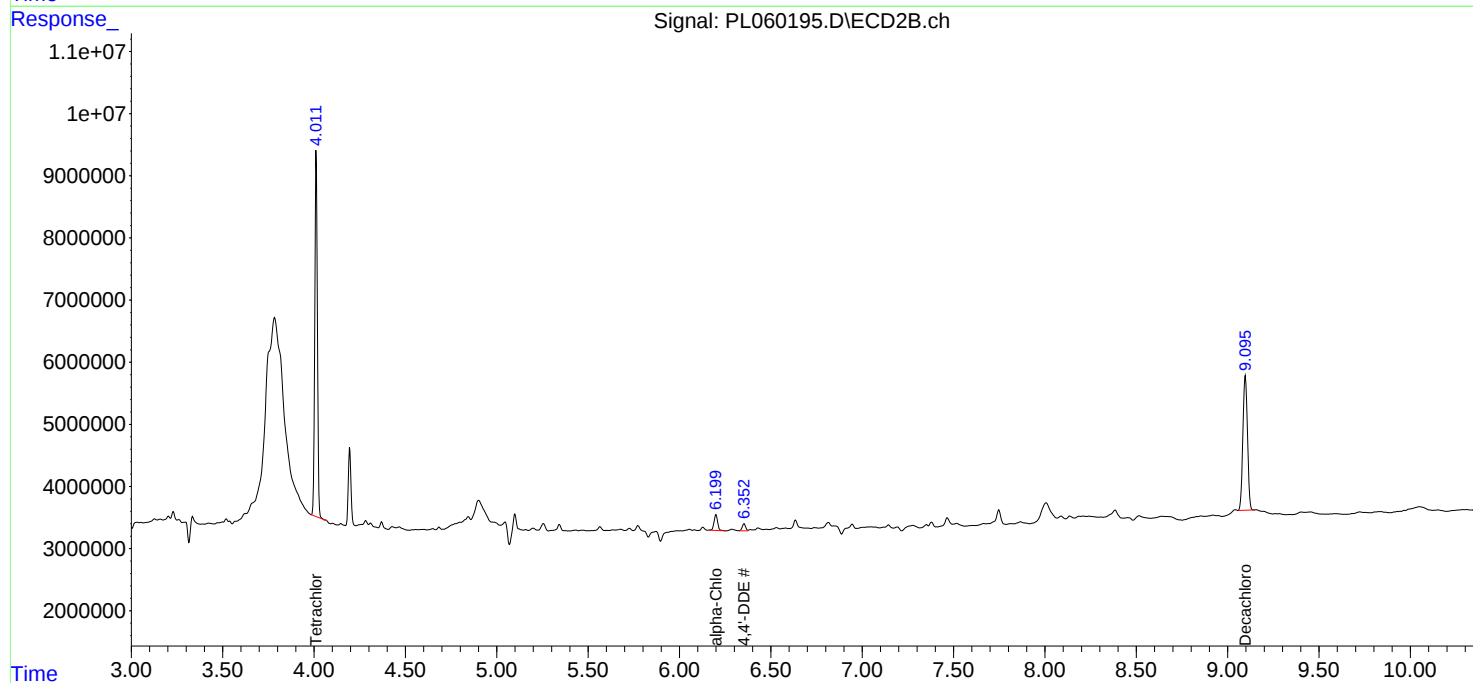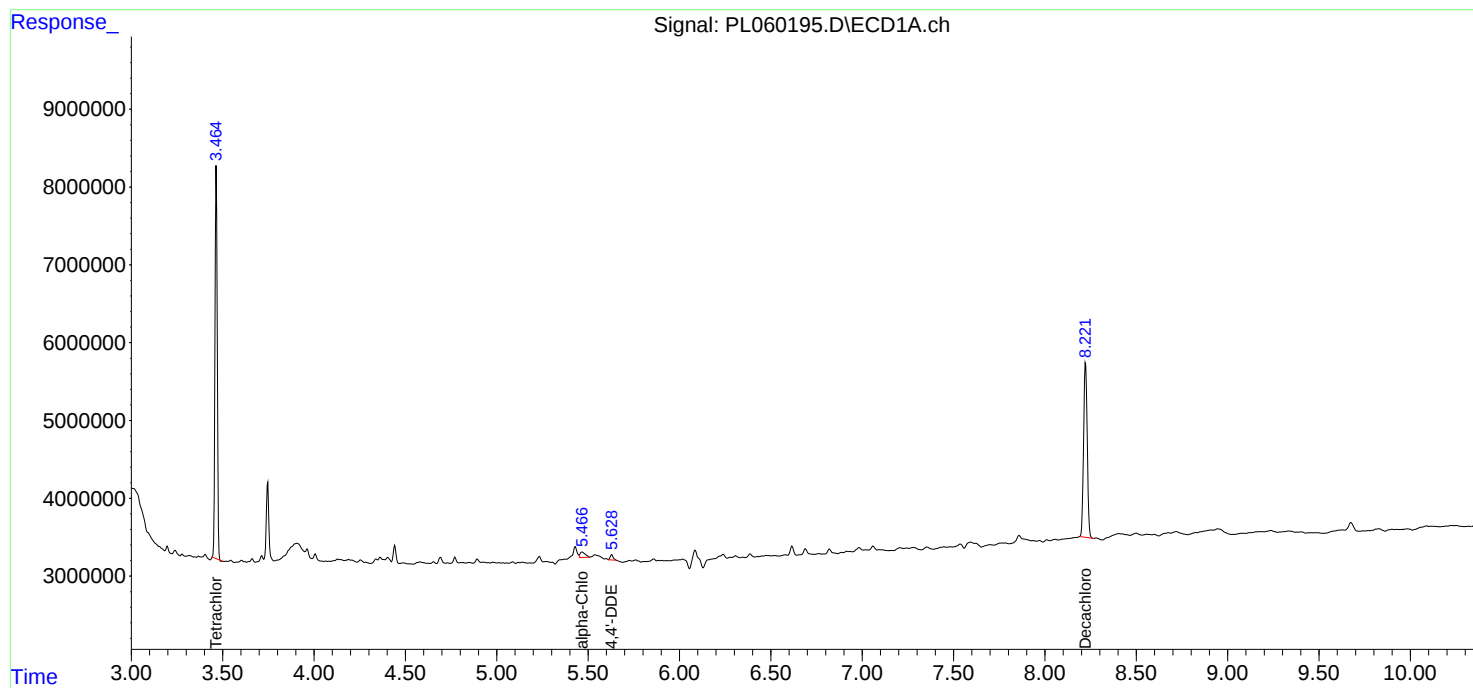

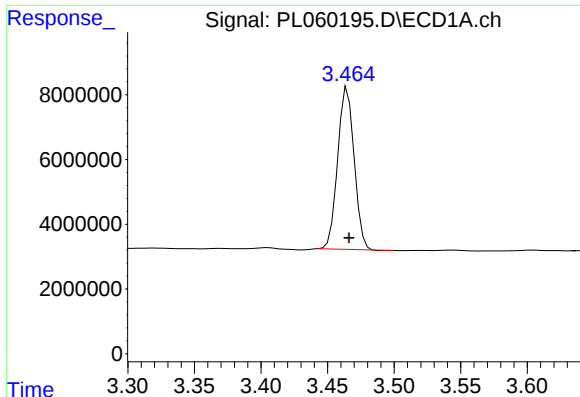


#1 Tetrachloro-m-xylene

R.T.: 3.465 min
Delta R.T.: 0.000 min
Response: 43038789
Conc: 22.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
DUCK-BANK


Manual Integrations
APPROVED

Ankita
7/27/2020 12:27:57 PM

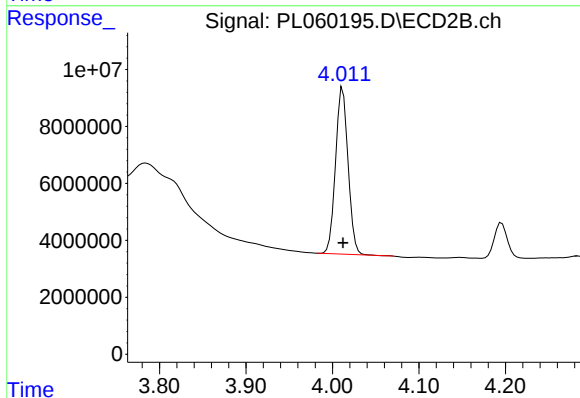


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 58506505
Conc: 22.08 ng/ml

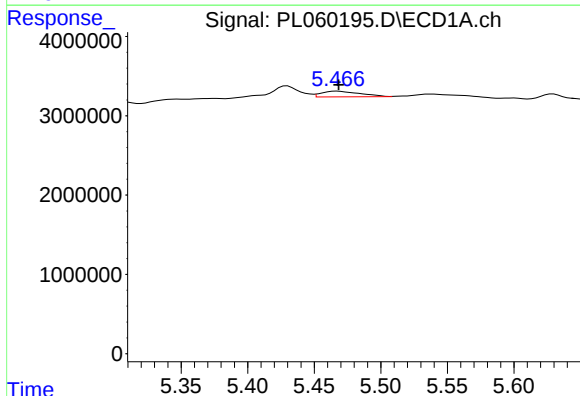


#11 alpha-Chlordane

R.T.: 5.466 min
Delta R.T.: -0.003 min
Response: 1392538
Conc: 0.77 ng/ml m

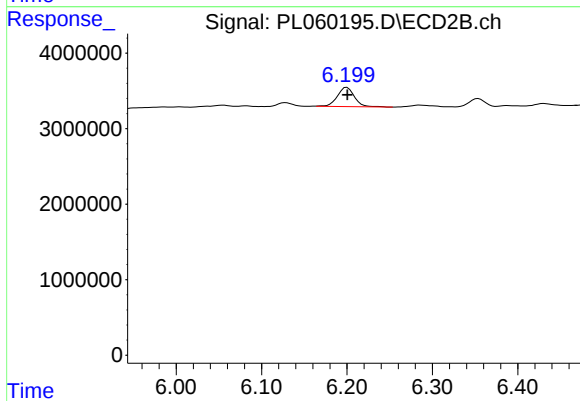

#11 alpha-Chlordane

R.T.: 6.200 min
Delta R.T.: 0.000 min
Response: 3533958
Conc: 1.24 ng/ml

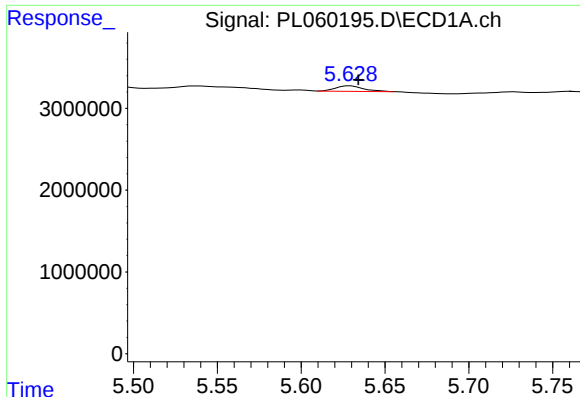


#12 4,4'-DDE

R.T.: 5.628 min
Delta R.T.: -0.006 min
Response: 782352
Conc: 0.47 ng/ml m

Instrument :
ECD_L
ClientSampleId :
DUCK-BANK


Manual Integrations
APPROVED

Ankita
7/27/2020 12:27:57 PM

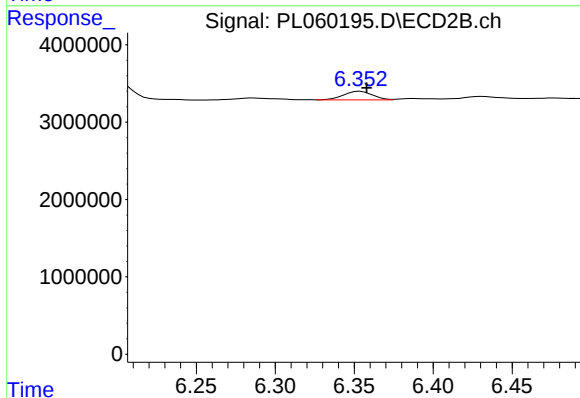


#12 4,4'-DDE

R.T.: 6.352 min
Delta R.T.: -0.006 min
Response: 1445292
Conc: 0.54 ng/ml m

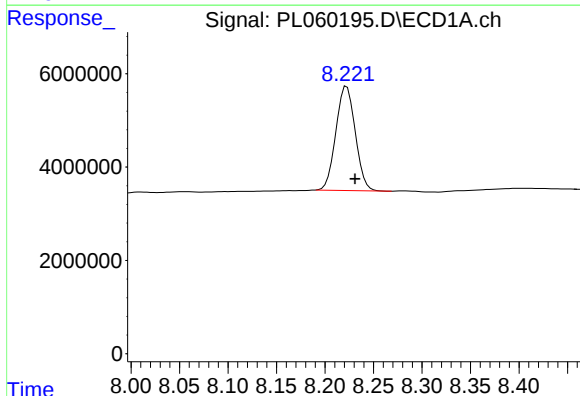

#28 Decachlorobiphenyl

R.T.: 8.222 min
Delta R.T.: -0.009 min
Response: 31052403
Conc: 18.88 ng/ml

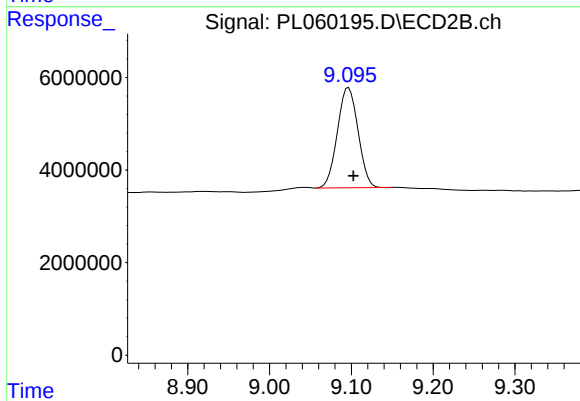

#28 Decachlorobiphenyl

R.T.: 9.097 min
Delta R.T.: -0.006 min
Response: 37900608
Conc: 18.12 ng/ml