

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072423\
 Data File : PL084153.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jul 2023 11:27
 Operator : AR\AJ
 Sample : 03707-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EO-01-072023

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/25/2023
 Supervised By :Ankita Jodhani 07/25/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 21:20:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 00:03:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.485	2.689	16396837	8323493	8.199	7.495
2) SA Decachlor...	9.033	7.874	11049185	9194301	8.489m	8.275

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072423\
Data File : PL084153.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2023 11:27
Operator : AR\AJ
Sample : 03707-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
EO-01-072023


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/25/2023
Supervised By :Ankita Jodhani 07/25/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 21:20:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 00:03:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

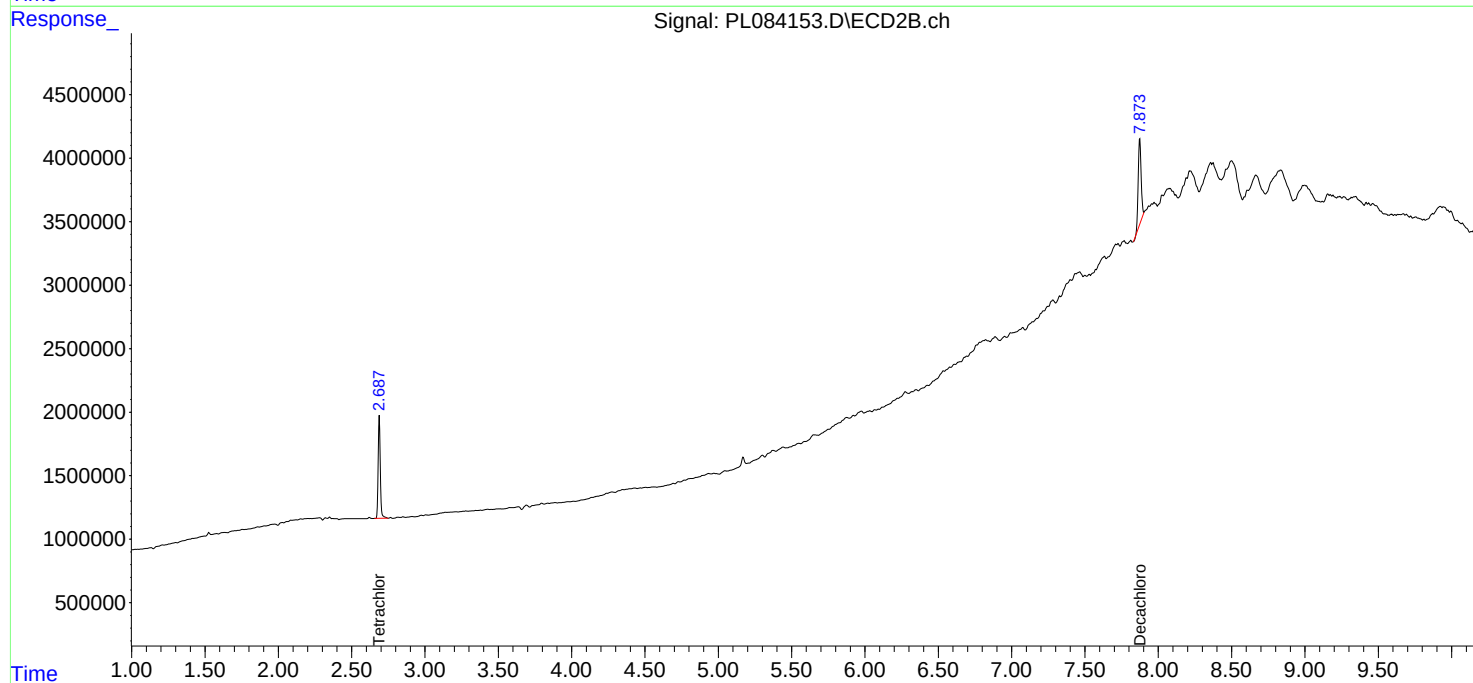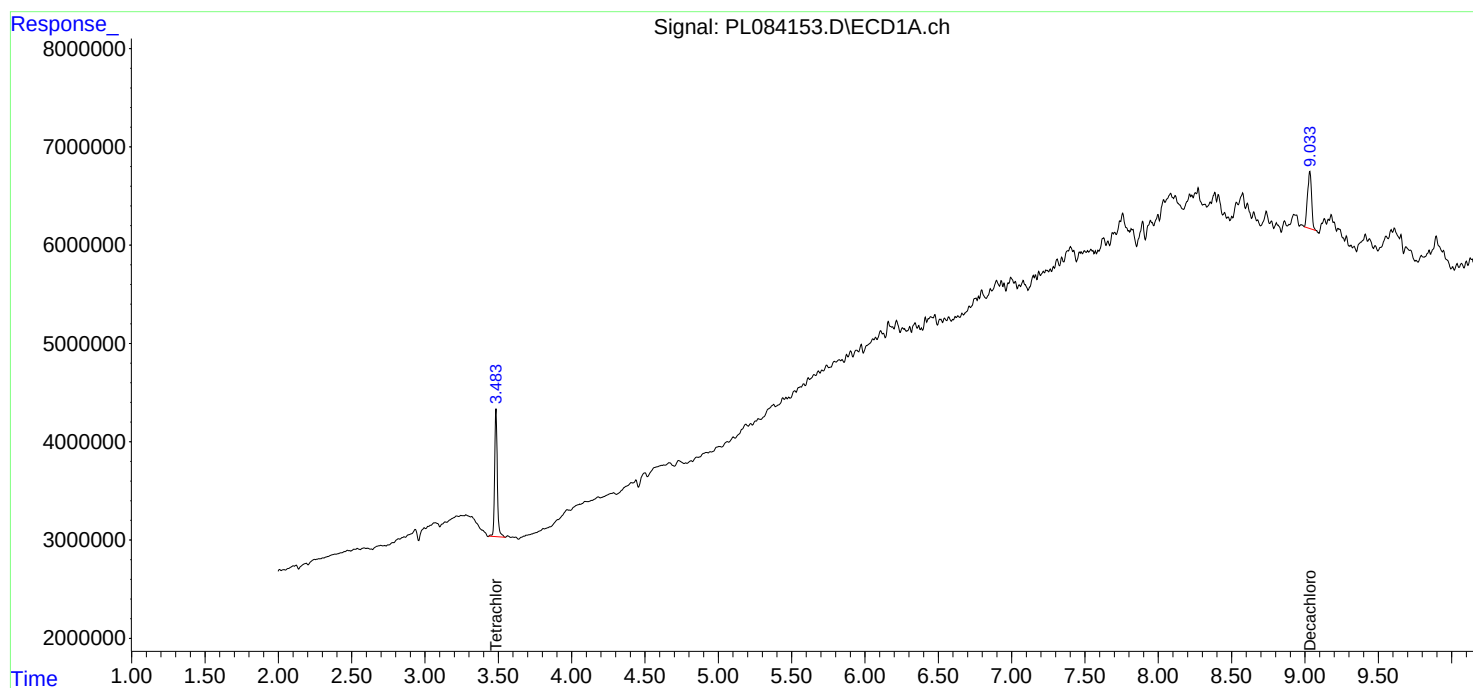

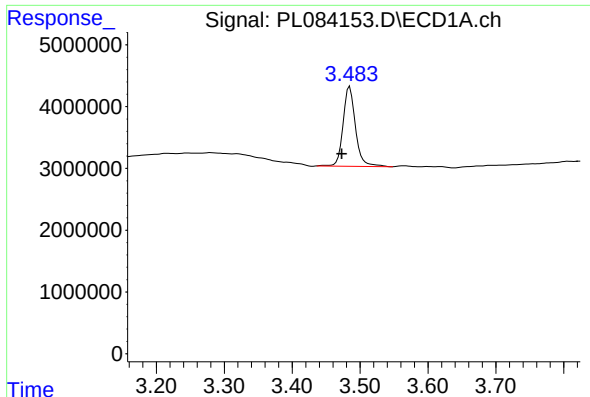


#1 Tetrachloro-m-xylene

R.T.: 3.485 min
Delta R.T.: 0.012 min
Response: 16396837
Conc: 8.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-01-072023


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/25/2023
Supervised By :Ankita Jodhani 07/25/2023

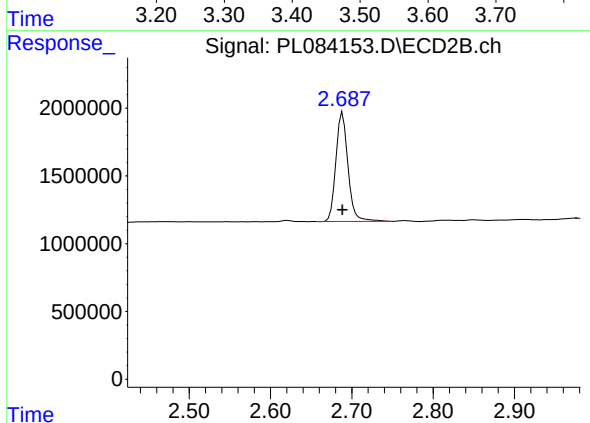


#1 Tetrachloro-m-xylene

R.T.: 2.689 min
Delta R.T.: 0.000 min
Response: 8323493
Conc: 7.49 ng/ml

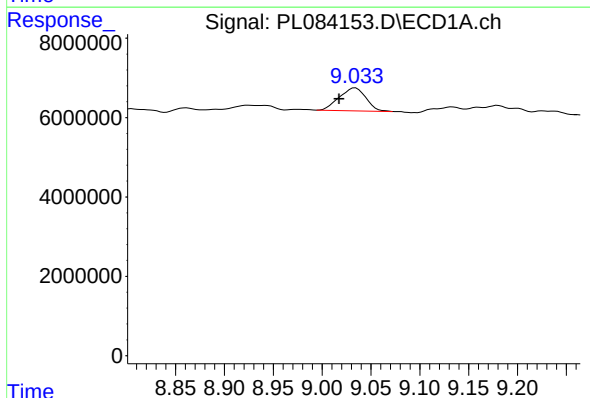

#28 Decachlorobiphenyl

R.T.: 9.033 min
Delta R.T.: 0.015 min
Response: 11049185
Conc: 8.49 ng/ml m

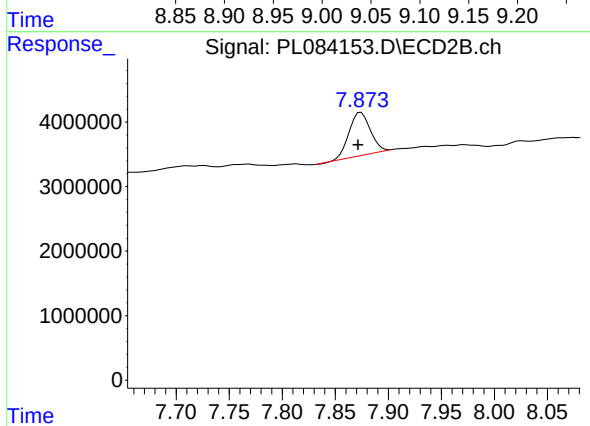

#28 Decachlorobiphenyl

R.T.: 7.874 min
Delta R.T.: 0.003 min
Response: 9194301
Conc: 8.27 ng/ml