

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072424\
Data File : PL090634.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2024 10:58
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/25/2024
Supervised By :Ankita Jodhani 07/25/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 01:00:43 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071524.M
Quant Title : GC Extractables
QLast Update : Mon Jul 15 14:16:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.552	2.789	44968977	36744127	21.597m	21.833
28)	SA Decachlor...	9.068	7.936	33414891	34770546	25.146m	23.847

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072424\
Data File : PL090634.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2024 10:58
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/25/2024
Supervised By : Ankita Jodhani 07/25/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 01:00:43 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071524.M
Quant Title : GC Extractables
QLast Update : Mon Jul 15 14:16:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

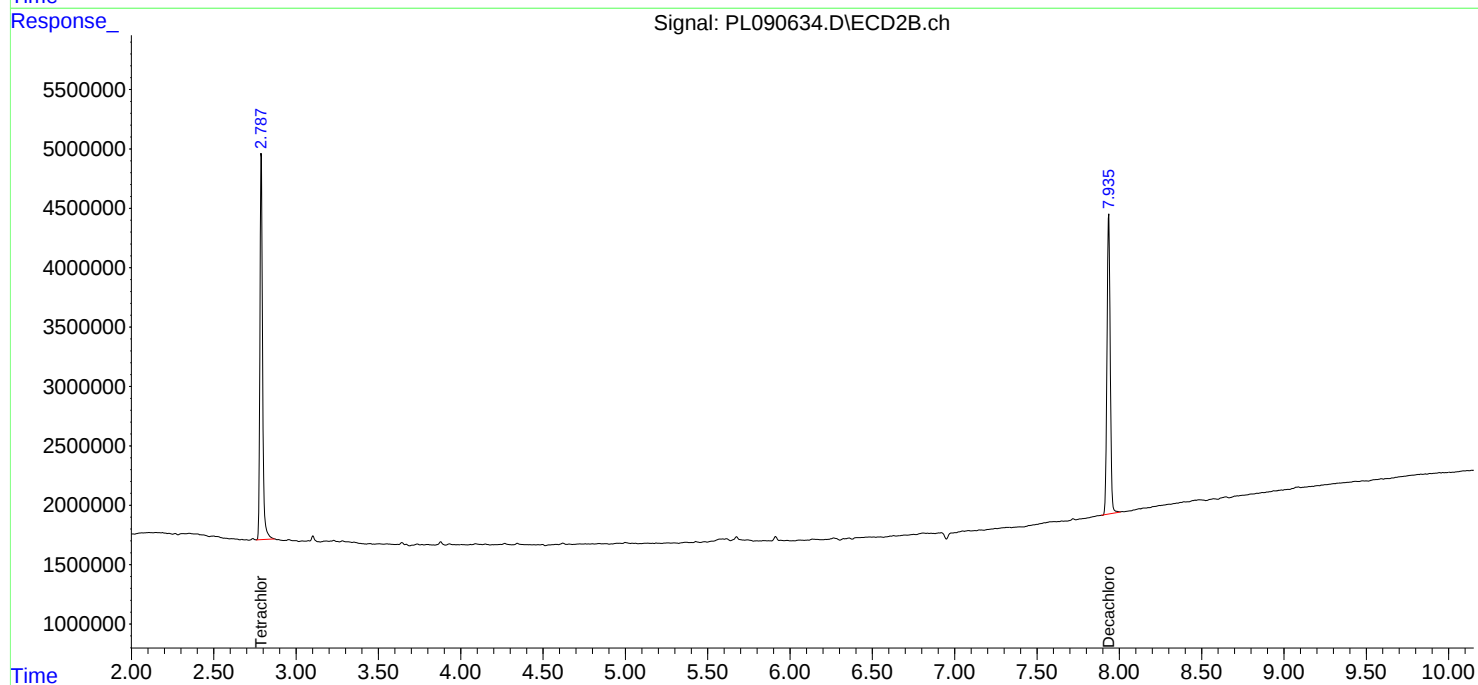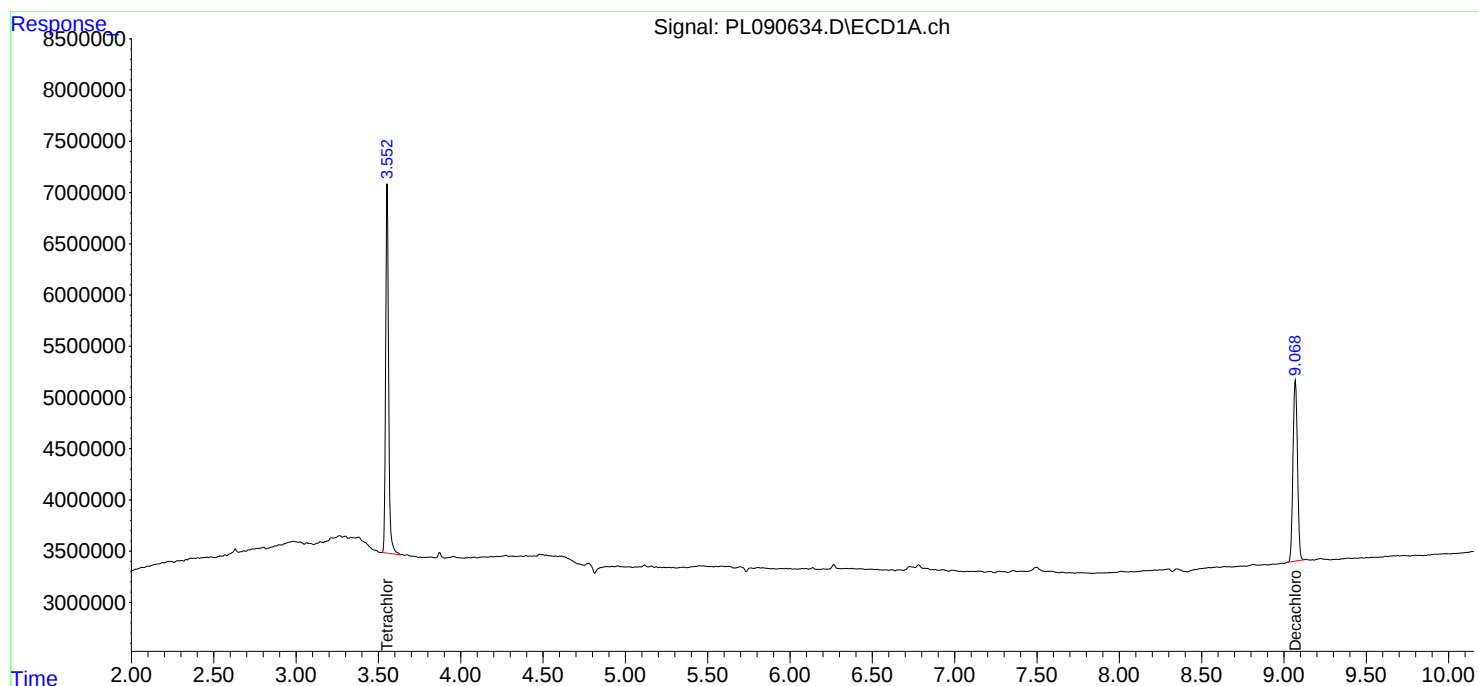

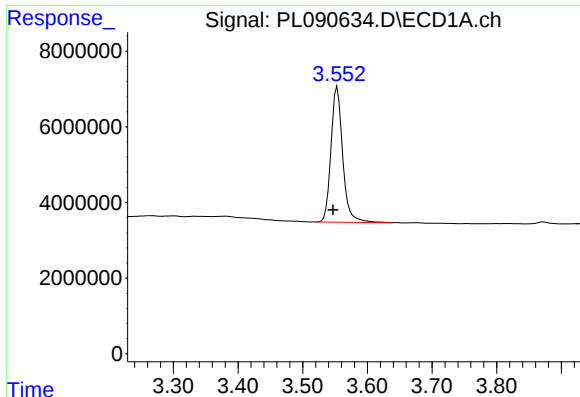


#1 Tetrachloro-m-xylene

R.T.: 3.552 min
Delta R.T.: 0.005 min
Response: 44968977
Conc: 21.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/25/2024
Supervised By :Ankita Jodhani 07/25/2024

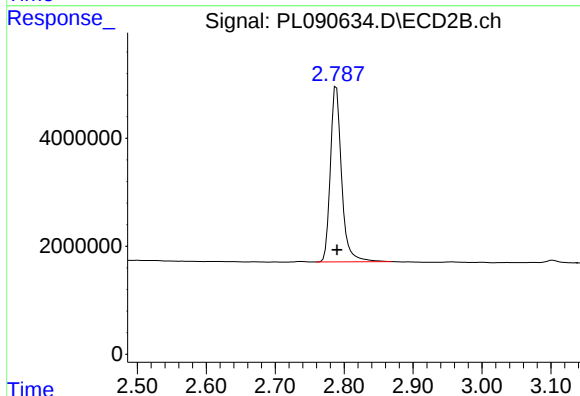


#1 Tetrachloro-m-xylene

R.T.: 2.789 min
Delta R.T.: 0.000 min
Response: 36744127
Conc: 21.83 ng/ml

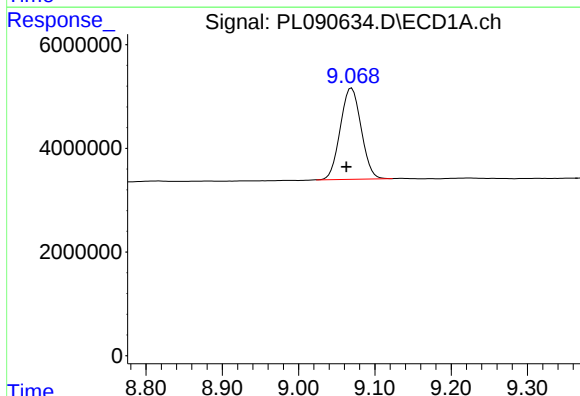

#28 Decachlorobiphenyl

R.T.: 9.068 min
Delta R.T.: 0.005 min
Response: 33414891
Conc: 25.15 ng/ml m

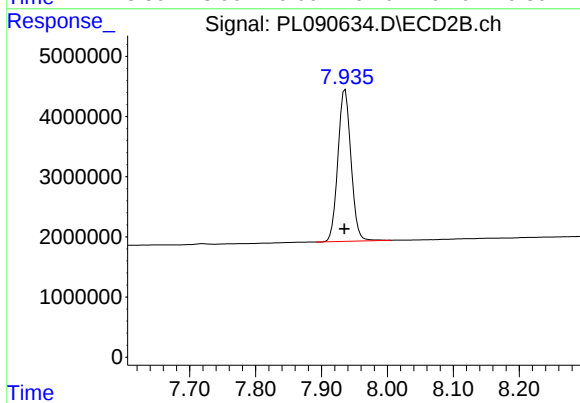

#28 Decachlorobiphenyl

R.T.: 7.936 min
Delta R.T.: 0.001 min
Response: 34770546
Conc: 23.85 ng/ml