

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072425\
 Data File : PL096550.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jul 2025 10:28
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 23:29:37 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 07 15:22:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

8) B	Heptachlo...	5.654	0.000	103.0E6	0	24.826	N.D.	#
9) A	Endosulfan I	6.030f	0.000	28089368	0	6.958	N.D.	#
10) B	gamma-Chl...	5.911	0.000	32185728	0	7.274	N.D.	#
12) B	4,4'-DDE	6.175	0.000	6495927	0	1.752	N.D.	#
13) MA	Dieldrin	0.000	5.437	0	48947721	N.D.	7.178	#
14) MA	Endrin	0.000	5.715	0	102.0E6	N.D.	16.734	#
15) B	Endosulfa...	6.748	0.000	7724048	0	2.226	N.D.	#
23)	Chlordane-1	0.000	3.835	0	6540608	N.D.	27.672	#
24)	Chlordane-2	0.000	4.411	0	19934234	N.D.	72.527	#
25)	Chlordane-3	5.911	0.000	32185728	0	43.686	N.D.	#
26)	Chlordane-4	6.030f	0.000	28089368	0	31.307	N.D.	#
27)	Chlordane-5	0.000	6.041f	0	16739004	N.D.	59.054	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072425\
Data File : PL096550.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2025 10:28
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 23:29:37 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
Quant Title : GC Extractables
QLast Update : Mon Jul 07 15:22:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

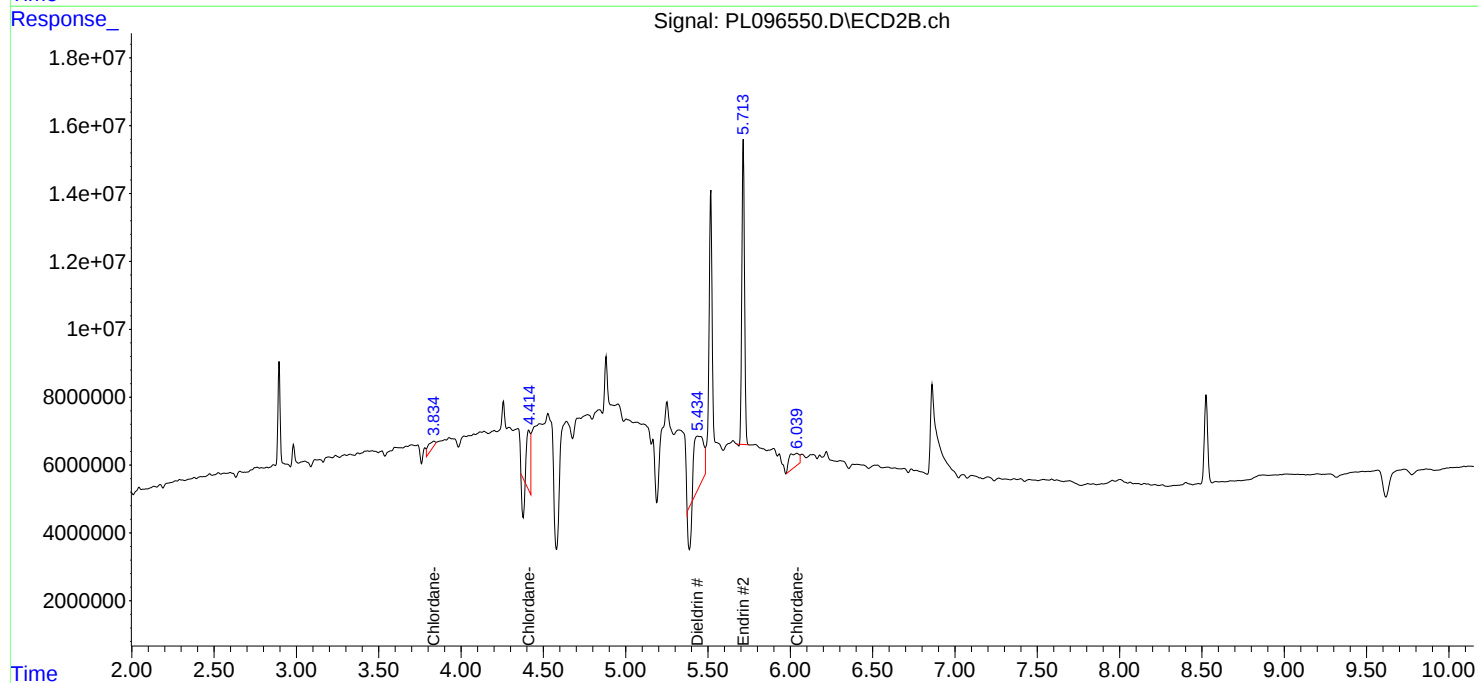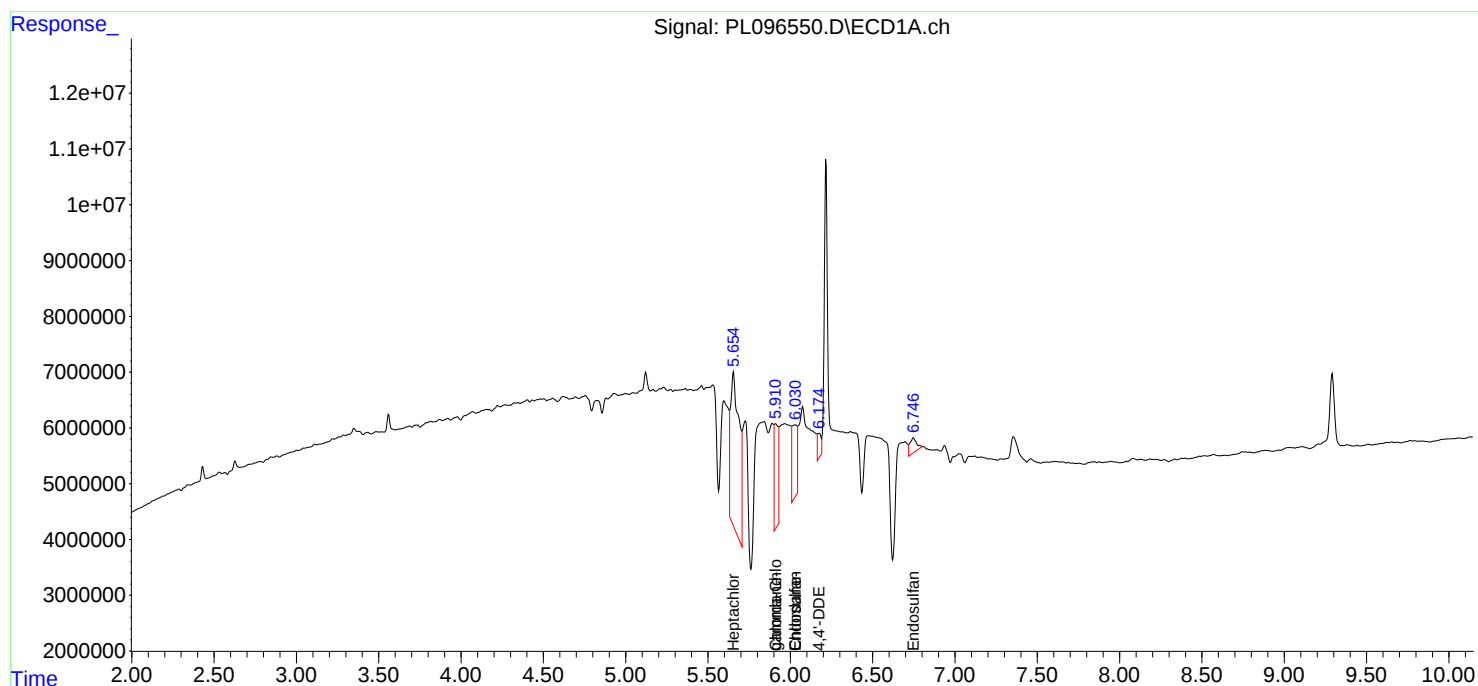


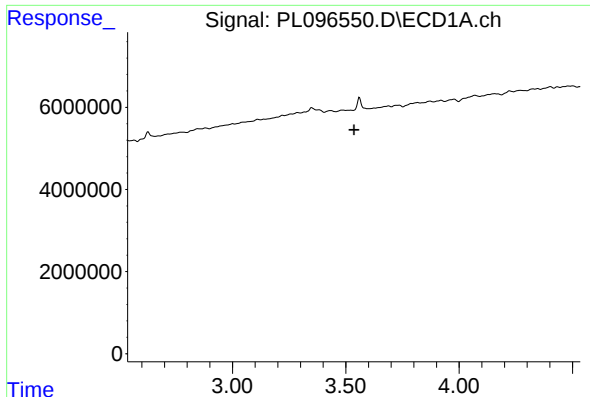

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.537 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

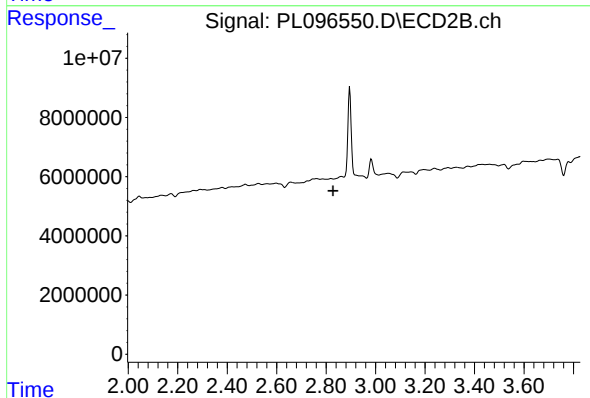


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 2.828 min
Response: 0
Conc: N.D.

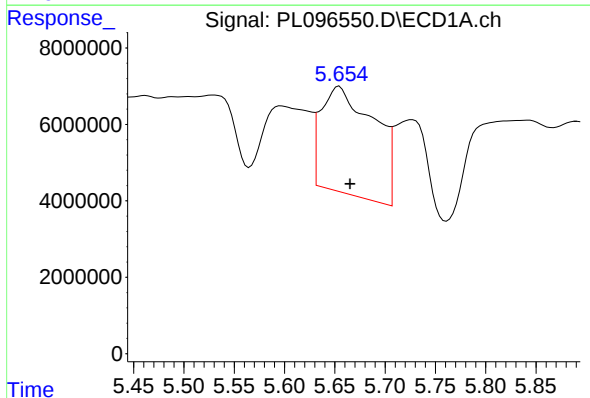


#8 Heptachlor epoxide

R.T.: 5.654 min
Delta R.T.: -0.011 min
Response: 103005603
Conc: 24.83 ng/ml

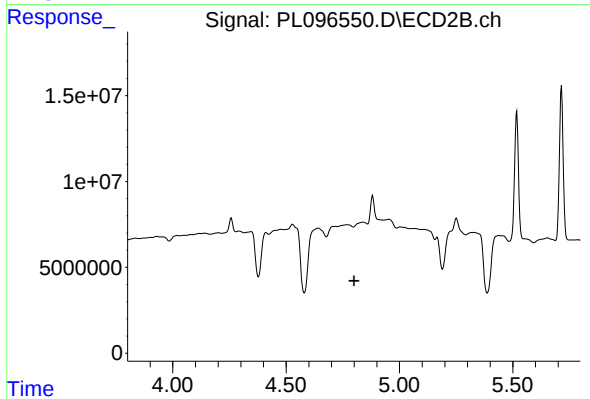

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.800 min
Response: 0
Conc: N.D.

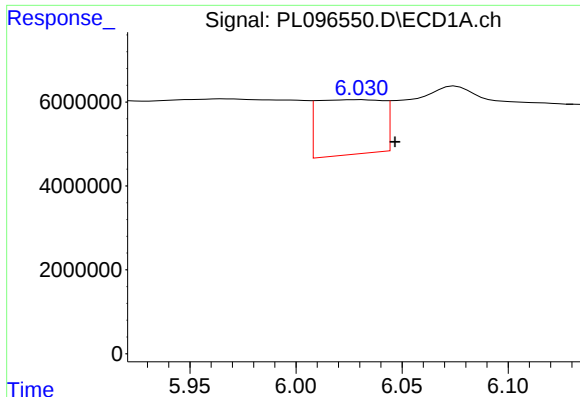

#9 Endosulfan I


R.T.: 6.030 min
Delta R.T.: -0.016 min
Response: 28089368
Conc: 6.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

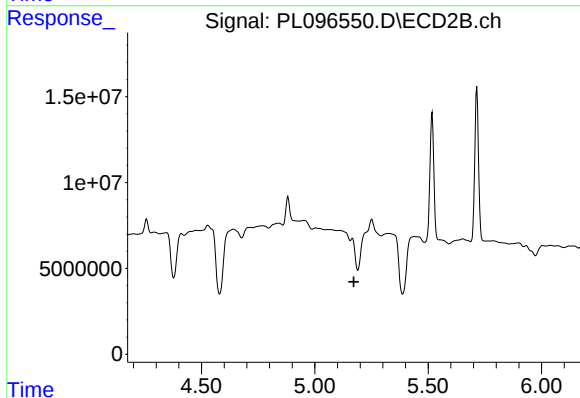


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.172 min
Response: 0
Conc: N.D.

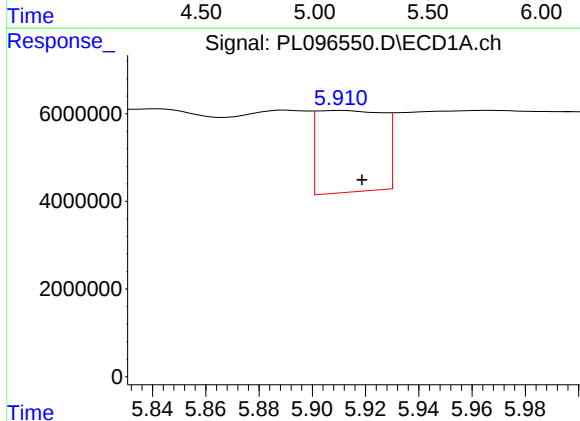


#10 gamma-Chlordane

R.T.: 5.911 min
Delta R.T.: -0.008 min
Response: 32185728
Conc: 7.27 ng/ml

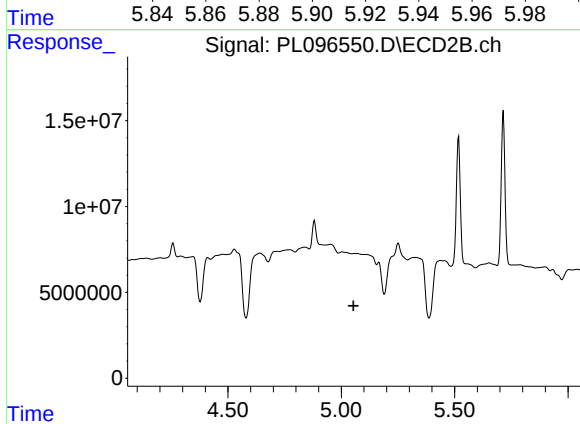

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.054 min
Response: 0
Conc: N.D.

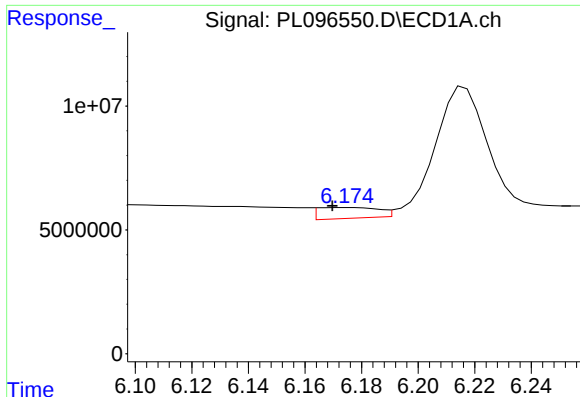

#12 4,4'-DDE


R.T.: 6.175 min
Delta R.T.: 0.006 min
Response: 6495927
Conc: 1.75 ng/ml

Instrument :
ECD_L
ClientSampleId :

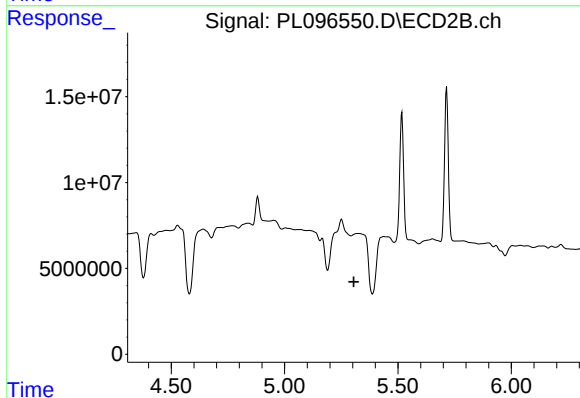


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 5.306 min
Response: 0
Conc: N.D.

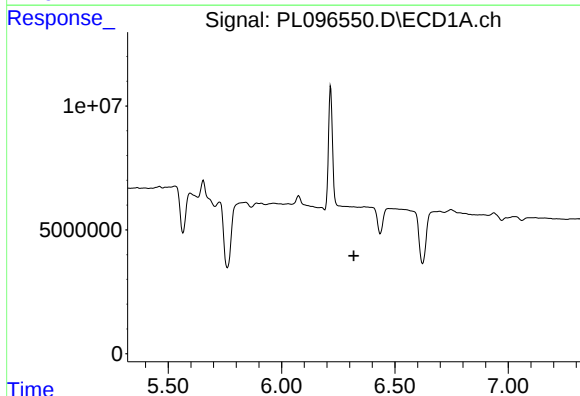


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.319 min
Response: 0
Conc: N.D.

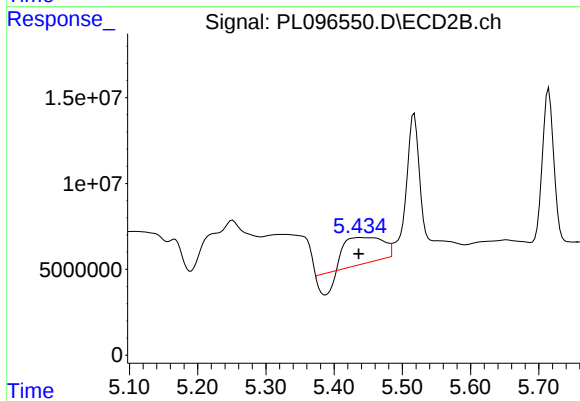

#13 Dieldrin


R.T.: 5.437 min
Delta R.T.: 0.001 min
Response: 48947721
Conc: 7.18 ng/ml

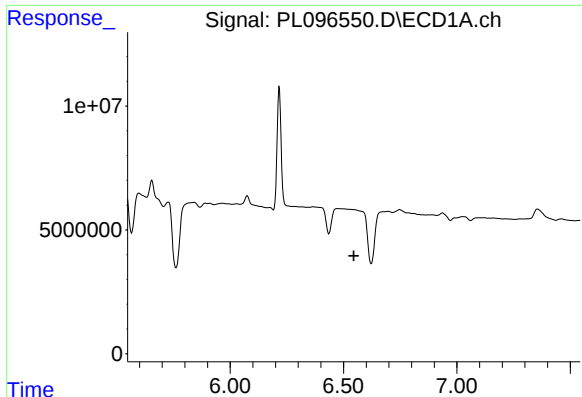

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

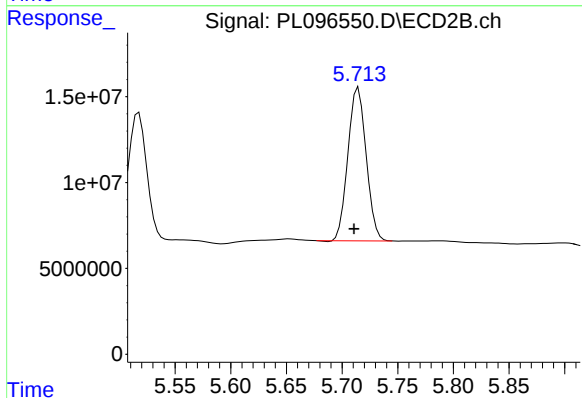


#14 Endrin

R.T.: 5.715 min
Delta R.T.: 0.004 min
Response: 102021116
Conc: 16.73 ng/ml

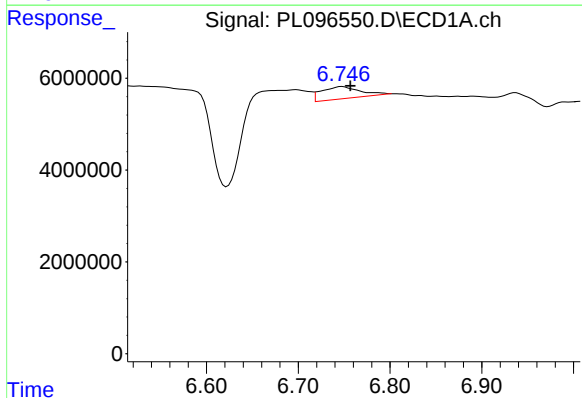


#15 Endosulfan II

R.T.: 6.748 min
Delta R.T.: -0.009 min
Response: 7724048
Conc: 2.23 ng/ml

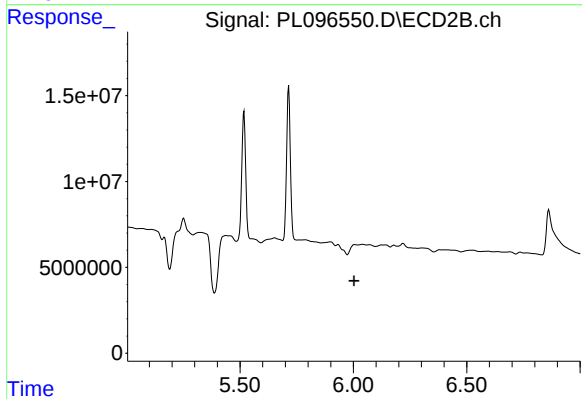

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.003 min
Response: 0
Conc: N.D.

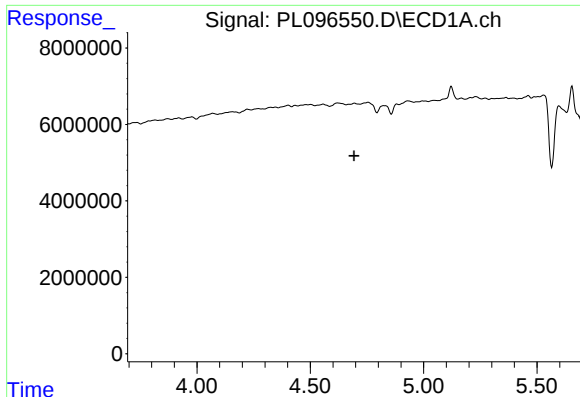

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.693 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

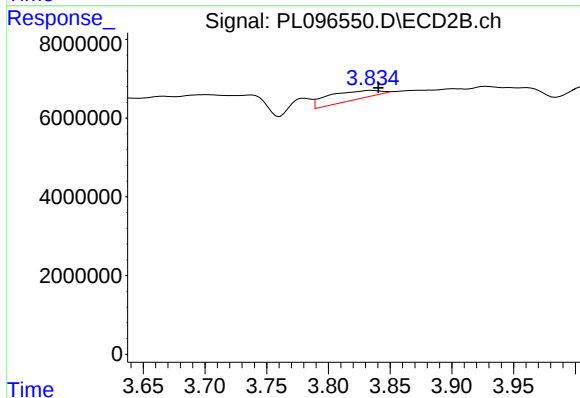


#23 Chlordane-1

R.T.: 3.835 min
Delta R.T.: -0.005 min
Response: 6540608
Conc: 27.67 ng/ml

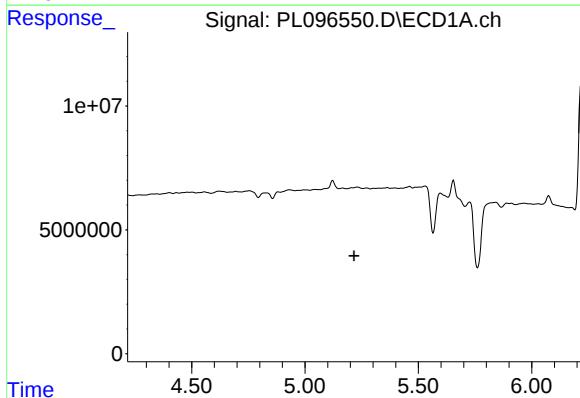


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 5.217 min
Response: 0
Conc: N.D.

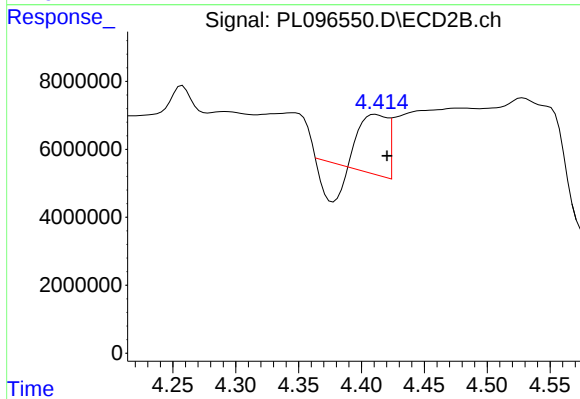

#24 Chlordane-2


R.T.: 4.411 min
Delta R.T.: -0.009 min
Response: 19934234
Conc: 72.53 ng/ml

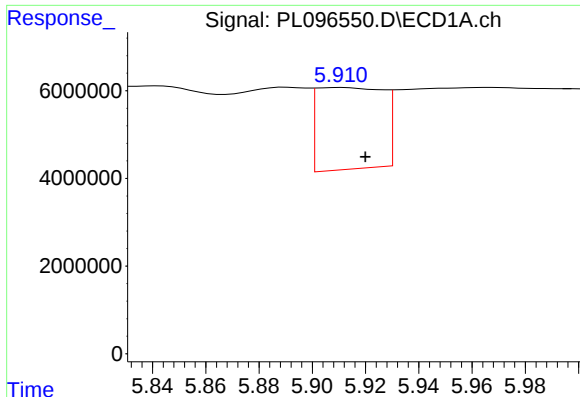

#25 Chlordane-3


R.T.: 5.911 min
Delta R.T.: -0.009 min
Response: 32185728
Conc: 43.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

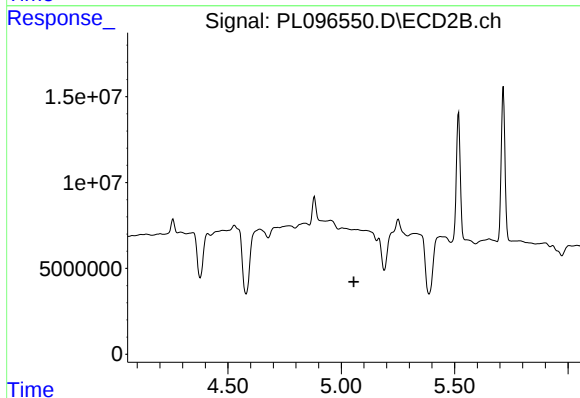


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.055 min
Response: 0
Conc: N.D.

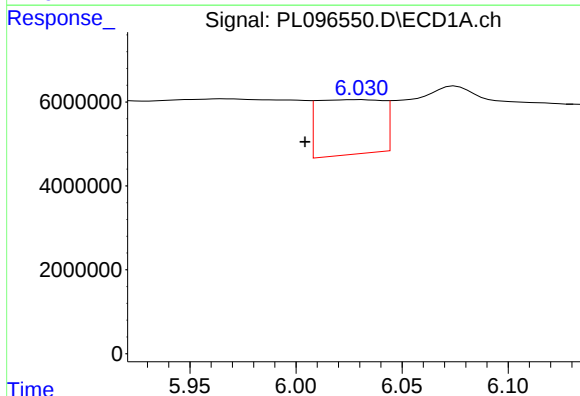


#26 Chlordane-4

R.T.: 6.030 min
Delta R.T.: 0.026 min
Response: 28089368
Conc: 31.31 ng/ml

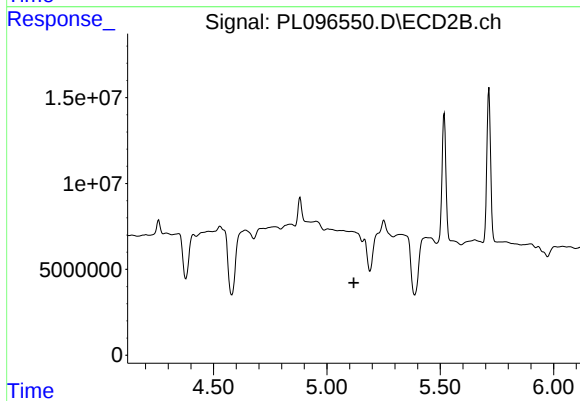

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 5.118 min
Response: 0
Conc: N.D.

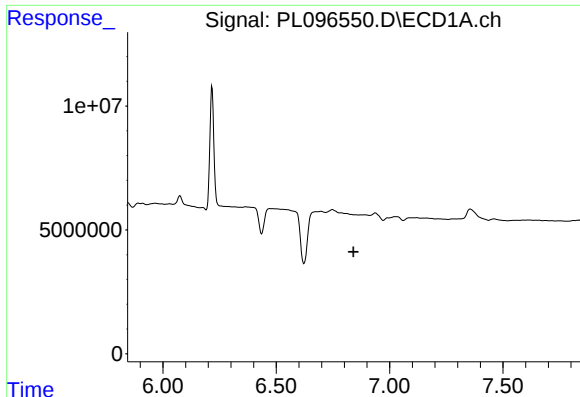

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 6.841 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

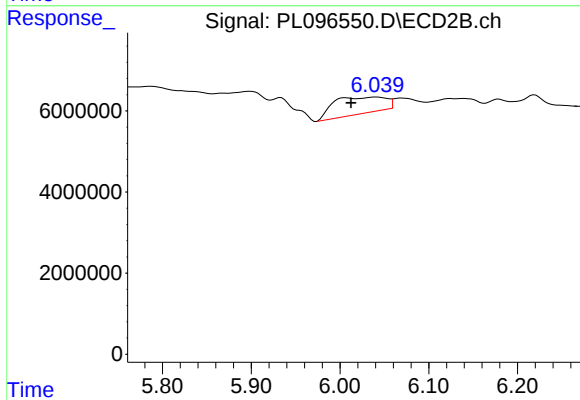


#27 Chlordane-5

R.T.: 6.041 min
Delta R.T.: 0.028 min
Response: 16739004
Conc: 59.05 ng/ml

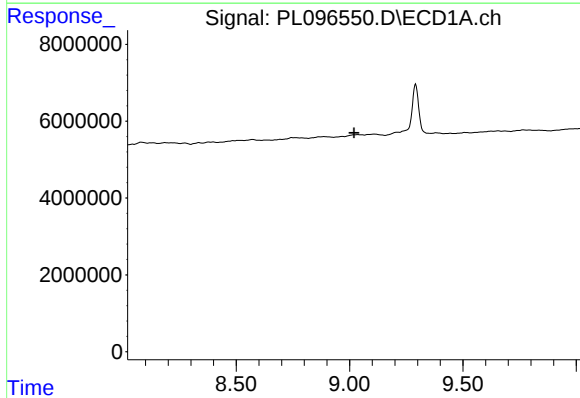

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.020 min
Response: 0
Conc: N.D.

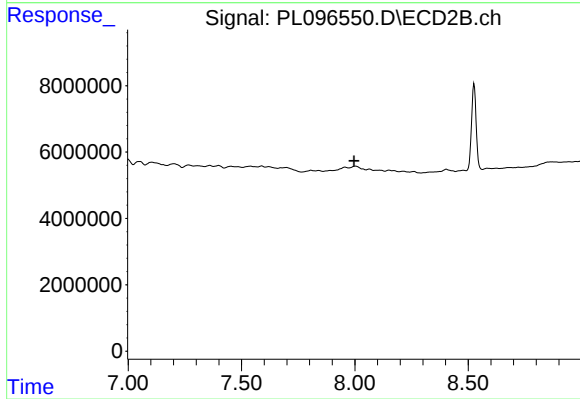

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.997 min
Response: 0
Conc: N.D.