

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072425\
 Data File : PL096566.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jul 2025 18:23
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 23:34:53 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 07 15:22:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	2.828	74689111	129.8E6	20.469	22.485
28)	SA Decachlor...	9.016	7.992	59798307	90723174	21.257	18.194
Target Compounds							
8)	B Heptachlo...	5.657	0.000	5716740	0	1.378	N.D. #
9)	A Endosulfan I	6.029f	0.000	21753002	0	5.388	N.D. #
10)	B gamma-Chl...	5.901f	0.000	34756064	0	7.855	N.D. #
11)	B alpha-Chl...	6.029f	0.000	21753002	0	4.968	N.D. #
14)	MA Endrin	0.000	5.717	0	9516568	N.D.	1.561 #
15)	B Endosulfa...	6.743	0.000	6107904	0	1.760	N.D. #
18)	B Endrin al...	0.000	6.172	0	32563593	N.D.	7.310 #
25)	Chlordane-3	5.901f	0.000	34756064	0	47.175	N.D. #
26)	Chlordane-4	6.029f	0.000	21753002	0	24.245	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072425\
Data File : PL096566.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2025 18:23
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 23:34:53 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
Quant Title : GC Extractables
QLast Update : Mon Jul 07 15:22:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

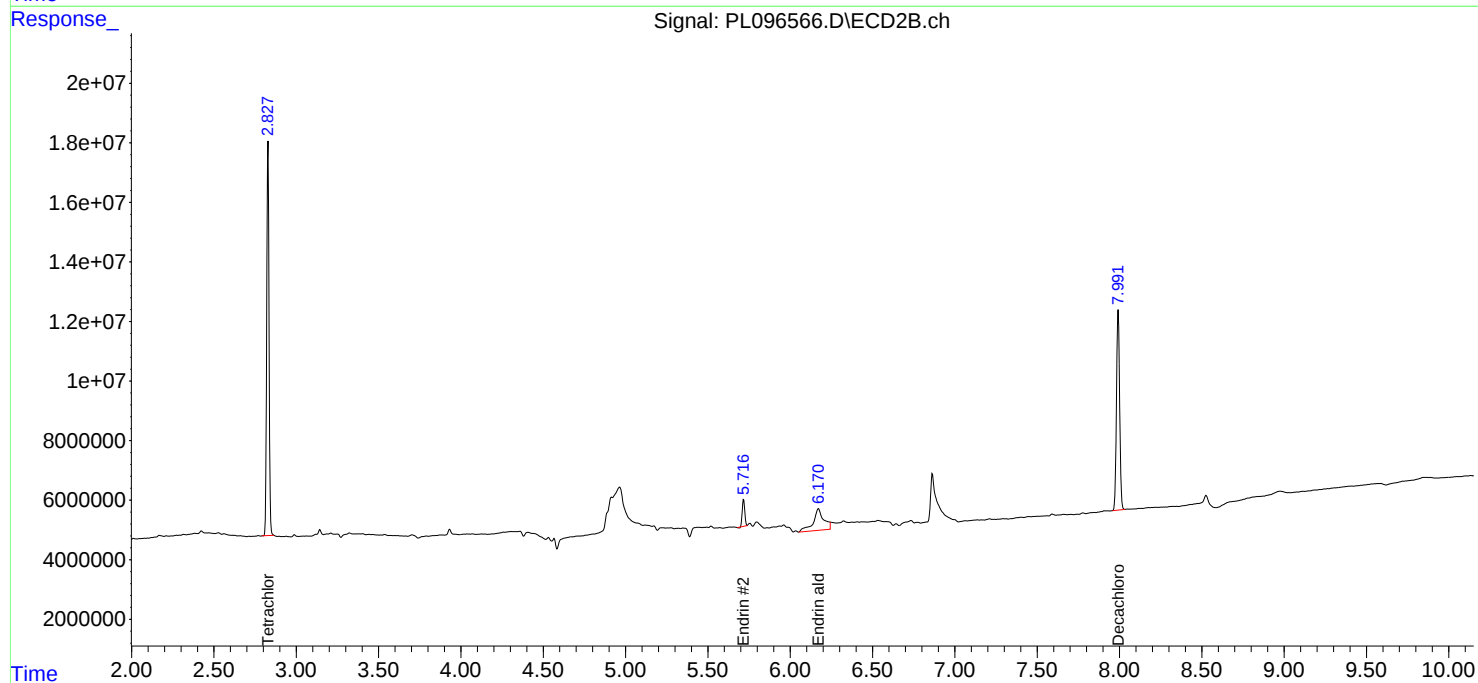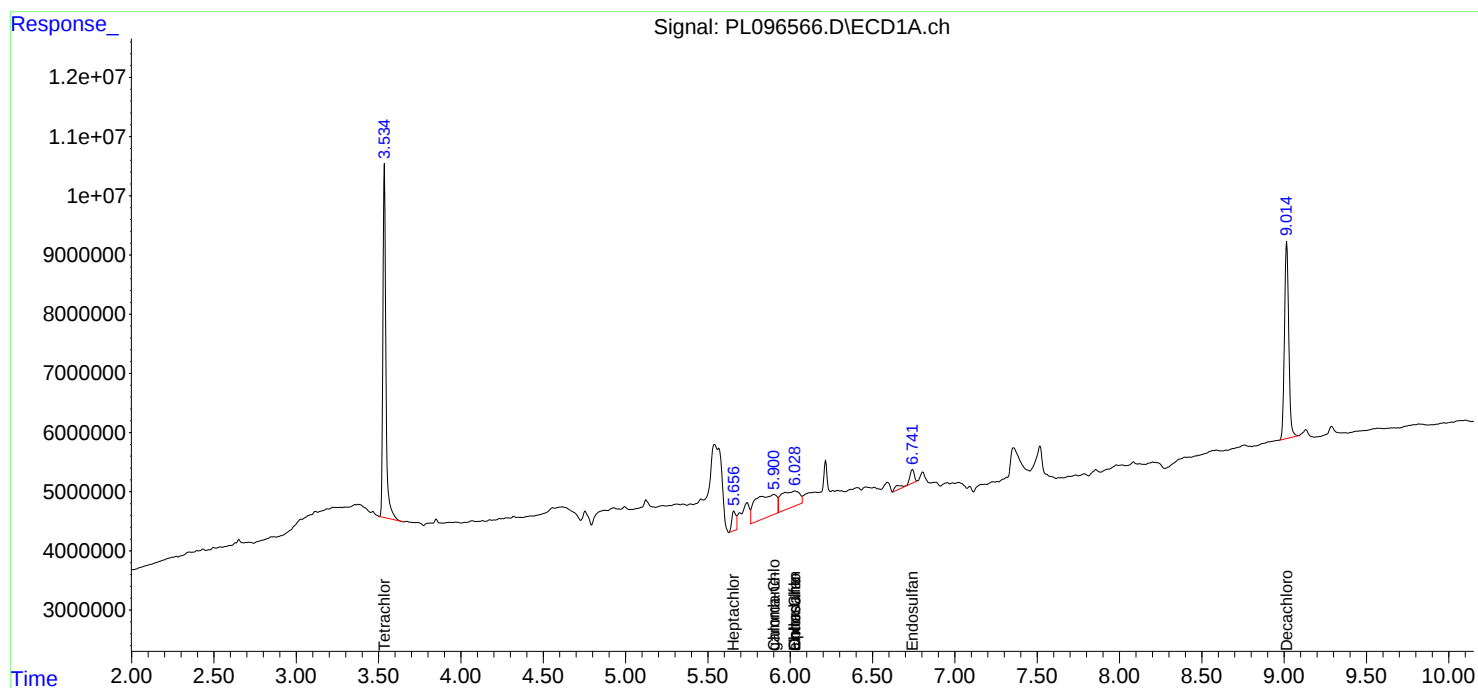


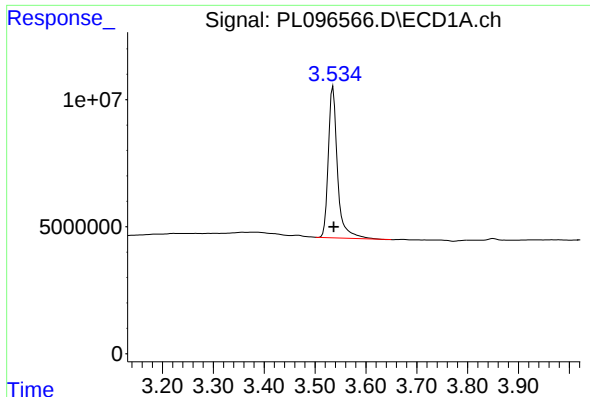

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: -0.002 min
Response: 74689111
Conc: 20.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

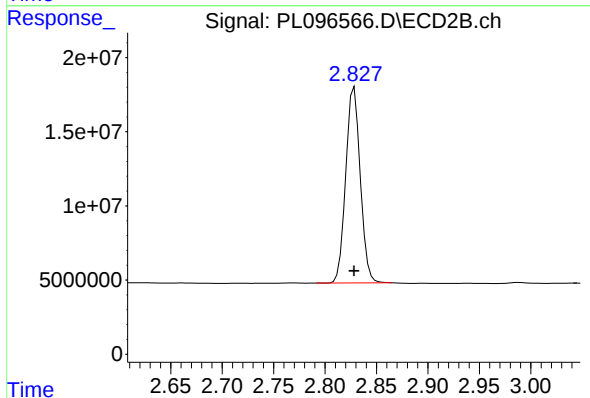


#1 Tetrachloro-m-xylene

R.T.: 2.828 min
Delta R.T.: 0.000 min
Response: 129767766
Conc: 22.49 ng/ml

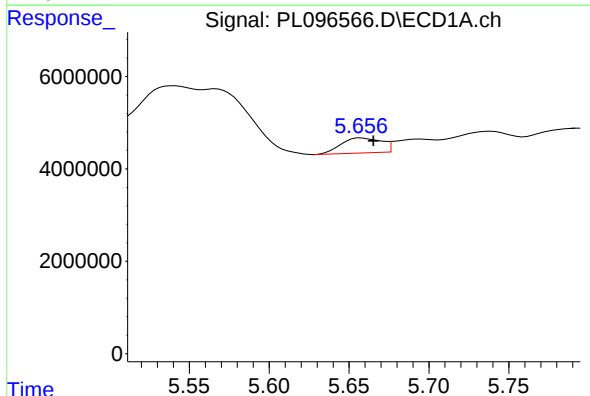


#8 Heptachlor epoxide

R.T.: 5.657 min
Delta R.T.: -0.008 min
Response: 5716740
Conc: 1.38 ng/ml

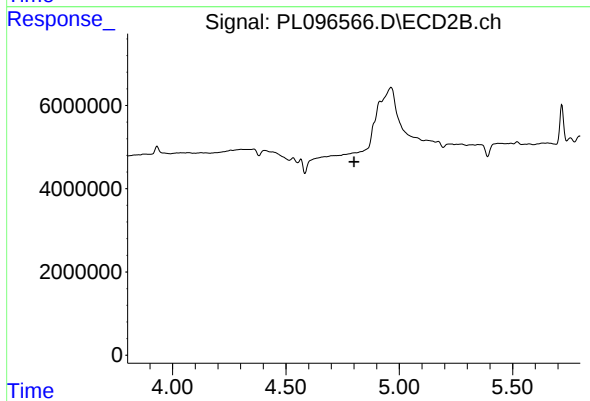

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.800 min
Response: 0
Conc: N.D.

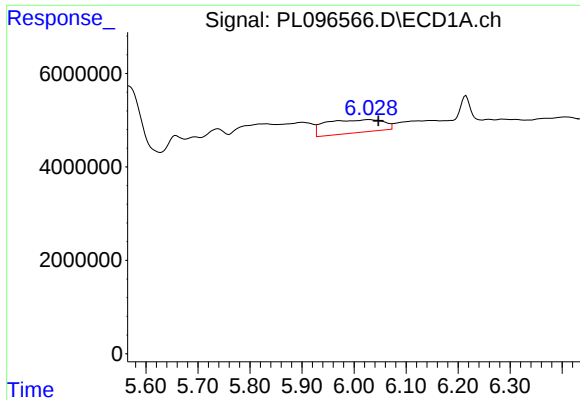

#9 Endosulfan I


R.T.: 6.029 min
Delta R.T.: -0.018 min
Response: 21753002
Conc: 5.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

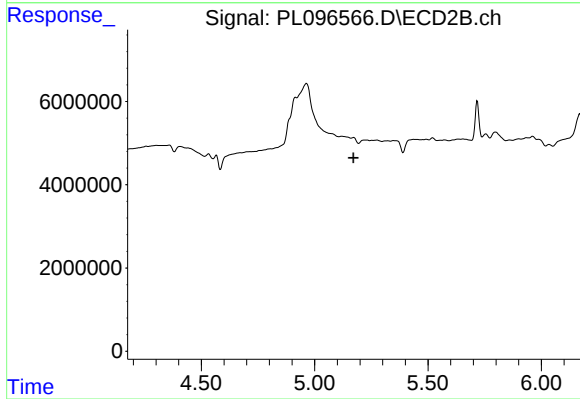


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.172 min
Response: 0
Conc: N.D.

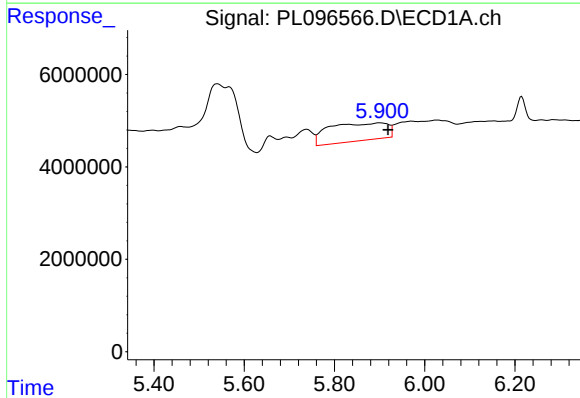


#10 gamma-Chlordane

R.T.: 5.901 min
Delta R.T.: -0.018 min
Response: 34756064
Conc: 7.85 ng/ml

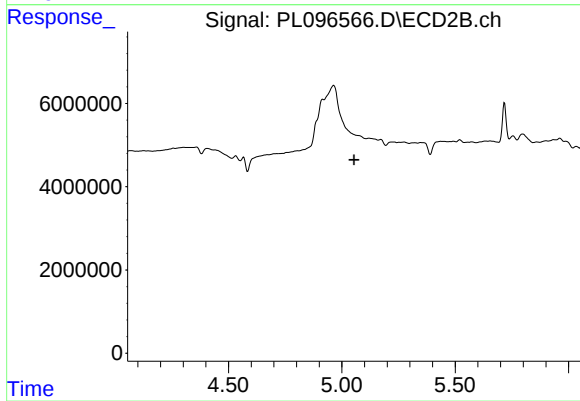

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.054 min
Response: 0
Conc: N.D.

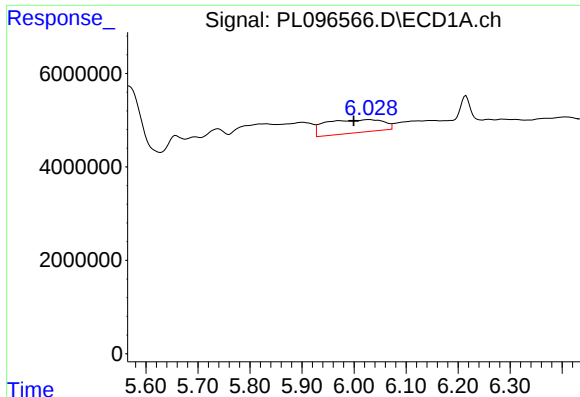

#11 alpha-Chlordane


R.T.: 6.029 min
Delta R.T.: 0.029 min
Response: 21753002
Conc: 4.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

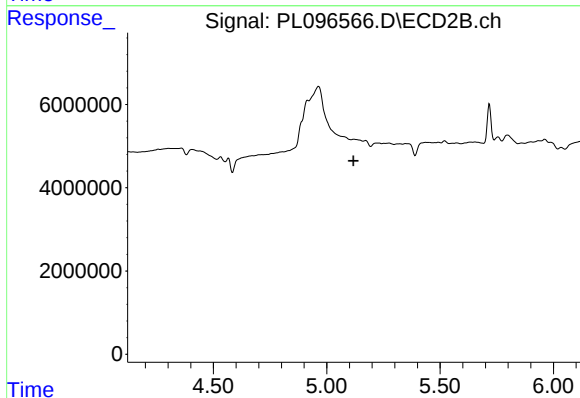


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.119 min
Response: 0
Conc: N.D.

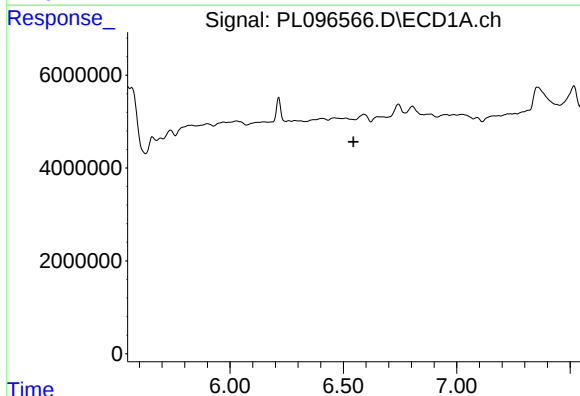


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.545 min
Response: 0
Conc: N.D.

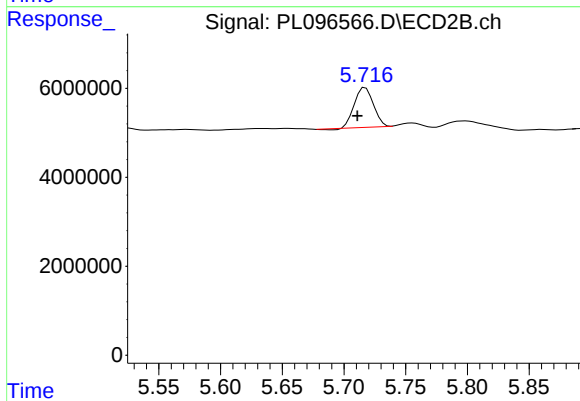

#14 Endrin


R.T.: 5.717 min
Delta R.T.: 0.007 min
Response: 9516568
Conc: 1.56 ng/ml

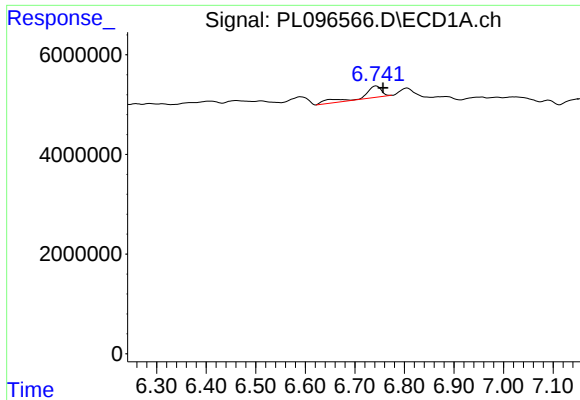

#15 Endosulfan II


R.T.: 6.743 min
Delta R.T.: -0.014 min
Response: 6107904
Conc: 1.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

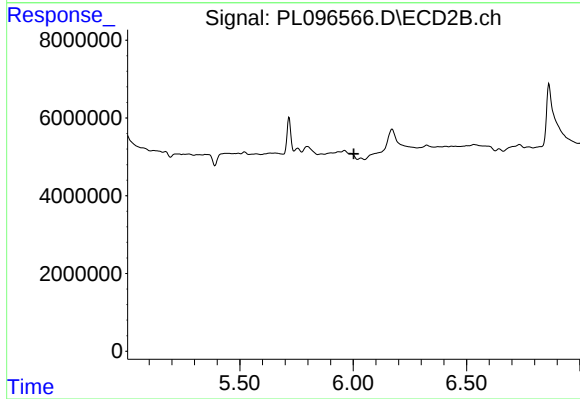


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.003 min
Response: 0
Conc: N.D.

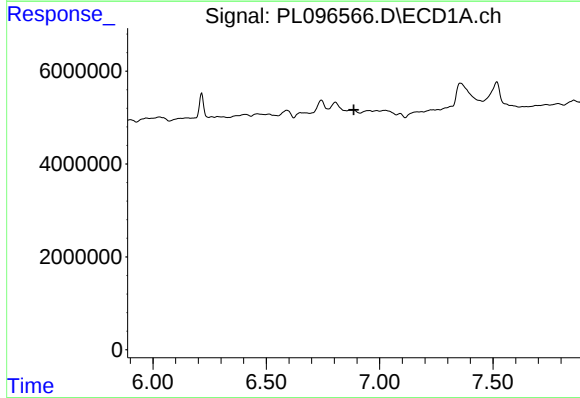


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.886 min
Response: 0
Conc: N.D.

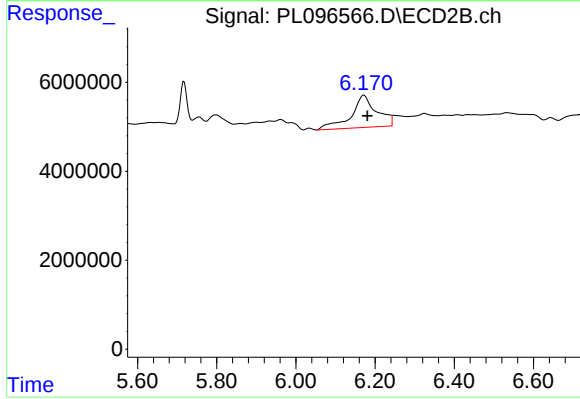

#18 Endrin aldehyde


R.T.: 6.172 min
Delta R.T.: -0.009 min
Response: 32563593
Conc: 7.31 ng/ml

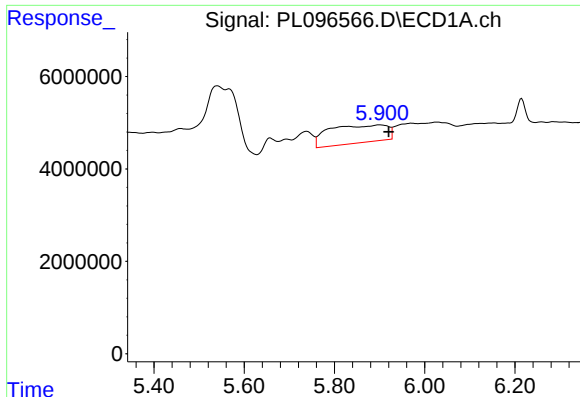

#25 Chlordane-3


R.T.: 5.901 min
Delta R.T.: -0.019 min
Response: 34756064
Conc: 47.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

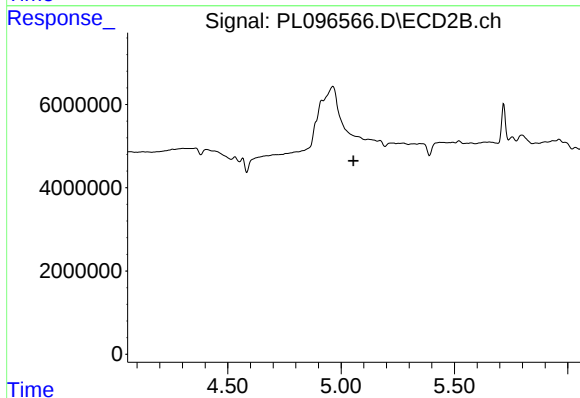


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.055 min
Response: 0
Conc: N.D.

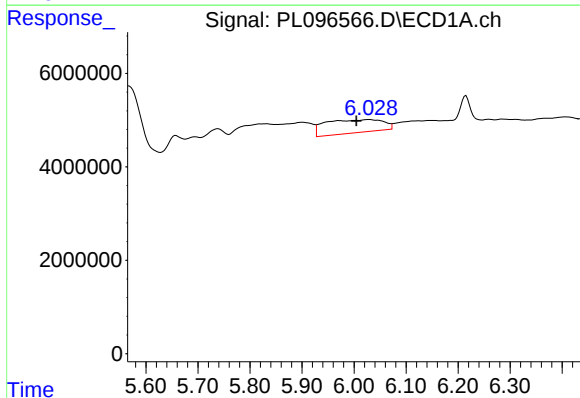


#26 Chlordane-4

R.T.: 6.029 min
Delta R.T.: 0.025 min
Response: 21753002
Conc: 24.24 ng/ml

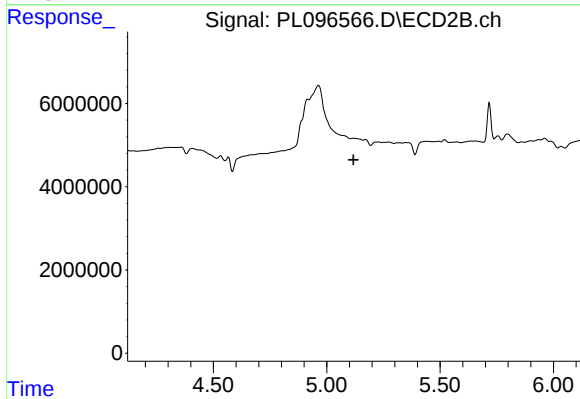

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 5.118 min
Response: 0
Conc: N.D.

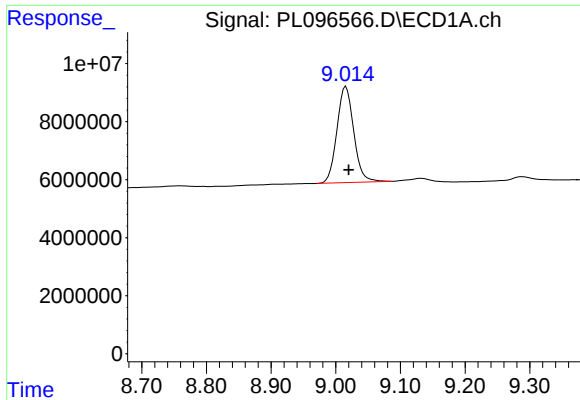

#28 Decachlorobiphenyl

R.T.: 9.016 min
Delta R.T.: -0.004 min
Response: 59798307
Conc: 21.26 ng/ml

Instrument :
ECD_L
ClientSampleId :

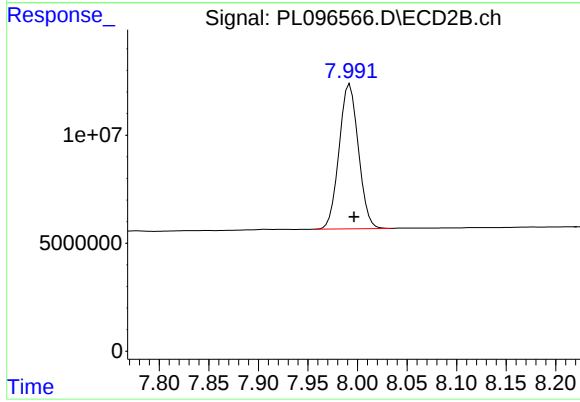

#28 Decachlorobiphenyl

R.T.: 7.992 min
Delta R.T.: -0.004 min
Response: 90723174
Conc: 18.19 ng/ml