

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072425\
 Data File : PL096572.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jul 2025 20:26
 Operator : AR\AJ
 Sample : Q2481-16 10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 23:38:15 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 07 15:22:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	0.000	2.829	0	9324747	N.D.	1.616 #
28)	SA Decachlor...	0.000	7.992	0	9577411	N.D.	1.921 #
Target Compounds							
4)	MA Heptachlor	4.908	4.006	262.1E6	33452734	57.204	4.397 #
6)	B beta-BHC	0.000	3.967	0	33395323	N.D.	9.754 #
7)	B delta-BHC	4.769f	0.000	128.4E6	0	28.660	N.D. #
8)	B Heptachlo...	5.676	4.798	128.1E6	20960672	30.862	3.136 #
18)	B Endrin al...	0.000	6.177	0	26100533	N.D.	5.859 #
19)	B Endosulfa...	0.000	6.403	0	875588	N.D.	0.156 #
21)	B Endrin ke...	0.000	6.882f	0	3047646	N.D.	0.487 #
23)	Chlordane-1	0.000	3.870f	0	87001659	N.D.	368.088 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072425\
Data File : PL096572.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2025 20:26
Operator : AR\AJ
Sample : Q2481-16 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 23:38:15 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
Quant Title : GC Extractables
QLast Update : Mon Jul 07 15:22:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

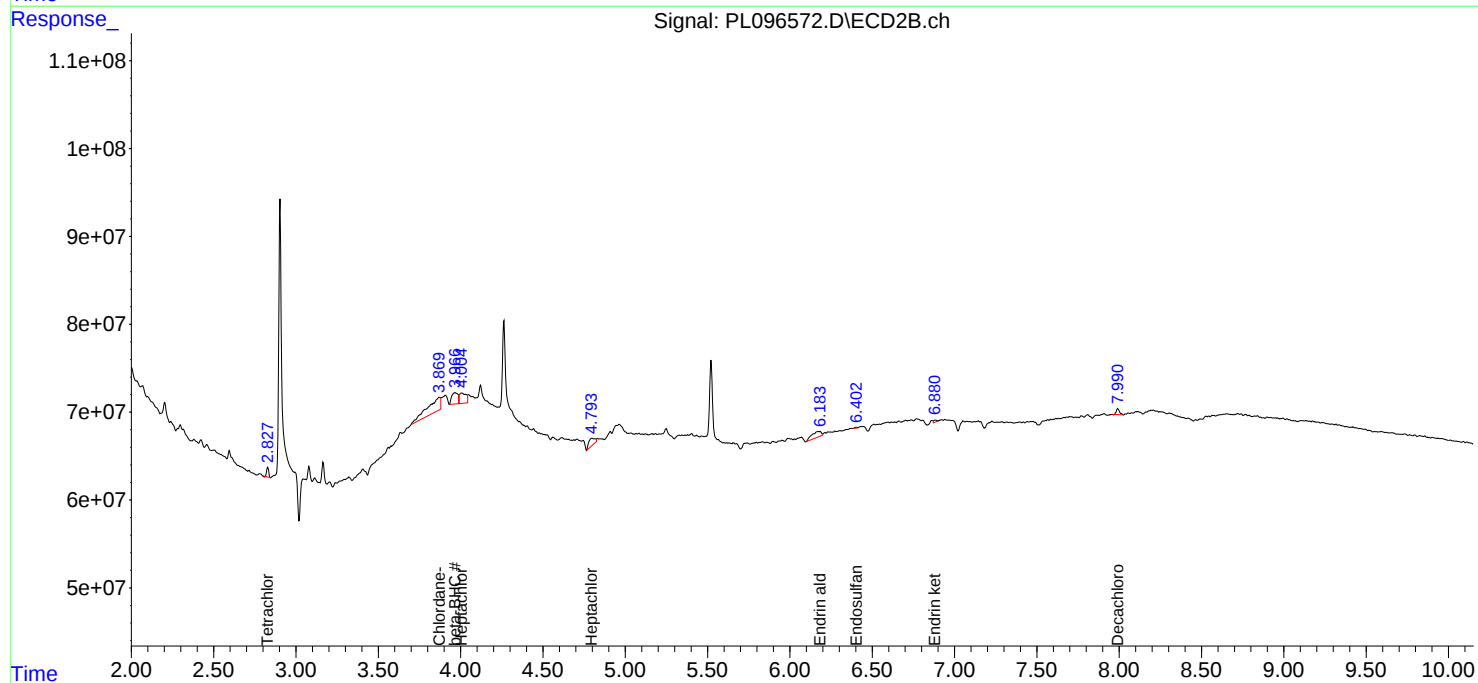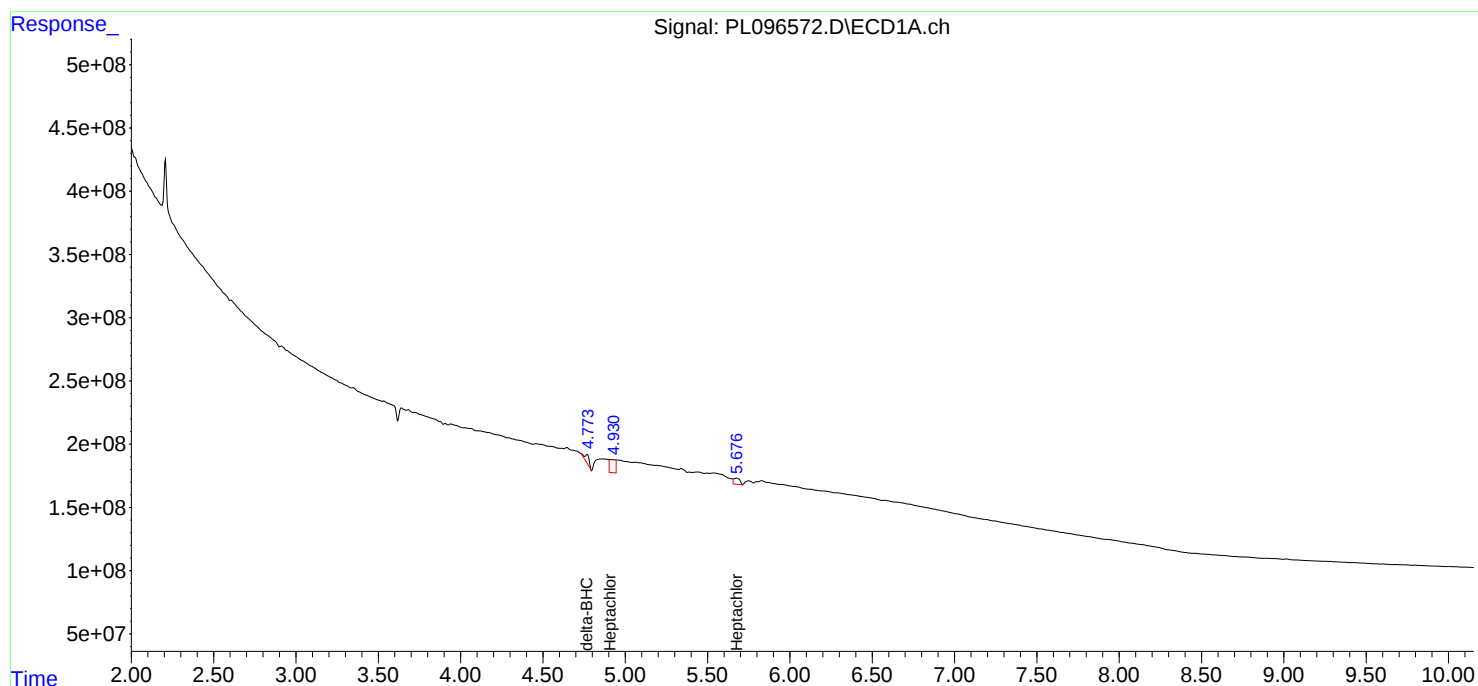


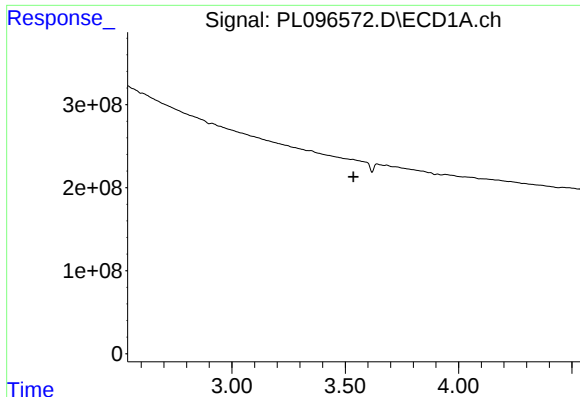

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.537 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

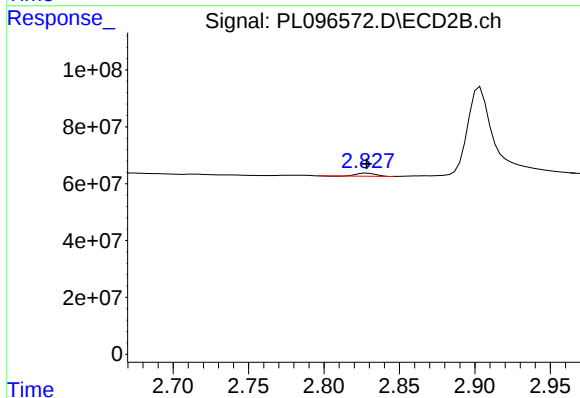


#1 Tetrachloro-m-xylene

R.T.: 2.829 min
Delta R.T.: 0.000 min
Response: 9324747
Conc: 1.62 ng/ml

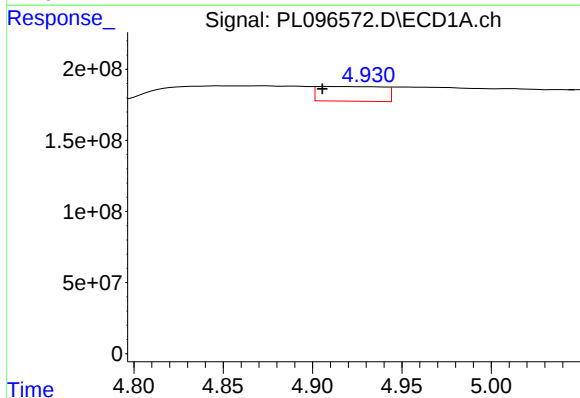


#4 Heptachlor

R.T.: 4.908 min
Delta R.T.: 0.003 min
Response: 262063664
Conc: 57.20 ng/ml

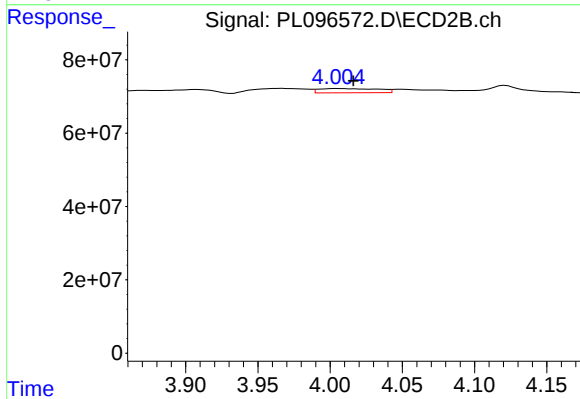

#4 Heptachlor


R.T.: 4.006 min
Delta R.T.: -0.011 min
Response: 33452734
Conc: 4.40 ng/ml

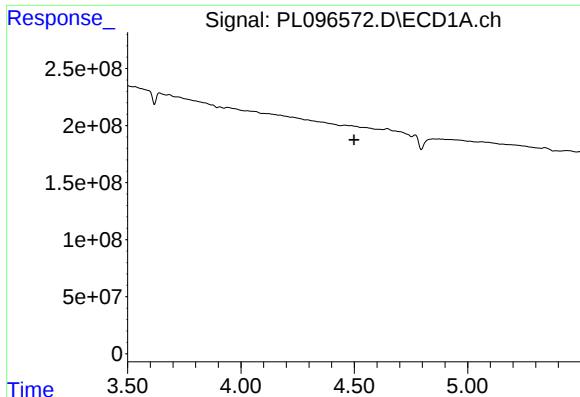

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.499 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

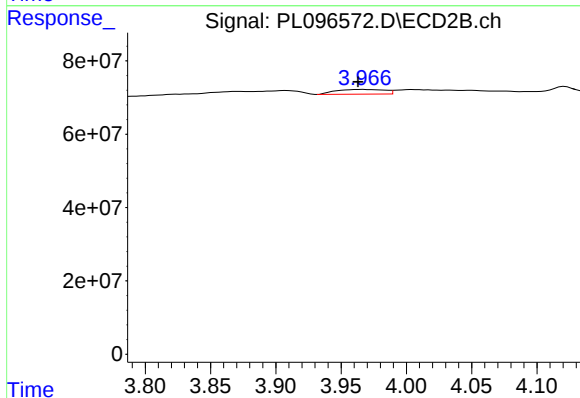


#6 beta-BHC

R.T.: 3.967 min
Delta R.T.: 0.004 min
Response: 33395323
Conc: 9.75 ng/ml

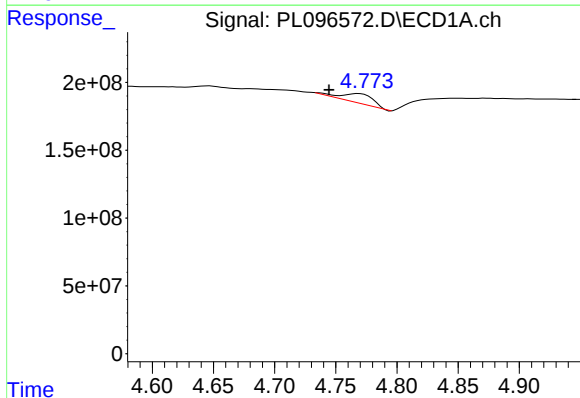


#7 delta-BHC

R.T.: 4.769 min
Delta R.T.: 0.024 min
Response: 128433097
Conc: 28.66 ng/ml

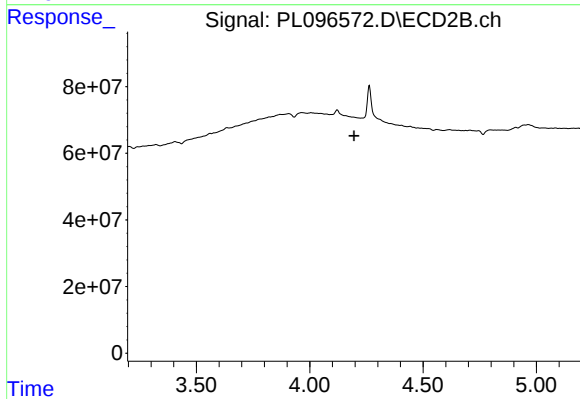

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.196 min
Response: 0
Conc: N.D.

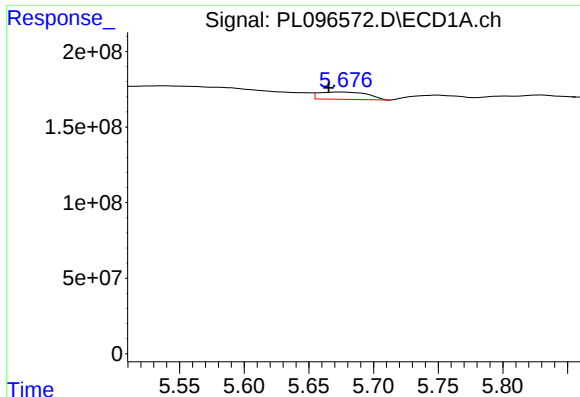

#8 Heptachlor epoxide


R.T.: 5.676 min
Delta R.T.: 0.011 min
Response: 128050185
Conc: 30.86 ng/ml

Instrument :
ECD_L
ClientSampleId :

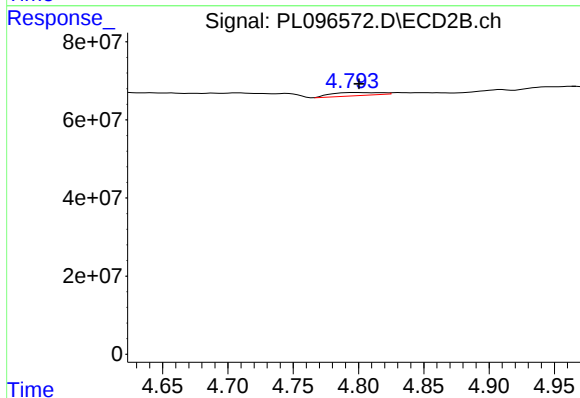


#8 Heptachlor epoxide

R.T.: 4.798 min
Delta R.T.: -0.003 min
Response: 20960672
Conc: 3.14 ng/ml

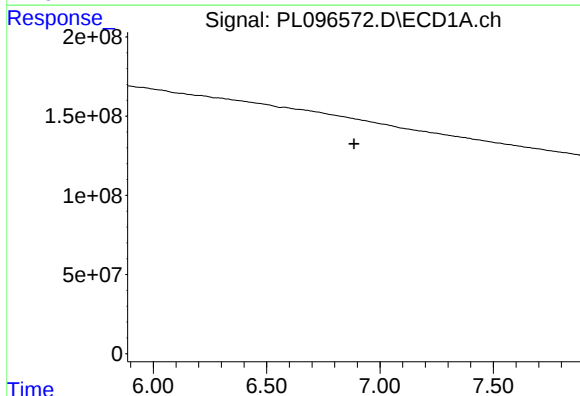


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.886 min
Response: 0
Conc: N.D.

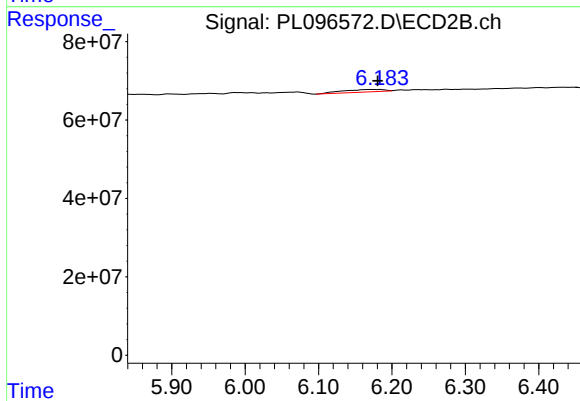

#18 Endrin aldehyde


R.T.: 6.177 min
Delta R.T.: -0.004 min
Response: 26100533
Conc: 5.86 ng/ml

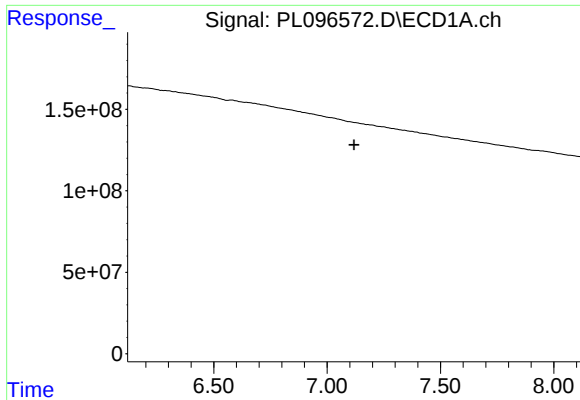

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.120 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

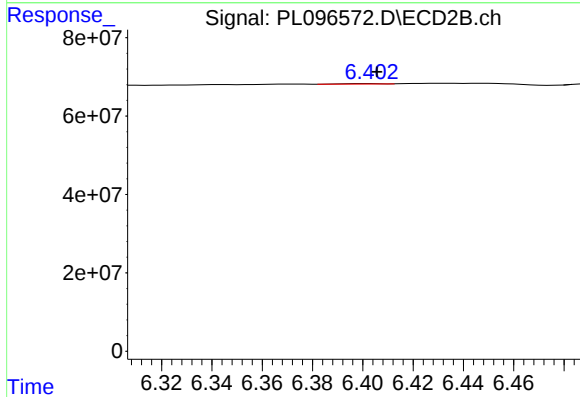


#19 Endosulfan Sulfate

R.T.: 6.403 min
Delta R.T.: -0.002 min
Response: 875588
Conc: 0.16 ng/ml

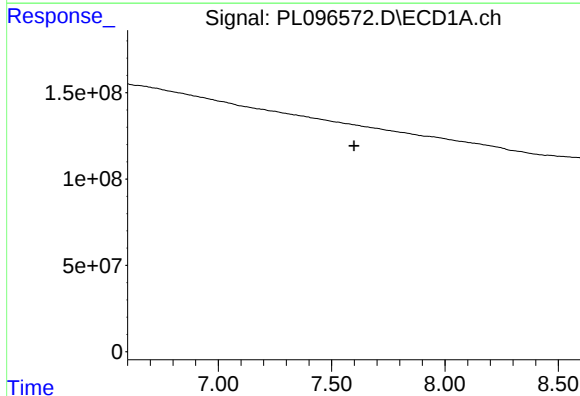


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.599 min
Response: 0
Conc: N.D.

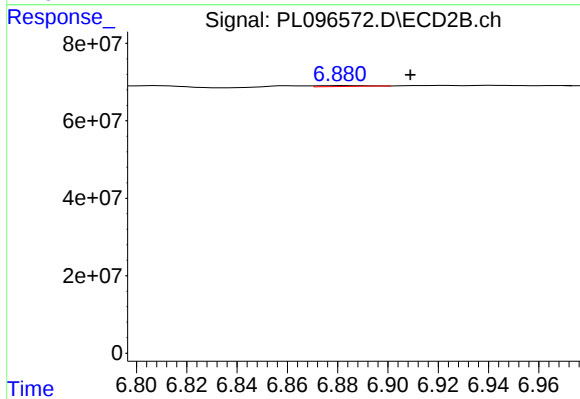

#21 Endrin ketone


R.T.: 6.882 min
Delta R.T.: -0.027 min
Response: 3047646
Conc: 0.49 ng/ml

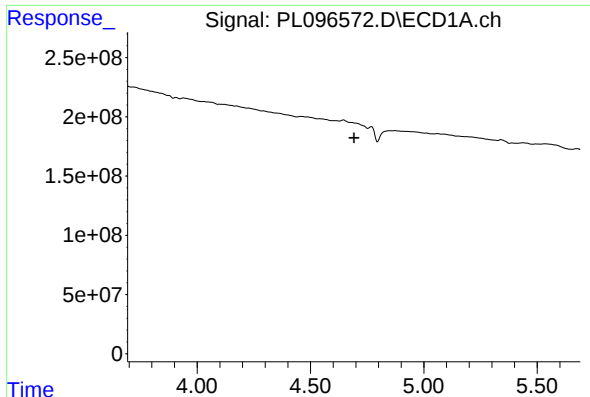

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.693 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

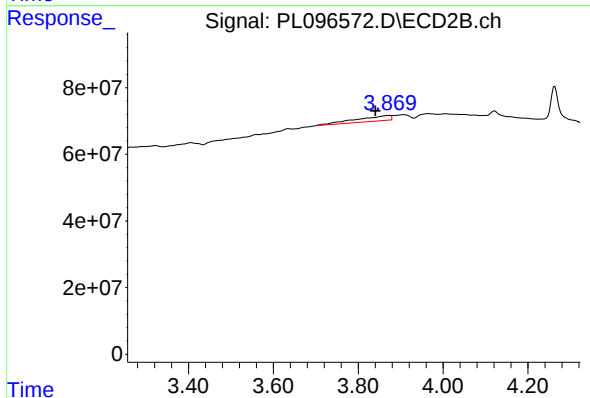


#23 Chlordane-1

R.T.: 3.870 min
Delta R.T.: 0.030 min
Response: 87001659
Conc: 368.09 ng/ml

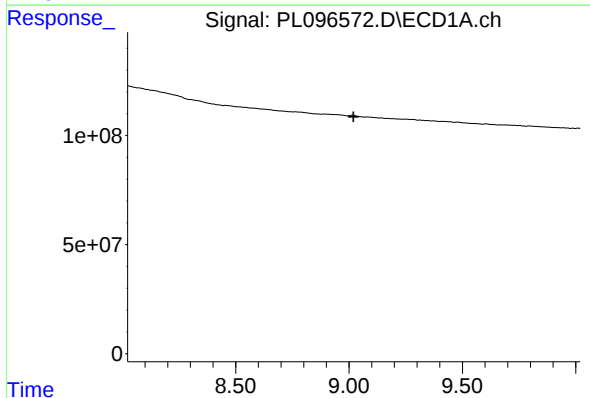

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.020 min
Response: 0
Conc: N.D.

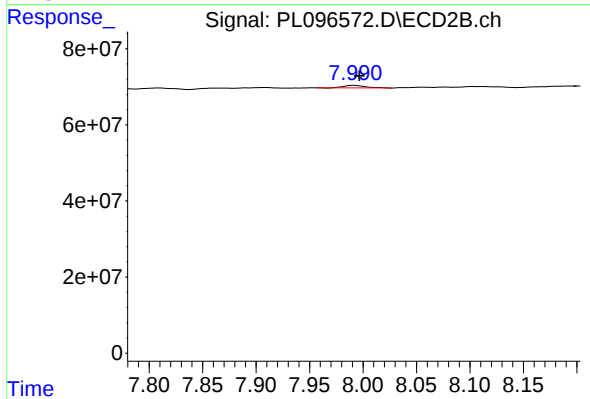

#28 Decachlorobiphenyl

R.T.: 7.992 min
Delta R.T.: -0.005 min
Response: 9577411
Conc: 1.92 ng/ml