

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072519\
 Data File : PL050778.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jul 2019 16:50
 Operator : SM\AJ
 Sample : K3990-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-1-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 00:51:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.319	3.929	193.2E6	51466505	19.226	18.038
28)	SA Decachlor...	7.979	8.959	165.9E6	46864351	16.386	16.572
Target Compounds							
8)	B Heptachlo...	0.000	5.806	0	5398122	N.D.	1.411 #
10)	B gamma-Chl...	5.195	0.000	34141371	0	2.163	N.D. #
11)	B alpha-Chl...	5.266	0.000	19119950	0	1.253	N.D. #
16)	A 4,4'-DDD	5.934	0.000	3568496	0	0.298	N.D. #
25)	Chlordane-3	5.195	0.000	34141371	0	24.390	N.D. #
26)	Chlordane-4	5.266	0.000	19119950	0	14.496	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072519\
Data File : PL050778.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jul 2019 16:50
Operator : SM\AJ
Sample : K3990-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-1-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 00:51:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

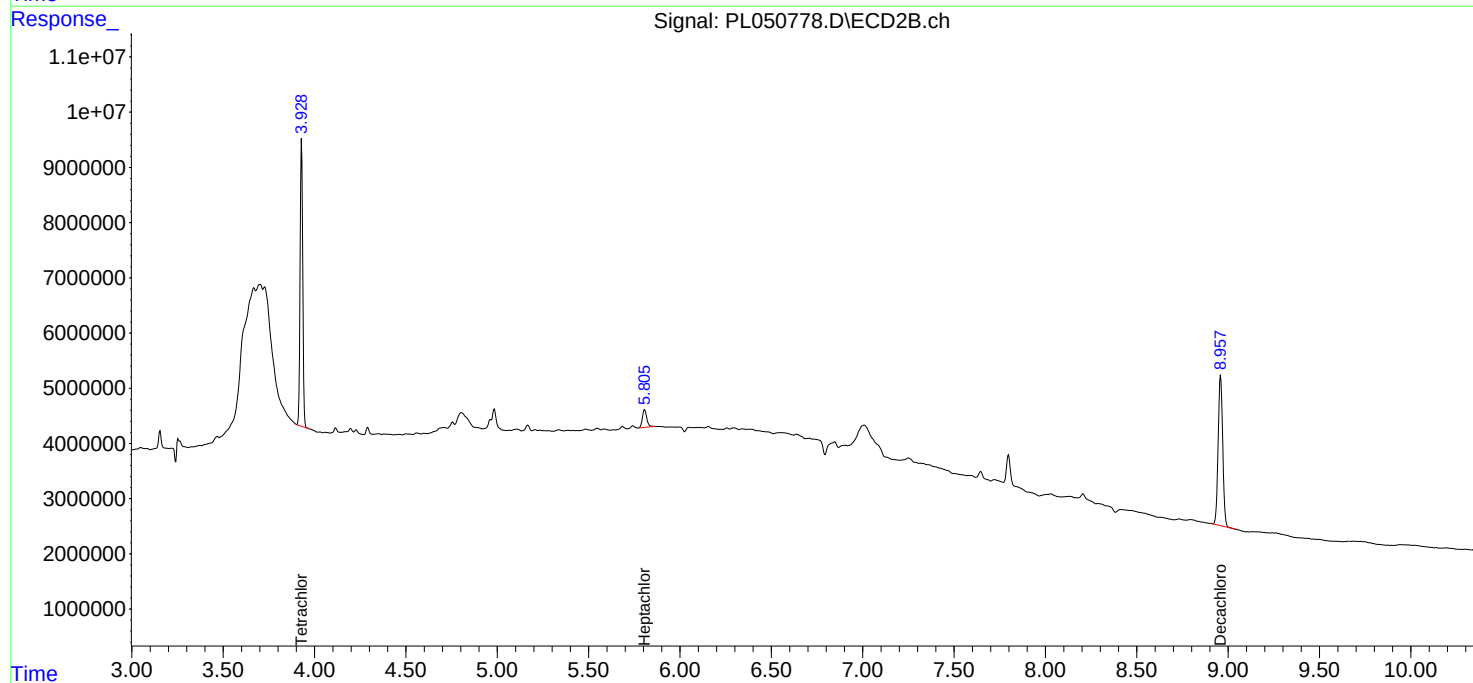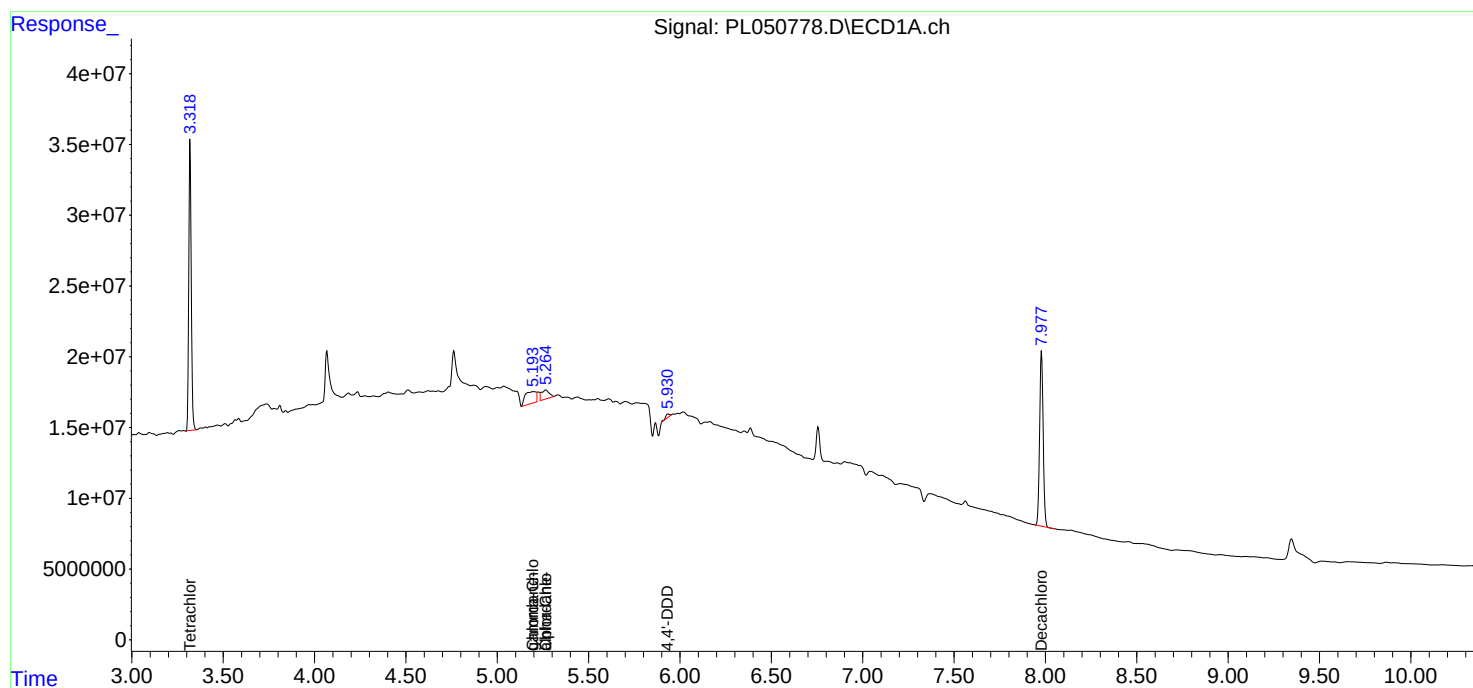


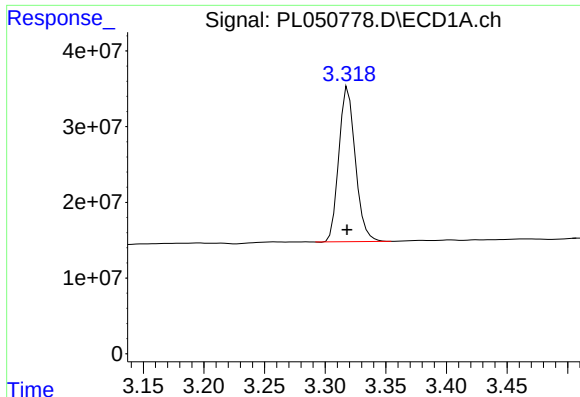

#1 Tetrachloro-m-xylene


R.T.: 3.319 min
Delta R.T.: 0.001 min
Response: 193178820
Conc: 19.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1-B

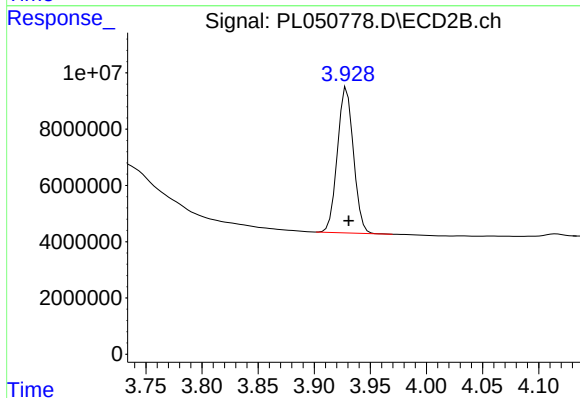


#1 Tetrachloro-m-xylene

R.T.: 3.929 min
Delta R.T.: -0.002 min
Response: 51466505
Conc: 18.04 ng/ml

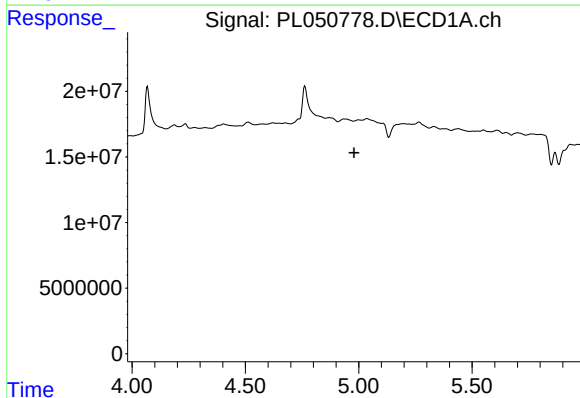


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.979 min
Response: 0
Conc: N.D.

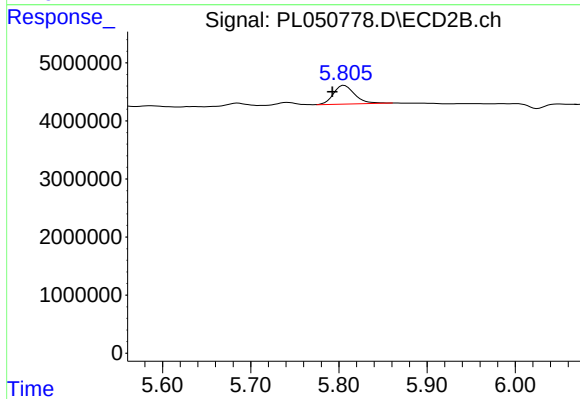

#8 Heptachlor epoxide


R.T.: 5.806 min
Delta R.T.: 0.014 min
Response: 5398122
Conc: 1.41 ng/ml

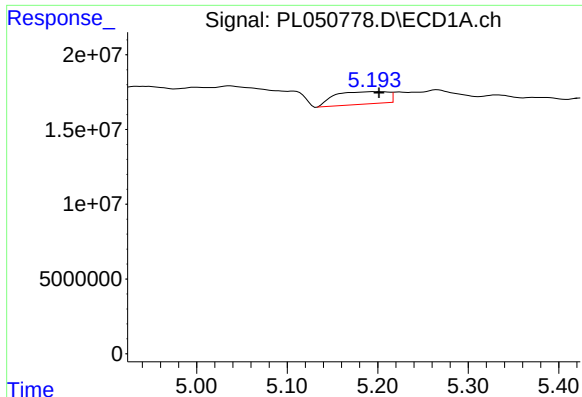

#10 gamma-Chlordane


R.T.: 5.195 min
Delta R.T.: -0.006 min
Response: 34141371
Conc: 2.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1-B

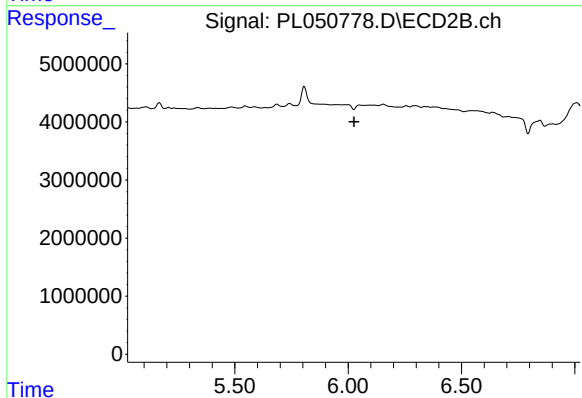


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.026 min
Response: 0
Conc: N.D.

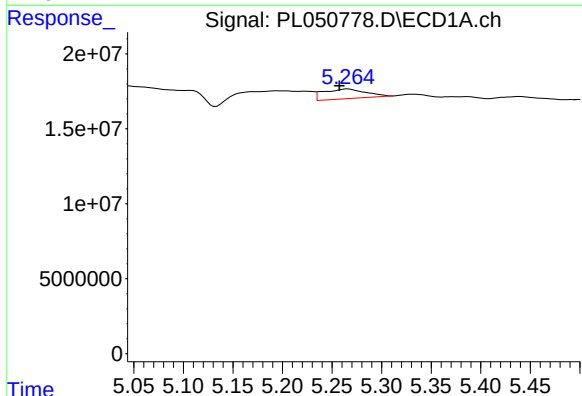


#11 alpha-Chlordane

R.T.: 5.266 min
Delta R.T.: 0.008 min
Response: 19119950
Conc: 1.25 ng/ml

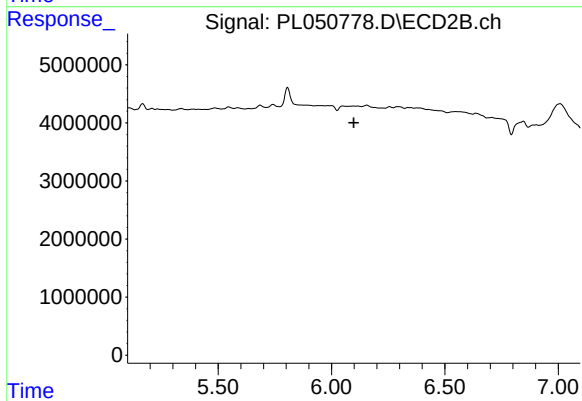

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

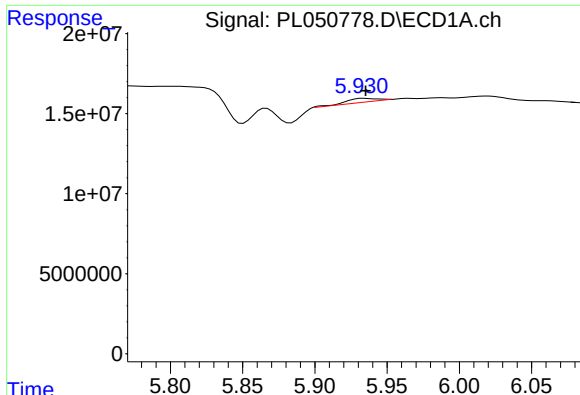

#16 4,4'-DDD


R.T.: 5.934 min
Delta R.T.: 0.000 min
Response: 3568496
Conc: 0.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1-B

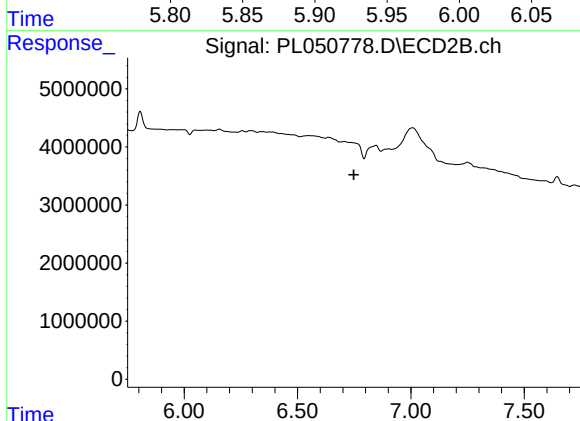


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.749 min
Response: 0
Conc: N.D.

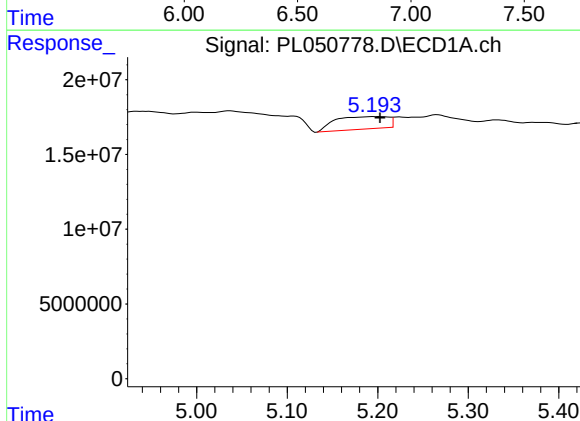


#25 Chlordane-3

R.T.: 5.195 min
Delta R.T.: -0.007 min
Response: 34141371
Conc: 24.39 ng/ml

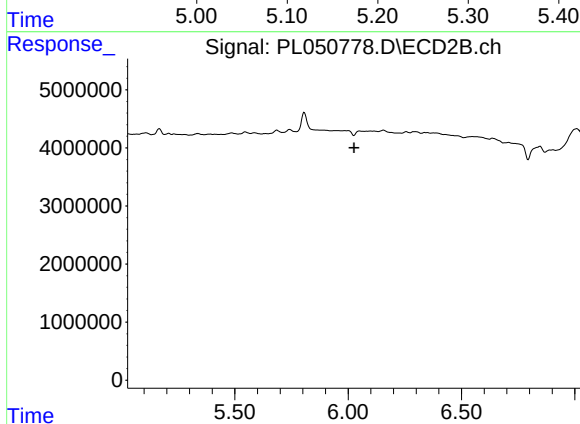

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.027 min
Response: 0
Conc: N.D.

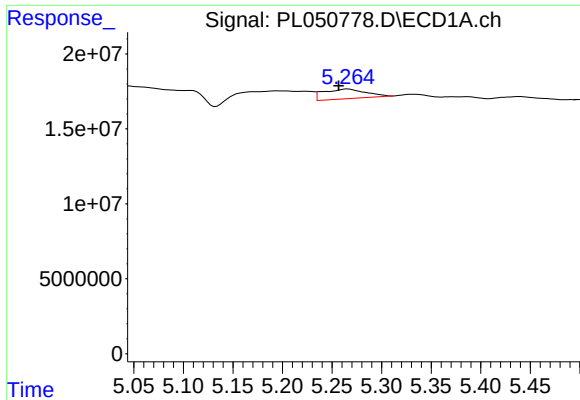

#26 Chlordane-4


R.T.: 5.266 min
Delta R.T.: 0.009 min
Response: 19119950
Conc: 14.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1-B

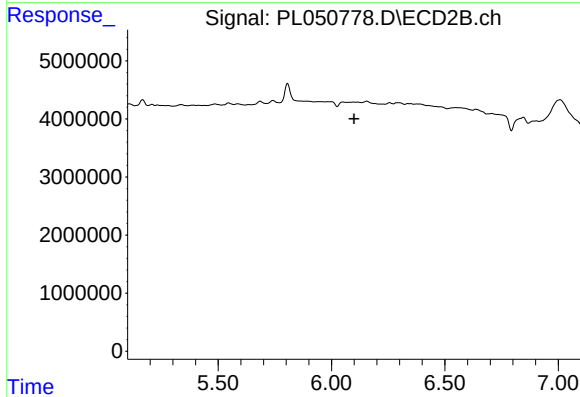


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 6.100 min
Response: 0
Conc: N.D.

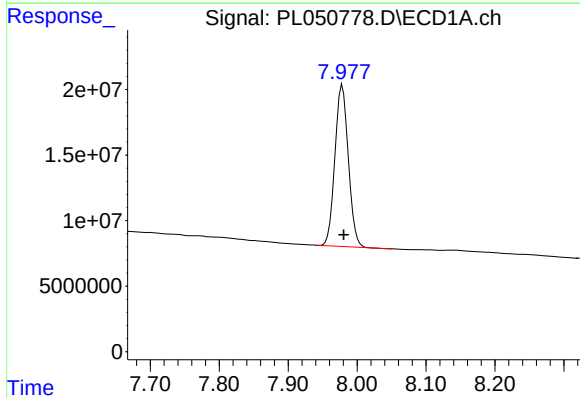

#28 Decachlorobiphenyl

R.T.: 7.979 min
Delta R.T.: -0.002 min
Response: 165918615
Conc: 16.39 ng/ml

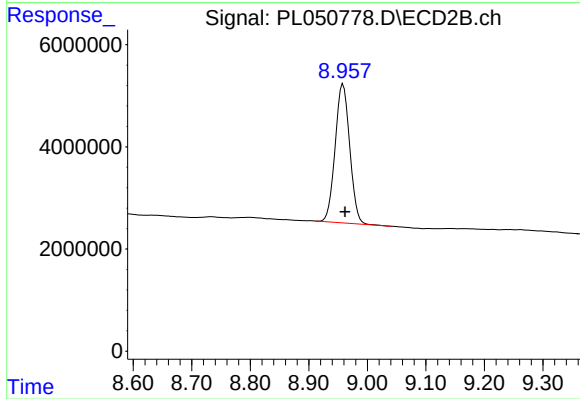

#28 Decachlorobiphenyl

R.T.: 8.959 min
Delta R.T.: -0.003 min
Response: 46864351
Conc: 16.57 ng/ml