

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072519\
 Data File : PL050784.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jul 2019 18:21
 Operator : SM\AJ
 Sample : K3990-06
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-3-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 00:53:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.319	3.929	216.0E6	57808013	21.500	20.261
28)	SA Decachlor...	7.980	8.958	200.2E6	53506813	19.771	18.921
Target Compounds							
6)	B beta-BHC	0.000	4.755f	0	659894	N.D.	0.382 #
8)	B Heptachlo...	0.000	5.807	0	6720788	N.D.	1.757 #
11)	B alpha-Chl...	5.267	0.000	8305114	0	0.544	N.D. #
12)	B 4,4'-DDE	5.425	0.000	8011336	0	0.535	N.D. #
13)	MA Dieldrin	5.548	0.000	12414680	0	0.801	N.D. #
26)	Chlordane-4	5.267	0.000	8305114	0	6.297	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072519\
Data File : PL050784.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jul 2019 18:21
Operator : SM\AJ
Sample : K3990-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-3-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 00:53:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

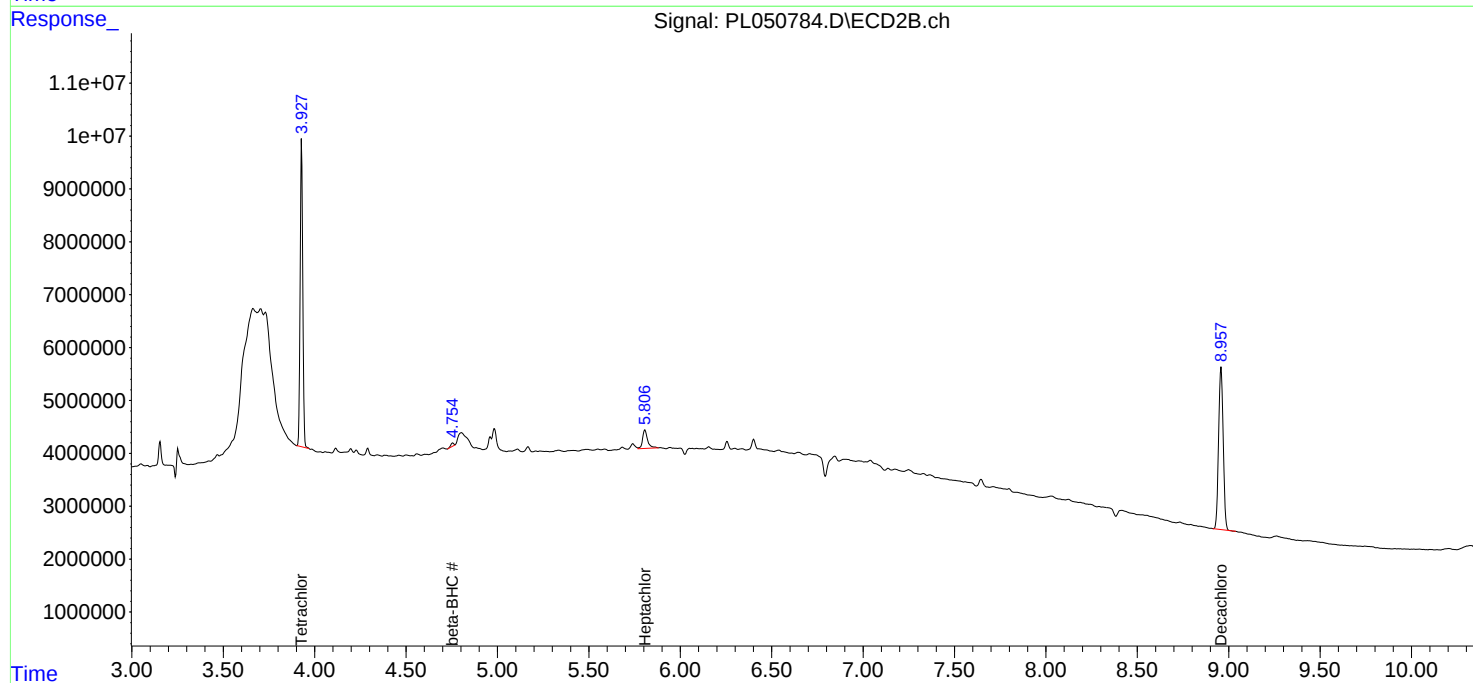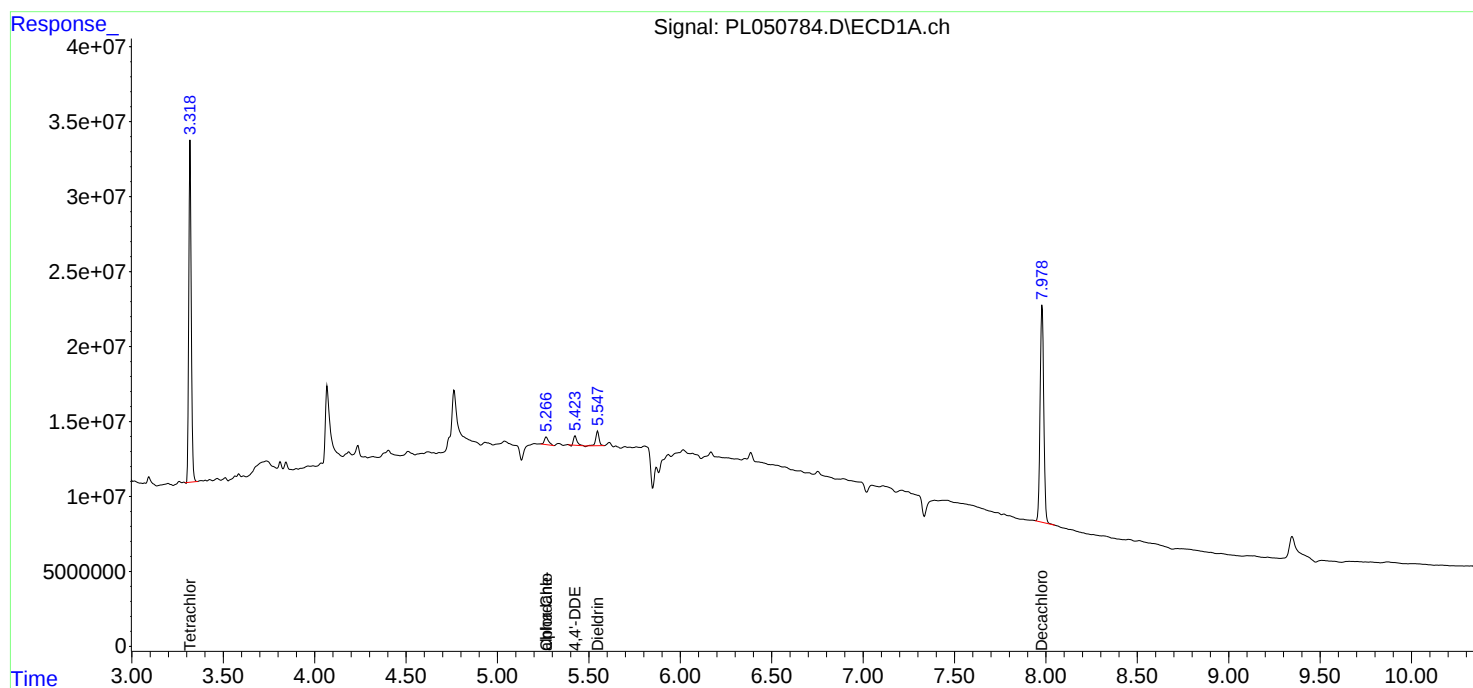


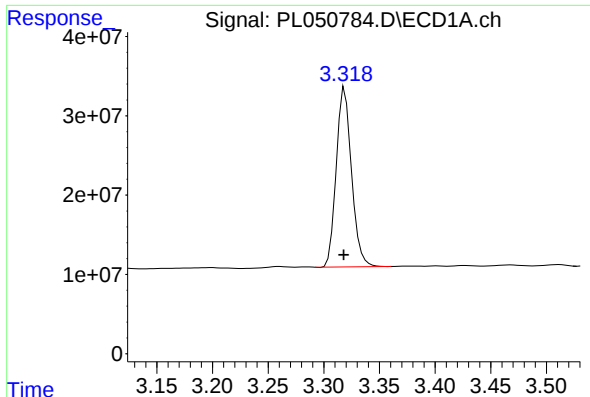

#1 Tetrachloro-m-xylene


R.T.: 3.319 min
Delta R.T.: 0.000 min
Response: 216033124
Conc: 21.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3-B

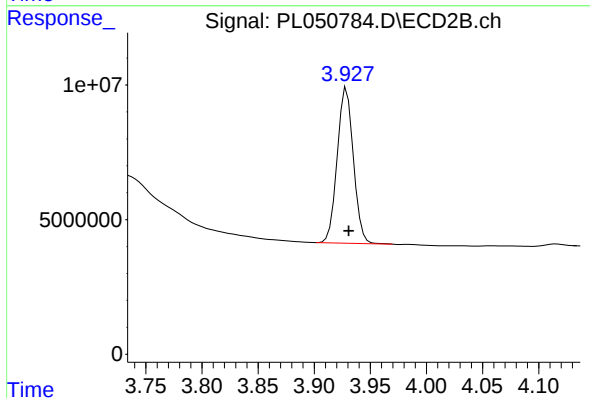


#1 Tetrachloro-m-xylene

R.T.: 3.929 min
Delta R.T.: -0.002 min
Response: 57808013
Conc: 20.26 ng/ml

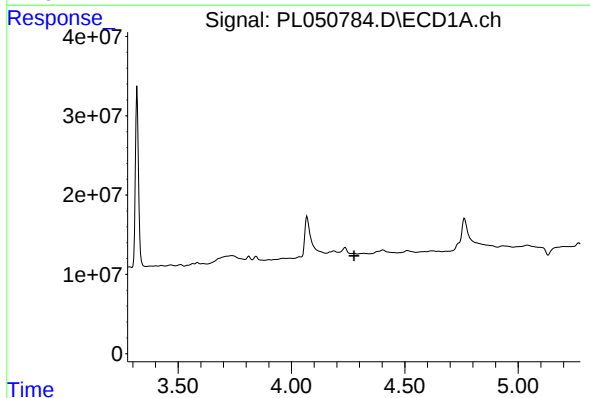


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

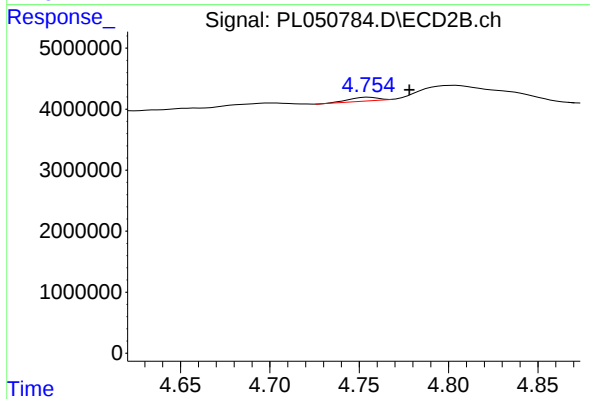

#6 beta-BHC


R.T.: 4.755 min
Delta R.T.: -0.023 min
Response: 659894
Conc: 0.38 ng/ml

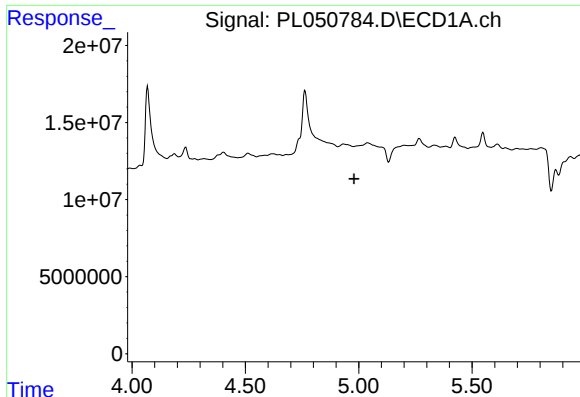

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.979 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-3-B

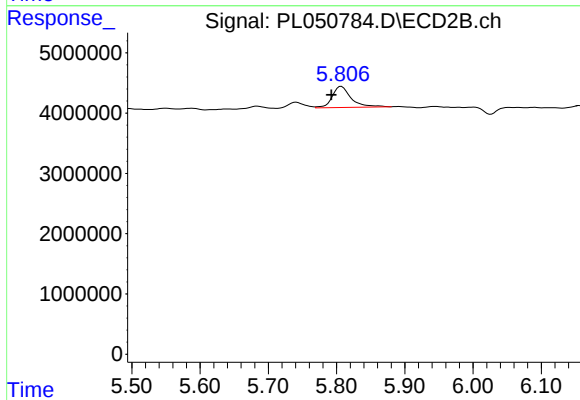


#8 Heptachlor epoxide

R.T.: 5.807 min
Delta R.T.: 0.014 min
Response: 6720788
Conc: 1.76 ng/ml

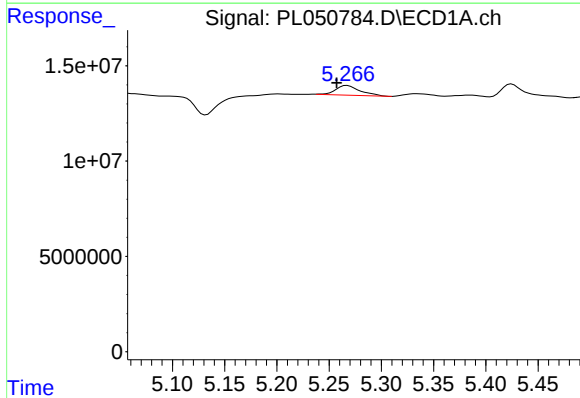


#11 alpha-Chlordane

R.T.: 5.267 min
Delta R.T.: 0.010 min
Response: 8305114
Conc: 0.54 ng/ml

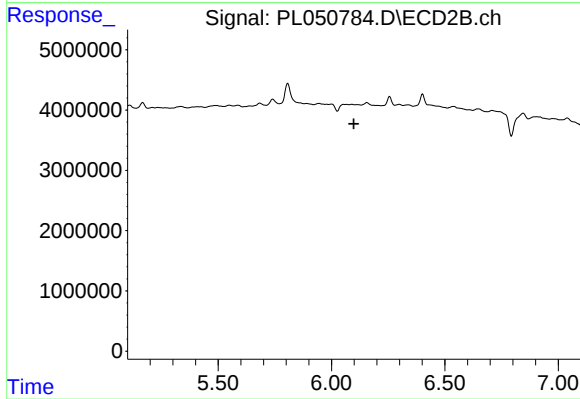

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

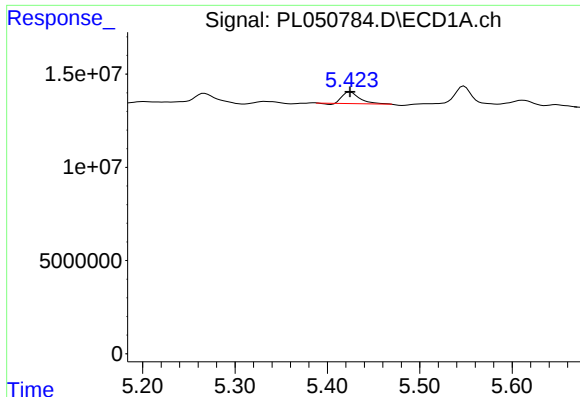

#12 4,4'-DDE


R.T.: 5.425 min
Delta R.T.: 0.000 min
Response: 8011336
Conc: 0.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3-B

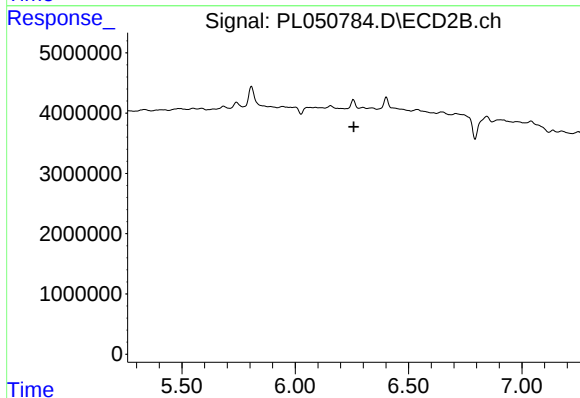


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.258 min
Response: 0
Conc: N.D.

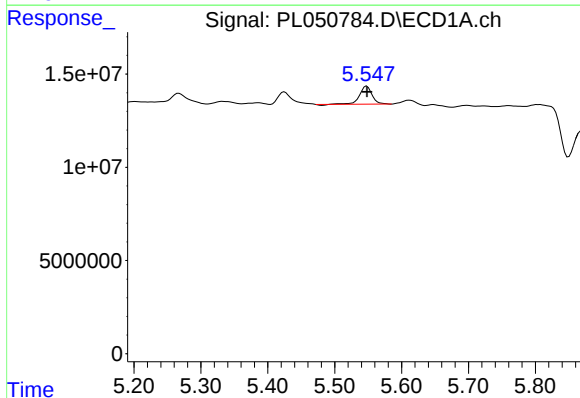


#13 Dieldrin

R.T.: 5.548 min
Delta R.T.: 0.000 min
Response: 12414680
Conc: 0.80 ng/ml

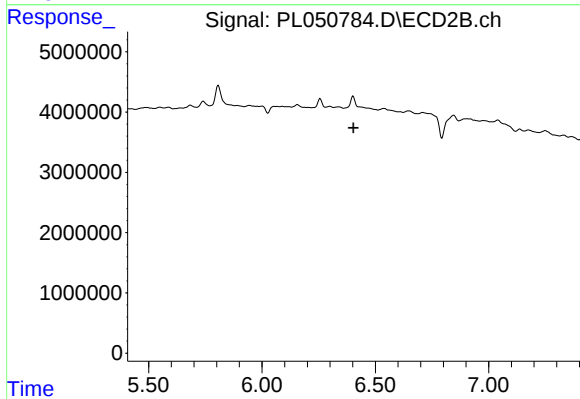

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.404 min
Response: 0
Conc: N.D.

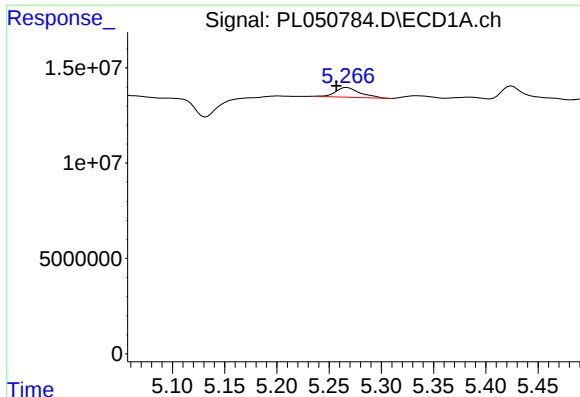

#26 Chlordane-4


R.T.: 5.267 min
Delta R.T.: 0.010 min
Response: 8305114
Conc: 6.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3-B

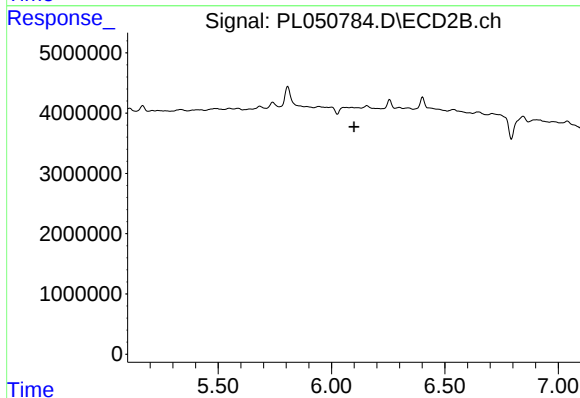


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 6.100 min
Response: 0
Conc: N.D.

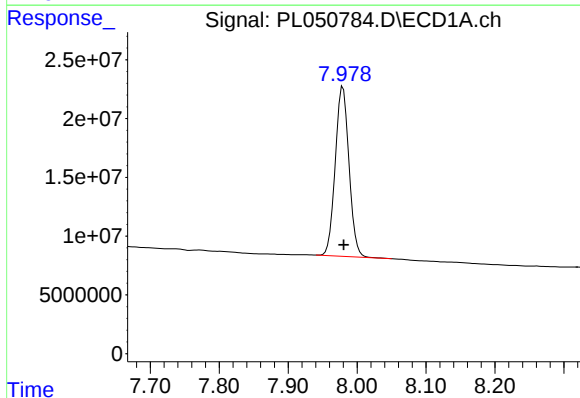

#28 Decachlorobiphenyl

R.T.: 7.980 min
Delta R.T.: -0.001 min
Response: 200186830
Conc: 19.77 ng/ml

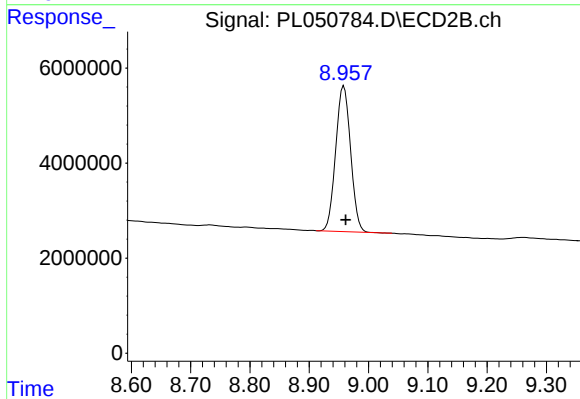

#28 Decachlorobiphenyl

R.T.: 8.958 min
Delta R.T.: -0.003 min
Response: 53506813
Conc: 18.92 ng/ml