

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072519\
 Data File : PL050788.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jul 2019 19:21
 Operator : SM\AJ
 Sample : K3990-08
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-4-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 00:54:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.319	3.929	208.6E6	55787916	20.762	19.553
28)	SA Decachlor...	7.979	8.959	194.1E6	52110973	19.174	18.427
Target Compounds							
6)	B beta-BHC	0.000	4.755f	0	786528	N.D.	0.455 #
7)	B delta-BHC	0.000	4.984	0	5784248	N.D.	1.496 #
8)	B Heptachlo...	0.000	5.806	0	10295386	N.D.	2.692 #
11)	B alpha-Chl...	5.272	0.000	5609688	0	0.368	N.D. #
15)	B Endosulfa...	0.000	6.848f	0	10893405	N.D.	3.426 #
26)	Chlordane-4	5.272f	0.000	5609688	0	4.253	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072519\
Data File : PL050788.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jul 2019 19:21
Operator : SM\AJ
Sample : K3990-08
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-4-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 00:54:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

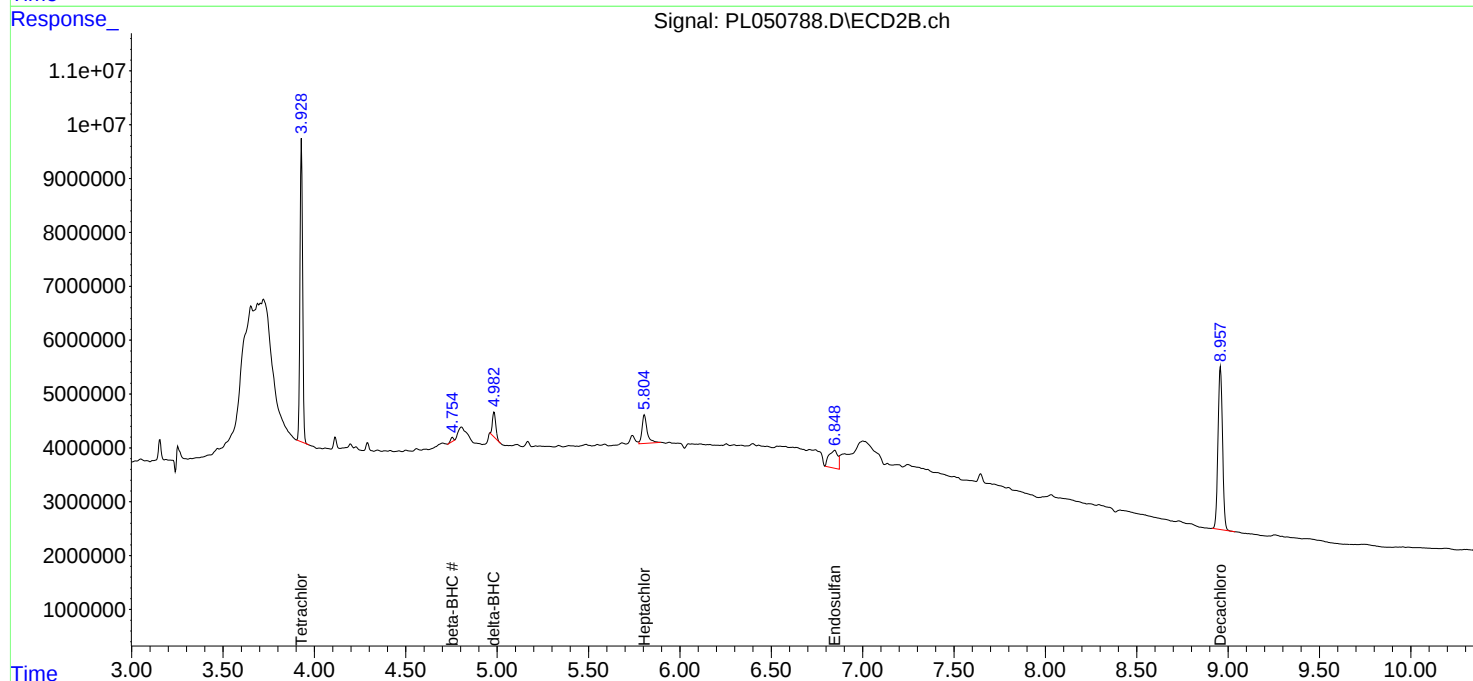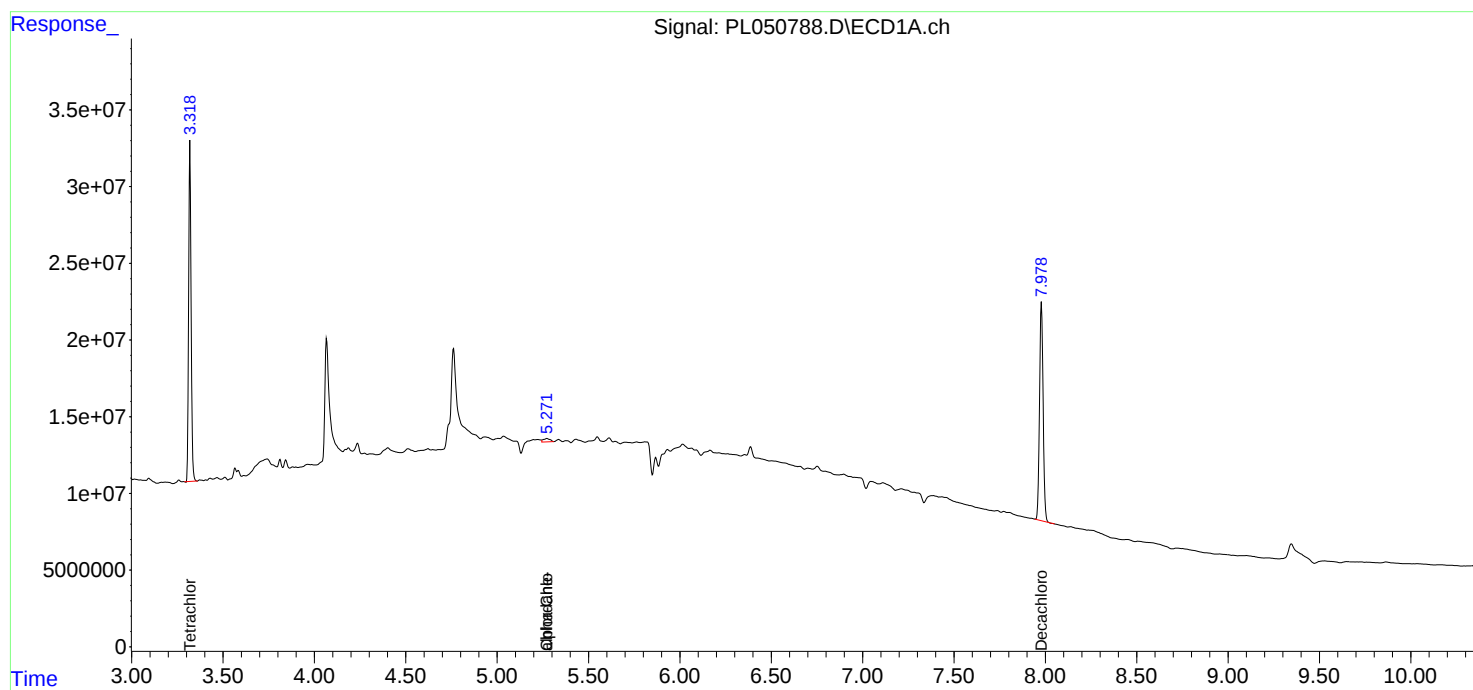


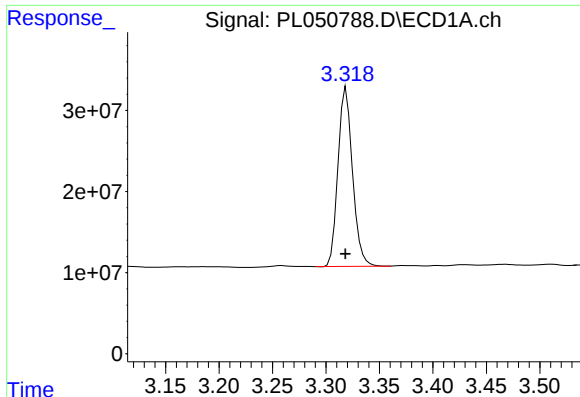

#1 Tetrachloro-m-xylene


R.T.: 3.319 min
Delta R.T.: 0.000 min
Response: 208608889
Conc: 20.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4-B

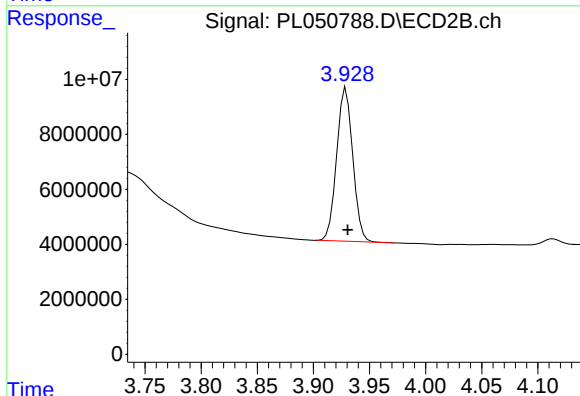


#1 Tetrachloro-m-xylene

R.T.: 3.929 min
Delta R.T.: -0.001 min
Response: 55787916
Conc: 19.55 ng/ml

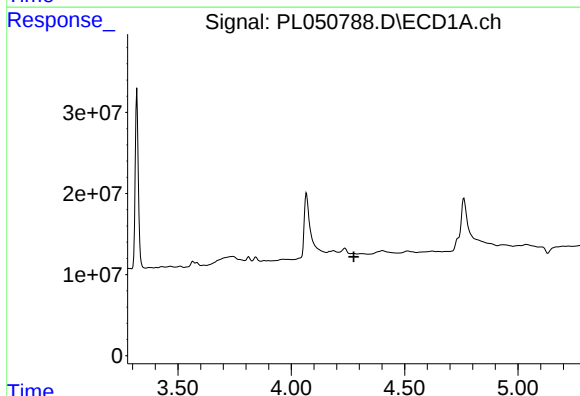


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

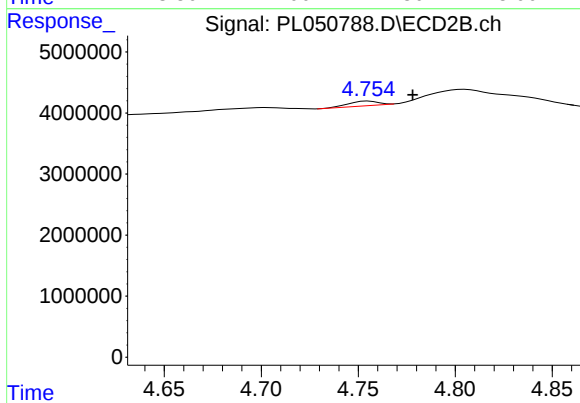

#6 beta-BHC


R.T.: 4.755 min
Delta R.T.: -0.023 min
Response: 786528
Conc: 0.45 ng/ml

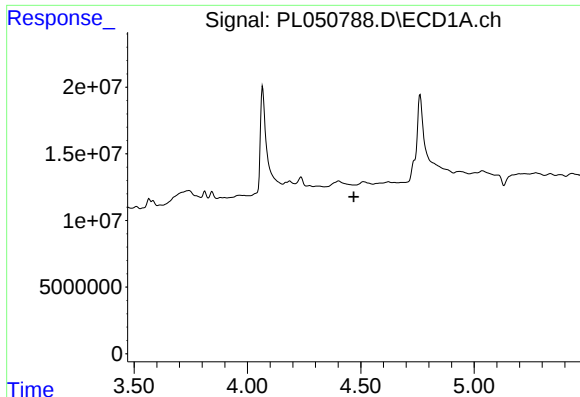

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.469 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-4-B

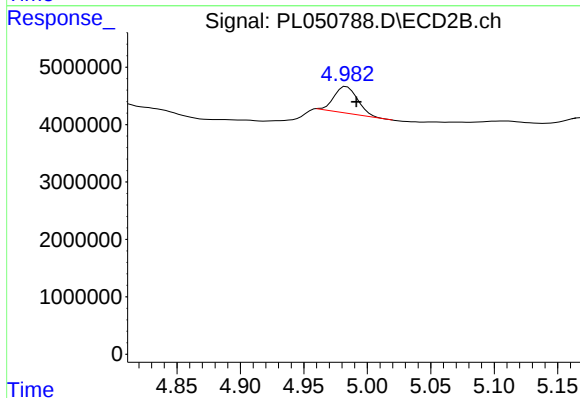


#7 delta-BHC

R.T.: 4.984 min
Delta R.T.: -0.008 min
Response: 5784248
Conc: 1.50 ng/ml

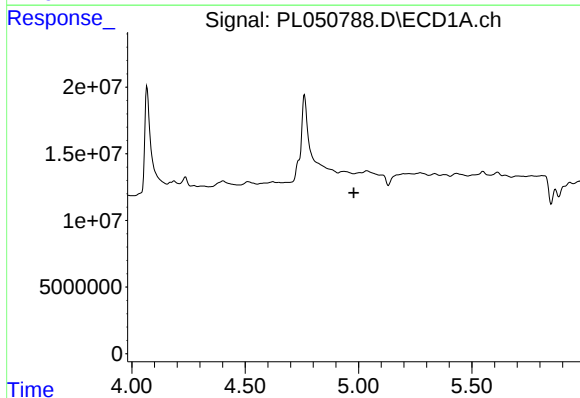


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.979 min
Response: 0
Conc: N.D.

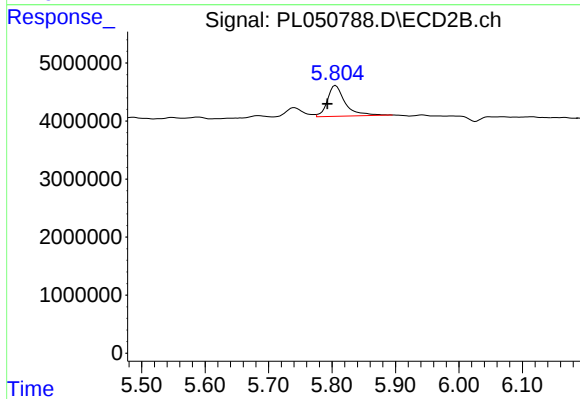

#8 Heptachlor epoxide


R.T.: 5.806 min
Delta R.T.: 0.013 min
Response: 10295386
Conc: 2.69 ng/ml

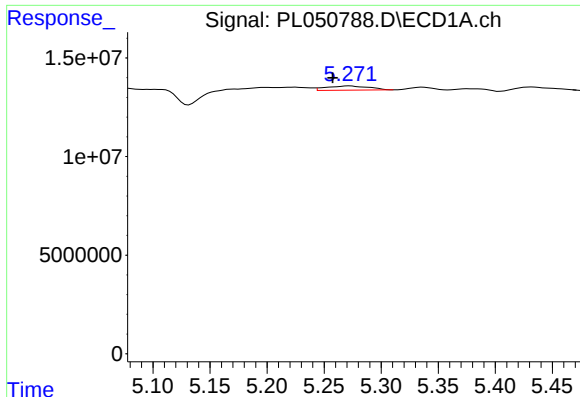

#11 alpha-Chlordane


R.T.: 5.272 min
Delta R.T.: 0.015 min
Response: 5609688
Conc: 0.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4-B

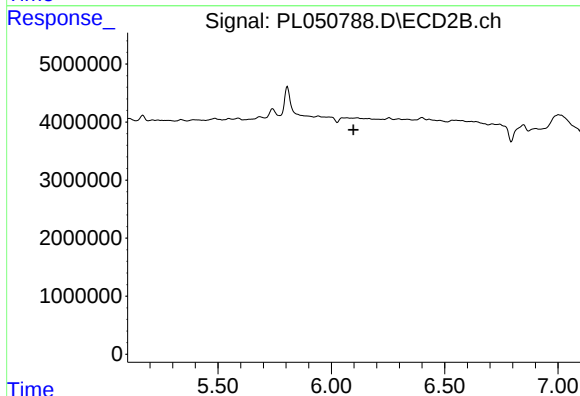


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

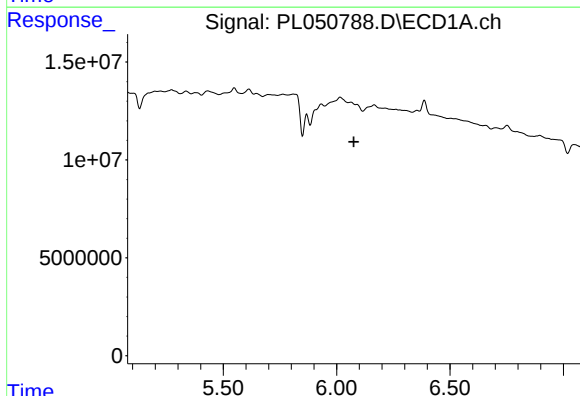


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.076 min
Response: 0
Conc: N.D.

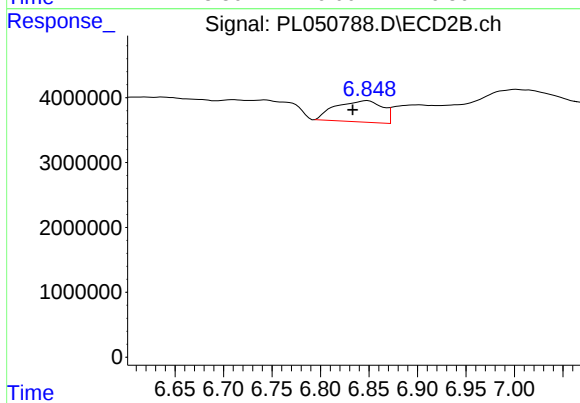

#15 Endosulfan II


R.T.: 6.848 min
Delta R.T.: 0.015 min
Response: 10893405
Conc: 3.43 ng/ml

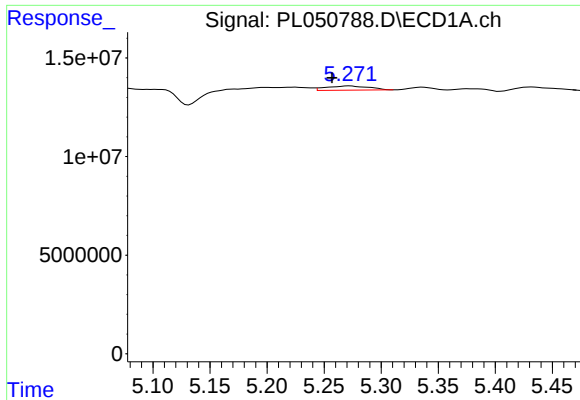

#26 Chlordane-4


R.T.: 5.272 min
Delta R.T.: 0.015 min
Response: 5609688
Conc: 4.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4-B

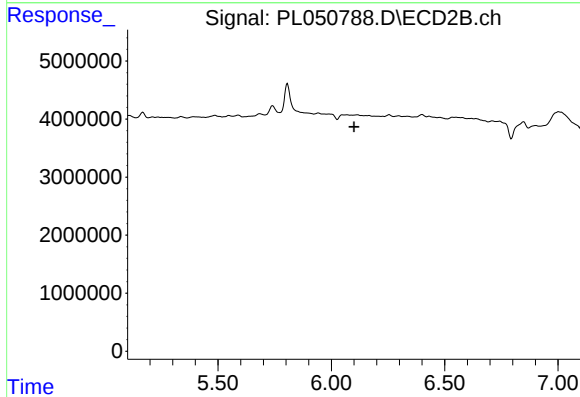


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 6.100 min
Response: 0
Conc: N.D.

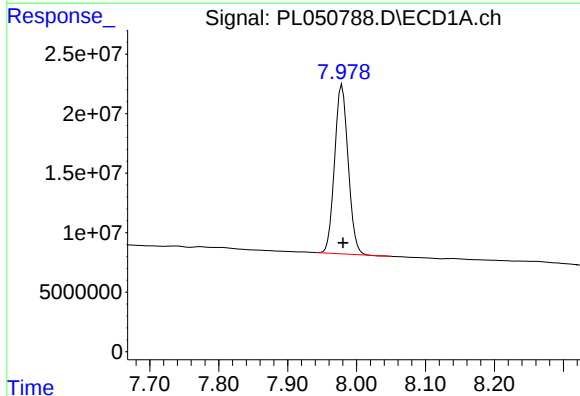

#28 Decachlorobiphenyl

R.T.: 7.979 min
Delta R.T.: -0.002 min
Response: 194140042
Conc: 19.17 ng/ml

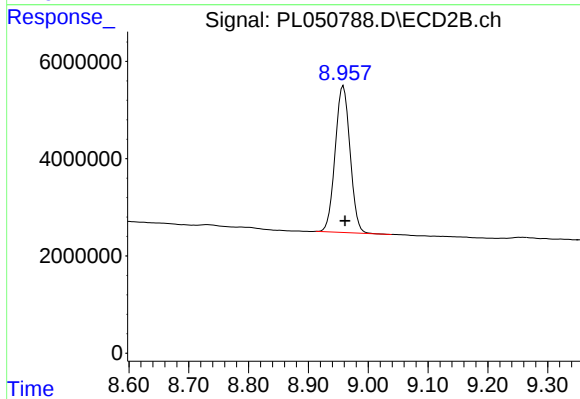

#28 Decachlorobiphenyl

R.T.: 8.959 min
Delta R.T.: -0.003 min
Response: 52110973
Conc: 18.43 ng/ml