

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072519\
 Data File : PL050783.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jul 2019 18:05
 Operator : SM\AJ
 Sample : K3990-05
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-3-A

Manual Integrations
 APPROVED

Ankita
 7/26/2019 1:42:33 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 00:53:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.319	3.929	209.4E6	52641763	20.836	18.450
28)	SA Decachlor...	7.979	8.959	159.3E6	44382470	15.737	15.694
Target Compounds							
13)	MA Dieldrin	5.546	6.400	10708069	1431036	0.691m	0.404m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072519\
Data File : PL050783.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jul 2019 18:05
Operator : SM\AJ
Sample : K3990-05
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-3-A


Manual Integrations
APPROVED

Ankita
7/26/2019 1:42:33 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 00:53:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

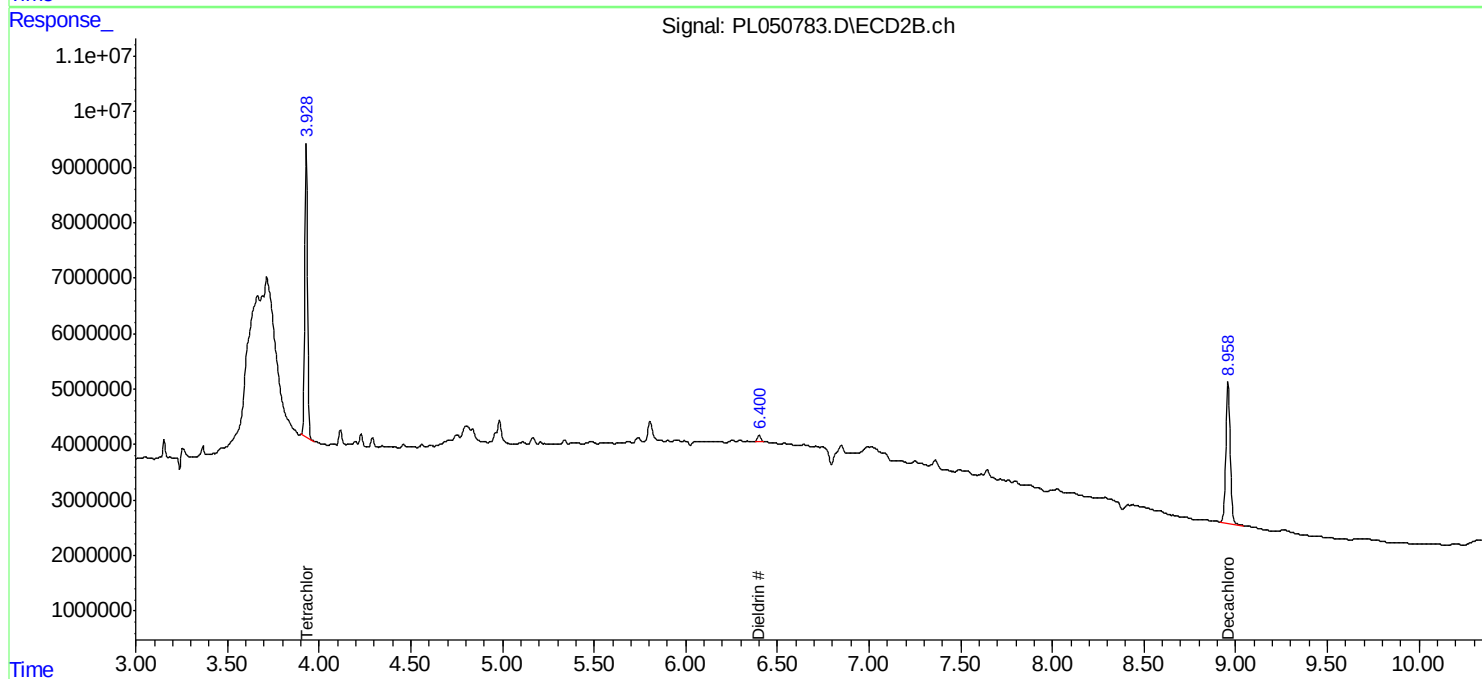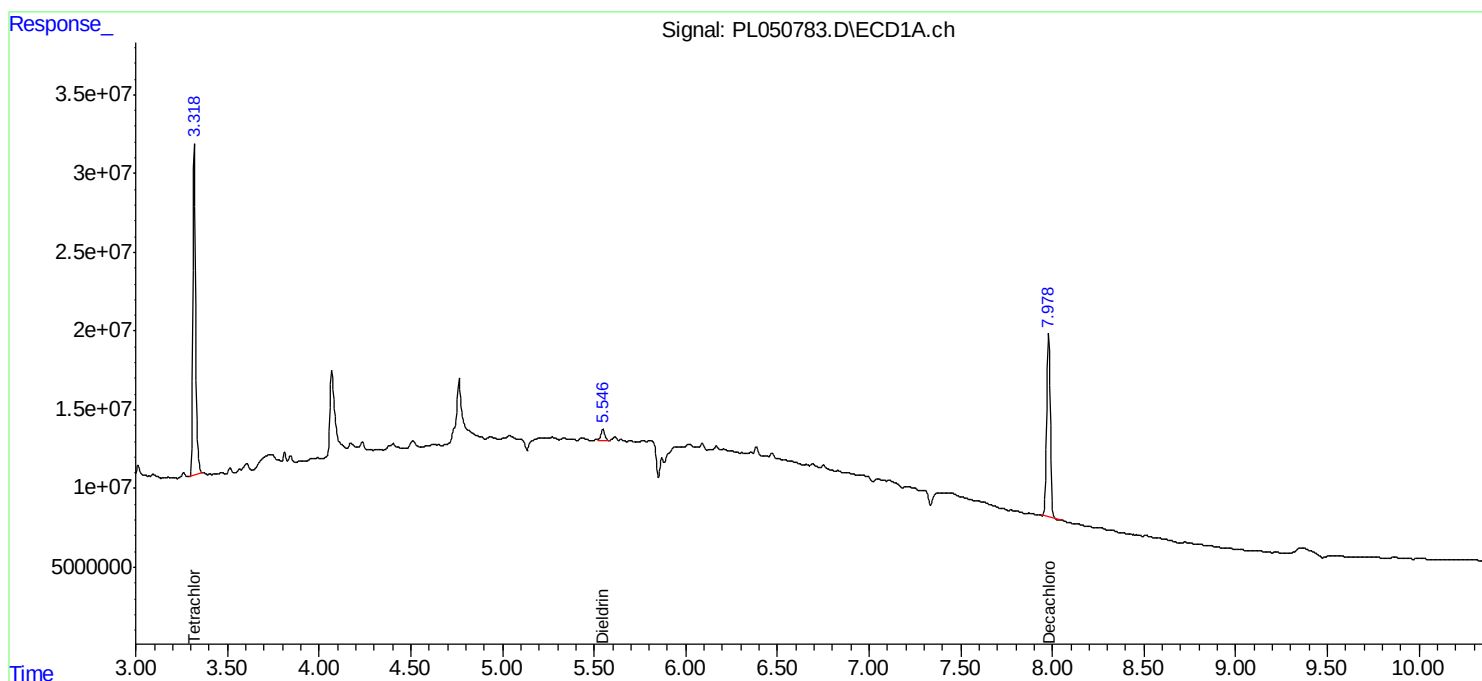

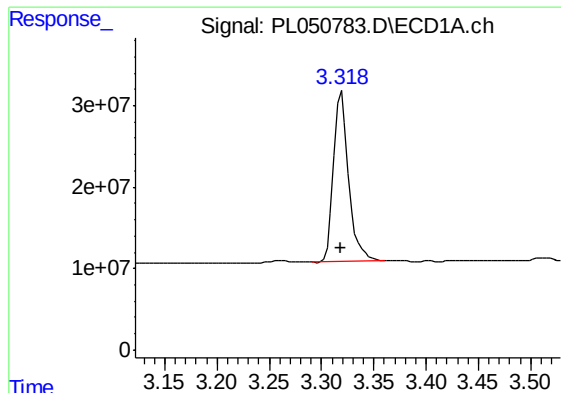


#1 Tetrachloro-m-xylene

R.T.: 3.319 min
Delta R.T.: 0.001 min
Response: 209360497
Conc: 20.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3-A


Manual Integrations
APPROVED

Ankita
7/26/2019 1:42:33 PM

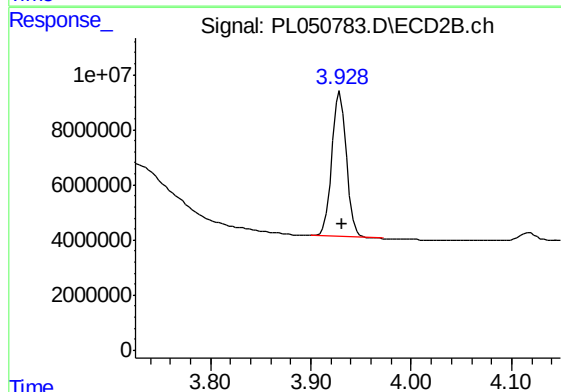


#1 Tetrachloro-m-xylene

R.T.: 3.929 min
Delta R.T.: -0.001 min
Response: 52641763
Conc: 18.45 ng/ml

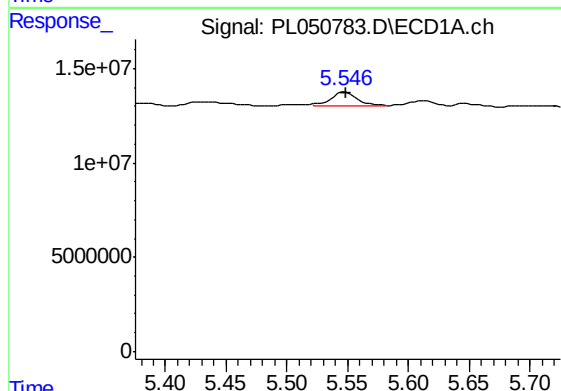


#13 Dieldrin

R.T.: 5.546 min
Delta R.T.: -0.002 min
Response: 10708069
Conc: 0.69 ng/ml m

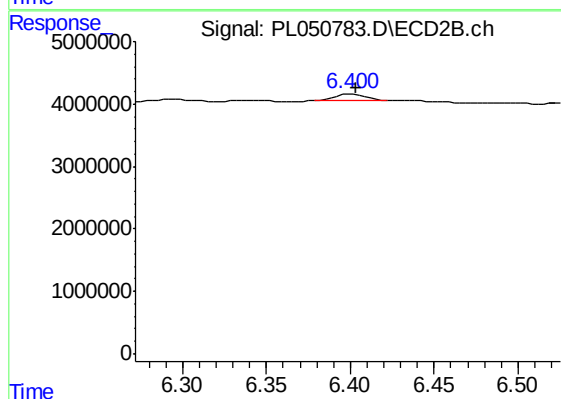

#13 Dieldrin

R.T.: 6.400 min
Delta R.T.: -0.004 min
Response: 1431036
Conc: 0.40 ng/ml m

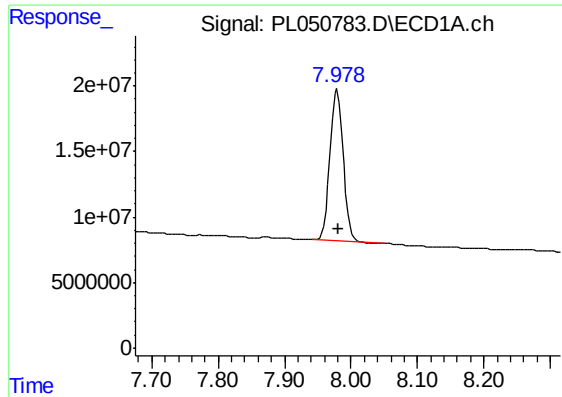


#28 Decachlorobiphenyl

R.T.: 7.979 min
Delta R.T.: -0.001 min
Response: 159341552
Conc: 15.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3-A

Manual Integrations
APPROVED

Ankita
7/26/2019 1:42:33 PM

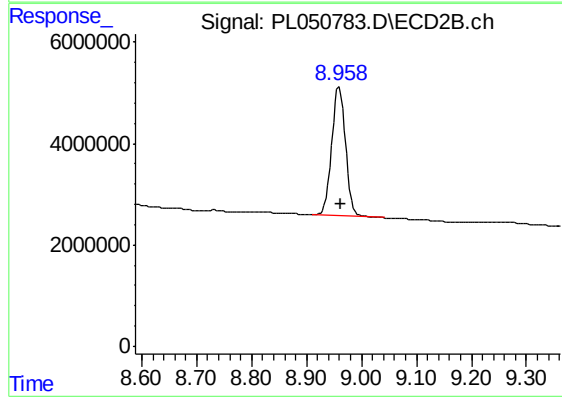

#28 Decachlorobiphenyl

R.T.: 8.959 min
Delta R.T.: -0.002 min
Response: 44382470
Conc: 15.69 ng/ml