

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072522\
 Data File : PL076594.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jul 2022 11:00
 Operator : AR\AJ
 Sample : N3704-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 23:54:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072122CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 25 05:54:24 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	2.643	16544892	38148451	18.259	16.270
27)	SA Decachlor...	8.915	7.755	26541959	63025046	33.896	31.386
Target Compounds							
3)	MA gamma-BHC...	0.000	3.428f	0	428837	N.D.	0.136
4)	MA Heptachlor	4.821	0.000	4348347	0	3.583	N.D. #
6)	B beta-BHC	4.409	0.000	7534809	0	12.672	N.D. #
10)	B trans-Chl...	0.000	4.842	0	992721	N.D.	0.376
11)	B cis-Chlor...	0.000	4.842f	0	992721	N.D.	0.385
15)	B Endosulfa...	0.000	5.701f	0	898191	N.D.	0.437
16)	A 4,4'-DDD	0.000	5.614	0	404292	N.D.	0.213
19)	B Endosulfa...	0.000	6.127f	0	778078	N.D.	0.373
21)	B Endrin ke...	7.541	0.000	275155	0	0.282	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072522\
Data File : PL076594.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jul 2022 11:00
Operator : AR\AJ
Sample : N3704-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 23:54:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072122CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jul 25 05:54:24 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

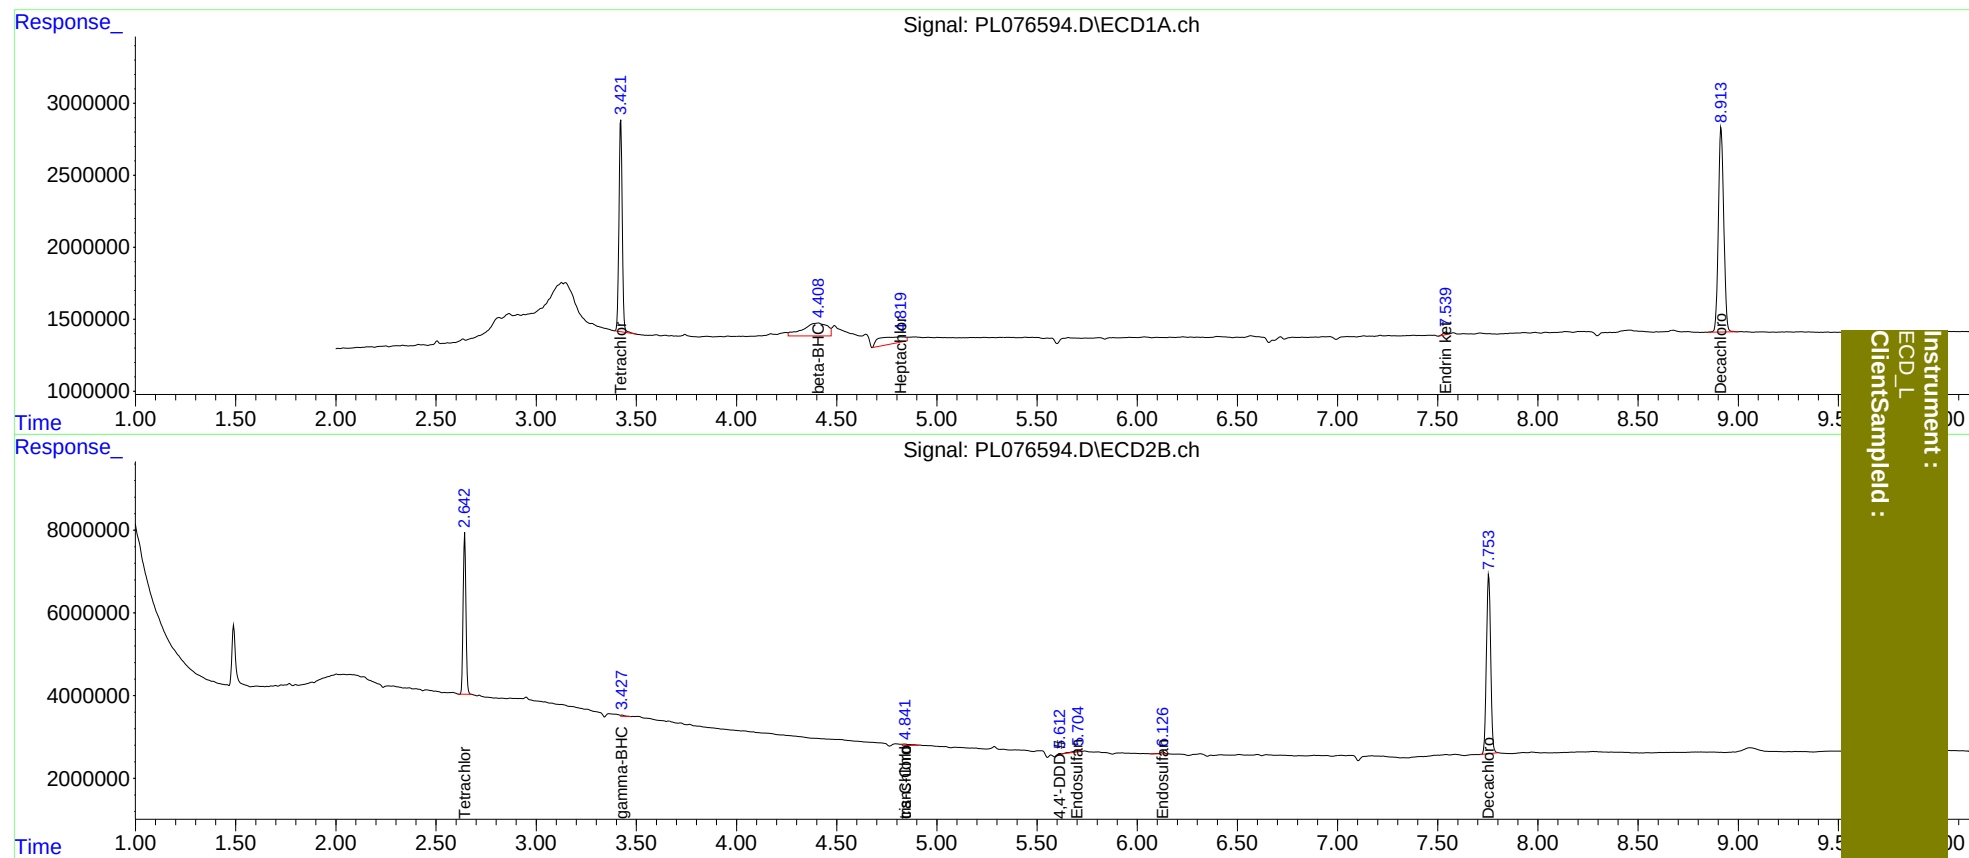


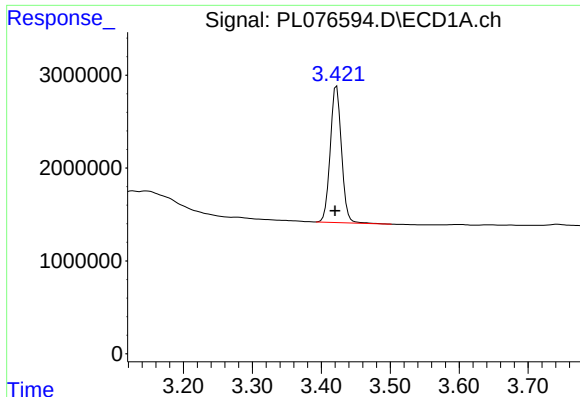

#1 Tetrachloro-m-xylene


R.T.: 3.422 min
Delta R.T.: 0.002 min
Response: 16544892
Conc: 18.26 ng/ml

Instrument :
ECD_L
ClientSampleId :

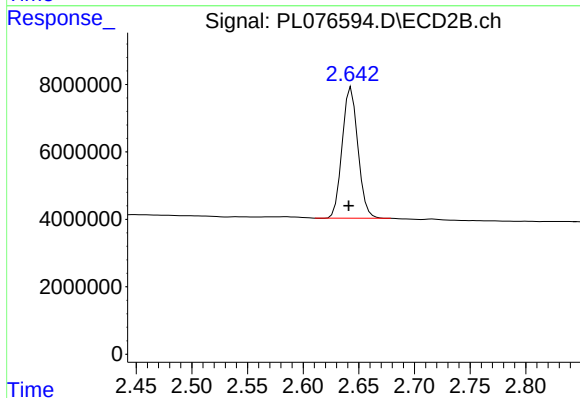


#1 Tetrachloro-m-xylene

R.T.: 2.643 min
Delta R.T.: 0.002 min
Response: 38148451
Conc: 16.27 ng/ml

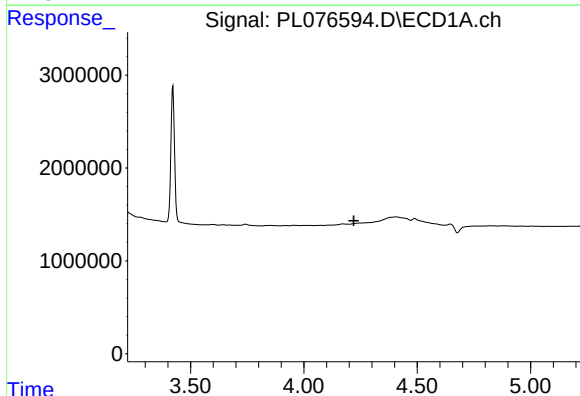


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.220 min
Response: 0
Conc: N.D.

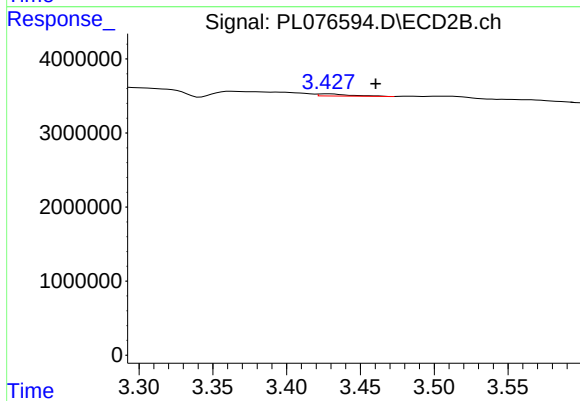

#3 gamma-BHC (Lindane)


R.T.: 3.428 min
Delta R.T.: -0.032 min
Response: 428837
Conc: 0.14 ng/ml

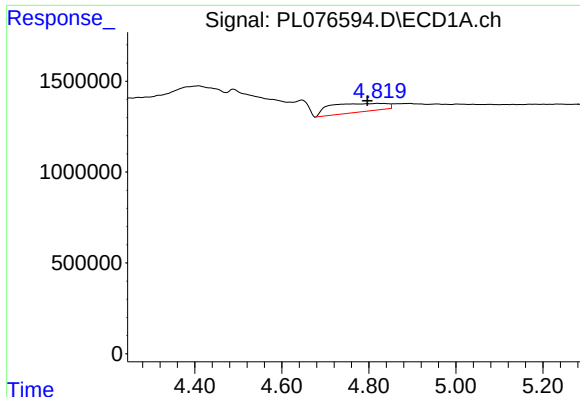

#4 Heptachlor


R.T.: 4.821 min
Delta R.T.: 0.024 min
Response: 4348347
Conc: 3.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

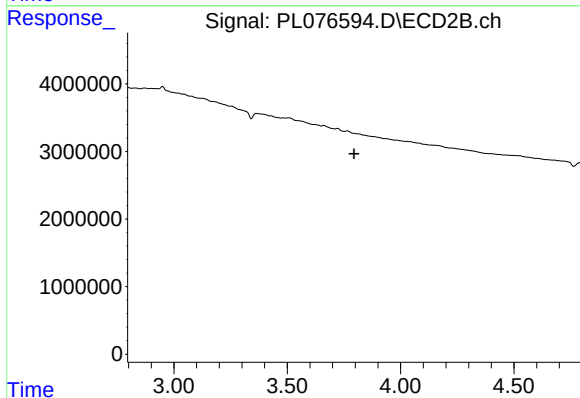


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 3.795 min
Response: 0
Conc: N.D.

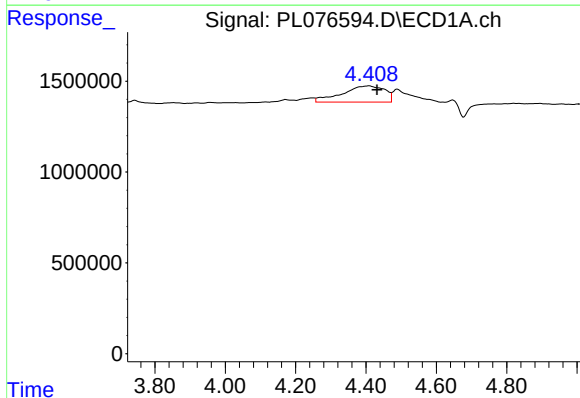


#6 beta-BHC

R.T.: 4.409 min
Delta R.T.: -0.022 min
Response: 7534809
Conc: 12.67 ng/ml

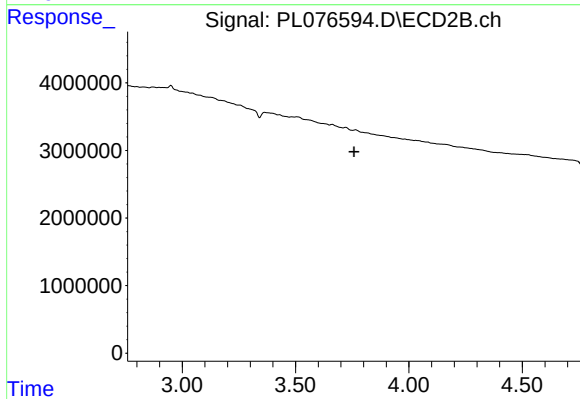

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 3.759 min
Response: 0
Conc: N.D.

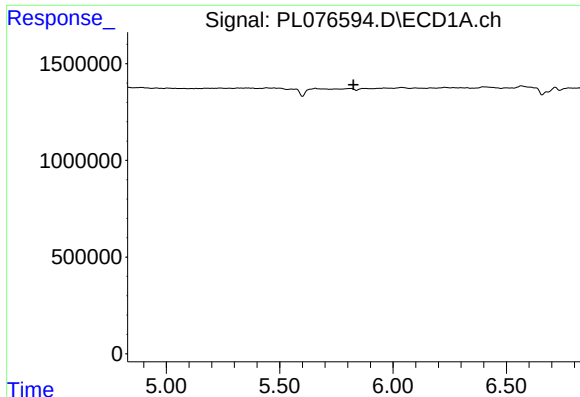

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.826 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

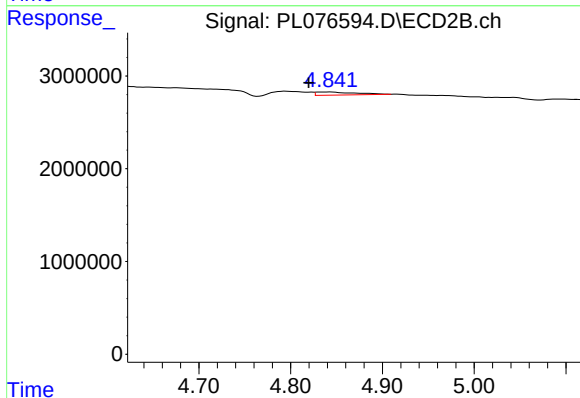


#10 trans-Chlordane

R.T.: 4.842 min
Delta R.T.: 0.022 min
Response: 992721
Conc: 0.38 ng/ml

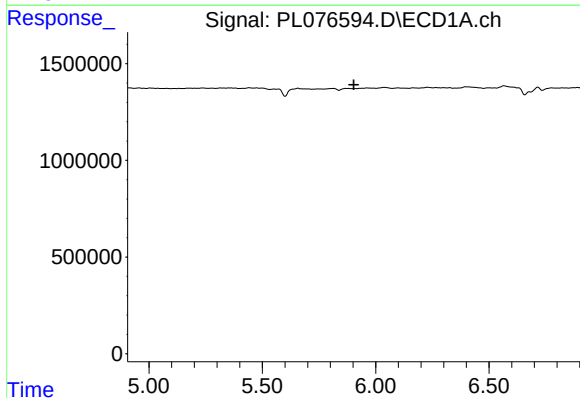


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.903 min
Response: 0
Conc: N.D.

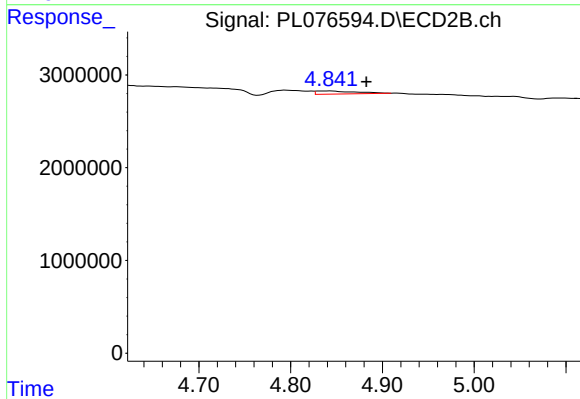

#11 cis-Chlordane


R.T.: 4.842 min
Delta R.T.: -0.041 min
Response: 992721
Conc: 0.38 ng/ml

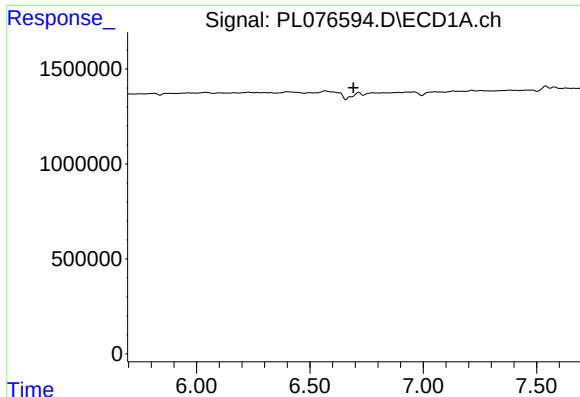

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.692 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

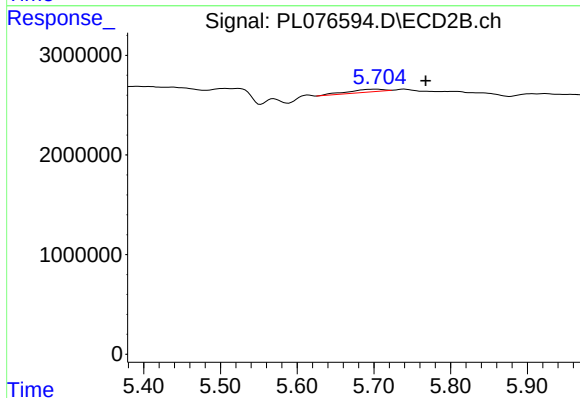


#15 Endosulfan II

R.T.: 5.701 min
Delta R.T.: -0.067 min
Response: 898191
Conc: 0.44 ng/ml

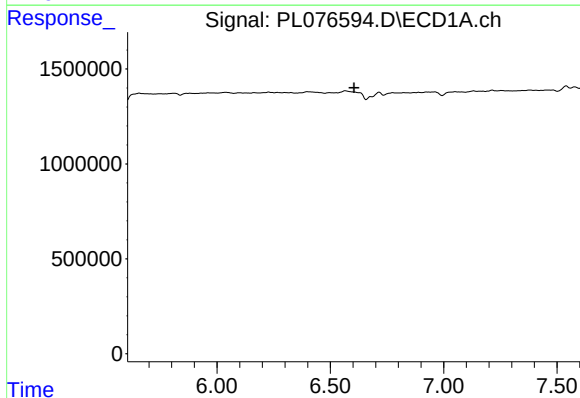


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.606 min
Response: 0
Conc: N.D.

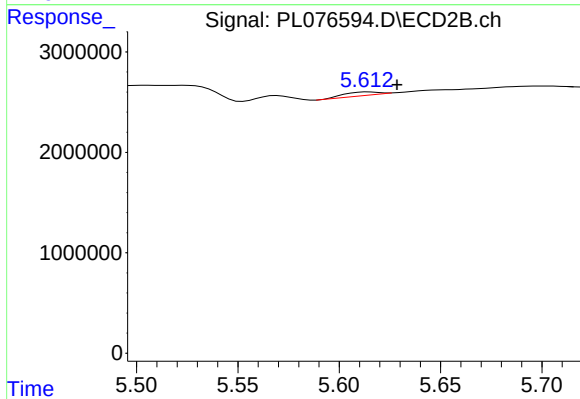

#16 4,4'-DDD


R.T.: 5.614 min
Delta R.T.: -0.014 min
Response: 404292
Conc: 0.21 ng/ml

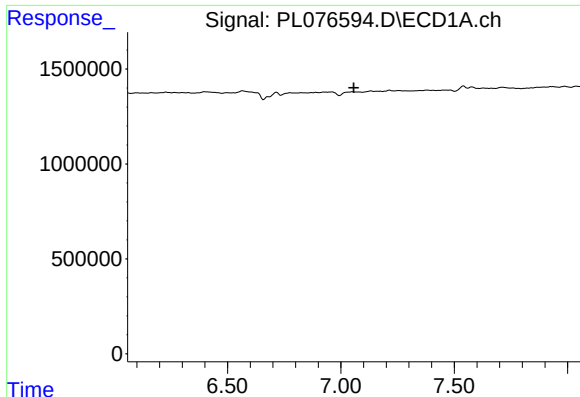

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.057 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

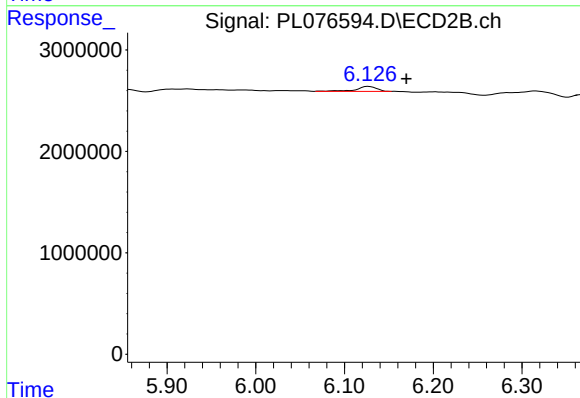


#19 Endosulfan Sulfate

R.T.: 6.127 min
Delta R.T.: -0.043 min
Response: 778078
Conc: 0.37 ng/ml

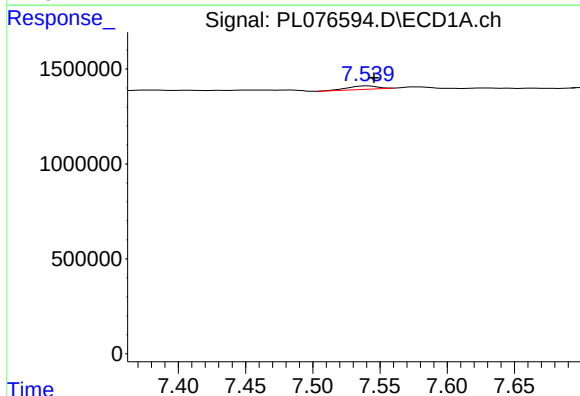


#21 Endrin ketone

R.T.: 7.541 min
Delta R.T.: -0.005 min
Response: 275155
Conc: 0.28 ng/ml

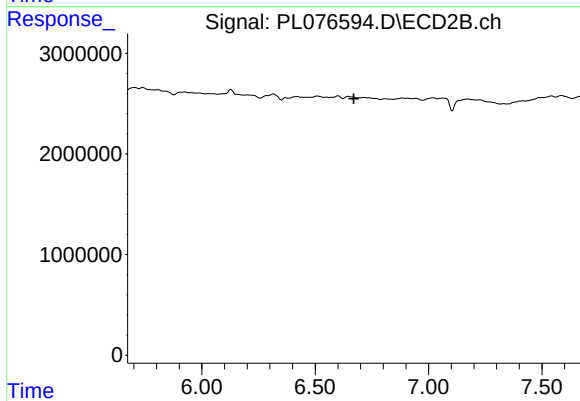

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 6.670 min
Response: 0
Conc: N.D.

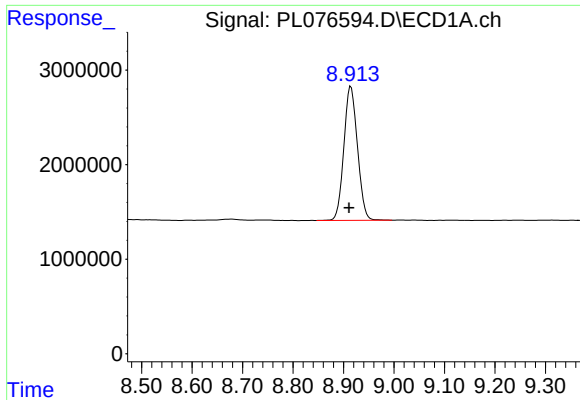

#27 Decachlorobiphenyl

R.T.: 8.915 min
Delta R.T.: 0.004 min
Response: 26541959
Conc: 33.90 ng/ml

Instrument :
ECD_L
ClientSampleId :

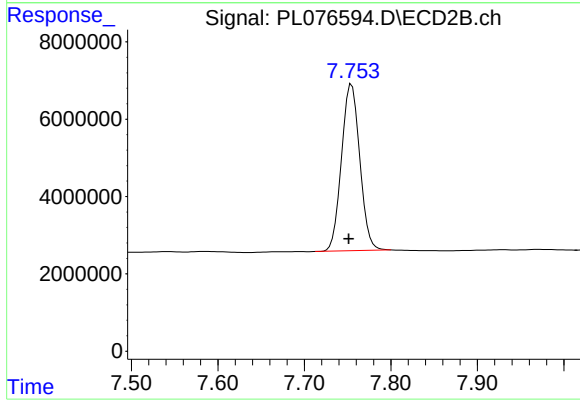

#27 Decachlorobiphenyl

R.T.: 7.755 min
Delta R.T.: 0.003 min
Response: 63025046
Conc: 31.39 ng/ml