

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072522\
 Data File : PL076595.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jul 2022 11:14
 Operator : AR\AJ
 Sample : N3704-04MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 C0AP9MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/26/2022
 Supervised By : Ankita Jodhani 07/26/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 23:54:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072122CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 25 05:54:24 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	2.644	15063463	35024738	16.624	14.938
27)	SA Decachlor...	8.916	7.754	25240024	59791108	32.234	29.775
Target Compounds							
2)	A alpha-BHC	3.887	3.138	68753800	162.8E6	56.008	48.692
3)	MA gamma-BHC...	4.223	3.463	66677645	151.3E6	55.514	48.030
4)	MA Heptachlor	4.800	3.797	63264810	139.8E6	52.123	46.923
5)	MB Aldrin	5.139	4.072	59067312	135.5E6	52.849m	47.077
6)	B beta-BHC	4.432	3.761	28519162	62432262	47.965m	43.439
7)	B delta-BHC	4.679	3.986	54864251	151.2E6	49.264	47.692
8)	B Heptachlo...	5.573	4.572	54455977	120.6E6	50.829	46.180
9)	A Endosulfan I	5.959	4.938	46794168	110.5E6	49.254	47.728
10)	B trans-Chl...	5.827	4.821	52853935	121.3E6	49.722m	45.978
11)	B cis-Chlor...	5.905	4.884	53863719	118.1E6	51.108m	45.805
12)	B 4,4'-DDE	6.084	5.078	100.7E6	227.6E6	104.991	93.859
13)	MA Dieldrin	6.237	5.202	109.4E6	243.2E6	108.863	97.918
14)	MA Endrin	6.469	5.475	91637515	210.0E6	112.354	104.422
15)	B Endosulfa...	6.694	5.770	88076756	199.0E6	100.450m	96.869
16)	A 4,4'-DDD	6.609	5.631	83779774	181.9E6	108.766	95.735
17)	MA 4,4'-DDT	6.919	5.881	88346375	190.1E6	108.461	99.207
18)	B Endrin al...	6.827	5.950	71390189	154.8E6	92.530	87.431
19)	B Endosulfa...	7.060	6.173	86204446	188.5E6	97.032	90.377
20)	A Methoxychlor	7.401	6.459	228.1E6	478.1E6	509.507	476.034
21)	B Endrin ke...	7.548	6.673	101.5E6	224.0E6	103.867	98.394

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072522\
Data File : PL076595.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jul 2022 11:14
Operator : AR\AJ
Sample : N3704-04MS
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 23:54:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072122CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jul 25 05:54:24 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

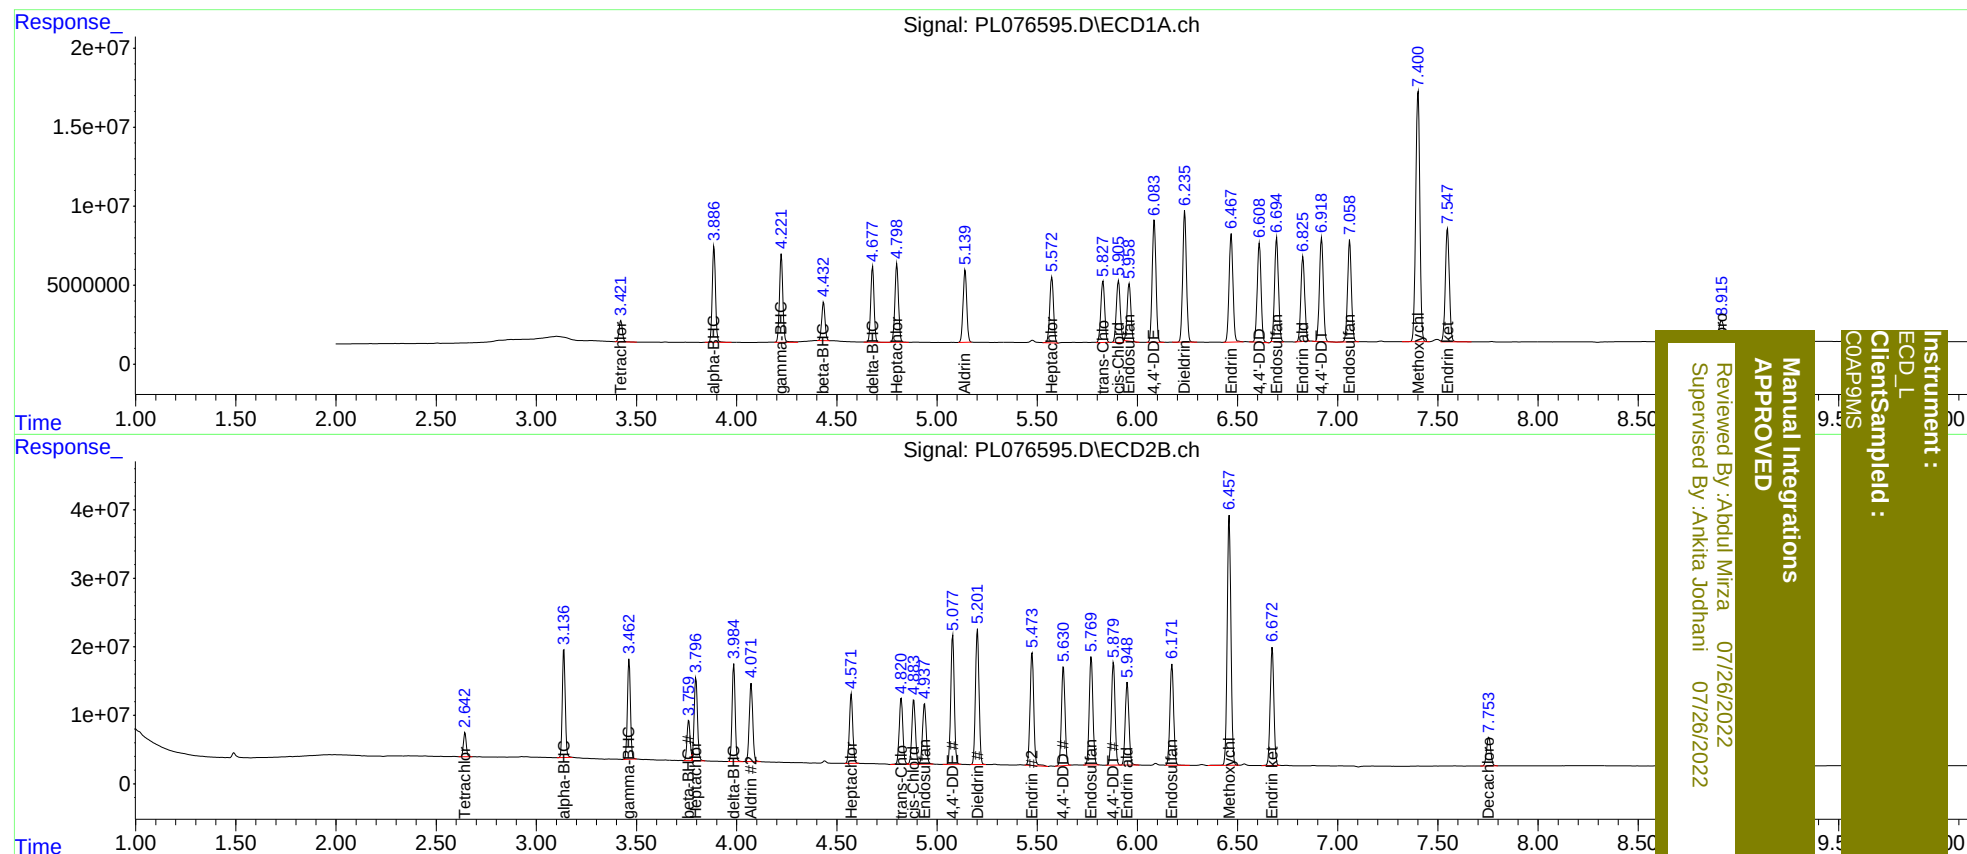

516.84
Reviewed By: Abul Mirza 07/26/2022
Supervised By: Ankita Jodhani 07/26/2022

Manual Integrations
APPROVED

Instrument :
ECD_L
Client/Sampled :
COAP9MS