

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072522\
 Data File : PL076596.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jul 2022 11:28
 Operator : AR\AJ
 Sample : N3704-05MSD
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 C0AP9MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/26/2022
 Supervised By : Ankita Jodhani 07/26/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 23:54:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072122CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 25 05:54:24 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	2.644	15408818	36185578	17.005	15.433
27)	SA Decachlor...	8.916	7.754	25573623	61707226	32.660	30.729
Target Compounds							
2)	A alpha-BHC	3.887	3.138	67077642	160.3E6	54.643	47.948
3)	MA gamma-BHC...	4.223	3.463	65849523	148.9E6	54.825	47.261
4)	MA Heptachlor	4.799	3.797	61895459	137.2E6	50.995	46.062
5)	MB Aldrin	5.138	4.072	58207240	133.3E6	52.080m	46.324
6)	B beta-BHC	4.432	3.760	27868786	61599241	46.871m	42.859
7)	B delta-BHC	4.678	3.986	52170287	148.3E6	46.845	46.748
8)	B Heptachlo...	5.572	4.572	53296778	118.6E6	49.747	45.419
9)	A Endosulfan I	5.959	4.938	45576728	108.8E6	47.972	46.979
10)	B trans-Chl...	5.826	4.821	52176746	119.2E6	49.085m	45.190
11)	B cis-Chlor...	5.903	4.884	51838712	116.2E6	49.187m	45.054
12)	B 4,4'-DDE	6.084	5.078	98399300	224.8E6	102.592	92.686
13)	MA Dieldrin	6.237	5.202	106.7E6	237.9E6	106.190	95.806
14)	MA Endrin	6.468	5.474	87893136	207.0E6	107.763	102.957
15)	B Endosulfa...	6.694	5.770	86986292	194.8E6	99.206m	94.826
16)	A 4,4'-DDD	6.609	5.631	81862997	179.8E6	106.277	94.680
17)	MA 4,4'-DDT	6.919	5.880	86302206	187.3E6	105.952	97.740
18)	B Endrin al...	6.827	5.949	69629165	151.5E6	90.247	85.572
19)	B Endosulfa...	7.060	6.172	84982017	184.0E6	95.656	88.237
20)	A Methoxychlor	7.401	6.458	224.7E6	466.9E6	501.843	464.879
21)	B Endrin ke...	7.548	6.673	99123058	218.9E6	101.475	96.164

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072522\
Data File : PL076596.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jul 2022 11:28
Operator : AR\AJ
Sample : N3704-05MSD
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 23:54:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072122CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jul 25 05:54:24 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

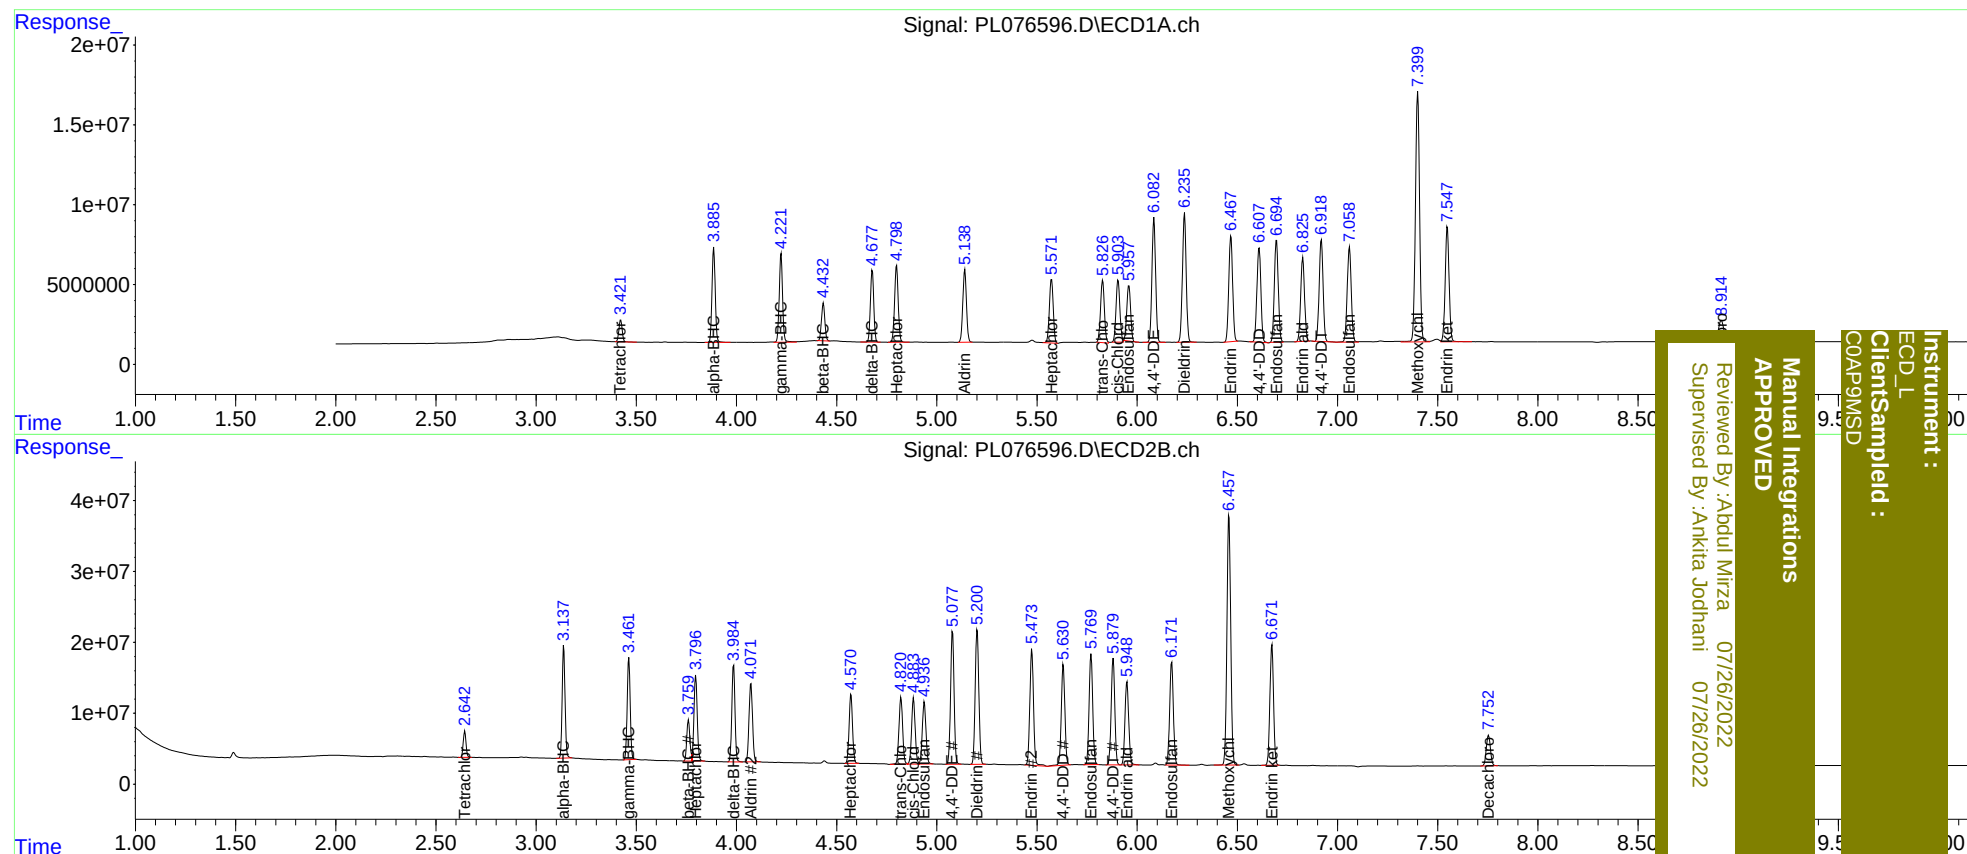

Instrument :
ECD_L
ClientSampled :
COAP9MSD

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/26/2022
Supervised By :Ankita Jodhani 07/26/2022