

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072523\
 Data File : PL084173.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jul 2023 09:49
 Operator : AR\AJ
 Sample : 03706-05
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 B-P20A

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/26/2023
 Supervised By : Ankita Jodhani 07/26/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 21:25:35 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 00:03:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	2.689	11340668	5233646	5.671m	4.713
28)	SA Decachlor...	9.038	7.875	7473398	6030464	5.741m	5.427

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072523\
Data File : PL084173.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jul 2023 09:49
Operator : AR\AJ
Sample : 03706-05
Misc :
ALS Vial : 5 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
B-P20A


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/26/2023
Supervised By : Ankita Jodhani 07/26/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 21:25:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 00:03:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

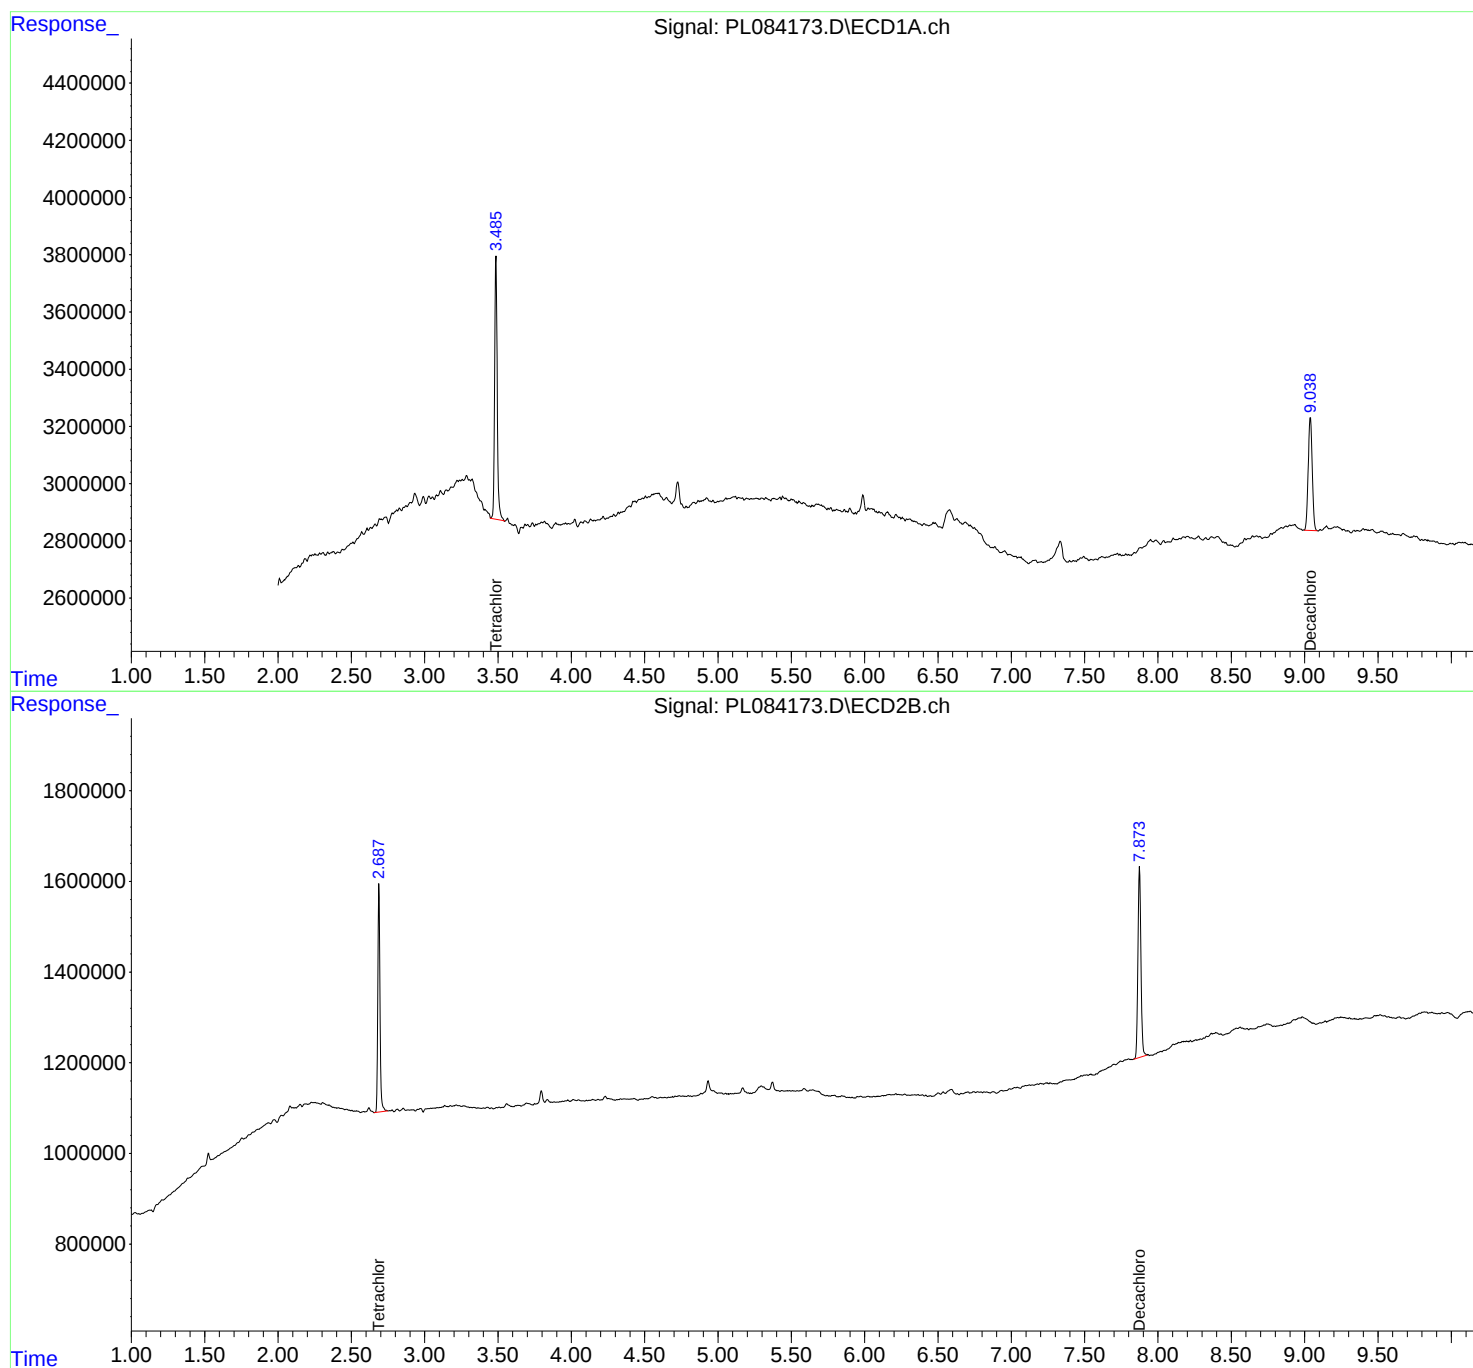

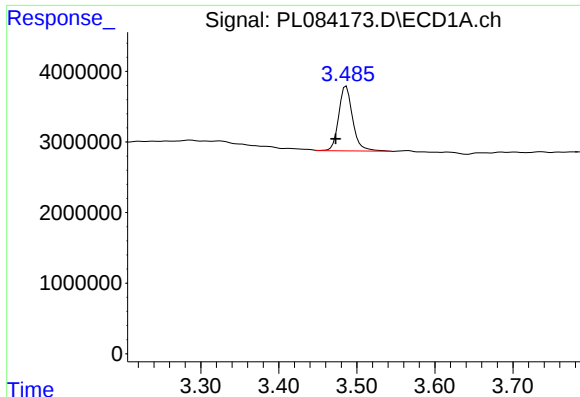


#1 Tetrachloro-m-xylene

R.T.: 3.485 min
Delta R.T.: 0.012 min
Response: 11340668
Conc: 5.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
B-P20A


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/26/2023
Supervised By :Ankita Jodhani 07/26/2023

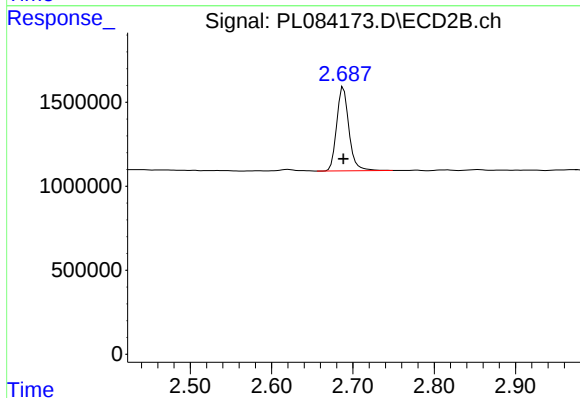


#1 Tetrachloro-m-xylene

R.T.: 2.689 min
Delta R.T.: 0.000 min
Response: 5233646
Conc: 4.71 ng/ml

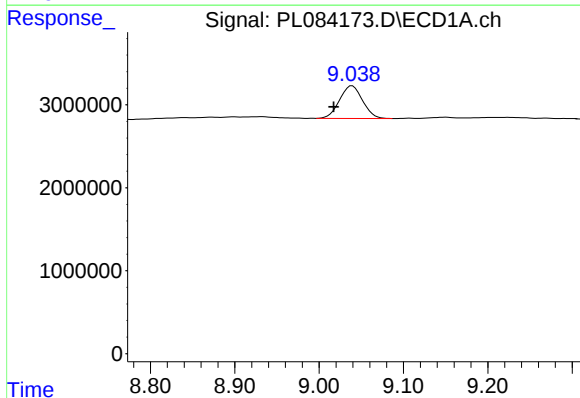

#28 Decachlorobiphenyl

R.T.: 9.038 min
Delta R.T.: 0.020 min
Response: 7473398
Conc: 5.74 ng/ml m

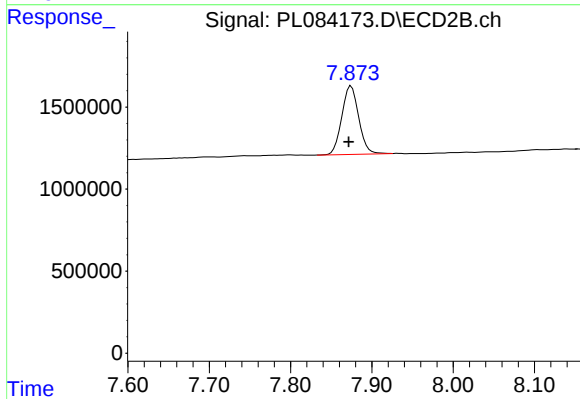

#28 Decachlorobiphenyl

R.T.: 7.875 min
Delta R.T.: 0.003 min
Response: 6030464
Conc: 5.43 ng/ml