

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072523\
 Data File : PL084204.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jul 2023 21:55
 Operator : AR\AJ
 Sample : 03741-12
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 B-P6A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 05:02:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 00:03:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	2.688	18379920	8898974	9.190	8.013
28)	SA Decachlor...	9.022	7.869	15880158	12651193	12.200	11.386
Target Compounds							
12)	B 4,4'-DDE	6.147	5.166	1363941	649555	0.678	0.529



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072523\
Data File : PL084204.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jul 2023 21:55
Operator : AR\AJ
Sample : 03741-12
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
B-P6A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 05:02:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 00:03:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

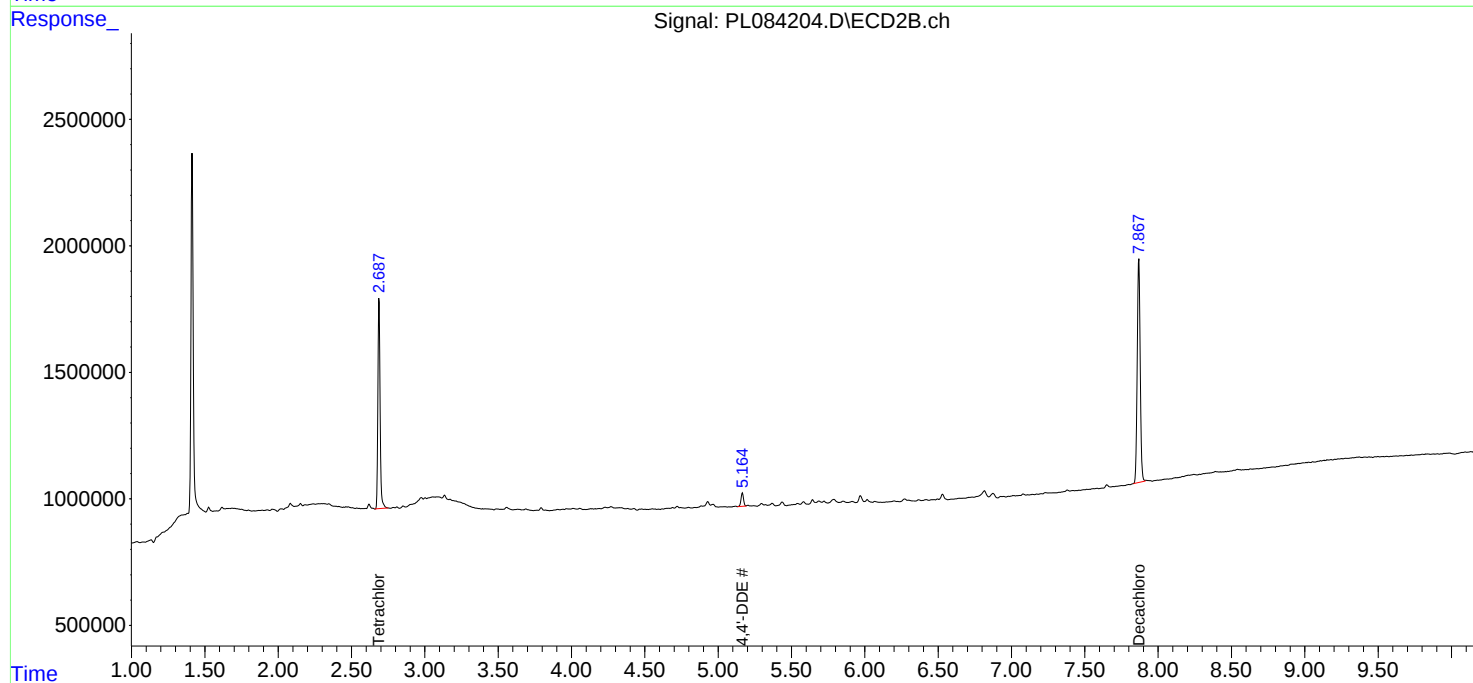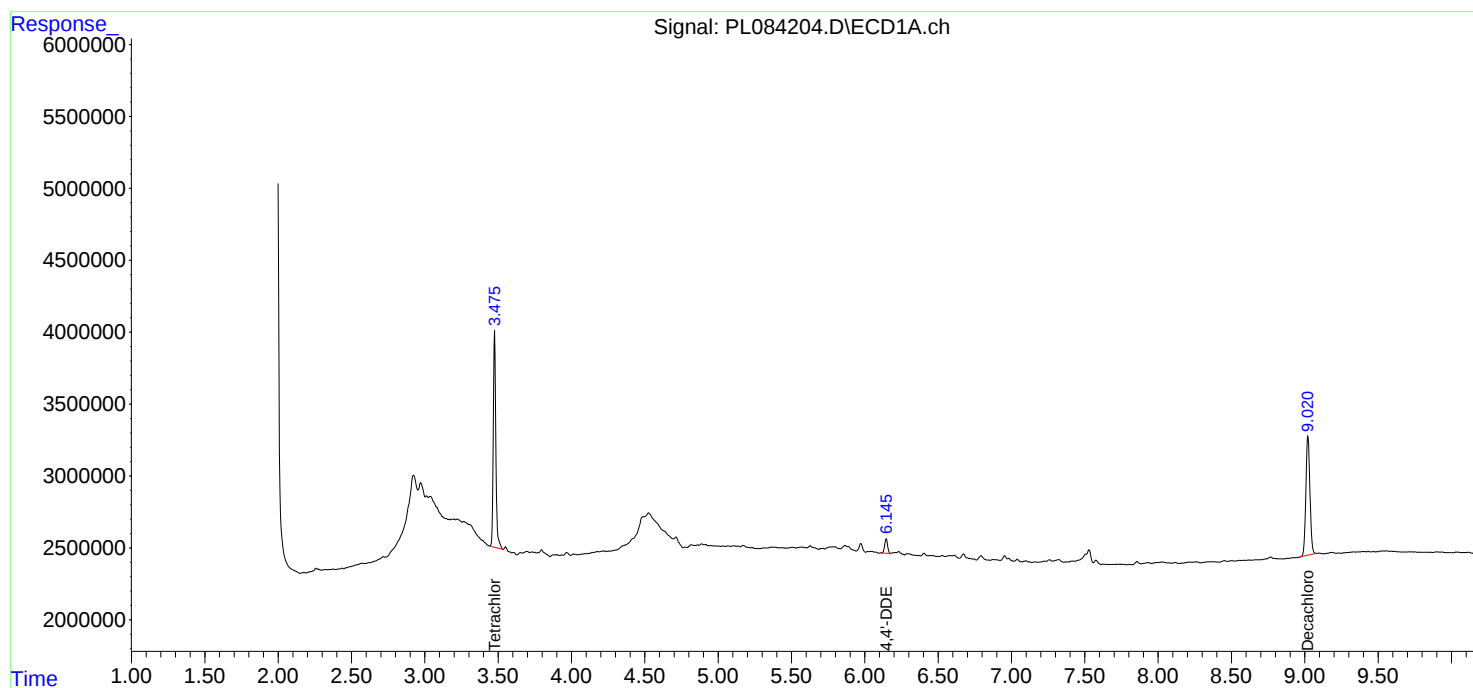


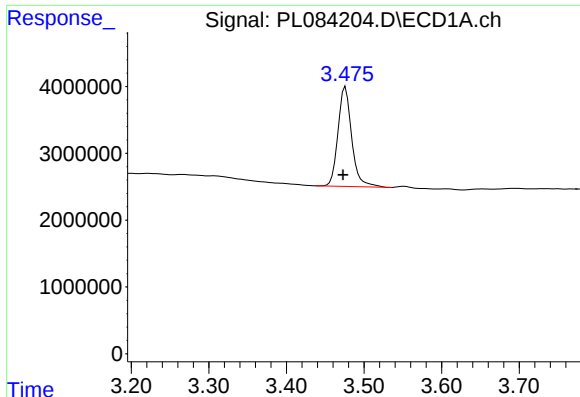

#1 Tetrachloro-m-xylene


R.T.: 3.476 min
Delta R.T.: 0.003 min
Response: 18379920
Conc: 9.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
B-P6A

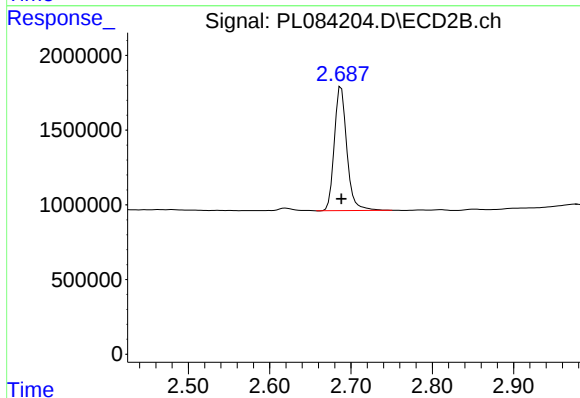


#1 Tetrachloro-m-xylene

R.T.: 2.688 min
Delta R.T.: 0.000 min
Response: 8898974
Conc: 8.01 ng/ml

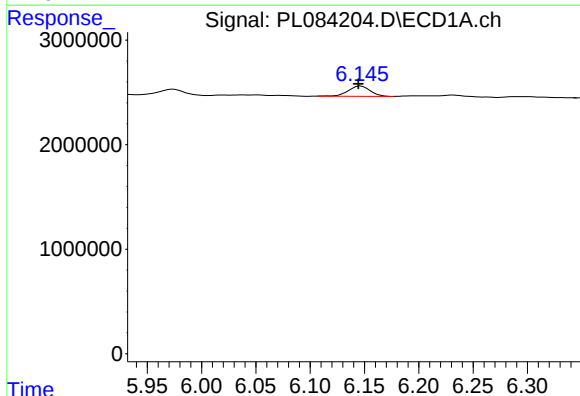


#12 4,4'-DDE

R.T.: 6.147 min
Delta R.T.: 0.002 min
Response: 1363941
Conc: 0.68 ng/ml

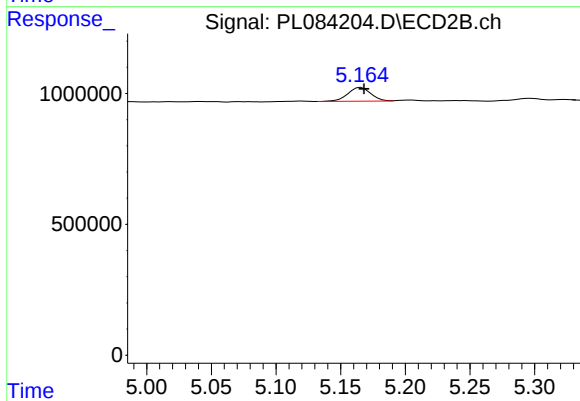

#12 4,4'-DDE


R.T.: 5.166 min
Delta R.T.: -0.002 min
Response: 649555
Conc: 0.53 ng/ml

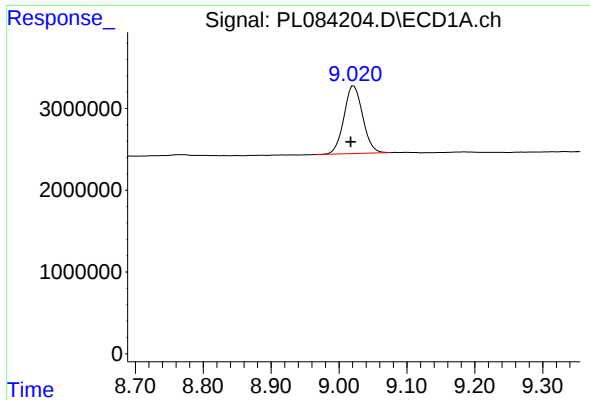

#28 Decachlorobiphenyl

R.T.: 9.022 min
Delta R.T.: 0.004 min
Response: 15880158
Conc: 12.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
B-P6A

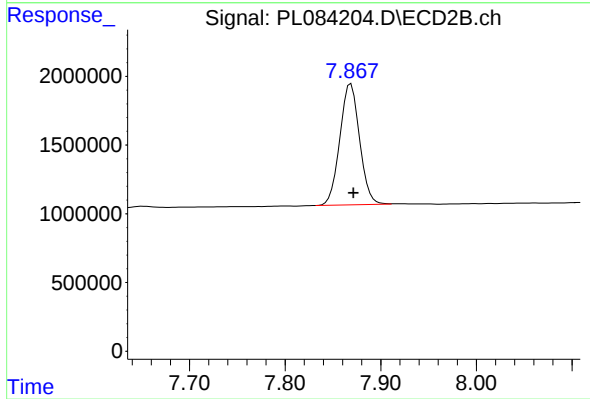

#28 Decachlorobiphenyl

R.T.: 7.869 min
Delta R.T.: -0.003 min
Response: 12651193
Conc: 11.39 ng/ml