

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072523\
 Data File : PL084208.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jul 2023 22:51
 Operator : AR\AJ
 Sample : 03741-16
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 B-P28A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 05:03:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 00:03:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	2.687	17359523	8104379	8.680	7.297
28)	SA Decachlor...	9.023	7.869	12243591	9464457	9.406	8.518
Target Compounds							
12)	B 4,4'-DDE	6.147	5.166	1992203	925186	0.990	0.753



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072523\
Data File : PL084208.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jul 2023 22:51
Operator : AR\AJ
Sample : 03741-16
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
B-P28A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 05:03:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 00:03:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

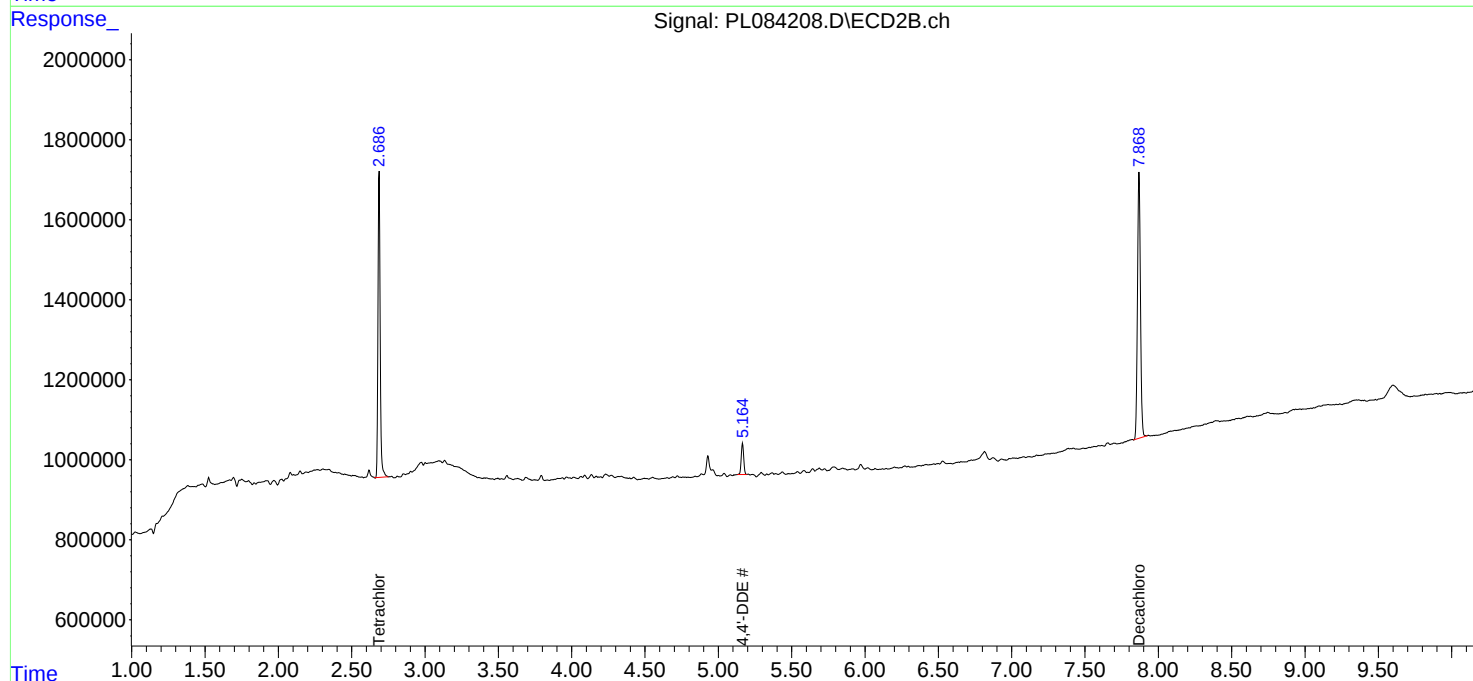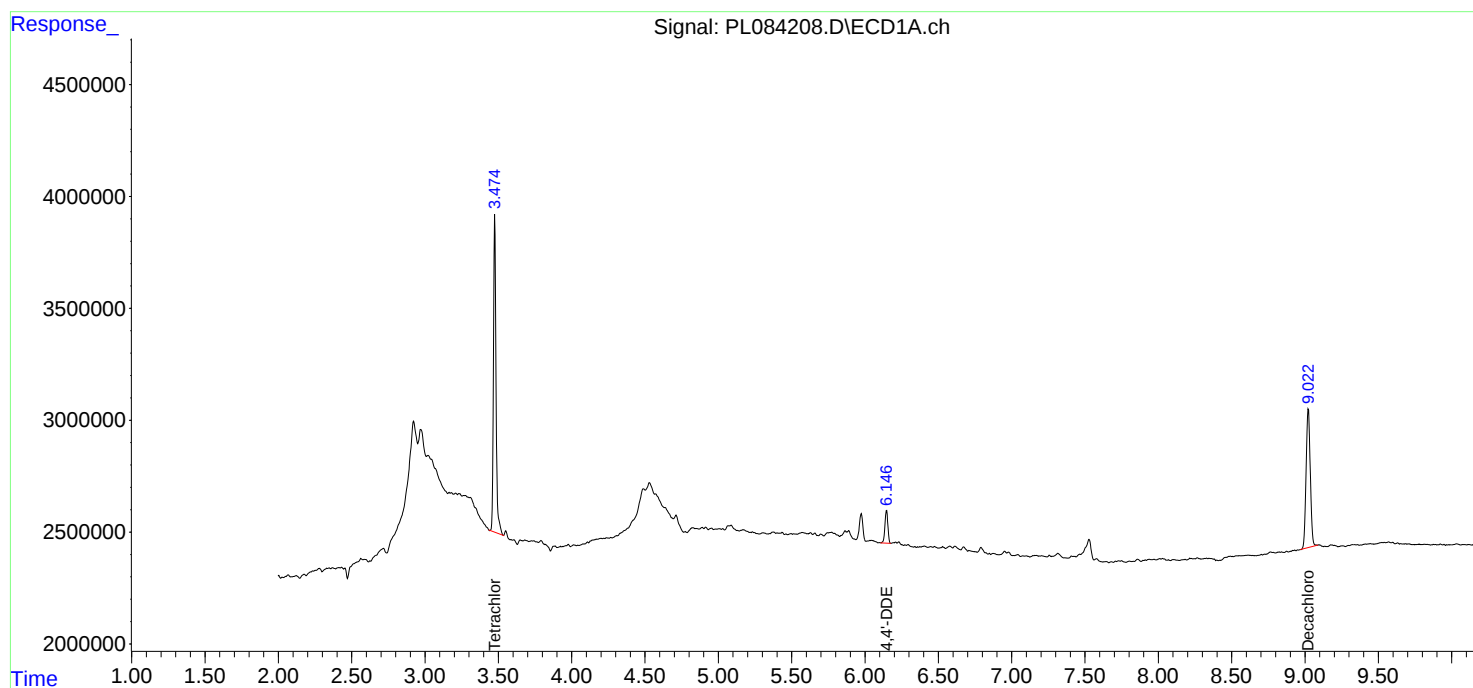


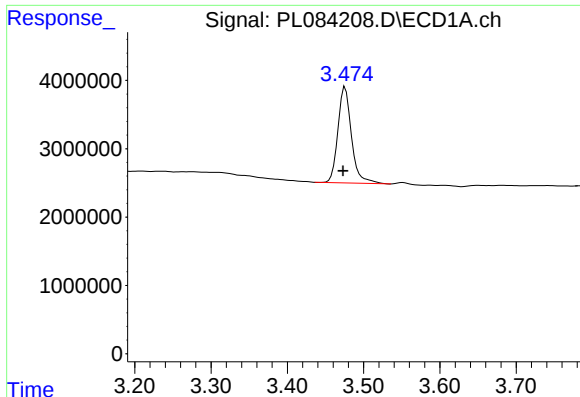

#1 Tetrachloro-m-xylene


R.T.: 3.476 min
Delta R.T.: 0.003 min
Response: 17359523
Conc: 8.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
B-P28A

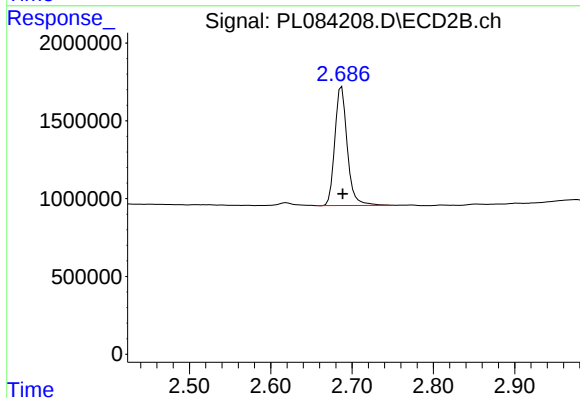


#1 Tetrachloro-m-xylene

R.T.: 2.687 min
Delta R.T.: -0.001 min
Response: 8104379
Conc: 7.30 ng/ml

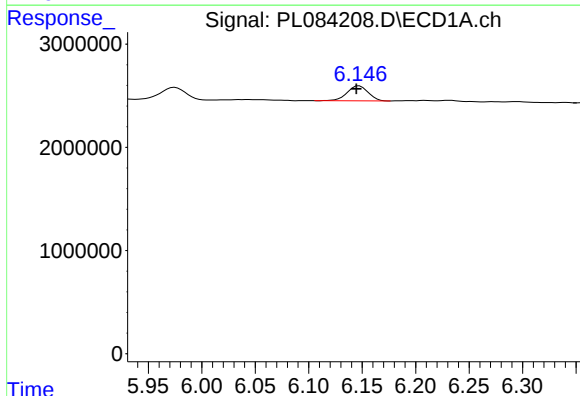


#12 4,4'-DDE

R.T.: 6.147 min
Delta R.T.: 0.003 min
Response: 1992203
Conc: 0.99 ng/ml

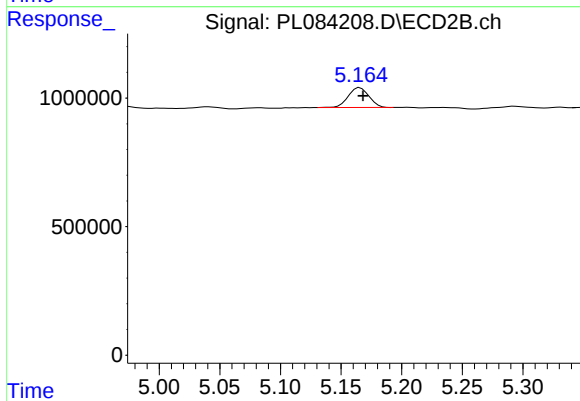

#12 4,4'-DDE


R.T.: 5.166 min
Delta R.T.: -0.002 min
Response: 925186
Conc: 0.75 ng/ml

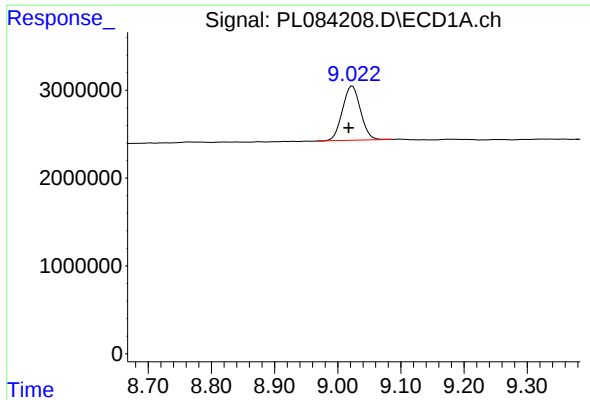

#28 Decachlorobiphenyl

R.T.: 9.023 min
Delta R.T.: 0.006 min
Response: 12243591
Conc: 9.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
B-P28A

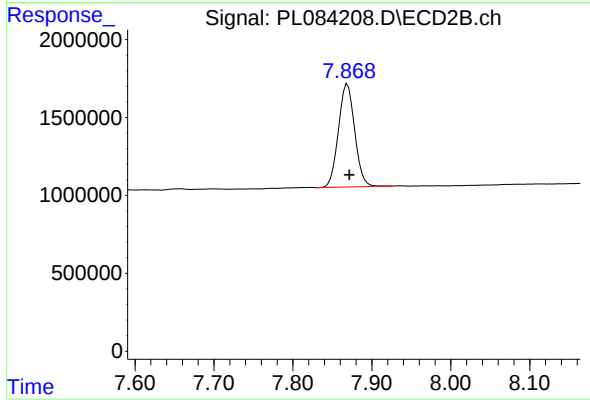

#28 Decachlorobiphenyl

R.T.: 7.869 min
Delta R.T.: -0.002 min
Response: 9464457
Conc: 8.52 ng/ml