

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072524\
 Data File : PL090651.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jul 2024 15:06
 Operator : AR\AJ
 Sample : PB162270BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB162270BL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/26/2024
 Supervised By : Ankita Jodhani 07/26/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 01:20:05 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071524.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 15 14:16:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.551	2.789	35000909	28481331	16.810m	16.923
2)	SA Decachlor...	9.068	7.937	24606350	29615228	18.517m	20.311

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072524\
Data File : PL090651.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jul 2024 15:06
Operator : AR\AJ
Sample : PB162270BL
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PB162270BL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/26/2024
Supervised By : Ankita Jodhani 07/26/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 01:20:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071524.M
Quant Title : GC Extractables
QLast Update : Mon Jul 15 14:16:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

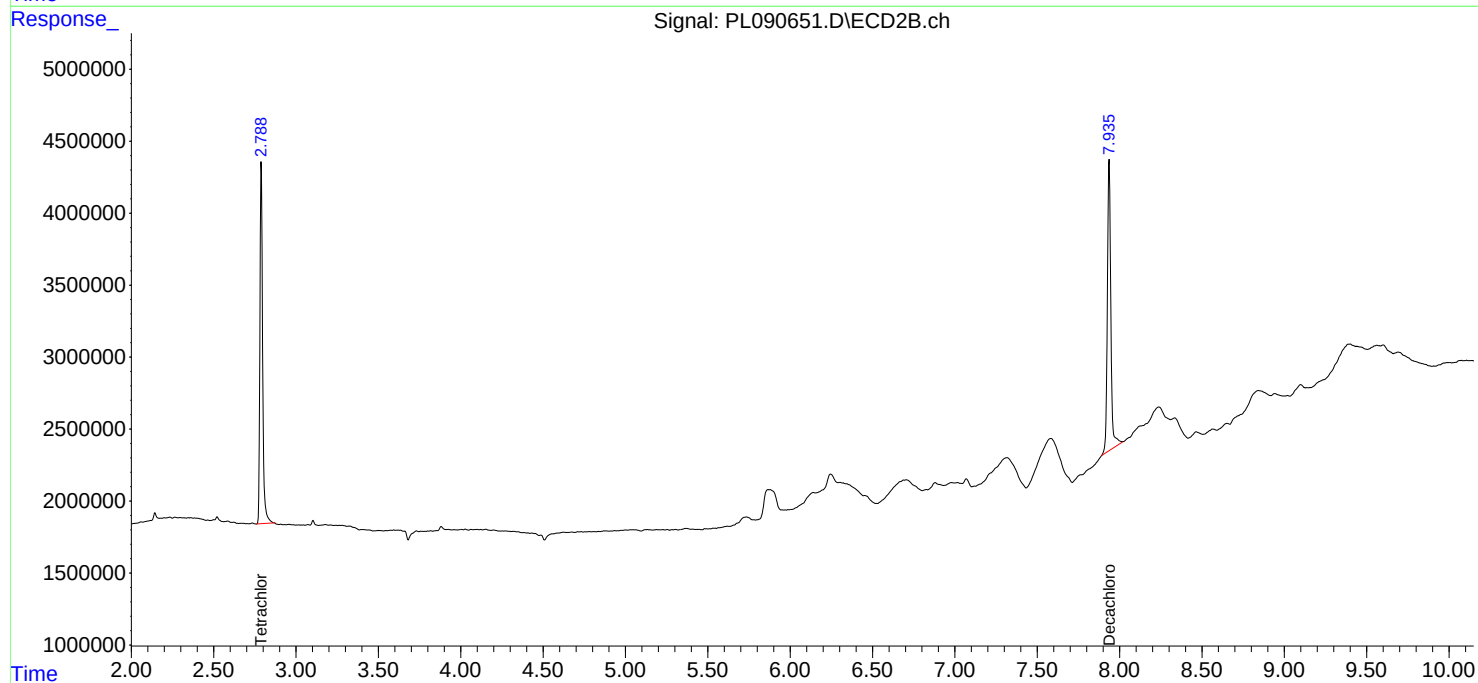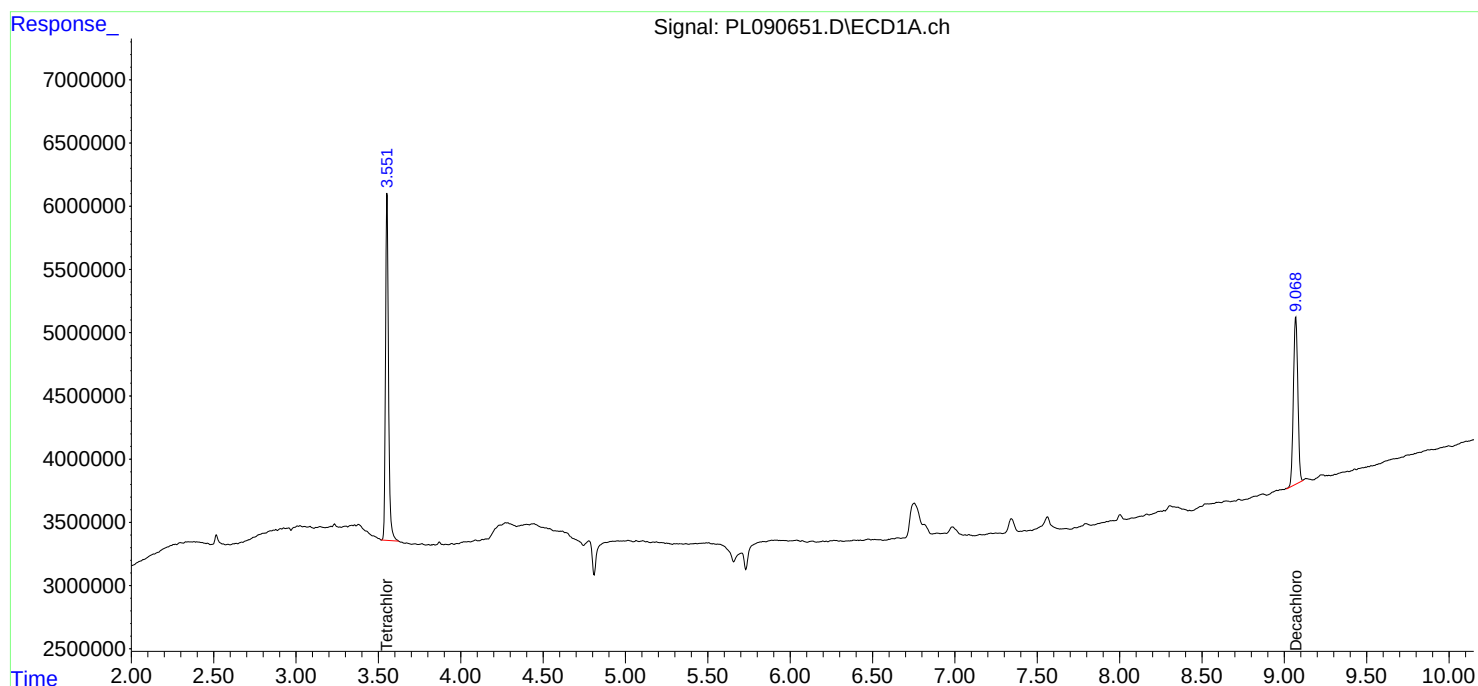

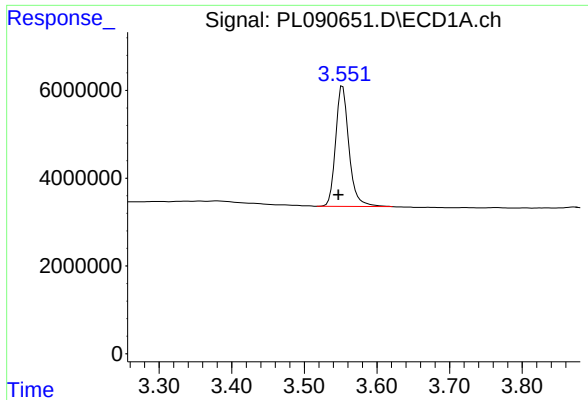


#1 Tetrachloro-m-xylene

R.T.: 3.551 min
Delta R.T.: 0.004 min
Response: 3500909
Conc: 16.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB162270BL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/26/2024
Supervised By :Ankita Jodhani 07/26/2024

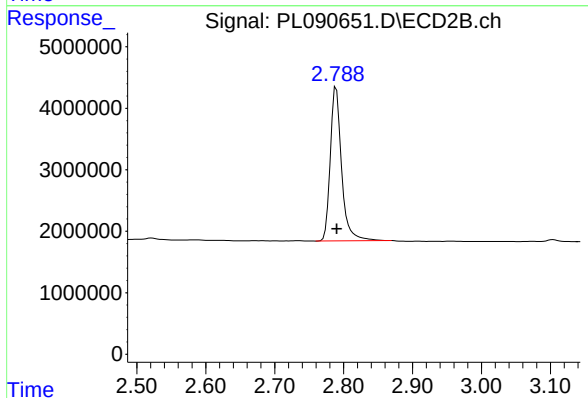


#1 Tetrachloro-m-xylene

R.T.: 2.789 min
Delta R.T.: 0.000 min
Response: 28481331
Conc: 16.92 ng/ml

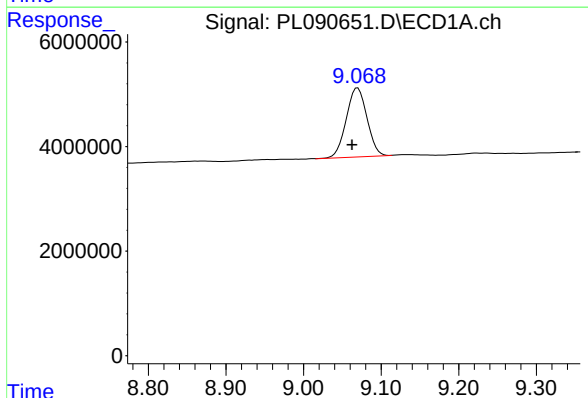

#28 Decachlorobiphenyl

R.T.: 9.068 min
Delta R.T.: 0.006 min
Response: 24606350
Conc: 18.52 ng/ml m

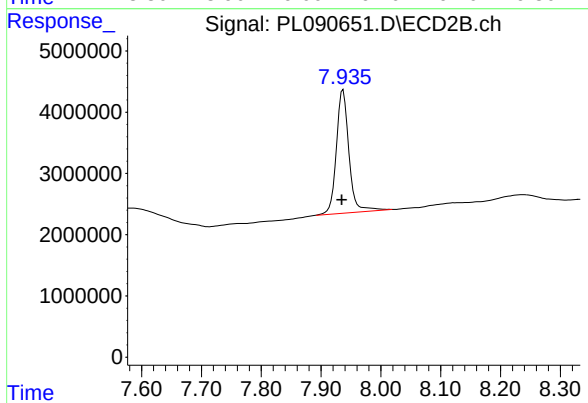

#28 Decachlorobiphenyl

R.T.: 7.937 min
Delta R.T.: 0.002 min
Response: 29615228
Conc: 20.31 ng/ml