

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072524\
 Data File : PL090657.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jul 2024 16:55
 Operator : AR\AJ
 Sample : P3358-01 10X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OK-02-07242024

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/26/2024
 Supervised By :Ankita Jodhani 07/26/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 07:38:59 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071524.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 15 14:16:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.544	2.786	2929298	2454760	1.407m	1.459m
28) SA Decachlor...	9.053	7.930	3855522	1916268	2.901m	1.314 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072524\
Data File : PL090657.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jul 2024 16:55
Operator : AR\AJ
Sample : P3358-01 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OK-02-07242024


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/26/2024
Supervised By : Ankita Jodhani 07/26/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 07:38:59 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071524.M
Quant Title : GC Extractables
QLast Update : Mon Jul 15 14:16:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

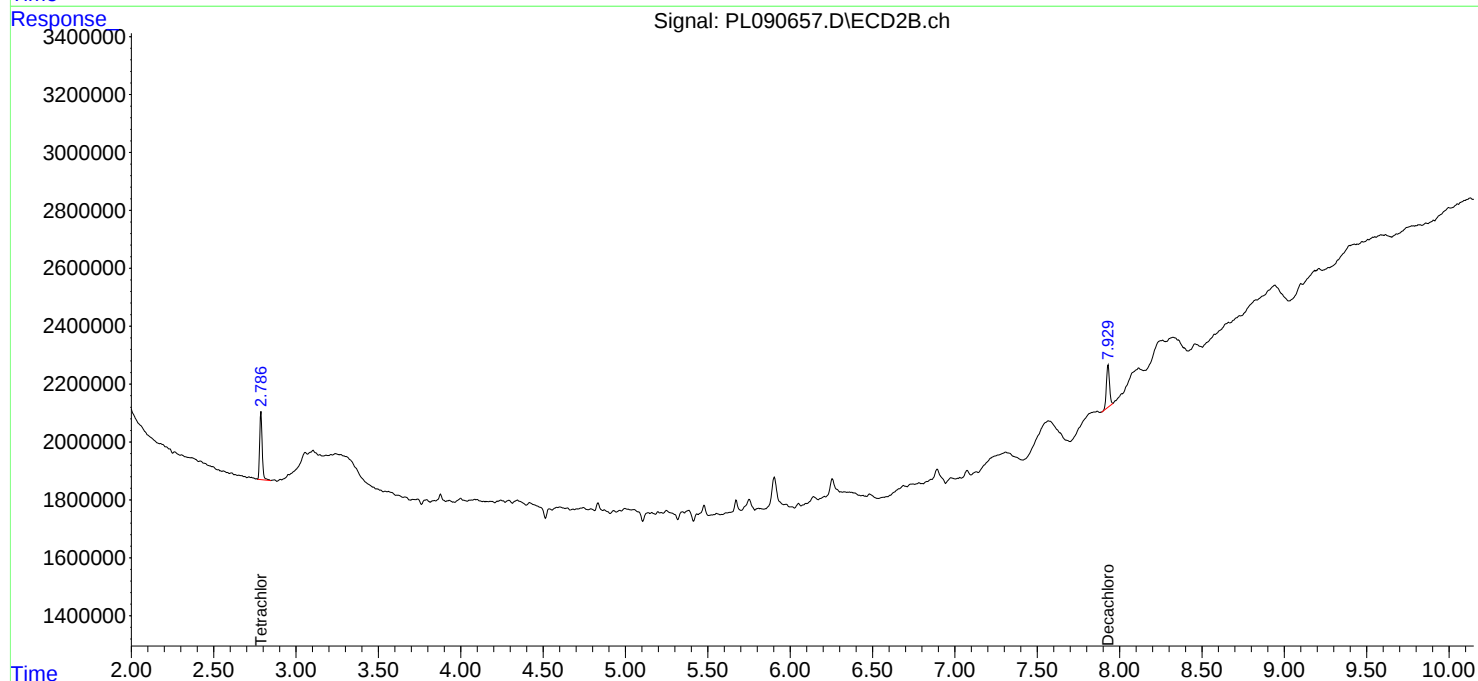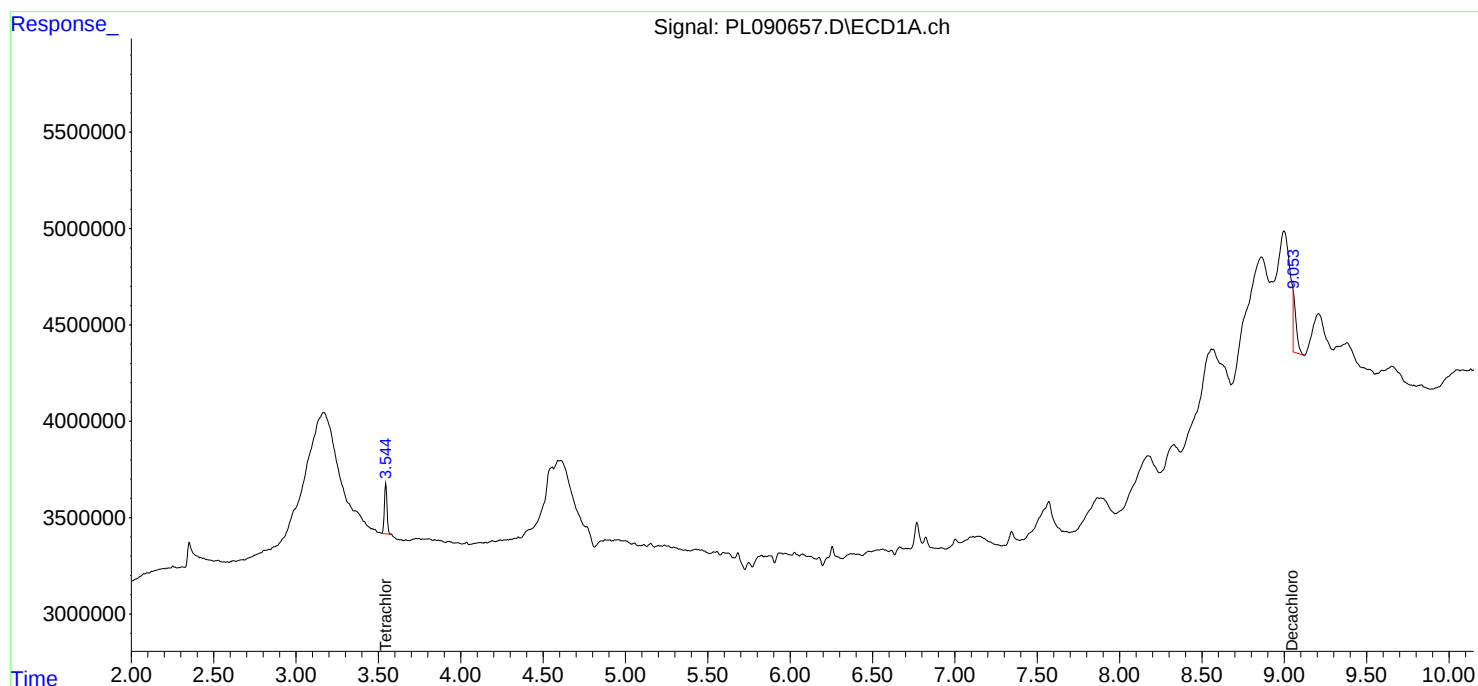

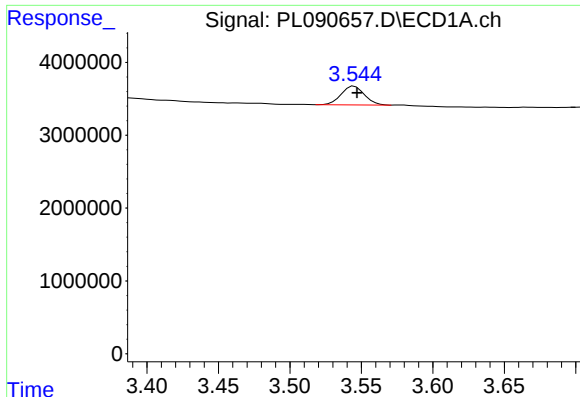


#1 Tetrachloro-m-xylene

R.T.: 3.544 min
Delta R.T.: -0.003 min
Response: 2929298
Conc: 1.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-02-07242024


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/26/2024
Supervised By :Ankita Jodhani 07/26/2024

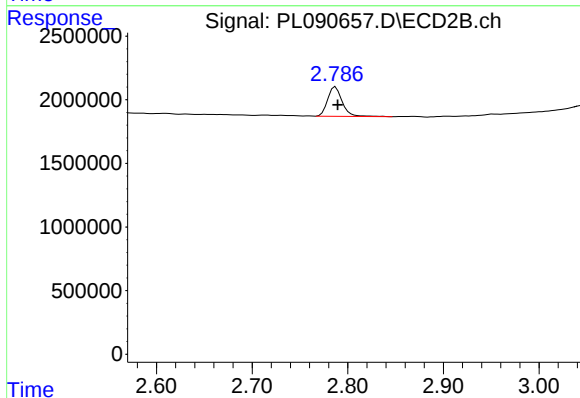


#1 Tetrachloro-m-xylene

R.T.: 2.786 min
Delta R.T.: -0.004 min
Response: 2454760
Conc: 1.46 ng/ml m

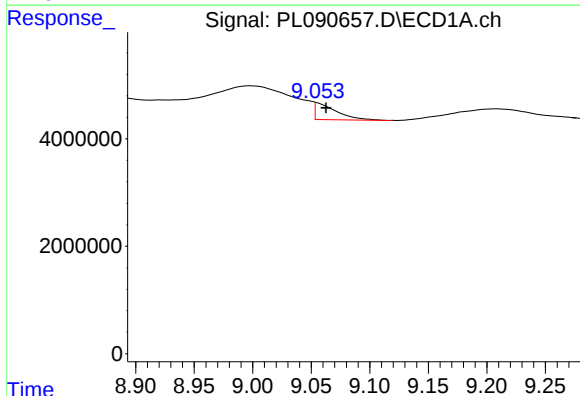

#28 Decachlorobiphenyl

R.T.: 9.053 min
Delta R.T.: -0.009 min
Response: 3855522
Conc: 2.90 ng/ml m

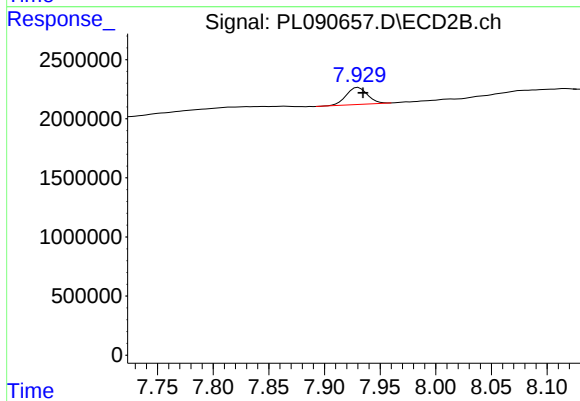

#28 Decachlorobiphenyl

R.T.: 7.930 min
Delta R.T.: -0.004 min
Response: 1916268
Conc: 1.31 ng/ml