

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072525\
 Data File : PL096579.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jul 2025 14:15
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 23:25:17 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 07 15:22:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	2.827	62386555	116.8E6	17.097	20.245
28)	SA Decachlor...	9.016	7.992	43425742	84381675	15.437	16.922
Target Compounds							
8)	B Heptachlo...	5.654	0.000	2003033	0	0.483	N.D. #
9)	A Endosulfan I	0.000	5.176	0	4105160	N.D.	0.572 #
11)	B alpha-Chl...	5.976f	0.000	2891024	0	0.660	N.D. #
14)	MA Endrin	0.000	5.721	0	3404971	N.D.	0.559 #
18)	B Endrin al...	0.000	6.182	0	2154563	N.D.	0.484 #
26)	Chlordane-4	5.976f	0.000	2891024	0	3.222	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072525\
Data File : PL096579.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jul 2025 14:15
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 23:25:17 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
Quant Title : GC Extractables
QLast Update : Mon Jul 07 15:22:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

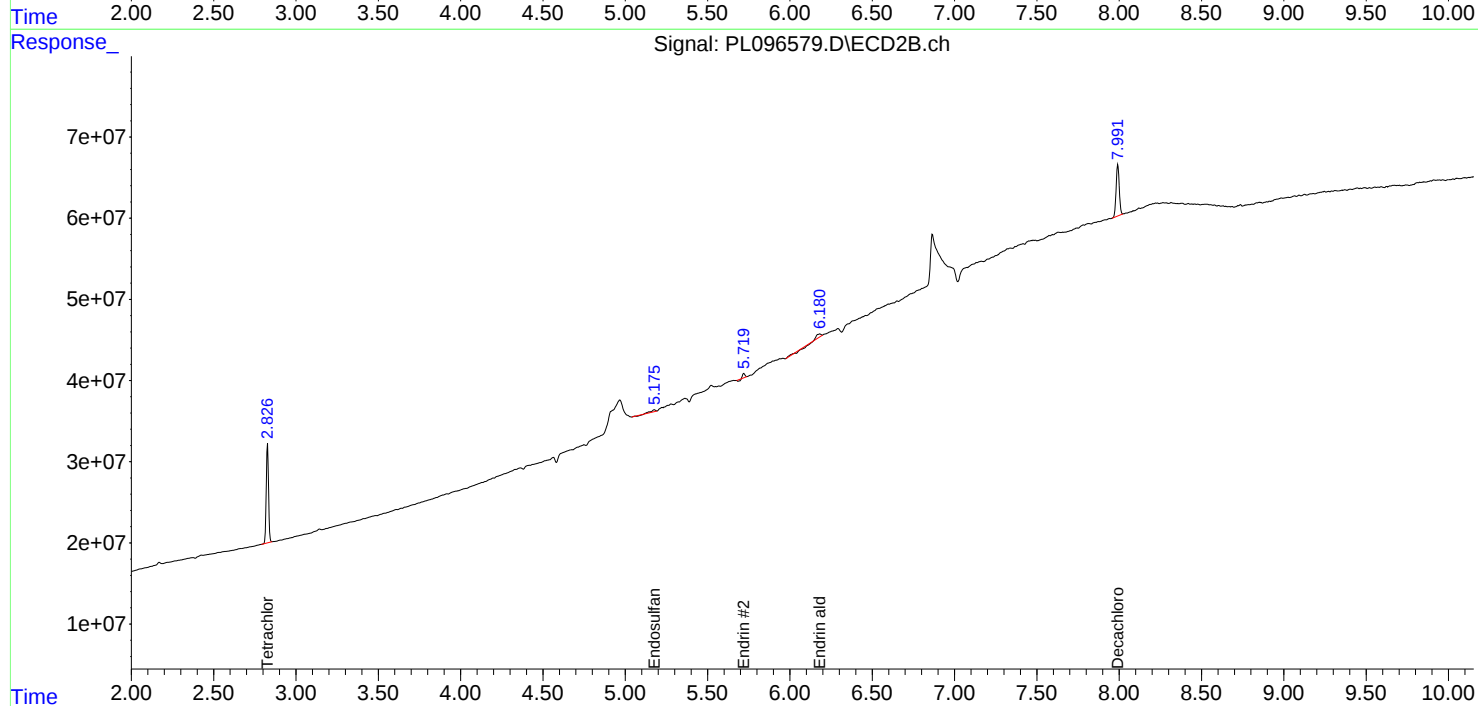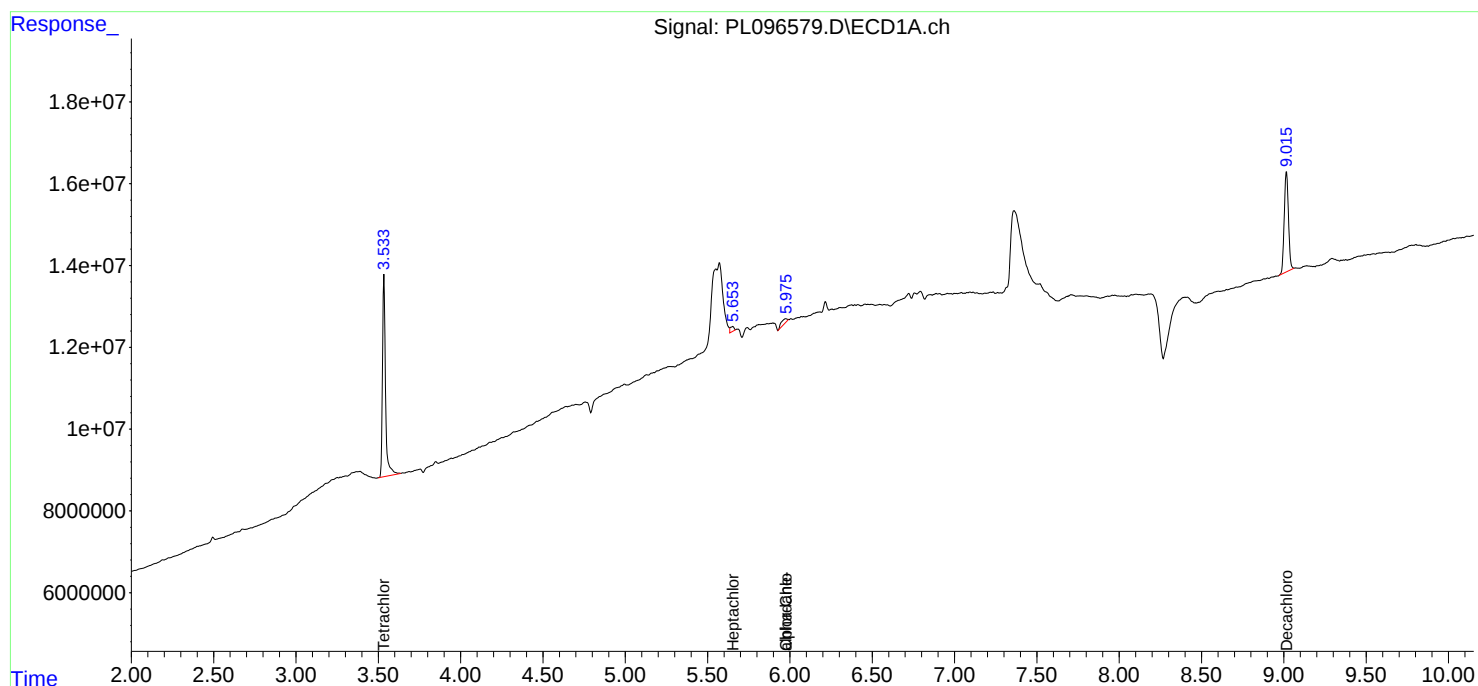


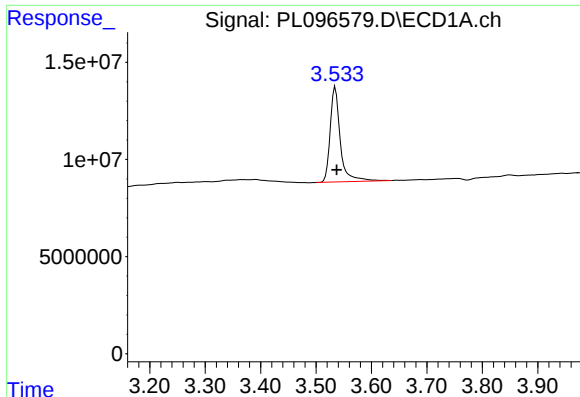

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: -0.002 min
Response: 62386555
Conc: 17.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

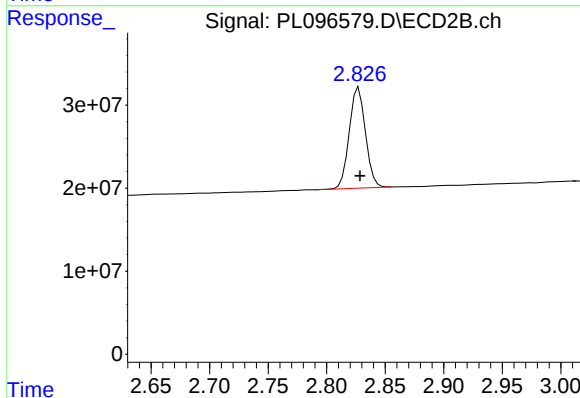


#1 Tetrachloro-m-xylene

R.T.: 2.827 min
Delta R.T.: 0.000 min
Response: 116835457
Conc: 20.24 ng/ml

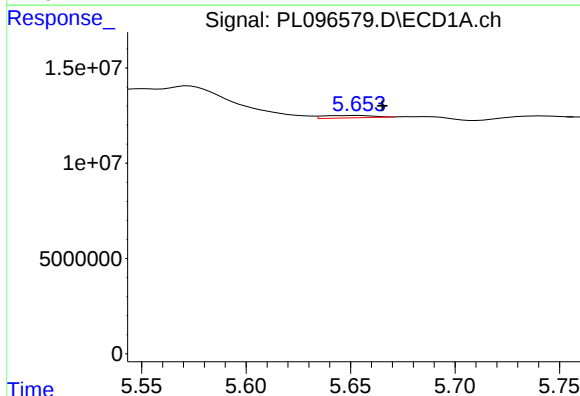


#8 Heptachlor epoxide

R.T.: 5.654 min
Delta R.T.: -0.011 min
Response: 2003033
Conc: 0.48 ng/ml

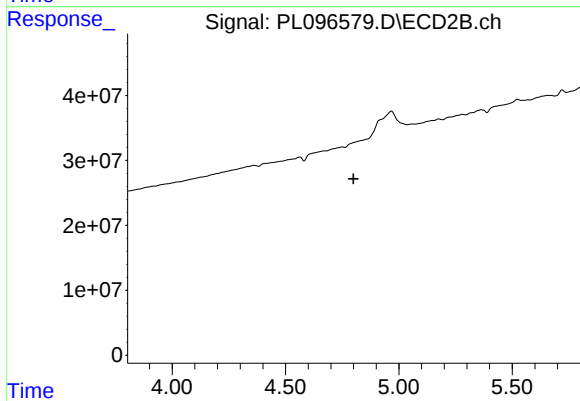

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.800 min
Response: 0
Conc: N.D.

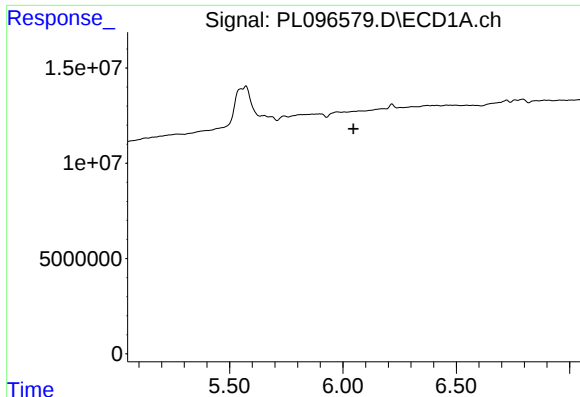

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.047 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

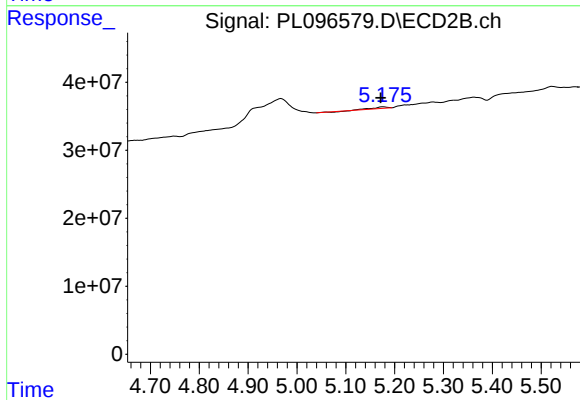


#9 Endosulfan I

R.T.: 5.176 min
Delta R.T.: 0.005 min
Response: 4105160
Conc: 0.57 ng/ml

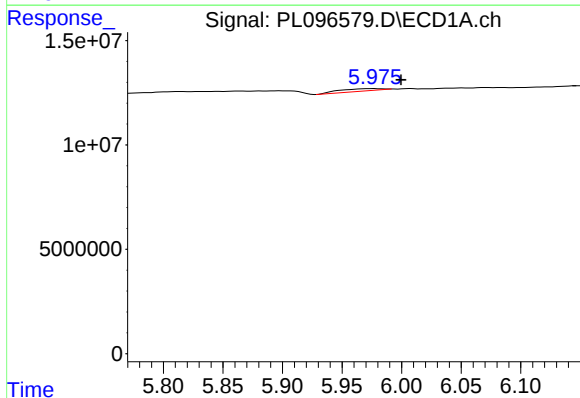


#11 alpha-Chlordane

R.T.: 5.976 min
Delta R.T.: -0.023 min
Response: 2891024
Conc: 0.66 ng/ml

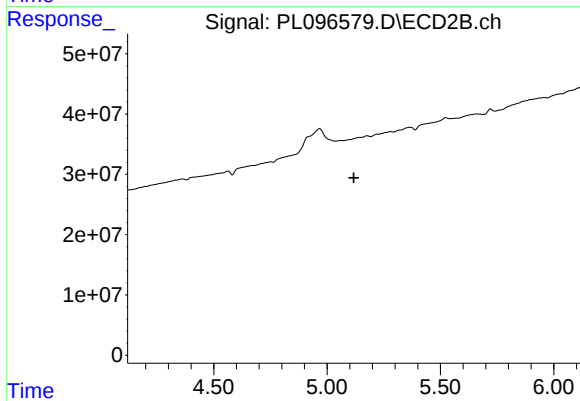

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.119 min
Response: 0
Conc: N.D.

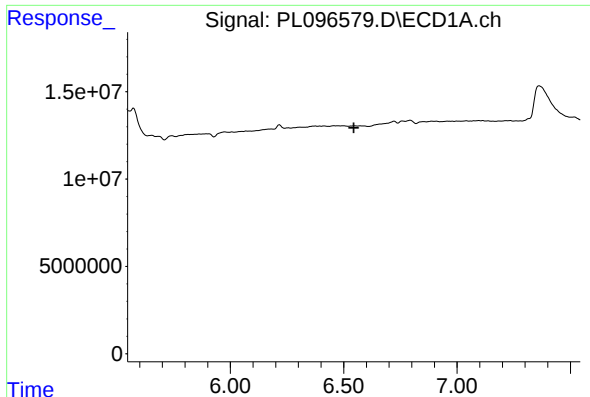

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

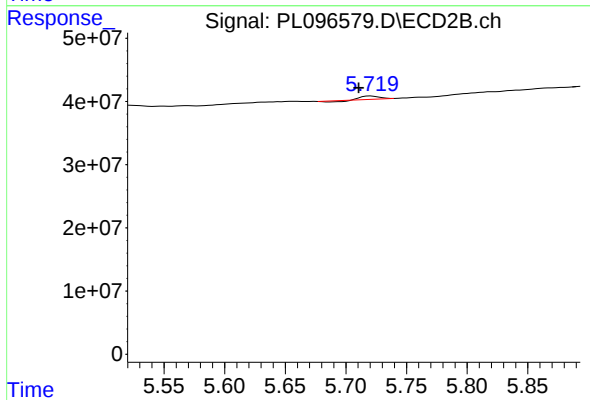


#14 Endrin

R.T.: 5.721 min
Delta R.T.: 0.010 min
Response: 3404971
Conc: 0.56 ng/ml

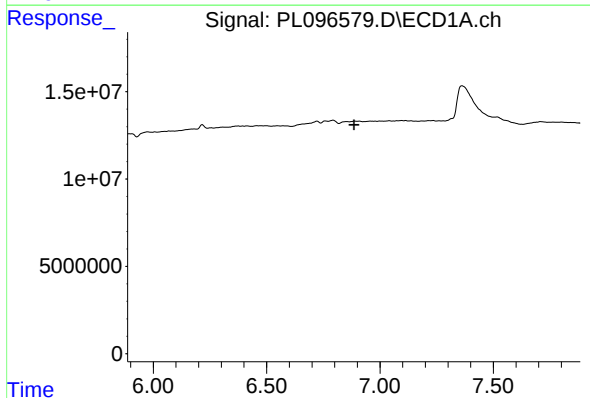


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.886 min
Response: 0
Conc: N.D.

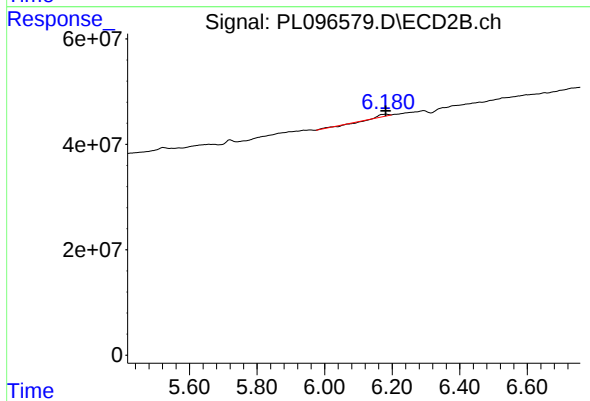

#18 Endrin aldehyde


R.T.: 6.182 min
Delta R.T.: 0.000 min
Response: 2154563
Conc: 0.48 ng/ml

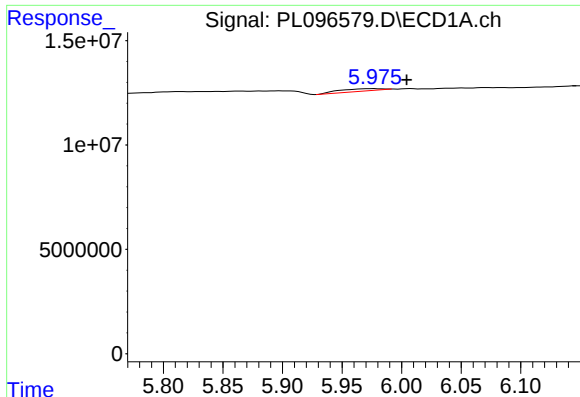

#26 Chlordane-4


R.T.: 5.976 min
Delta R.T.: -0.028 min
Response: 2891024
Conc: 3.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

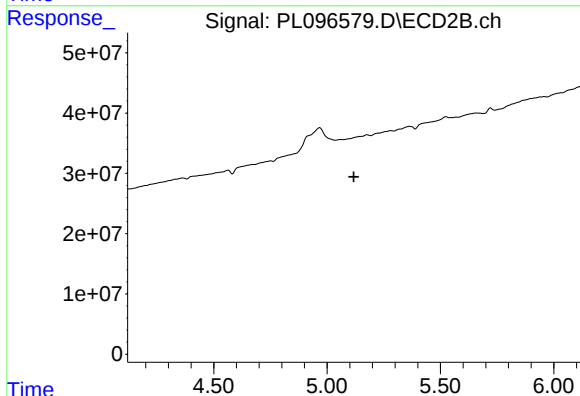


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.118 min
Response: 0
Conc: N.D.

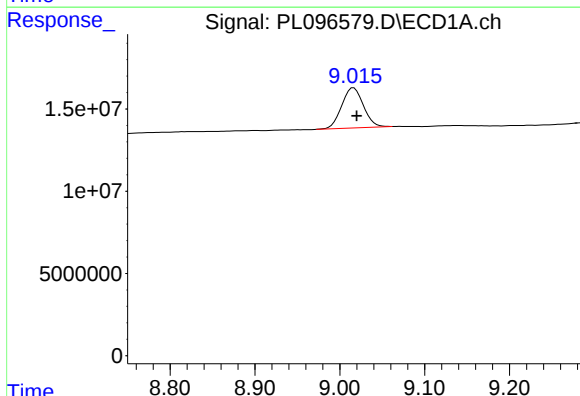

#28 Decachlorobiphenyl

R.T.: 9.016 min
Delta R.T.: -0.004 min
Response: 43425742
Conc: 15.44 ng/ml

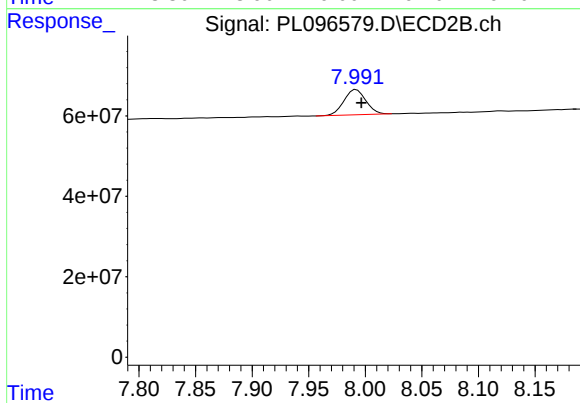

#28 Decachlorobiphenyl

R.T.: 7.992 min
Delta R.T.: -0.004 min
Response: 84381675
Conc: 16.92 ng/ml