

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072525\
 Data File : PL096584.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jul 2025 15:37
 Operator : AR\AJ
 Sample : PB169003BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB169003BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 23:28:05 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 07 15:22:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	2.828	57121170	104.8E6	15.654	18.152
28)	SA Decachlor...	9.017	7.992	42374532	55878618	15.063	11.206 #
Target Compounds							
8)	B Heptachlo...	5.646f	0.000	1695226	0	0.409	N.D. #
14)	MA Endrin	0.000	5.718	0	8404047	N.D.	1.379 #
15)	B Endosulfa...	6.745	6.017	4341937	1606140	1.251	0.274 #
18)	B Endrin al...	0.000	6.174	0	14880887	N.D.	3.341 #
19)	B Endosulfa...	0.000	6.394	0	6012811	N.D.	1.069 #
21)	B Endrin ke...	0.000	6.896	0	12178328	N.D.	1.948 #
22)	Mirex	0.000	7.098	0	2683968	N.D.	0.540 #
27)	Chlordane-5	0.000	6.017	0	1606140	N.D.	5.666 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072525\
Data File : PL096584.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jul 2025 15:37
Operator : AR\AJ
Sample : PB169003BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB169003BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 23:28:05 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
Quant Title : GC Extractables
QLast Update : Mon Jul 07 15:22:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

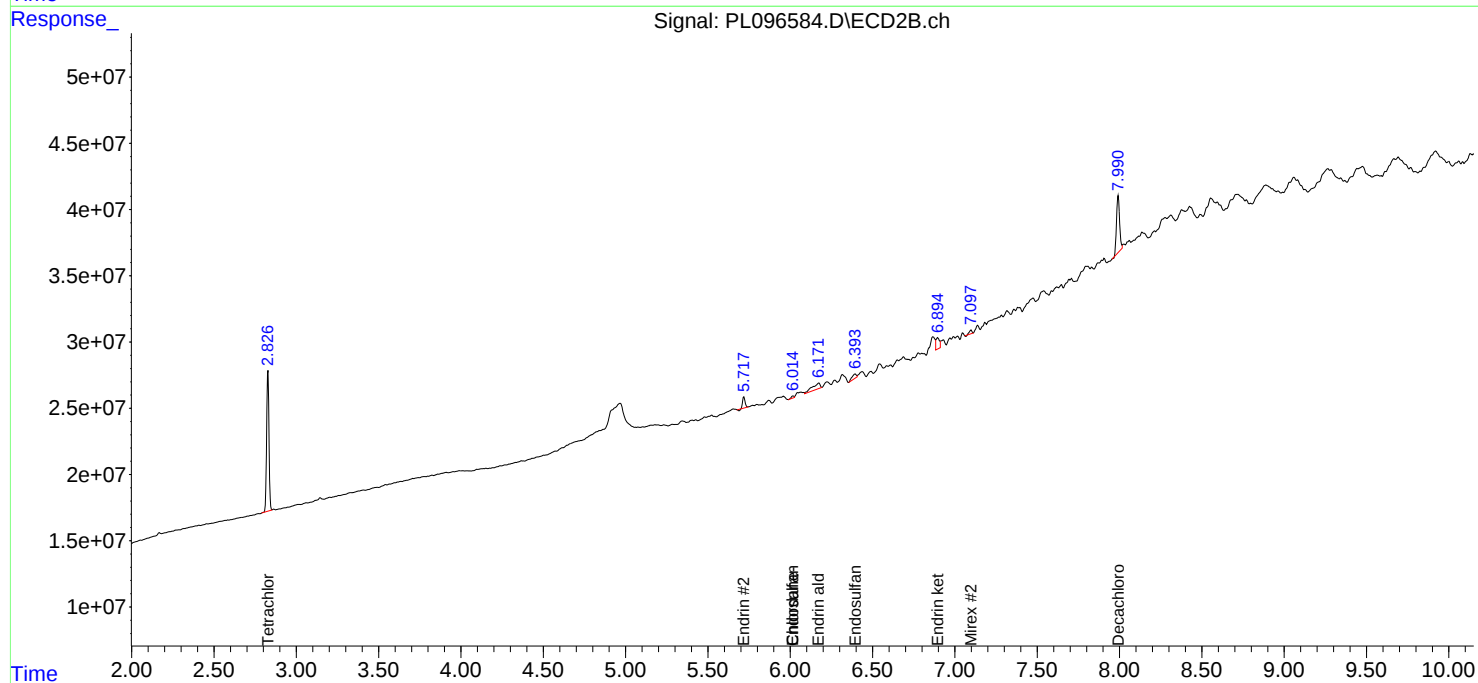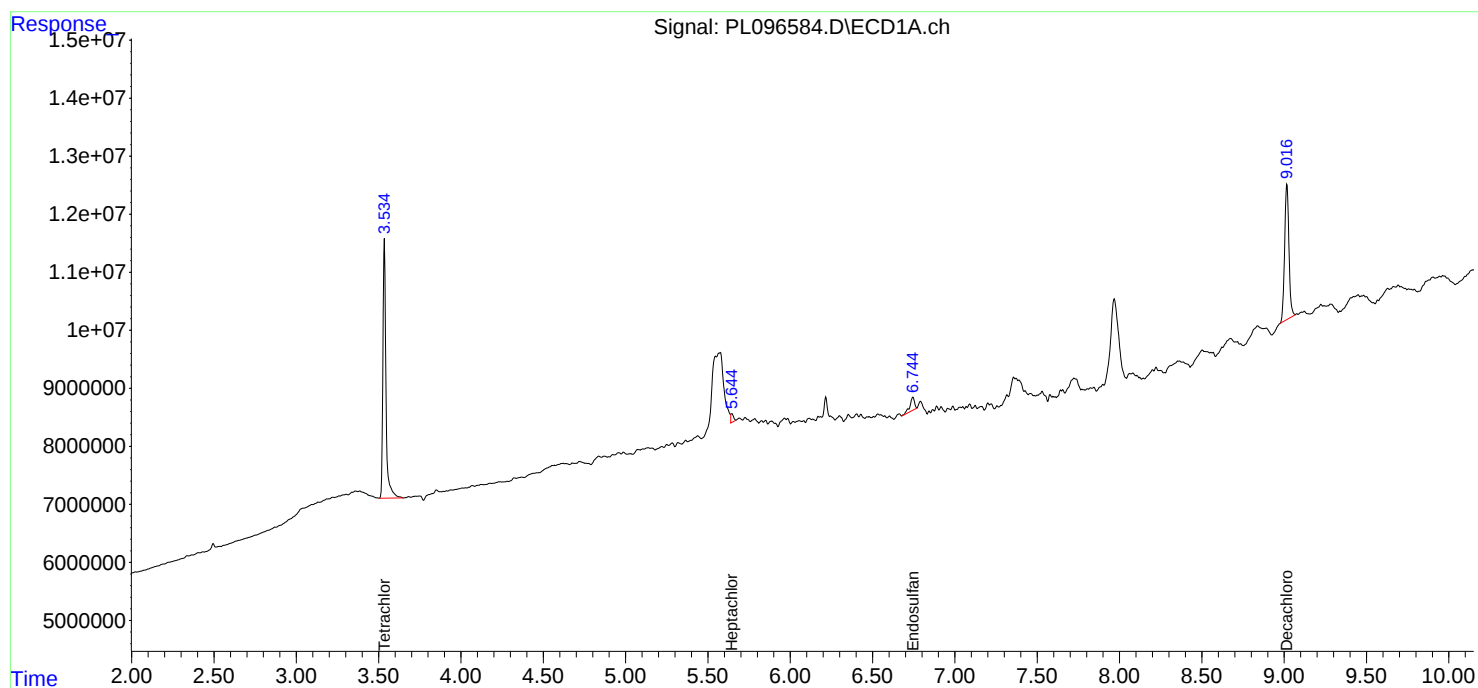


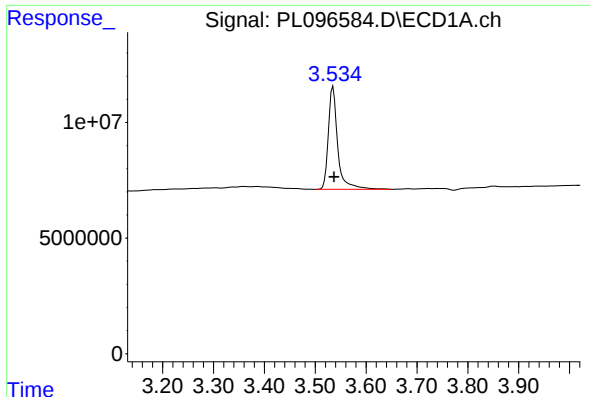

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: -0.002 min
Response: 57121170
Conc: 15.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB169003BL

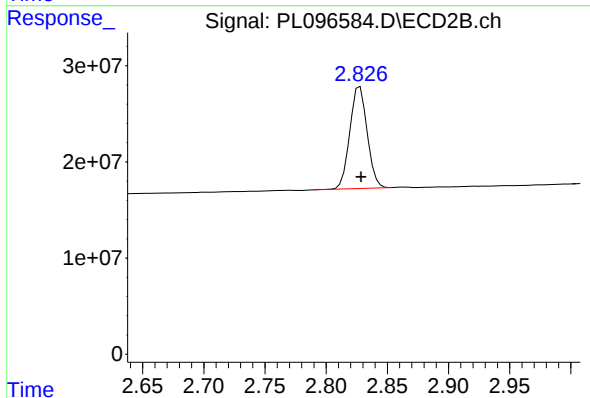


#1 Tetrachloro-m-xylene

R.T.: 2.828 min
Delta R.T.: 0.000 min
Response: 104756683
Conc: 18.15 ng/ml

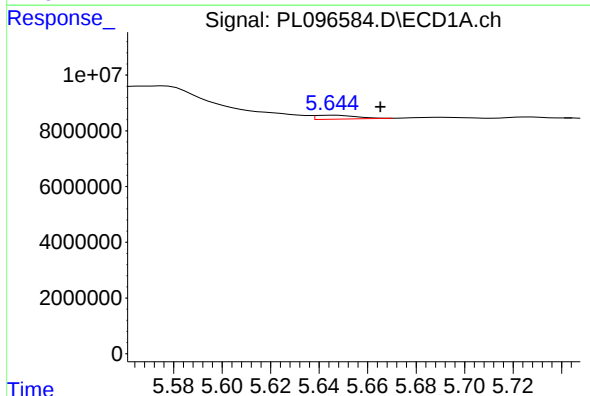


#8 Heptachlor epoxide

R.T.: 5.646 min
Delta R.T.: -0.019 min
Response: 1695226
Conc: 0.41 ng/ml

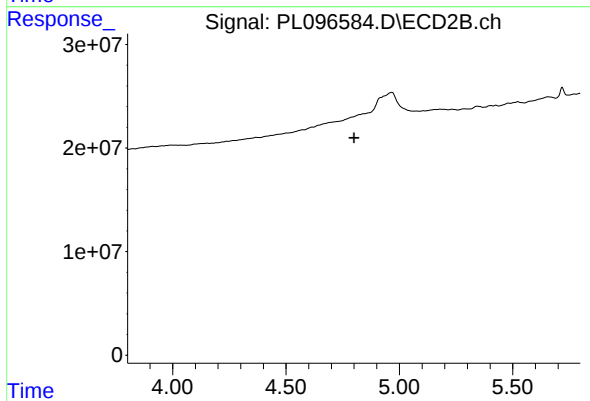

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.800 min
Response: 0
Conc: N.D.

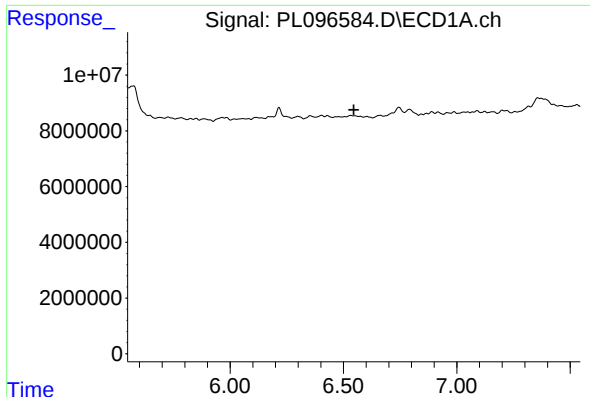

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB169003BL

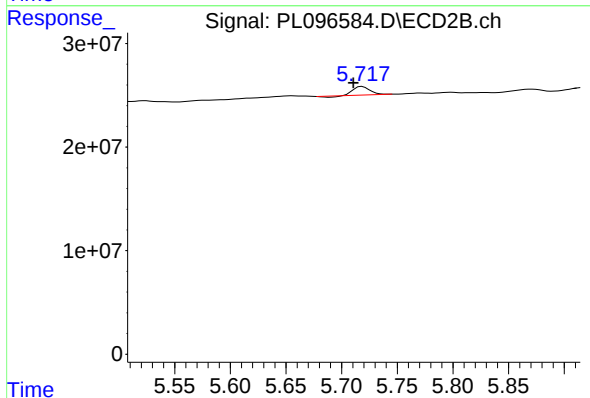


#14 Endrin

R.T.: 5.718 min
Delta R.T.: 0.008 min
Response: 8404047
Conc: 1.38 ng/ml

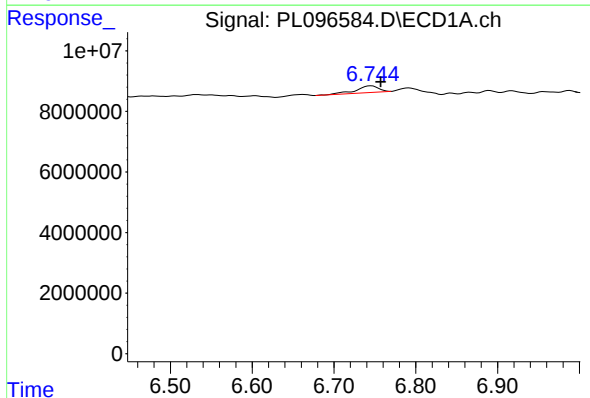


#15 Endosulfan II

R.T.: 6.745 min
Delta R.T.: -0.012 min
Response: 4341937
Conc: 1.25 ng/ml

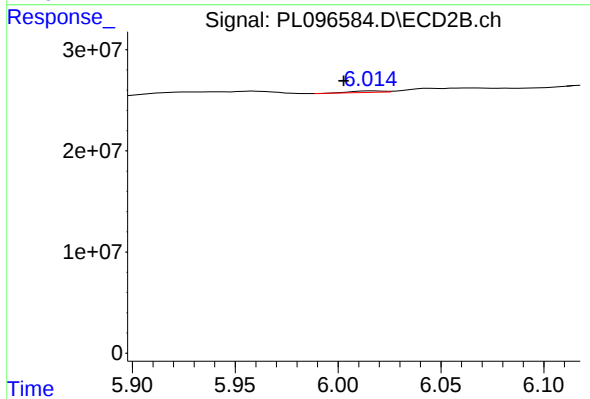

#15 Endosulfan II


R.T.: 6.017 min
Delta R.T.: 0.014 min
Response: 1606140
Conc: 0.27 ng/ml

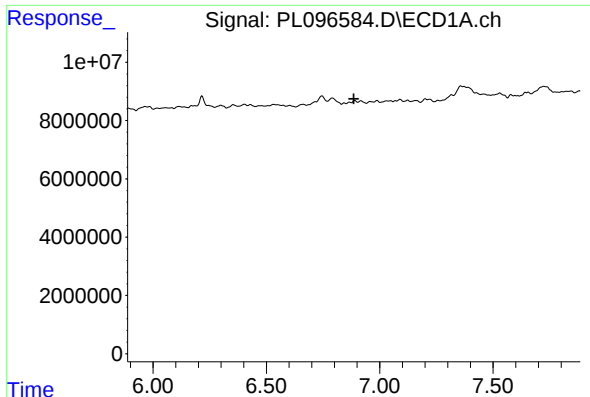

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.886 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB169003BL

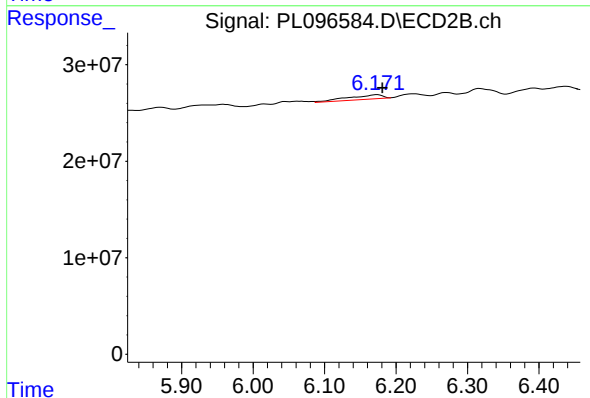


#18 Endrin aldehyde

R.T.: 6.174 min
Delta R.T.: -0.007 min
Response: 14880887
Conc: 3.34 ng/ml

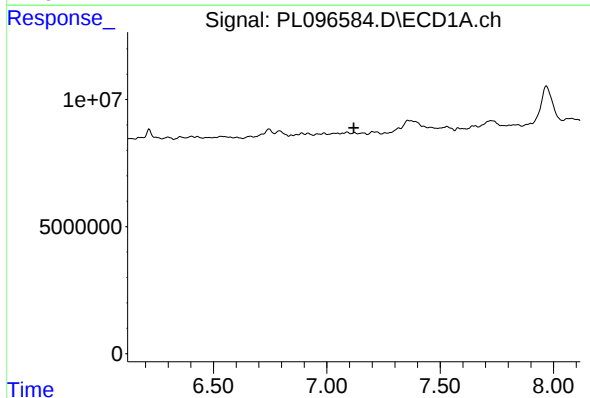


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 7.120 min
Response: 0
Conc: N.D.

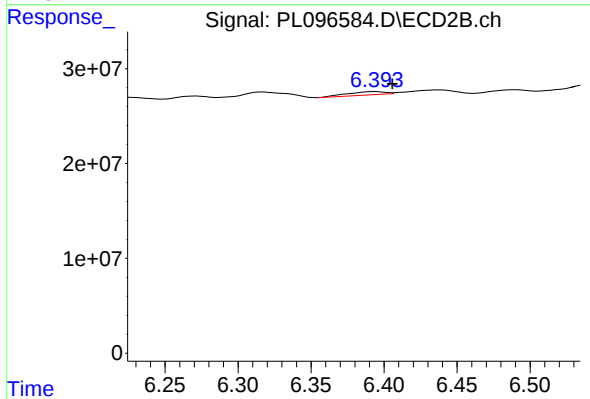

#19 Endosulfan Sulfate


R.T.: 6.394 min
Delta R.T.: -0.011 min
Response: 6012811
Conc: 1.07 ng/ml

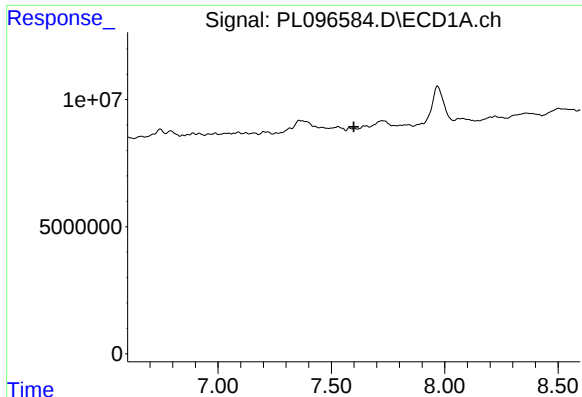

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.599 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB169003BL

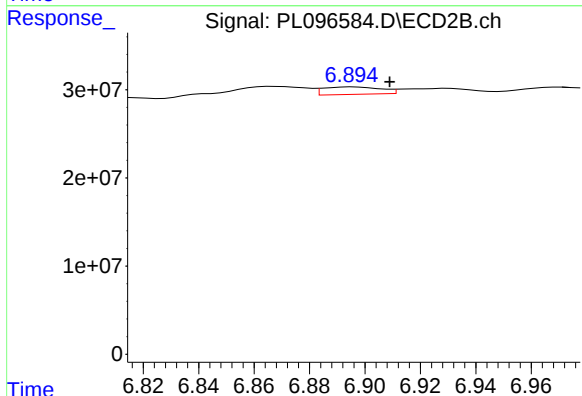


#21 Endrin ketone

R.T.: 6.896 min
Delta R.T.: -0.013 min
Response: 12178328
Conc: 1.95 ng/ml

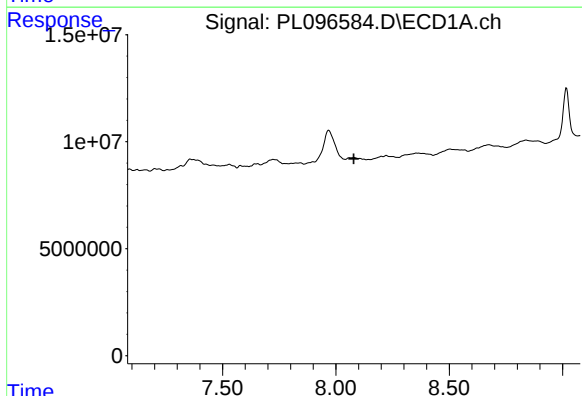


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 8.079 min
Response: 0
Conc: N.D.

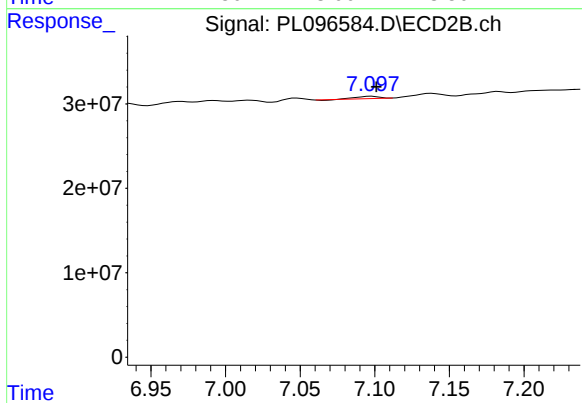

#22 Mirex


R.T.: 7.098 min
Delta R.T.: -0.003 min
Response: 2683968
Conc: 0.54 ng/ml

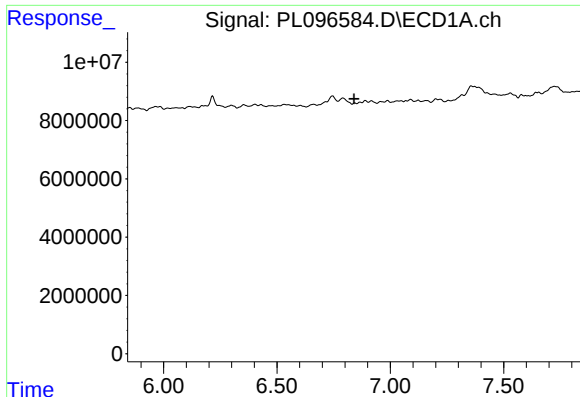

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.841 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB169003BL

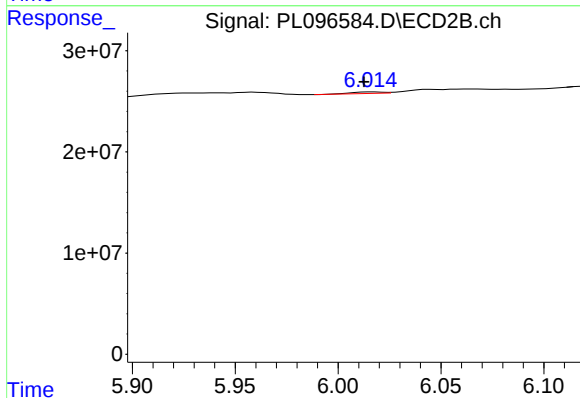


#27 Chlordane-5

R.T.: 6.017 min
Delta R.T.: 0.004 min
Response: 1606140
Conc: 5.67 ng/ml

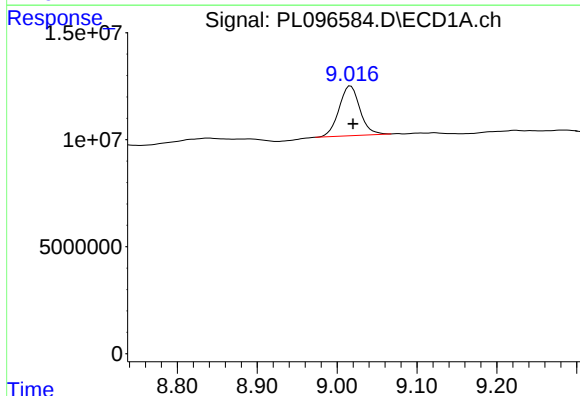

#28 Decachlorobiphenyl

R.T.: 9.017 min
Delta R.T.: -0.003 min
Response: 42374532
Conc: 15.06 ng/ml

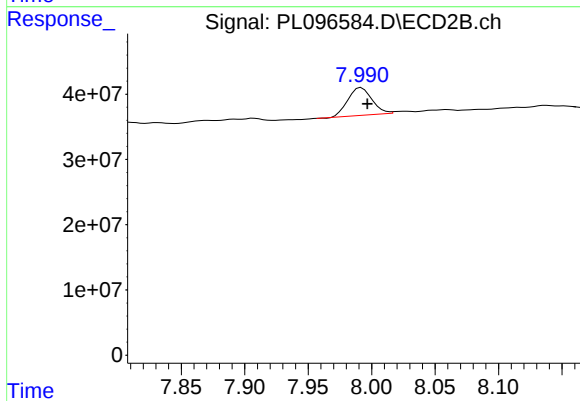

#28 Decachlorobiphenyl

R.T.: 7.992 min
Delta R.T.: -0.005 min
Response: 55878618
Conc: 11.21 ng/ml