

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072525\
 Data File : PL096590.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jul 2025 17:36
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 23:30:59 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 07 15:22:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.534	2.827	62195326	115.1E6	17.045	19.941
28)	SA Decachlor...	9.015	7.992	40920137	58449832	14.546	11.722
Target Compounds							
8)	B Heptachlo...	5.653	0.000	3656879	0	0.881	N.D. #
13)	MA Dieldrin	0.000	5.445	0	8138491	N.D.	1.193 #
14)	MA Endrin	0.000	5.718	0	4667288	N.D.	0.766 #
15)	B Endosulfa...	6.744	0.000	3947114	0	1.137	N.D. #
18)	B Endrin al...	0.000	6.171	0	11984715	N.D.	2.690 #
21)	B Endrin ke...	0.000	6.930f	0	8265419	N.D.	1.322 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072525\
Data File : PL096590.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jul 2025 17:36
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 23:30:59 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
Quant Title : GC Extractables
QLast Update : Mon Jul 07 15:22:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

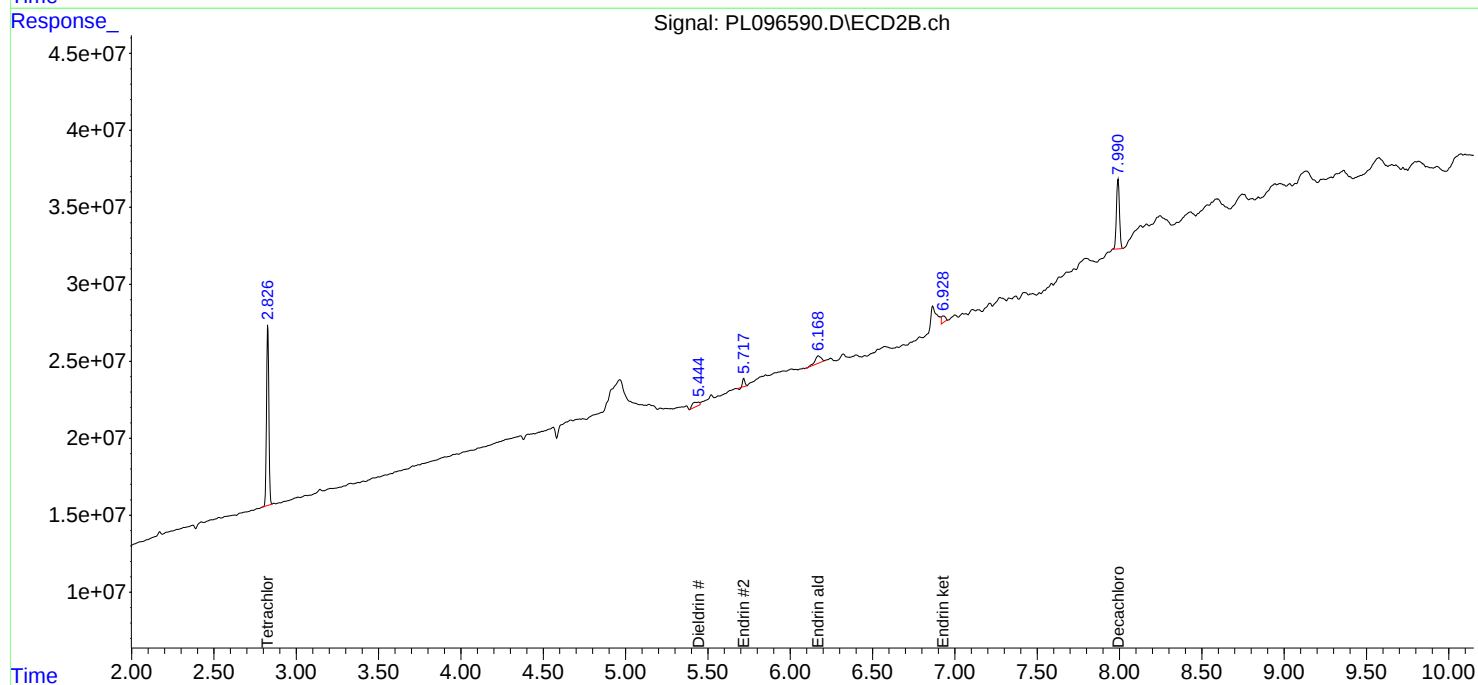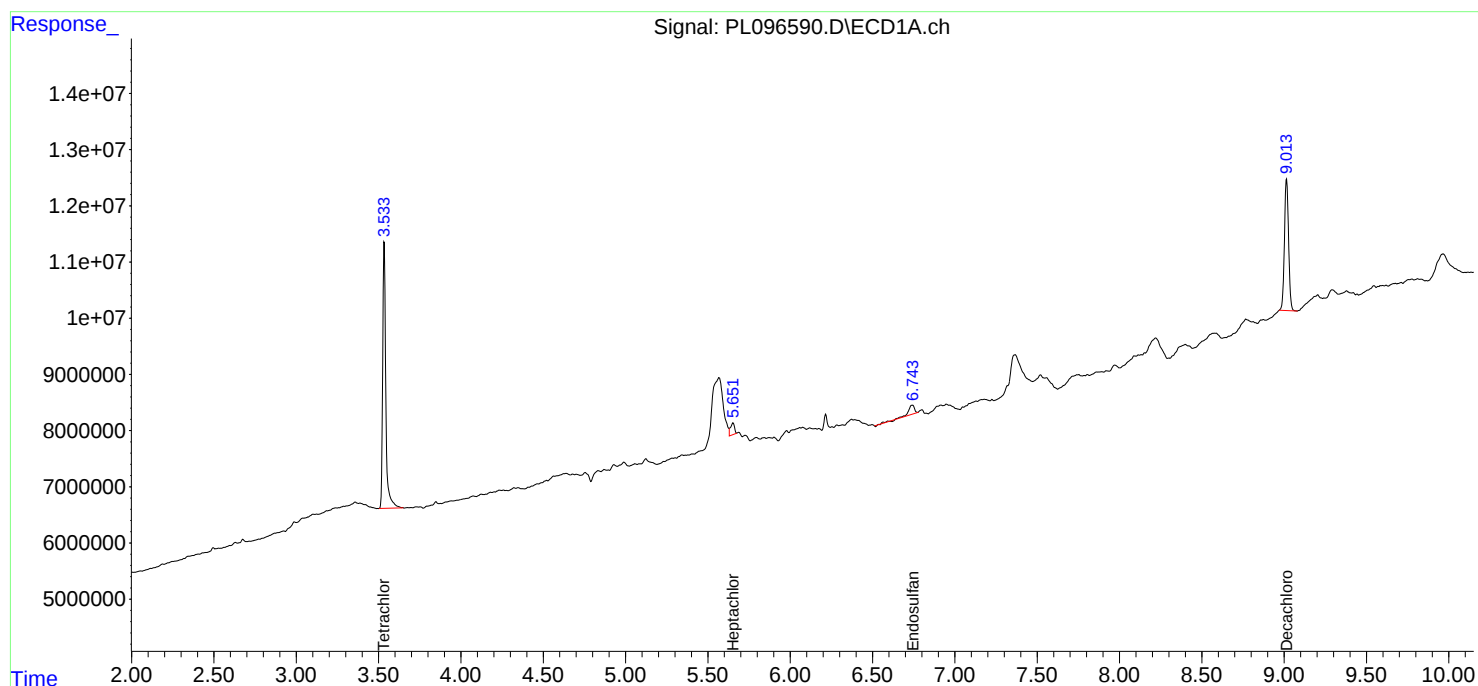


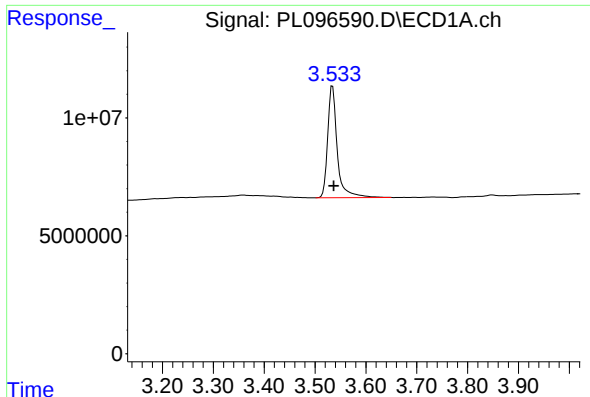

#1 Tetrachloro-m-xylene


R.T.: 3.534 min
Delta R.T.: -0.003 min
Response: 62195326
Conc: 17.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

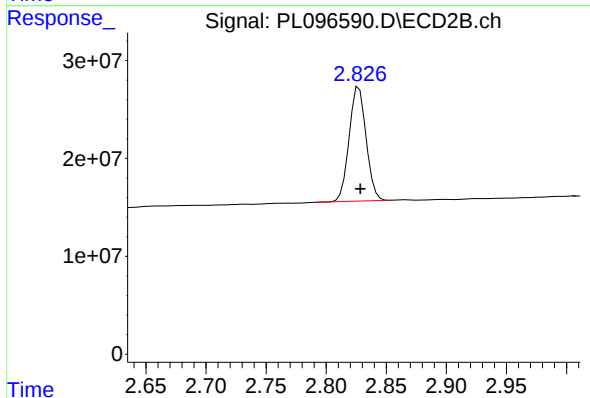


#1 Tetrachloro-m-xylene

R.T.: 2.827 min
Delta R.T.: 0.000 min
Response: 115084714
Conc: 19.94 ng/ml

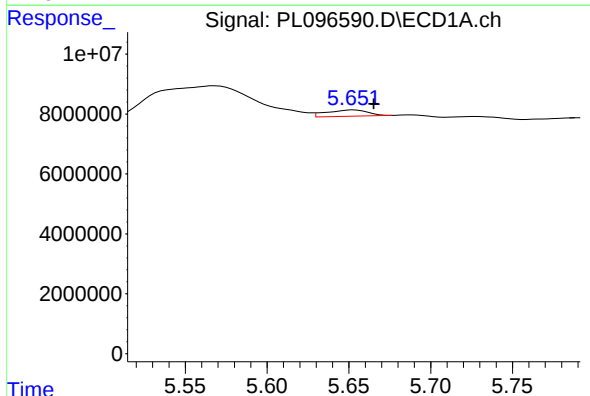


#8 Heptachlor epoxide

R.T.: 5.653 min
Delta R.T.: -0.012 min
Response: 3656879
Conc: 0.88 ng/ml

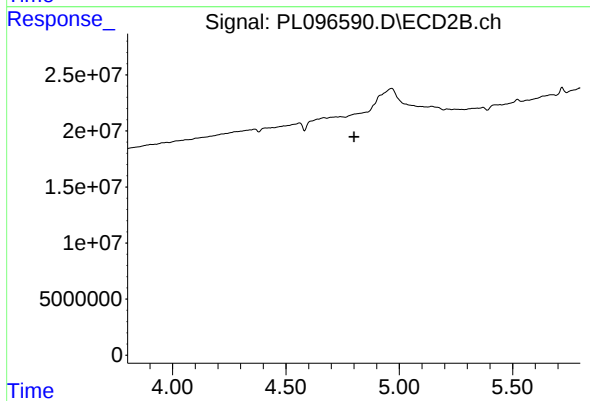

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.800 min
Response: 0
Conc: N.D.

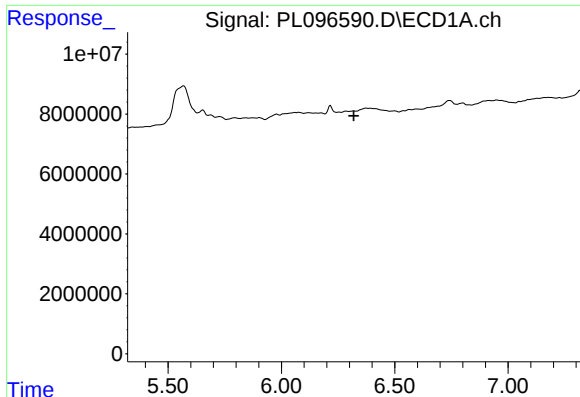

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

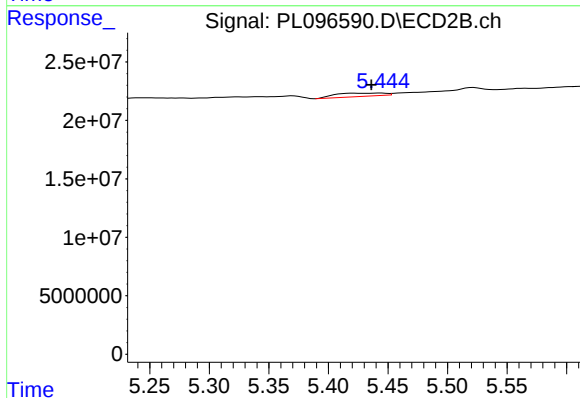


#13 Dieldrin

R.T.: 5.445 min
Delta R.T.: 0.009 min
Response: 8138491
Conc: 1.19 ng/ml

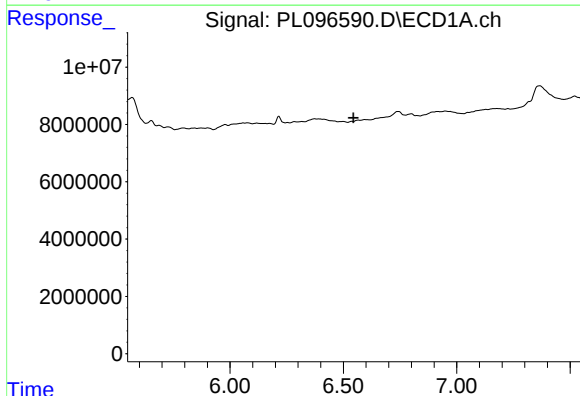


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.545 min
Response: 0
Conc: N.D.

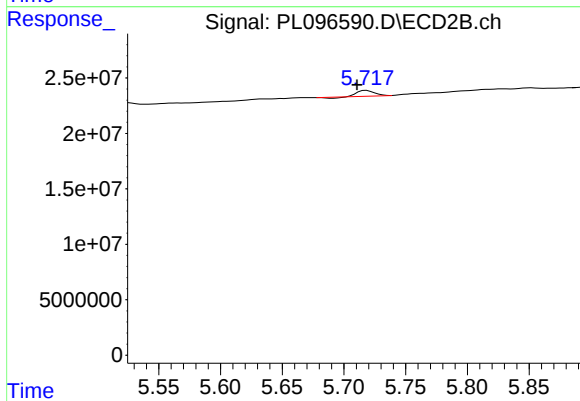

#14 Endrin


R.T.: 5.718 min
Delta R.T.: 0.008 min
Response: 4667288
Conc: 0.77 ng/ml

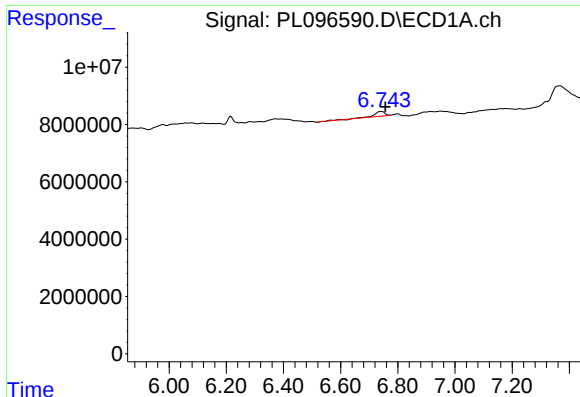

#15 Endosulfan II


R.T.: 6.744 min
Delta R.T.: -0.013 min
Response: 3947114
Conc: 1.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

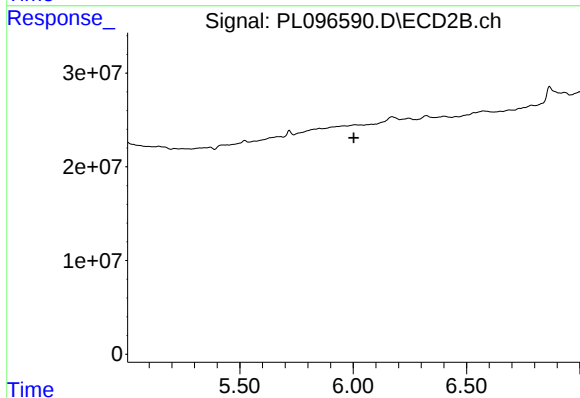


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.003 min
Response: 0
Conc: N.D.

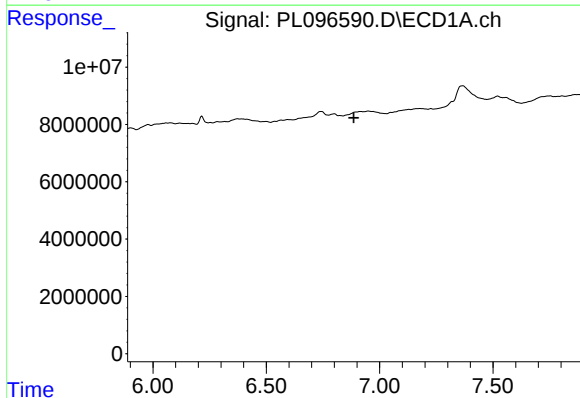


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.886 min
Response: 0
Conc: N.D.

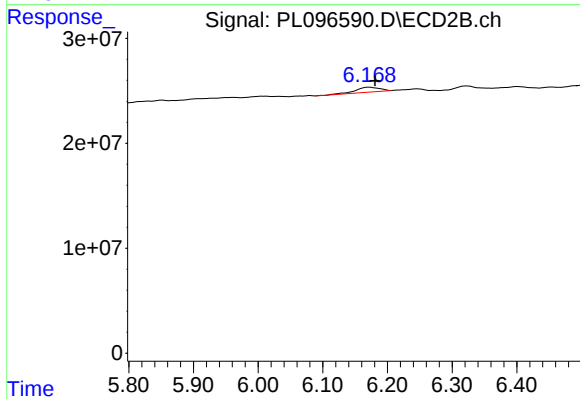

#18 Endrin aldehyde


R.T.: 6.171 min
Delta R.T.: -0.010 min
Response: 11984715
Conc: 2.69 ng/ml

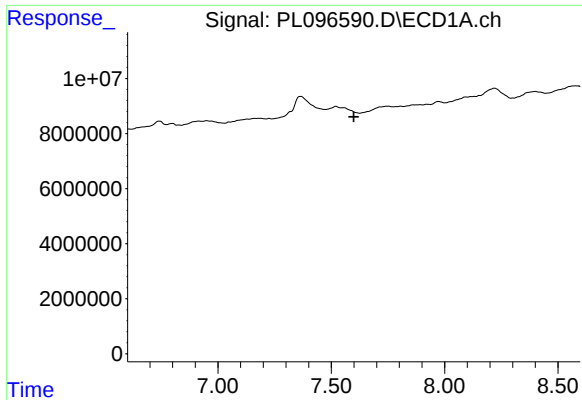

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.599 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

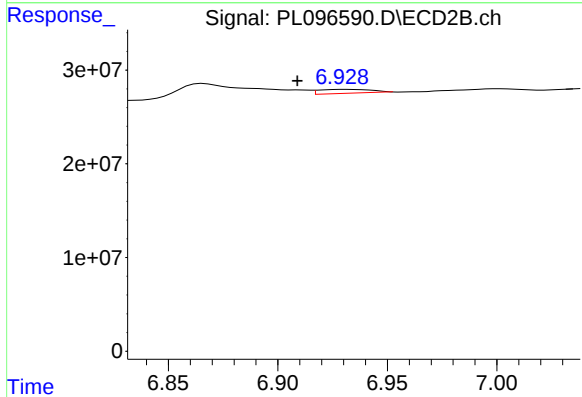


#21 Endrin ketone

R.T.: 6.930 min
Delta R.T.: 0.021 min
Response: 8265419
Conc: 1.32 ng/ml

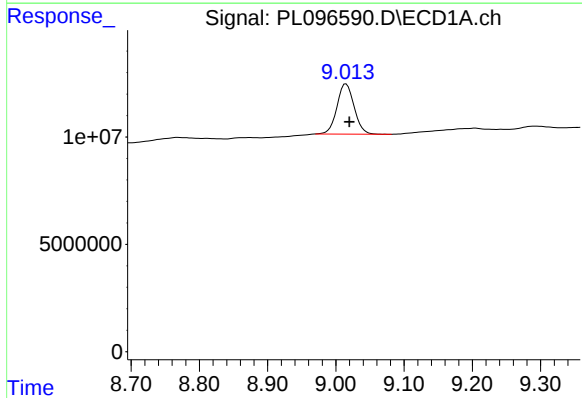

#28 Decachlorobiphenyl

R.T.: 9.015 min
Delta R.T.: -0.005 min
Response: 40920137
Conc: 14.55 ng/ml

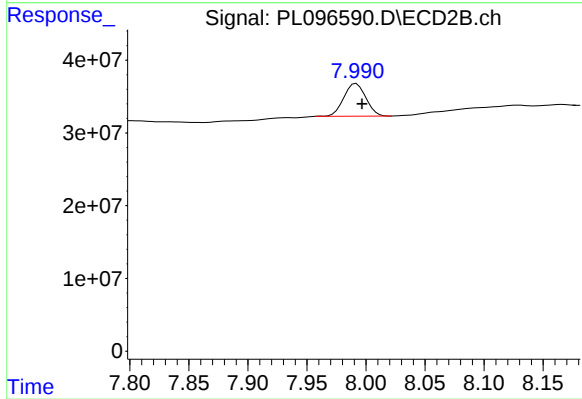

#28 Decachlorobiphenyl

R.T.: 7.992 min
Delta R.T.: -0.005 min
Response: 58449832
Conc: 11.72 ng/ml