

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072619\
 Data File : PL050799.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jul 2019 10:55
 Operator : SM\AJ
 Sample : K3990-08
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-4-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 22:44:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.319	3.928	216.9E6	56427659	21.589	19.777
28)	SA Decachlor...	7.977	8.956	204.3E6	53363658	20.173	18.870
Target Compounds							
6)	B beta-BHC	0.000	4.800f	0	3000261	N.D.	1.735 #
7)	B delta-BHC	0.000	4.982	0	5998052	N.D.	1.551 #
8)	B Heptachlo...	0.000	5.804	0	9066069	N.D.	2.370 #
9)	A Endosulfan I	5.339f	0.000	1767853	0	0.122	N.D. #
10)	B gamma-Chl...	5.198	0.000	836264	0	0.053	N.D. #
11)	B alpha-Chl...	5.271	0.000	4169715	0	0.273	N.D. #
25)	Chlordane-3	5.198	0.000	836264	0	0.597	N.D. #
26)	Chlordane-4	5.271	0.000	4169715	0	3.161	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072619\
Data File : PL050799.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jul 2019 10:55
Operator : SM\AJ
Sample : K3990-08
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-4-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 22:44:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

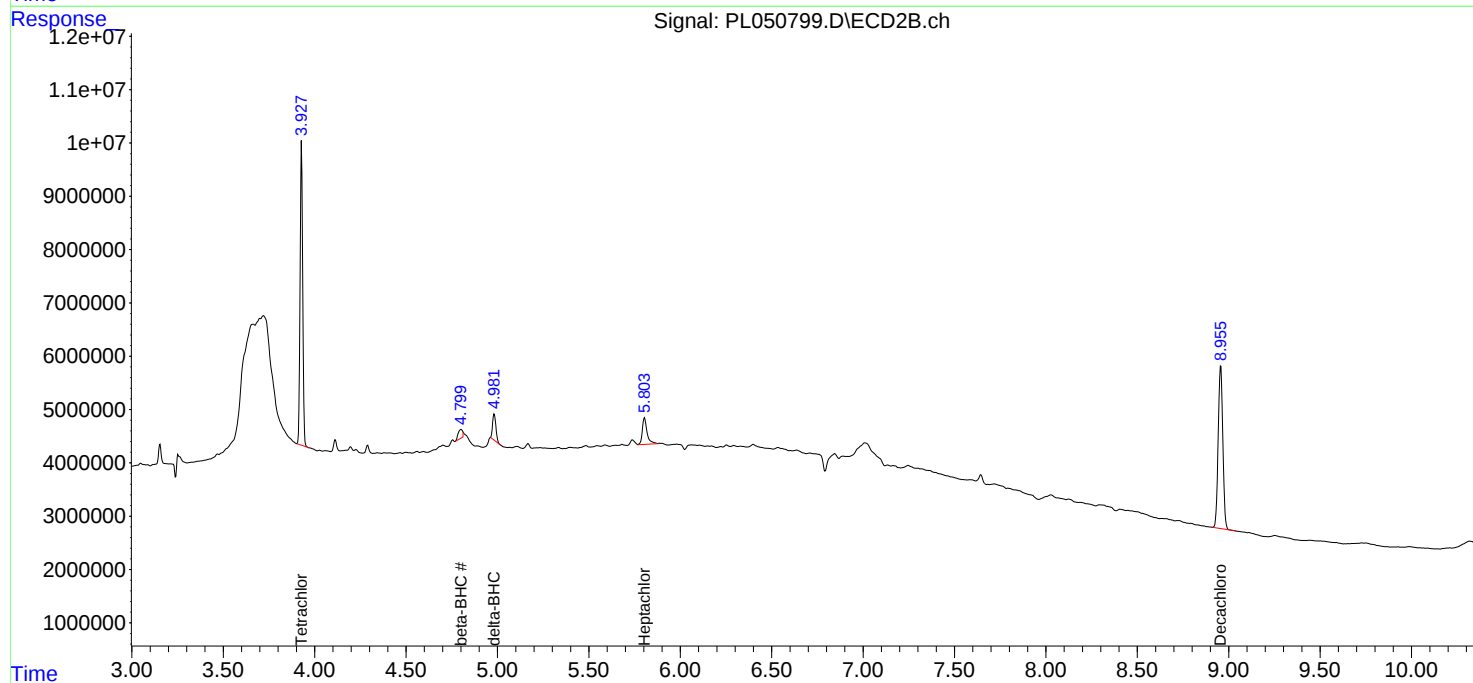


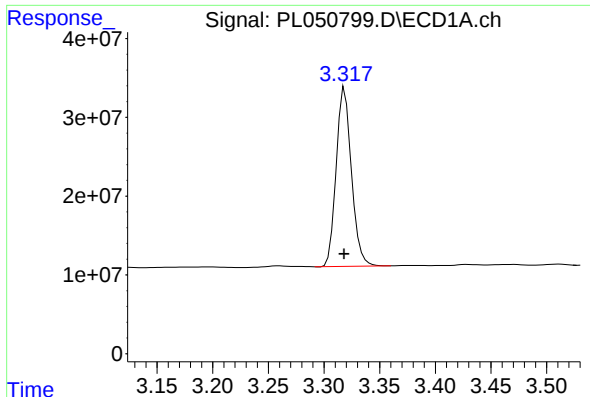

#1 Tetrachloro-m-xylene


R.T.: 3.319 min
Delta R.T.: 0.000 min
Response: 216918397
Conc: 21.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4-B

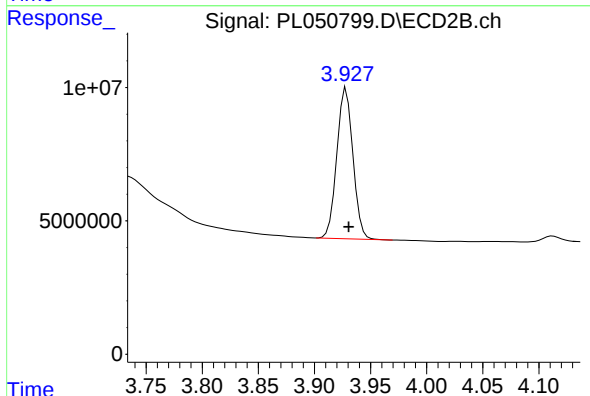


#1 Tetrachloro-m-xylene

R.T.: 3.928 min
Delta R.T.: -0.002 min
Response: 56427659
Conc: 19.78 ng/ml

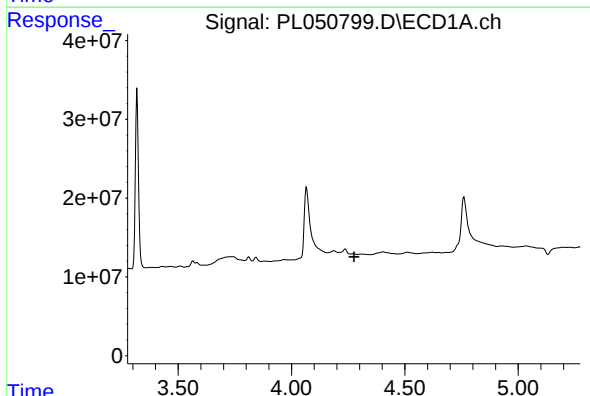


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

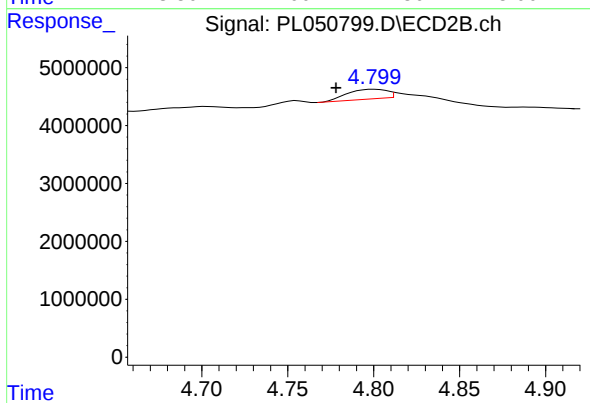

#6 beta-BHC


R.T.: 4.800 min
Delta R.T.: 0.022 min
Response: 3000261
Conc: 1.74 ng/ml

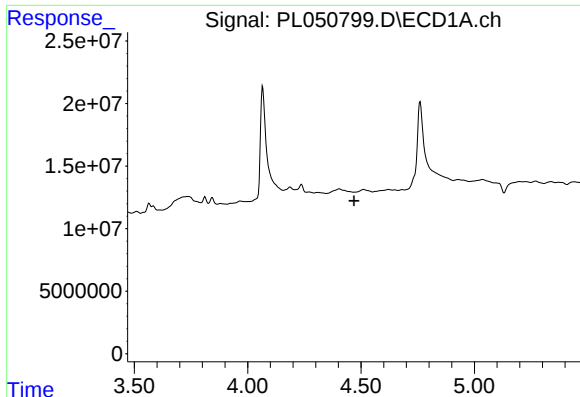

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.469 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-4-B

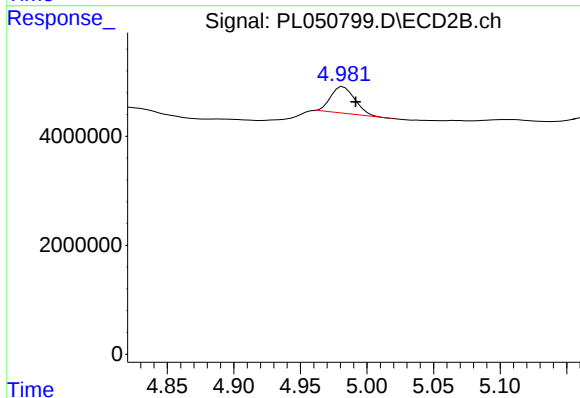


#7 delta-BHC

R.T.: 4.982 min
Delta R.T.: -0.009 min
Response: 5998052
Conc: 1.55 ng/ml

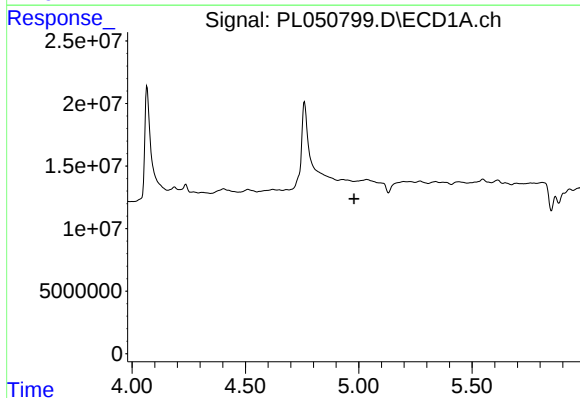


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.979 min
Response: 0
Conc: N.D.

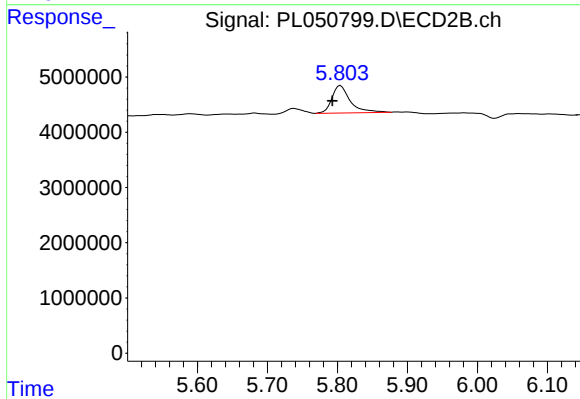

#8 Heptachlor epoxide


R.T.: 5.804 min
Delta R.T.: 0.012 min
Response: 9066069
Conc: 2.37 ng/ml

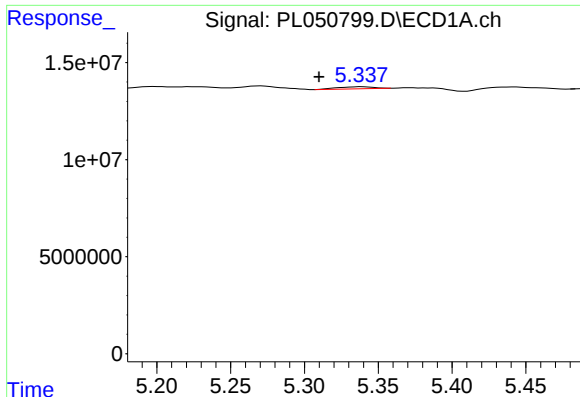

#9 Endosulfan I


R.T.: 5.339 min
Delta R.T.: 0.029 min
Response: 1767853
Conc: 0.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4-B

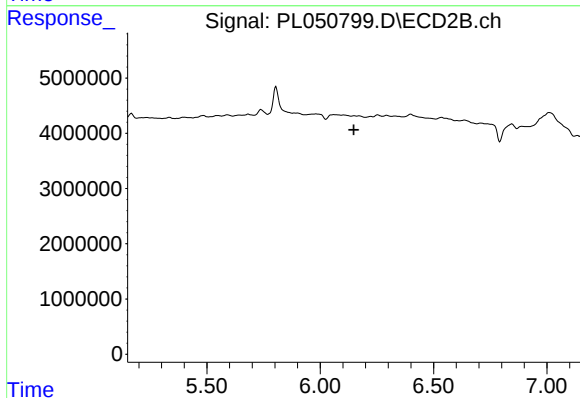


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.148 min
Response: 0
Conc: N.D.

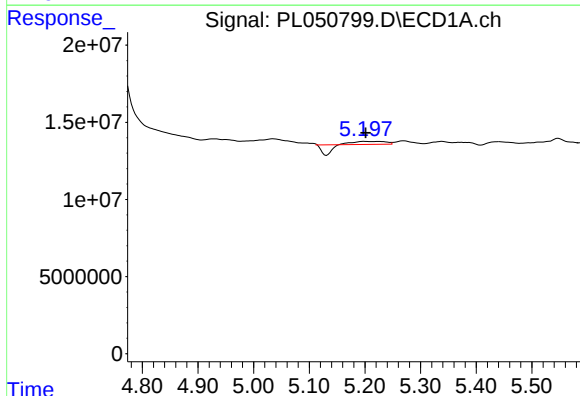


#10 gamma-Chlordane

R.T.: 5.198 min
Delta R.T.: -0.003 min
Response: 836264
Conc: 0.05 ng/ml

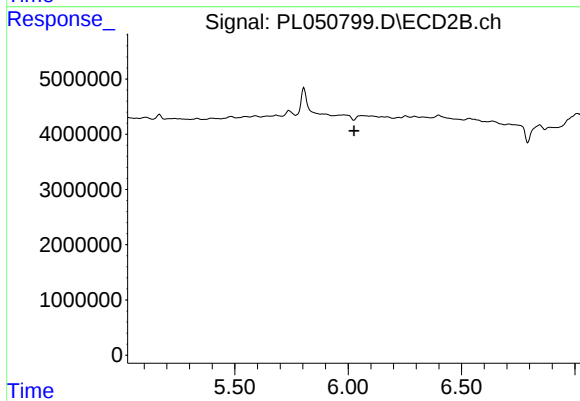

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.026 min
Response: 0
Conc: N.D.

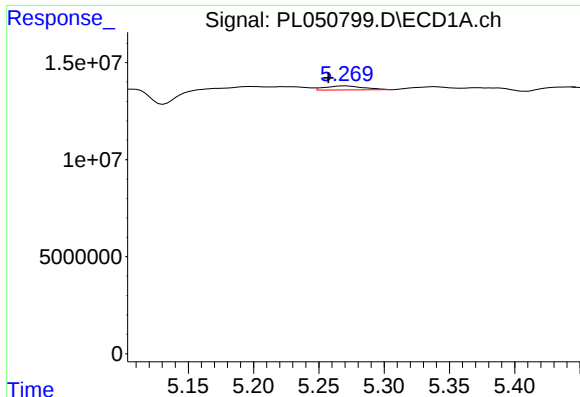

#11 alpha-Chlordane


R.T.: 5.271 min
Delta R.T.: 0.013 min
Response: 4169715
Conc: 0.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4-B

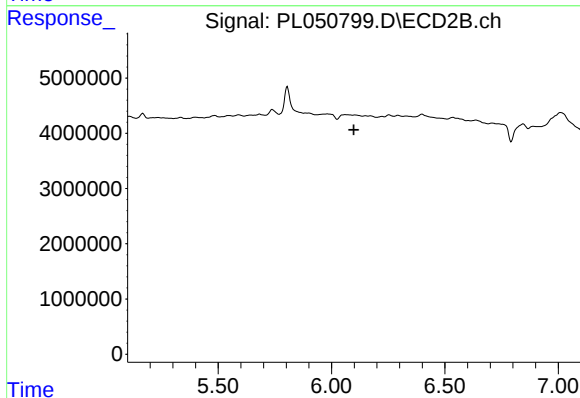


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

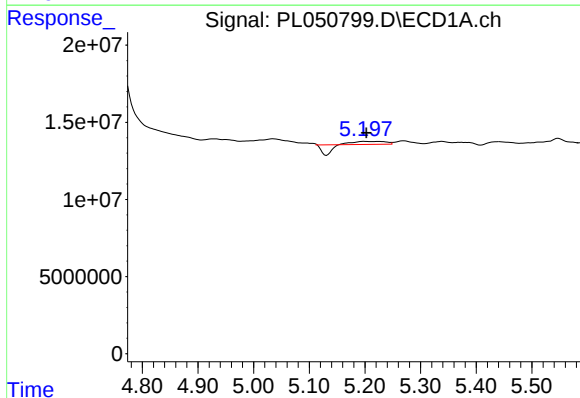


#25 Chlordane-3

R.T.: 5.198 min
Delta R.T.: -0.004 min
Response: 836264
Conc: 0.60 ng/ml

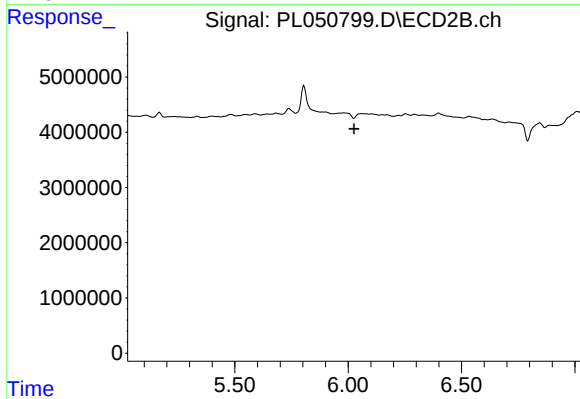

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.027 min
Response: 0
Conc: N.D.

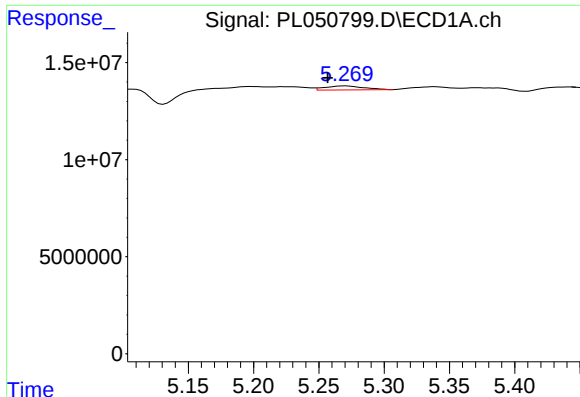

#26 Chlordane-4


R.T.: 5.271 min
Delta R.T.: 0.014 min
Response: 4169715
Conc: 3.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4-B

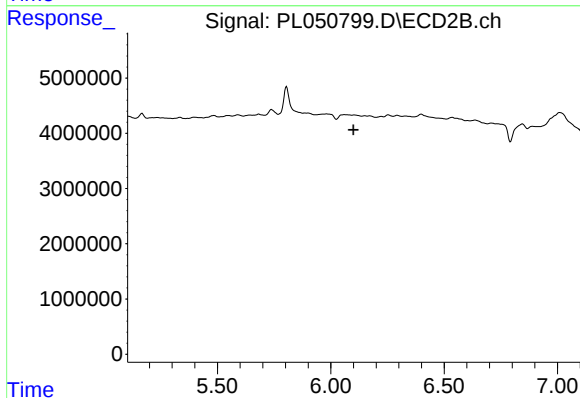


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 6.100 min
Response: 0
Conc: N.D.

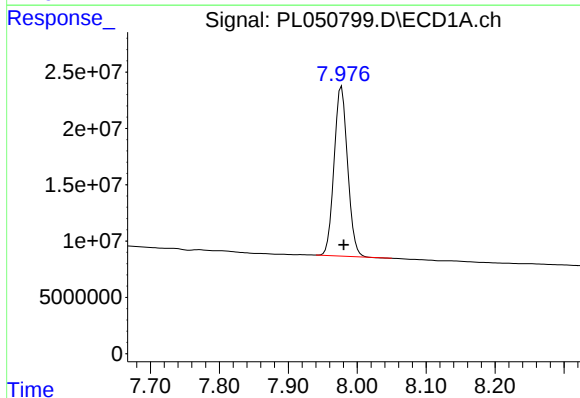

#28 Decachlorobiphenyl

R.T.: 7.977 min
Delta R.T.: -0.003 min
Response: 204256499
Conc: 20.17 ng/ml

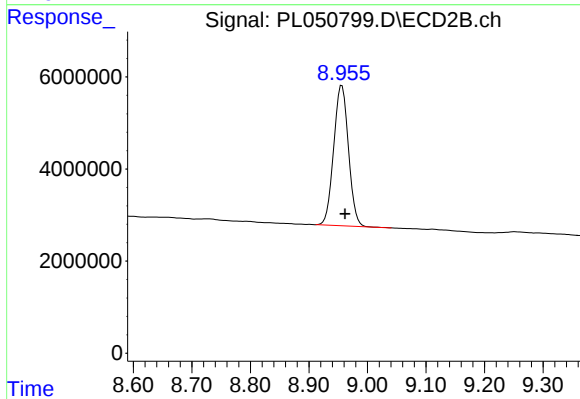

#28 Decachlorobiphenyl

R.T.: 8.956 min
Delta R.T.: -0.005 min
Response: 53363658
Conc: 18.87 ng/ml