

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072619\
 Data File : PL050801.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jul 2019 11:25
 Operator : SM\AJ
 Sample : K3990-10
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-5-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 22:45:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.319	3.928	188.8E6	49939229	18.794	17.503
28)	SA Decachlor...	7.977	8.957	173.0E6	45377428	17.081	16.046
Target Compounds							
6)	B beta-BHC	0.000	4.803f	0	2014129	N.D.	1.165 #
8)	B Heptachlo...	0.000	5.804	0	6271228	N.D.	1.640 #
9)	A Endosulfan I	5.338f	0.000	3752497	0	0.258	N.D. #
11)	B alpha-Chl...	5.266	0.000	45564487	0	2.987	N.D. #
15)	B Endosulfa...	0.000	6.847	0	11725438	N.D.	3.688 #
26)	Chlordane-4	5.266	0.000	45564487	0	34.545	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072619\
Data File : PL050801.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jul 2019 11:25
Operator : SM\AJ
Sample : K3990-10
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-5-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 22:45:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

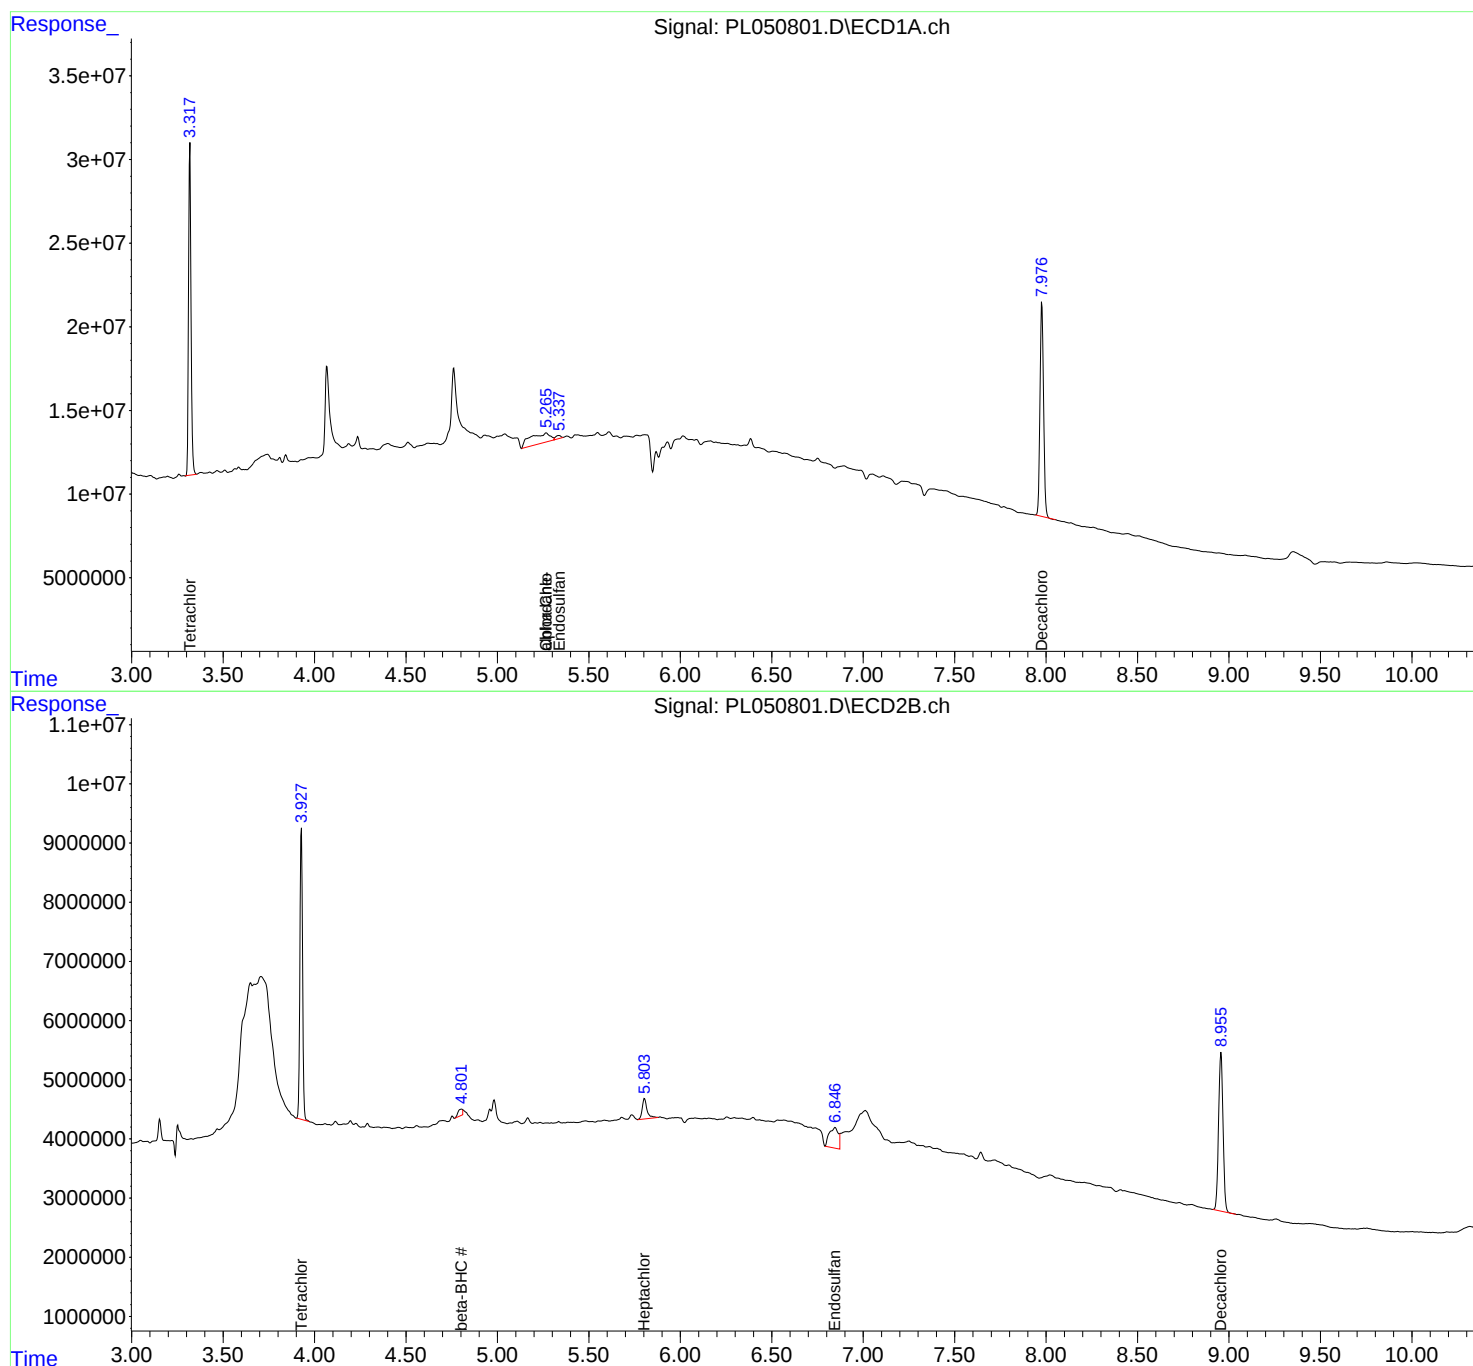


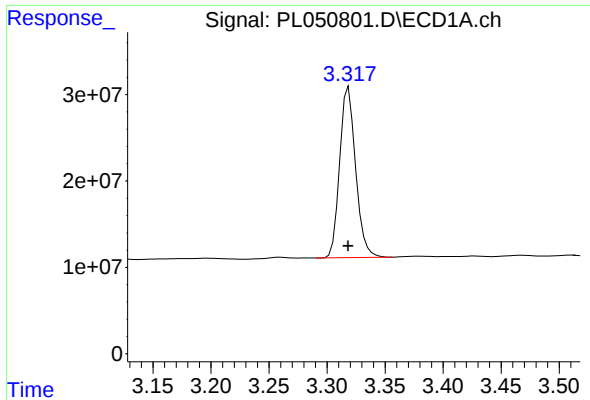

#1 Tetrachloro-m-xylene


R.T.: 3.319 min
Delta R.T.: 0.000 min
Response: 188838424
Conc: 18.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-5-B

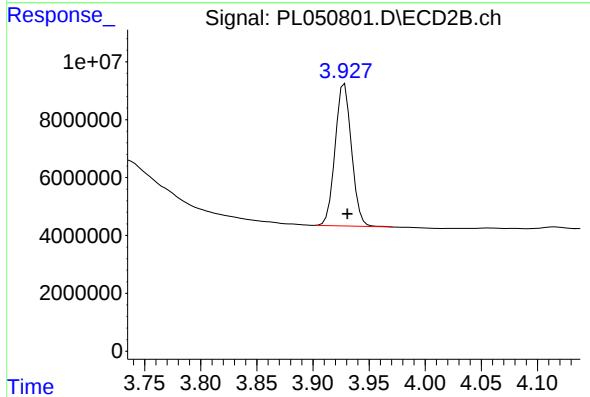


#1 Tetrachloro-m-xylene

R.T.: 3.928 min
Delta R.T.: -0.002 min
Response: 49939229
Conc: 17.50 ng/ml

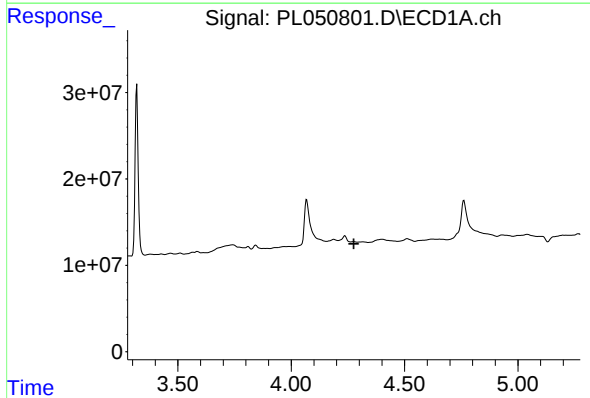


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

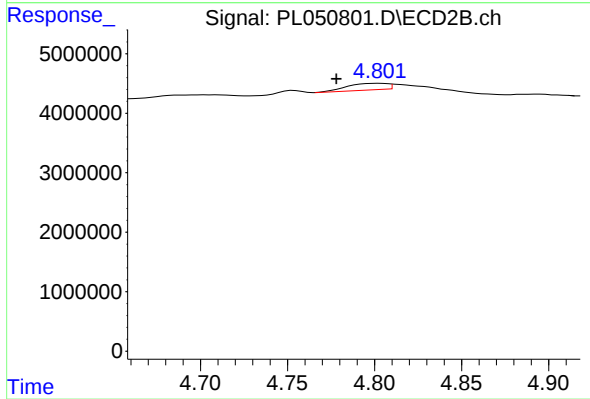

#6 beta-BHC


R.T.: 4.803 min
Delta R.T.: 0.025 min
Response: 2014129
Conc: 1.17 ng/ml

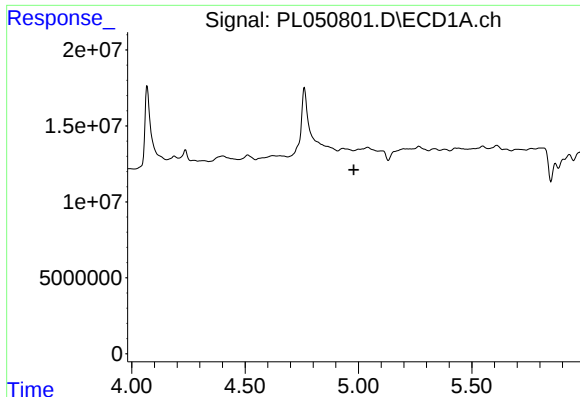

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.979 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-5-B

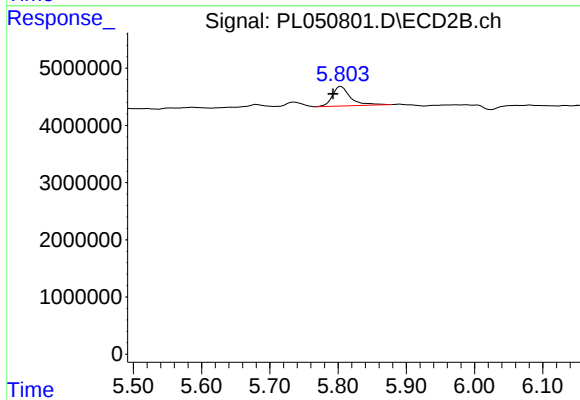


#8 Heptachlor epoxide

R.T.: 5.804 min
Delta R.T.: 0.012 min
Response: 6271228
Conc: 1.64 ng/ml

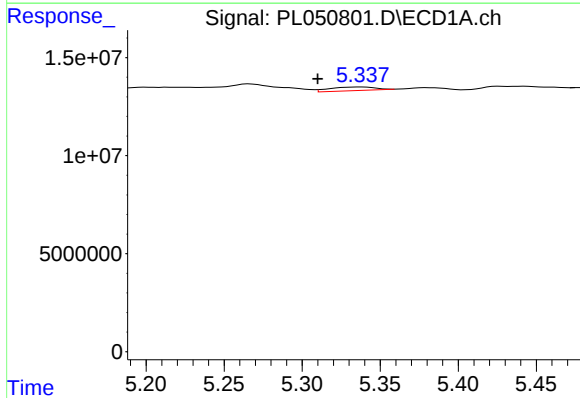


#9 Endosulfan I

R.T.: 5.338 min
Delta R.T.: 0.028 min
Response: 3752497
Conc: 0.26 ng/ml

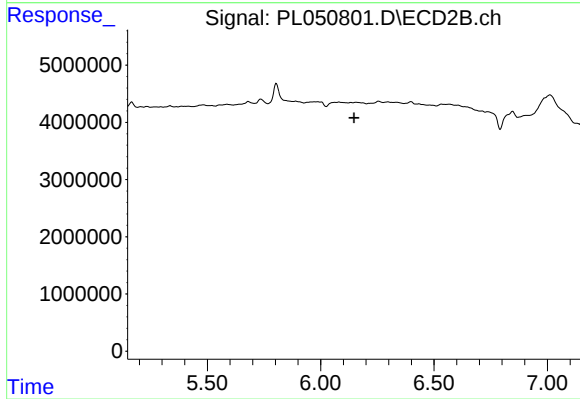

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.148 min
Response: 0
Conc: N.D.

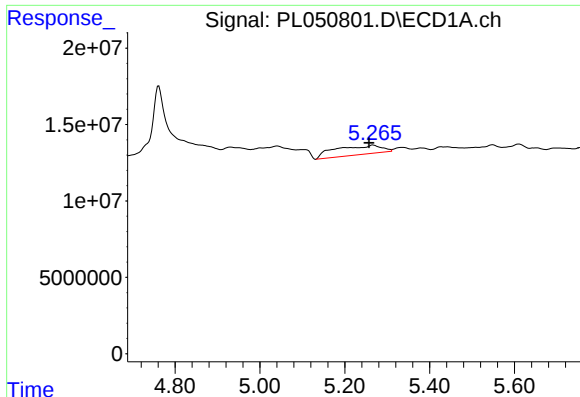

#11 alpha-Chlordane


R.T.: 5.266 min
Delta R.T.: 0.009 min
Response: 45564487
Conc: 2.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-5-B

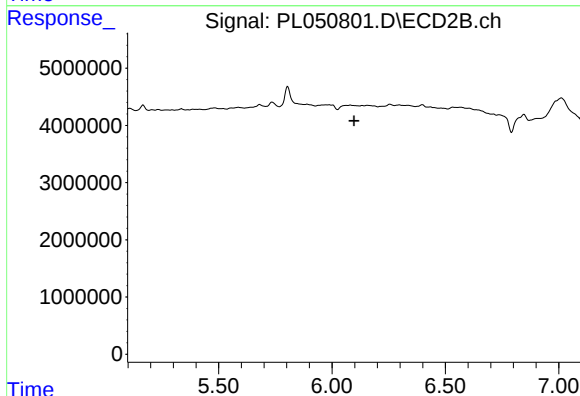


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

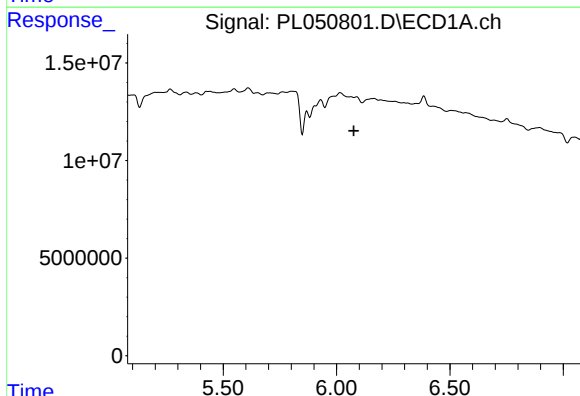


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.076 min
Response: 0
Conc: N.D.

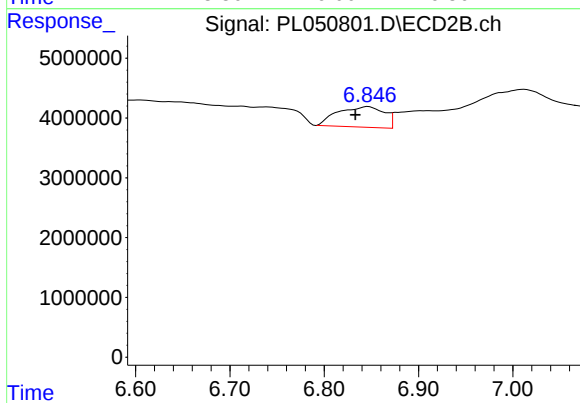

#15 Endosulfan II


R.T.: 6.847 min
Delta R.T.: 0.014 min
Response: 11725438
Conc: 3.69 ng/ml

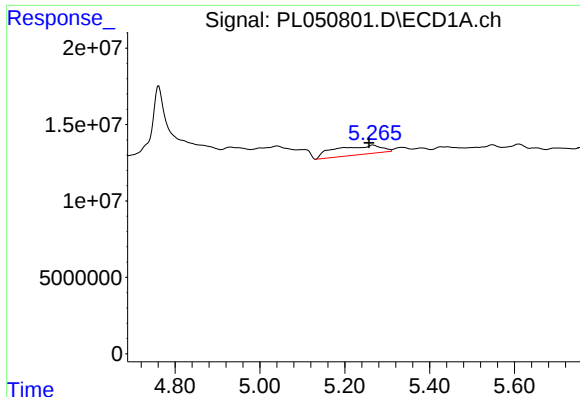

#26 Chlordane-4


R.T.: 5.266 min
Delta R.T.: 0.010 min
Response: 45564487
Conc: 34.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-5-B

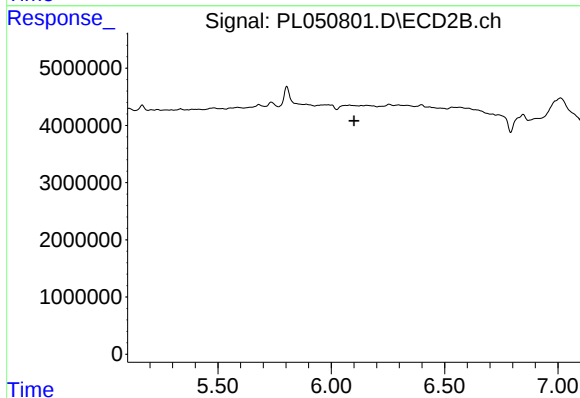


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 6.100 min
Response: 0
Conc: N.D.

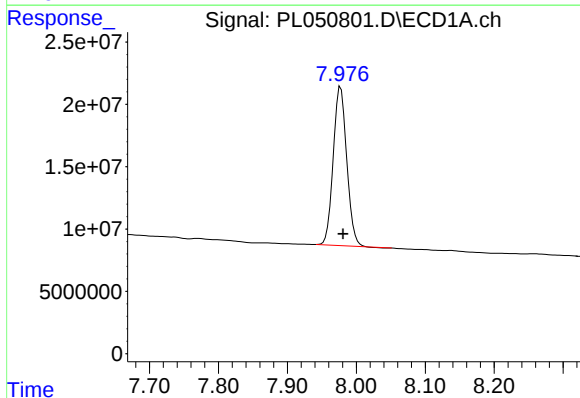

#28 Decachlorobiphenyl

R.T.: 7.977 min
Delta R.T.: -0.003 min
Response: 172955131
Conc: 17.08 ng/ml

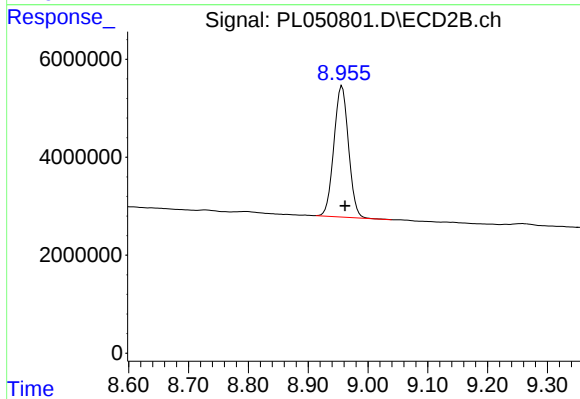

#28 Decachlorobiphenyl

R.T.: 8.957 min
Delta R.T.: -0.005 min
Response: 45377428
Conc: 16.05 ng/ml