

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072619\
 Data File : PL050803.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jul 2019 11:55
 Operator : SM\AJ
 Sample : K3990-01DL 2X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-1-ADL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 22:46:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.319	3.929	95060780	24129976	9.461	8.457
28)	SA Decachlor...	7.977	8.957	68762644	17755589	6.791	6.279
Target Compounds							
7)	B delta-BHC	0.000	4.983	0	3559532	N.D.	0.920 #
8)	B Heptachlo...	0.000	5.804	0	6591171	N.D.	1.723 #
10)	B gamma-Chl...	5.203	0.000	5629276	0	0.357	N.D. #
12)	B 4,4'-DDE	5.423	6.255	257.8E6	59326408	17.203	16.464
13)	MA Dieldrin	5.547	6.400	811.1E6	180.4E6	52.342	50.953
14)	MA Endrin	5.803	0.000	28510417	0	1.937	N.D. #
16)	A 4,4'-DDD	5.933	6.745	29619292	8512065	2.472	3.197 #
17)	MA 4,4'-DDT	6.167	7.041	31042229	6891562	2.506	2.553
25)	Chlordane-3	5.203	0.000	5629276	0	4.022	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072619\
Data File : PL050803.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jul 2019 11:55
Operator : SM\AJ
Sample : K3990-01DL 2X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-1-ADL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 22:46:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

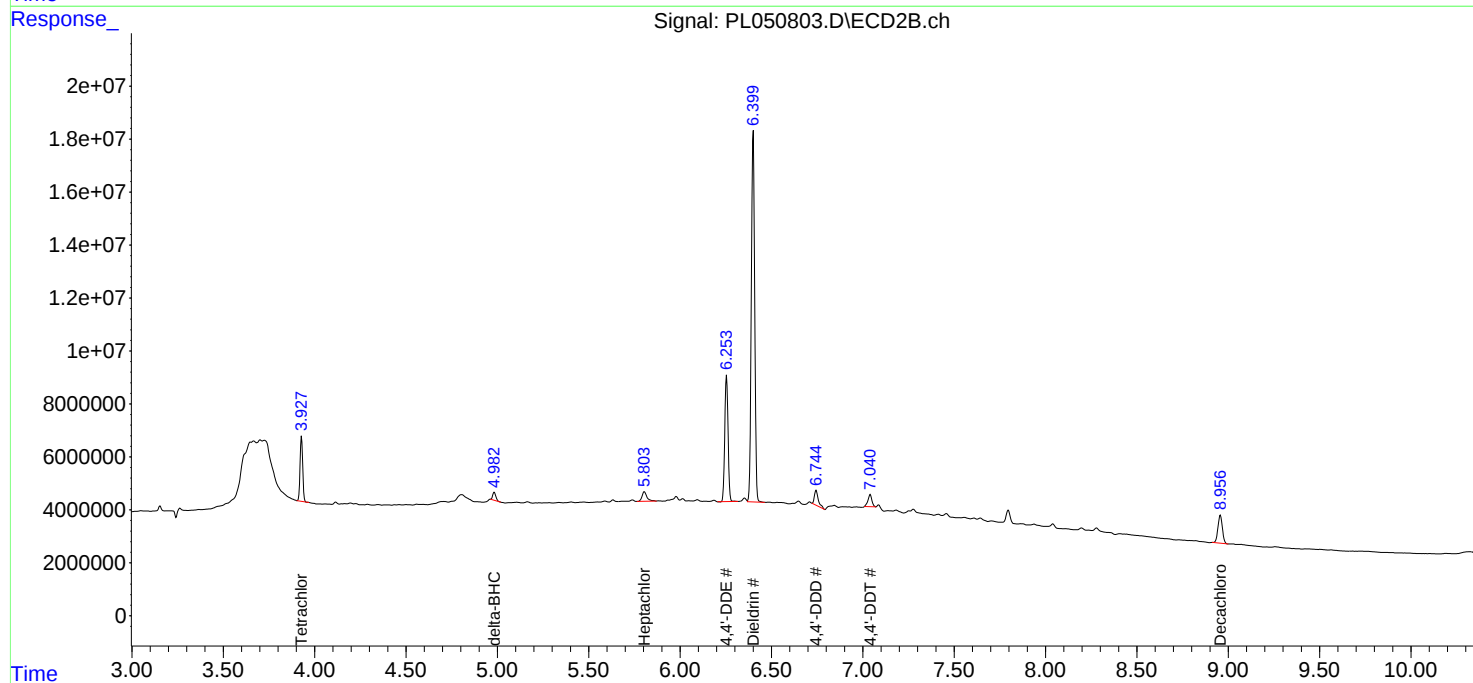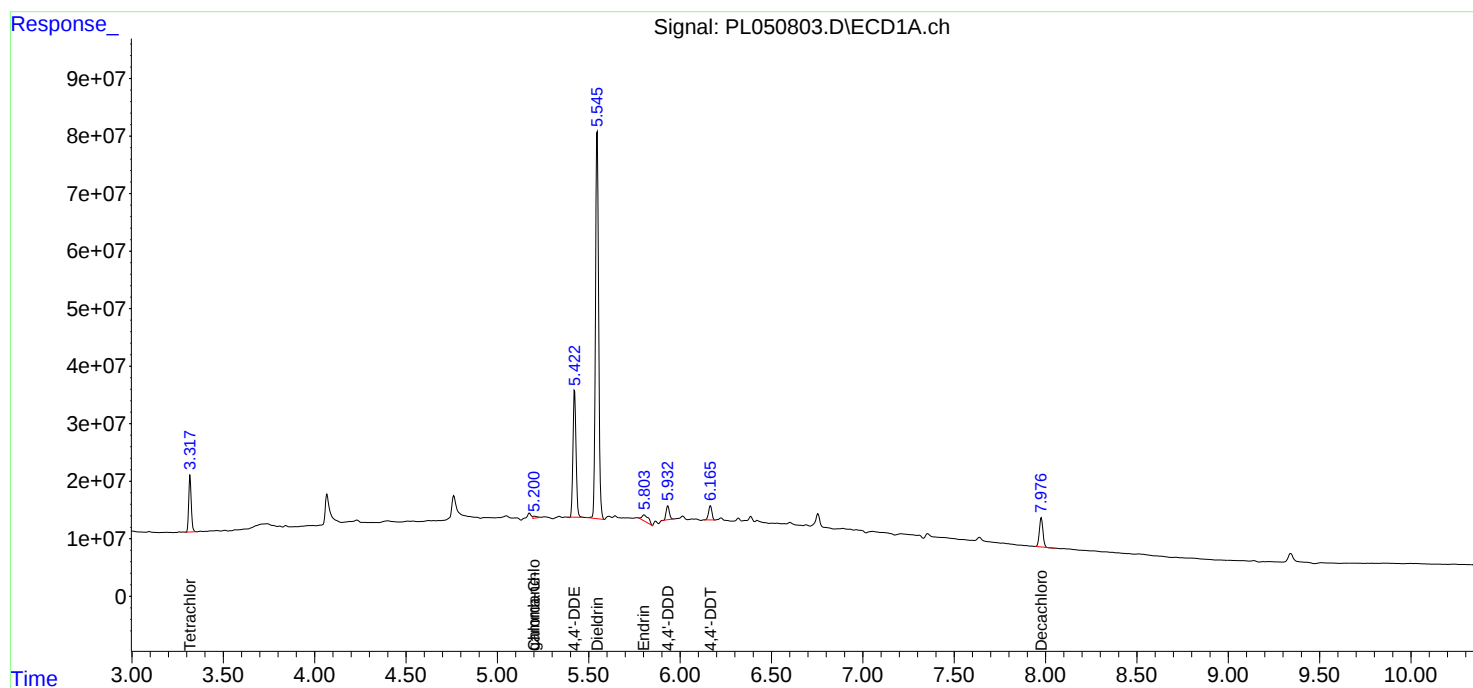


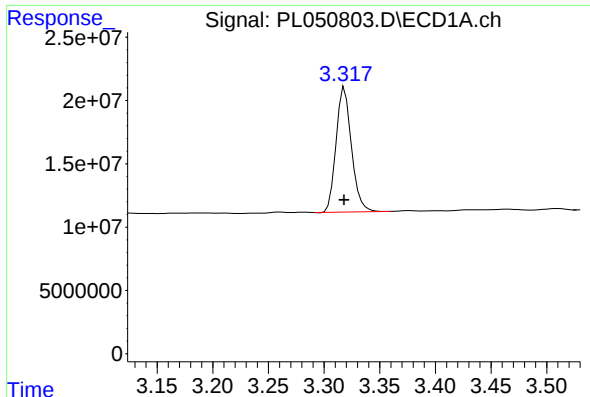

#1 Tetrachloro-m-xylene


R.T.: 3.319 min
Delta R.T.: 0.000 min
Response: 95060780
Conc: 9.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1-ADL

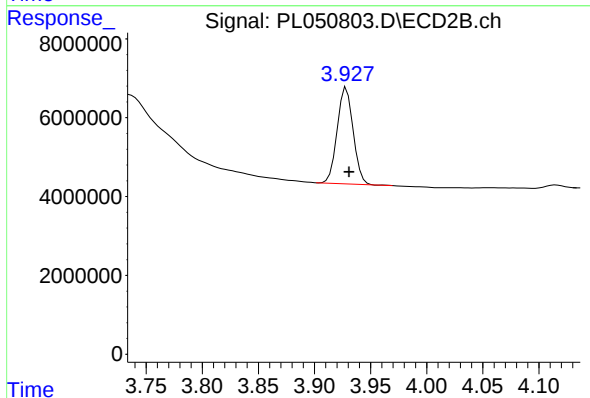


#1 Tetrachloro-m-xylene

R.T.: 3.929 min
Delta R.T.: -0.002 min
Response: 24129976
Conc: 8.46 ng/ml

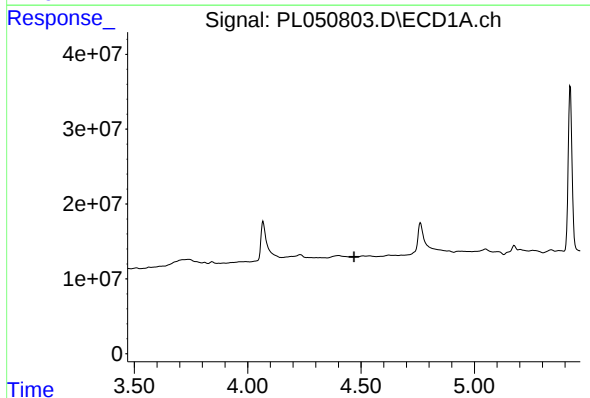


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.469 min
Response: 0
Conc: N.D.

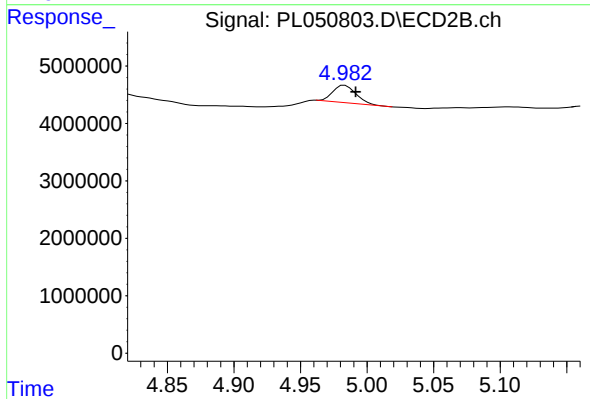

#7 delta-BHC


R.T.: 4.983 min
Delta R.T.: -0.008 min
Response: 3559532
Conc: 0.92 ng/ml

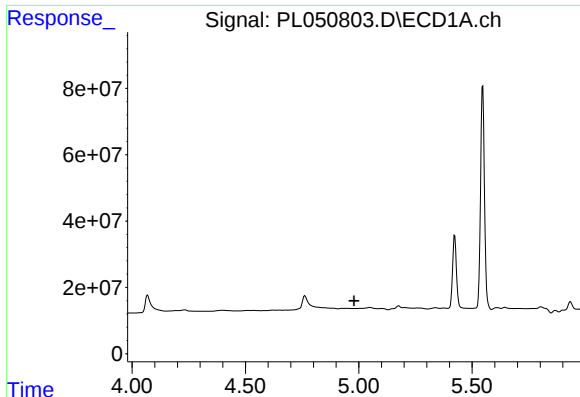

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.979 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-1-ADL

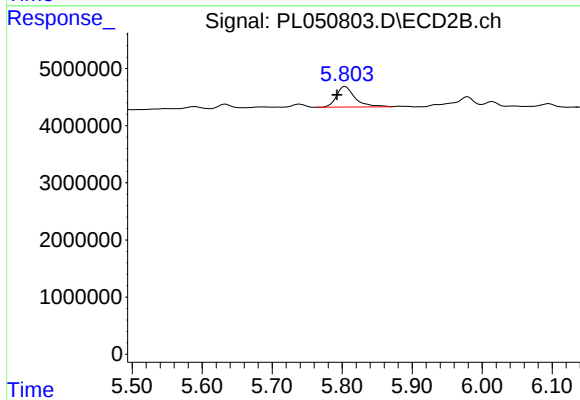


#8 Heptachlor epoxide

R.T.: 5.804 min
Delta R.T.: 0.012 min
Response: 6591171
Conc: 1.72 ng/ml

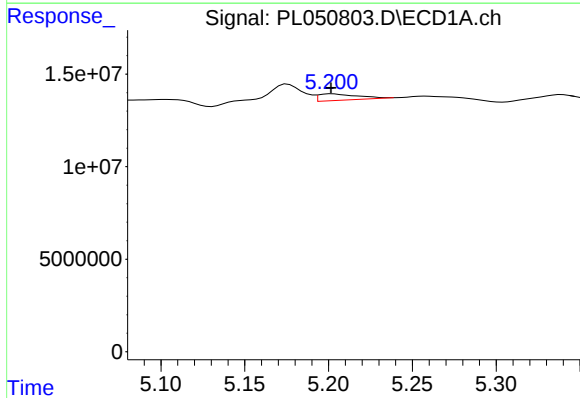


#10 gamma-Chlordane

R.T.: 5.203 min
Delta R.T.: 0.001 min
Response: 5629276
Conc: 0.36 ng/ml

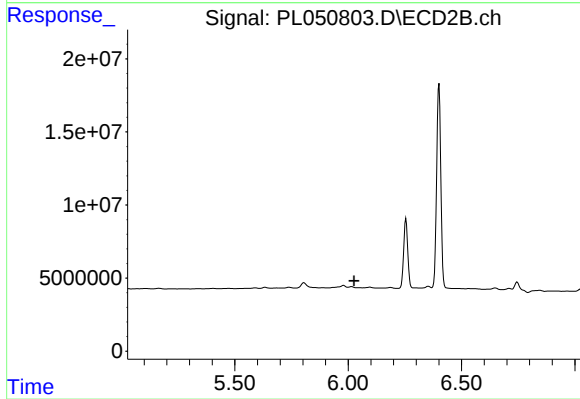

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.026 min
Response: 0
Conc: N.D.

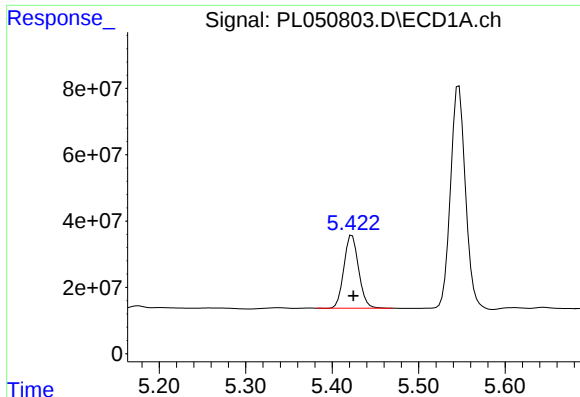

#12 4,4'-DDE


R.T.: 5.423 min
Delta R.T.: -0.002 min
Response: 257799294
Conc: 17.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1-ADL

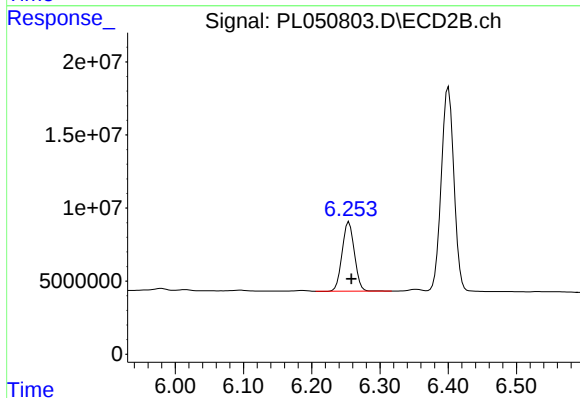


#12 4,4'-DDE

R.T.: 6.255 min
Delta R.T.: -0.004 min
Response: 59326408
Conc: 16.46 ng/ml

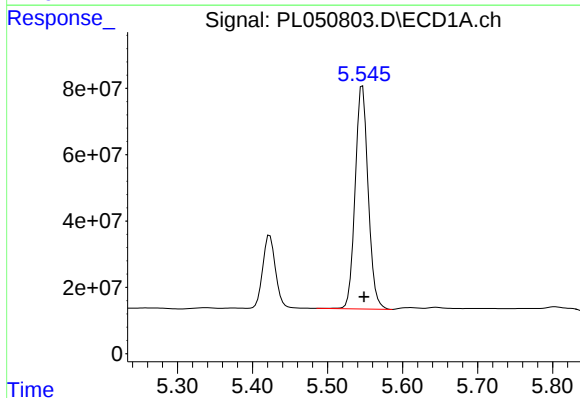


#13 Dieldrin

R.T.: 5.547 min
Delta R.T.: -0.002 min
Response: 811124527
Conc: 52.34 ng/ml

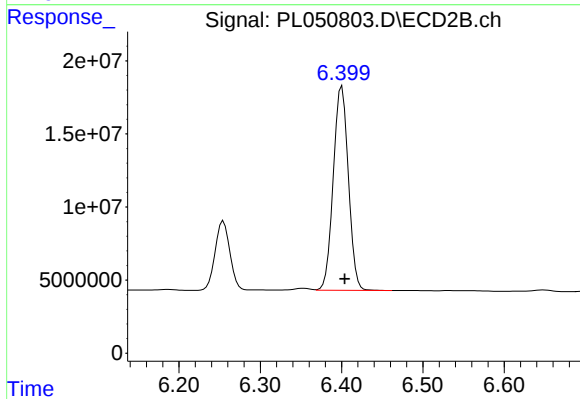

#13 Dieldrin


R.T.: 6.400 min
Delta R.T.: -0.003 min
Response: 180432893
Conc: 50.95 ng/ml

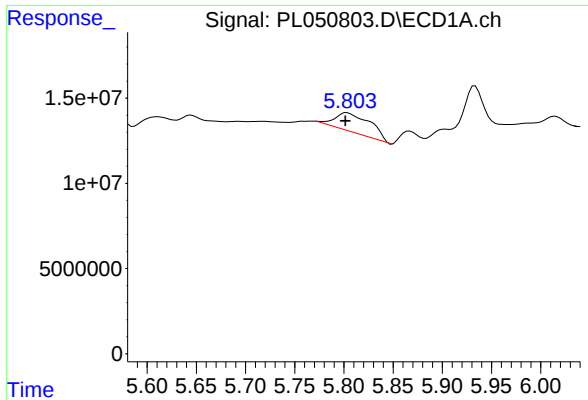

#14 Endrin


R.T.: 5.803 min
Delta R.T.: 0.002 min
Response: 28510417
Conc: 1.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1-ADL

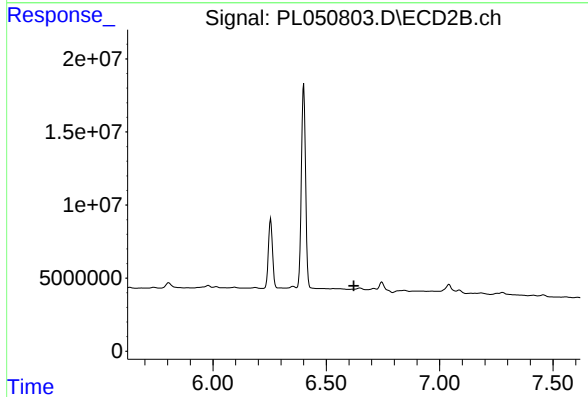


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.621 min
Response: 0
Conc: N.D.

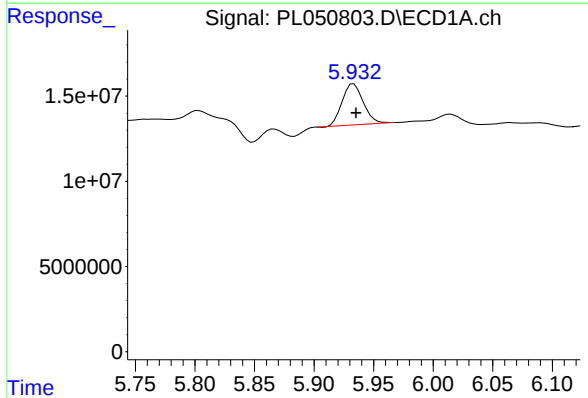


#16 4,4'-DDD

R.T.: 5.933 min
Delta R.T.: -0.002 min
Response: 29619292
Conc: 2.47 ng/ml

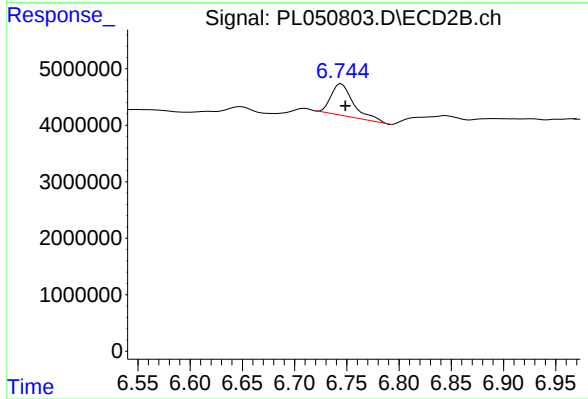

#16 4,4'-DDD


R.T.: 6.745 min
Delta R.T.: -0.004 min
Response: 8512065
Conc: 3.20 ng/ml

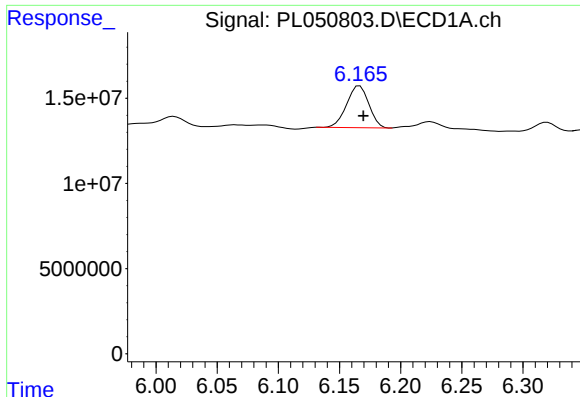

#17 4,4'-DDT


R.T.: 6.167 min
Delta R.T.: -0.003 min
Response: 31042229
Conc: 2.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1-ADL

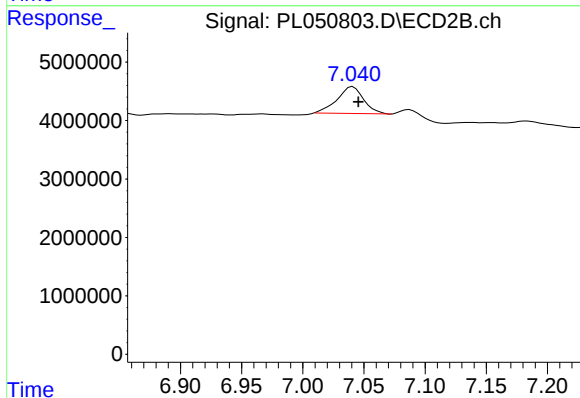


#17 4,4'-DDT

R.T.: 7.041 min
Delta R.T.: -0.005 min
Response: 6891562
Conc: 2.55 ng/ml

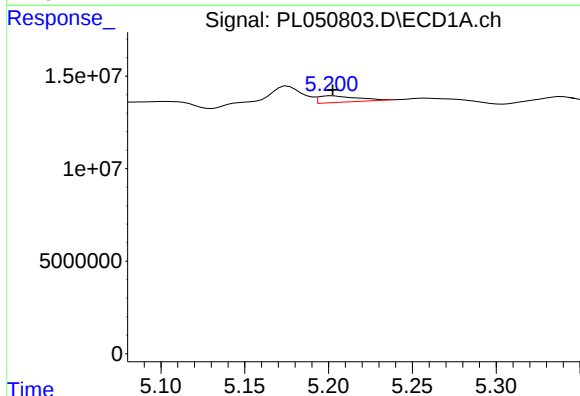


#25 Chlordane-3

R.T.: 5.203 min
Delta R.T.: 0.000 min
Response: 5629276
Conc: 4.02 ng/ml

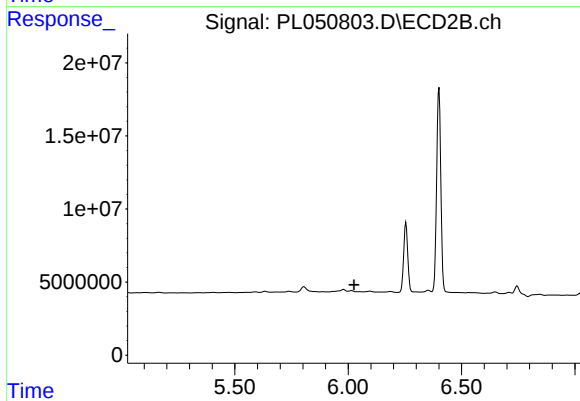

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 6.027 min
Response: 0
Conc: N.D.

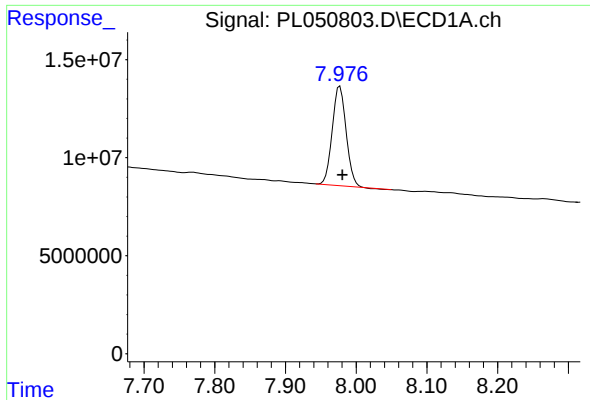

#28 Decachlorobiphenyl

R.T.: 7.977 min
Delta R.T.: -0.004 min
Response: 68762644
Conc: 6.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1-ADL

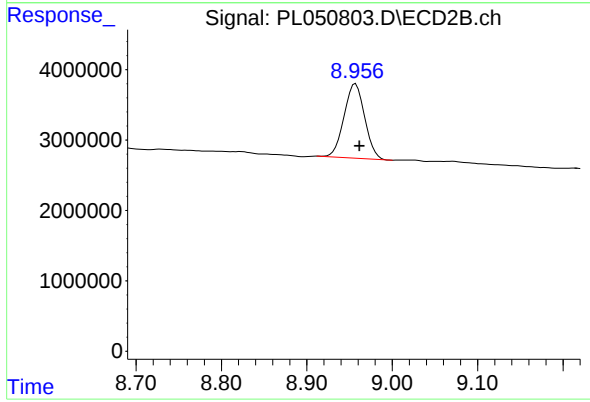

#28 Decachlorobiphenyl

R.T.: 8.957 min
Delta R.T.: -0.004 min
Response: 17755589
Conc: 6.28 ng/ml