

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072619\
 Data File : PL050826.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jul 2019 19:25
 Operator : SM\AJ
 Sample : PEM
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PEM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 22:52:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.319	3.929	210.7E6	55133794	20.968	19.323
28)	SA Decachlor...	7.978	8.957	227.7E6	61342187	22.484	21.692
Target Compounds							
2)	A alpha-BHC	3.746	4.317	164.8E6	35221987	9.832	8.537
3)	MA gamma-BHC...	4.021	4.600	139.0E6	34751299	9.039	8.972
4)	MA Heptachlor	4.276f	0.000	71631035	0	4.366	N.D. #
6)	B beta-BHC	4.276	4.777	71631035	19244539	10.926	11.131
8)	B Heptachlo...	0.000	5.803	0	8067538	N.D.	2.109 #
14)	MA Endrin	5.800	6.619	788.5E6	156.4E6	53.562	50.433
17)	MA 4,4'-DDT	6.168	7.043	1331.9E6	302.0E6	107.537	111.882
20)	A Methoxychlor	6.713	7.504	1557.8E6	394.3E6	249.689	268.745



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072619\
Data File : PL050826.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jul 2019 19:25
Operator : SM\AJ
Sample : PEM
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PEM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 22:52:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

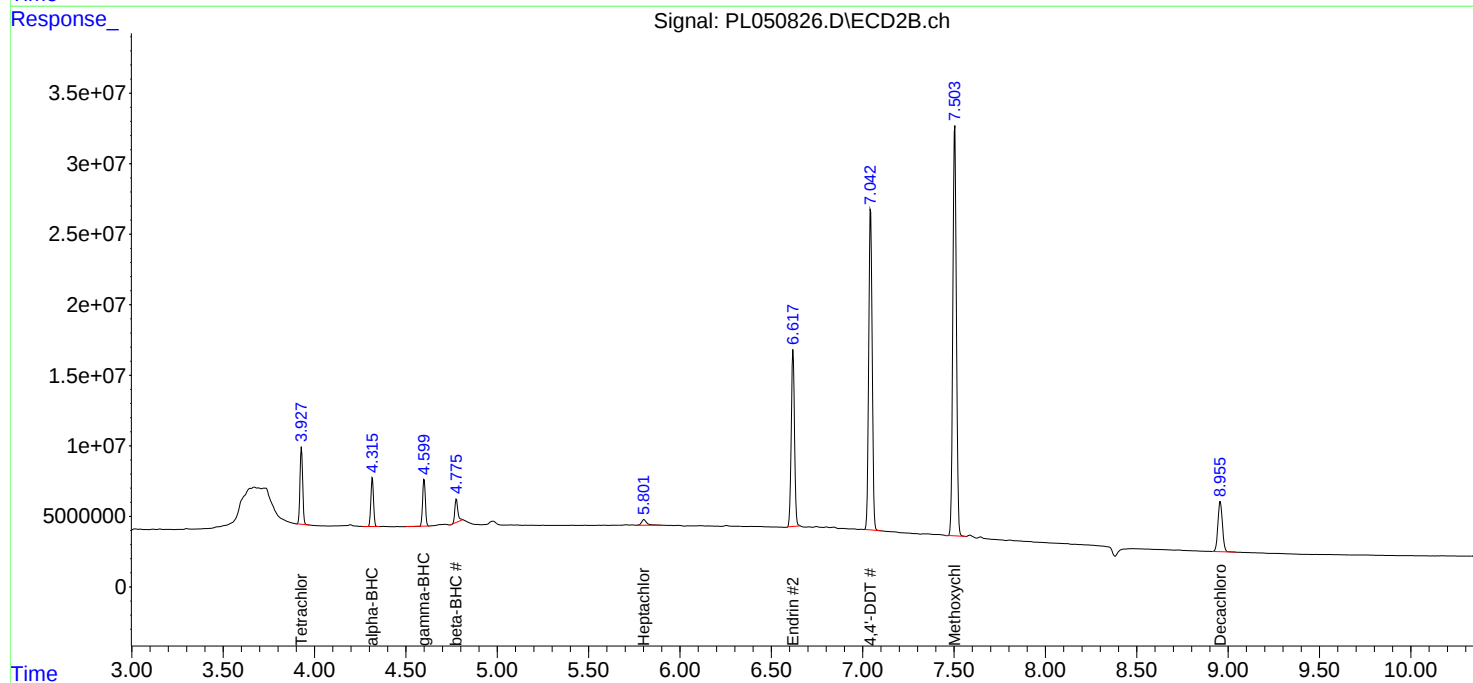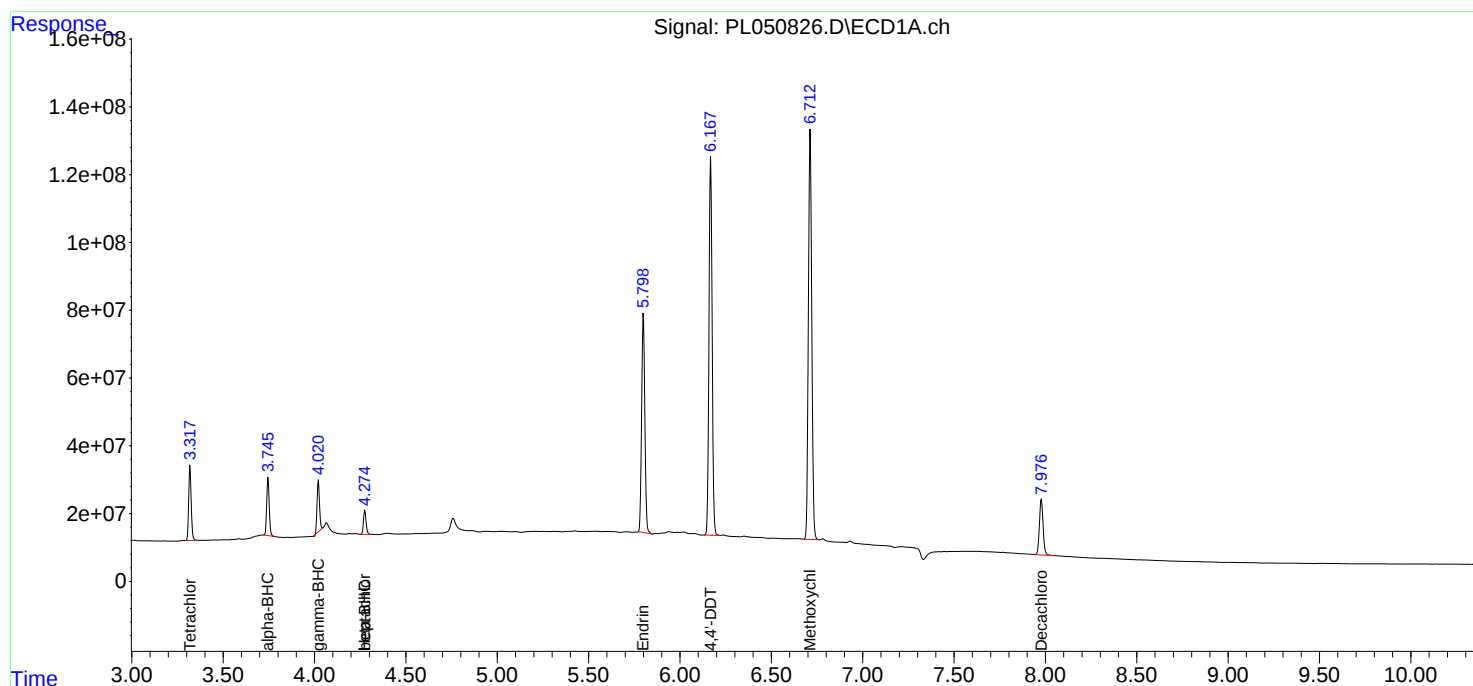


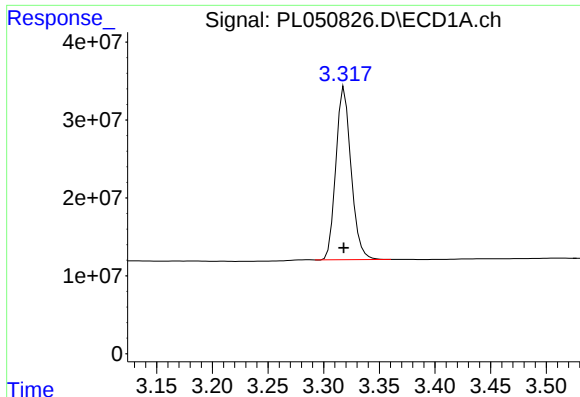

#1 Tetrachloro-m-xylene


R.T.: 3.319 min
Delta R.T.: 0.000 min
Response: 210684495
Conc: 20.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
PEM

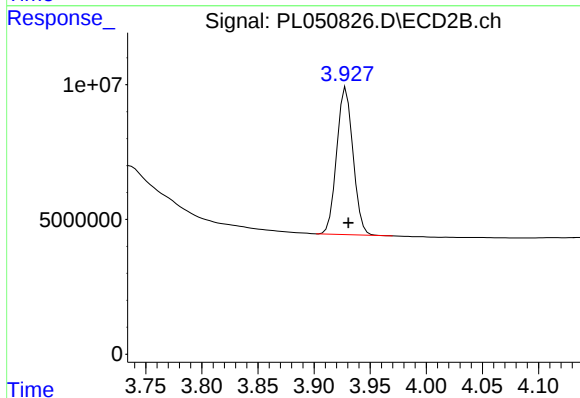


#1 Tetrachloro-m-xylene

R.T.: 3.929 min
Delta R.T.: -0.002 min
Response: 55133794
Conc: 19.32 ng/ml

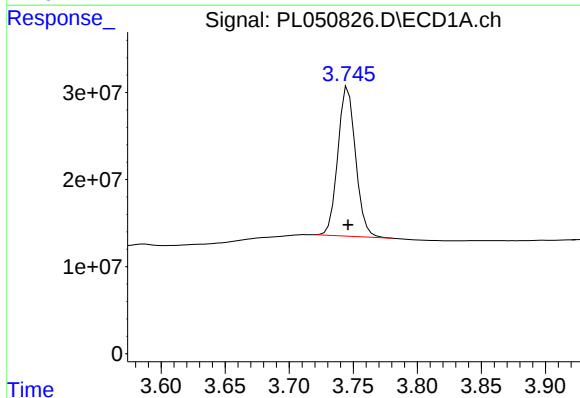


#2 alpha-BHC

R.T.: 3.746 min
Delta R.T.: 0.000 min
Response: 164766991
Conc: 9.83 ng/ml

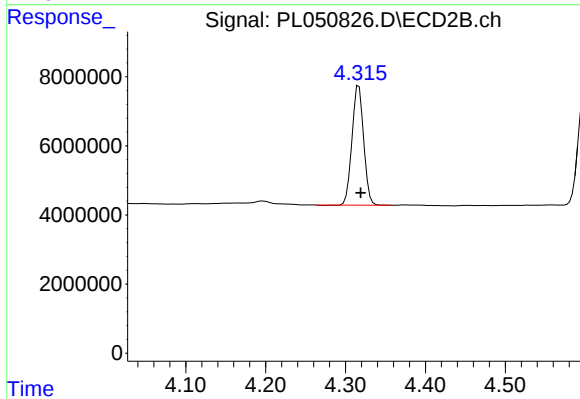

#2 alpha-BHC


R.T.: 4.317 min
Delta R.T.: -0.002 min
Response: 35221987
Conc: 8.54 ng/ml

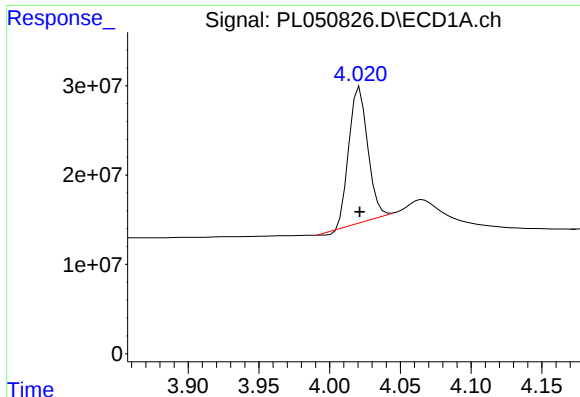

#3 gamma-BHC (Lindane)


R.T.: 4.021 min
Delta R.T.: 0.000 min
Response: 139038900
Conc: 9.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
PEM

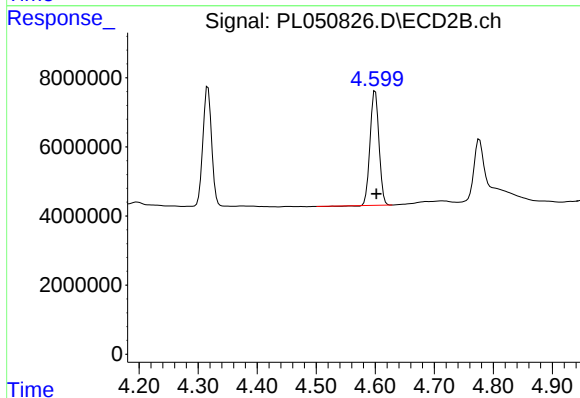


#3 gamma-BHC (Lindane)

R.T.: 4.600 min
Delta R.T.: -0.002 min
Response: 34751299
Conc: 8.97 ng/ml

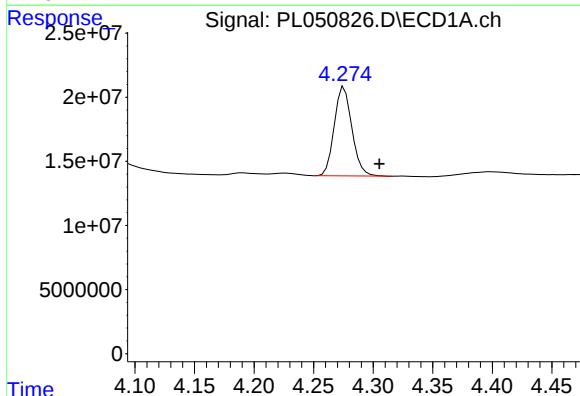


#4 Heptachlor

R.T.: 4.276 min
Delta R.T.: -0.030 min
Response: 71631035
Conc: 4.37 ng/ml

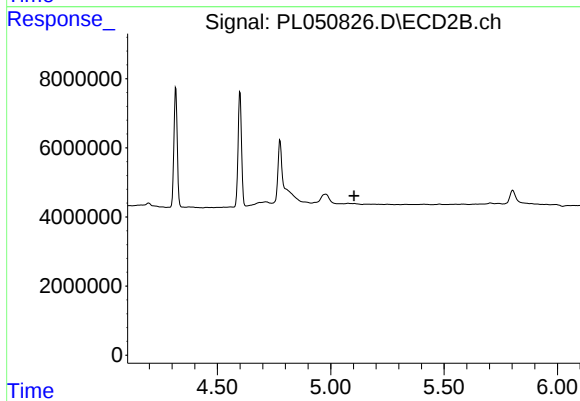

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.104 min
Response: 0
Conc: N.D.

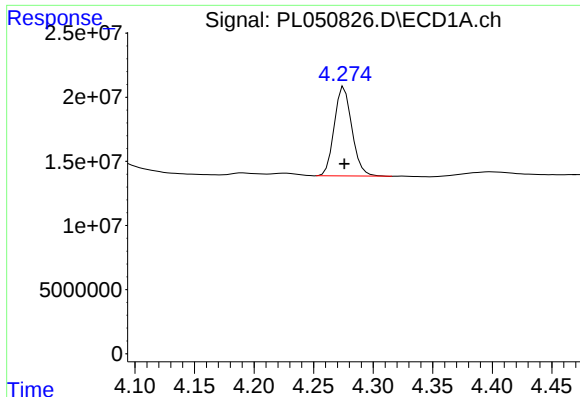

#6 beta-BHC


R.T.: 4.276 min
Delta R.T.: 0.000 min
Response: 71631035
Conc: 10.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
PEM

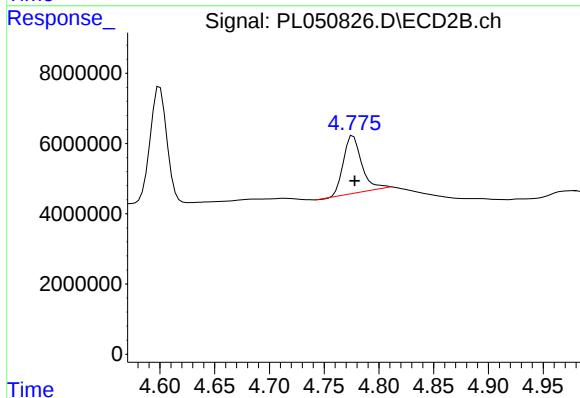


#6 beta-BHC

R.T.: 4.777 min
Delta R.T.: -0.002 min
Response: 19244539
Conc: 11.13 ng/ml

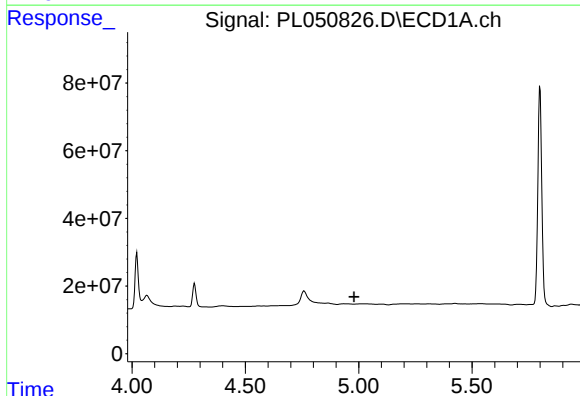


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.979 min
Response: 0
Conc: N.D.

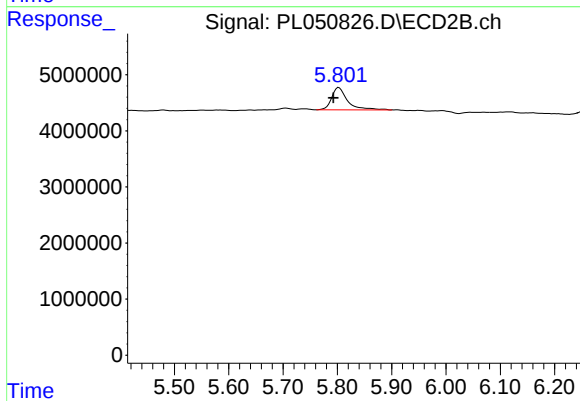

#8 Heptachlor epoxide


R.T.: 5.803 min
Delta R.T.: 0.010 min
Response: 8067538
Conc: 2.11 ng/ml

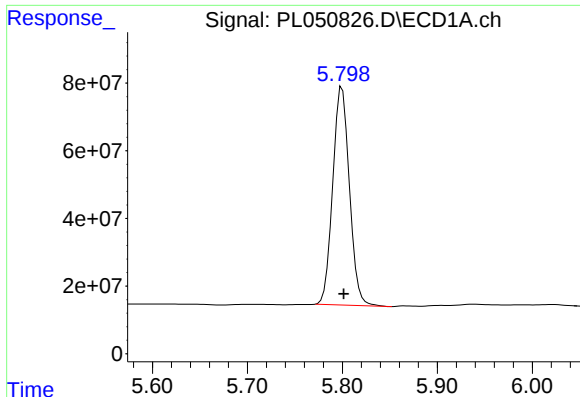

#14 Endrin


R.T.: 5.800 min
Delta R.T.: -0.002 min
Response: 788452931
Conc: 53.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
PEM

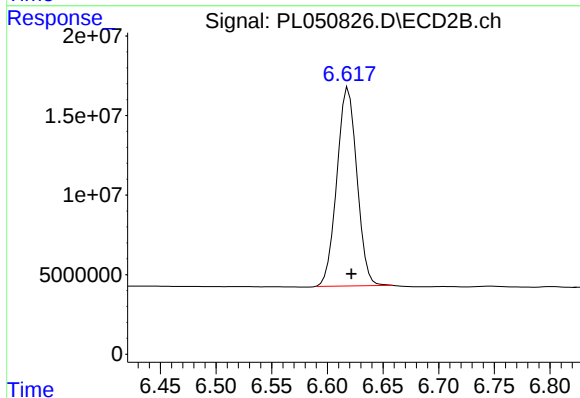


#14 Endrin

R.T.: 6.619 min
Delta R.T.: -0.003 min
Response: 156413648
Conc: 50.43 ng/ml

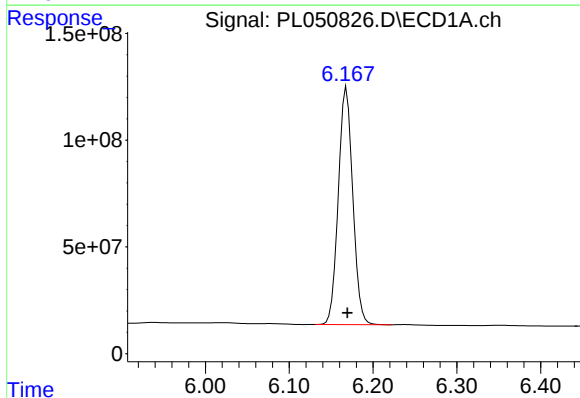


#17 4,4'-DDT

R.T.: 6.168 min
Delta R.T.: -0.001 min
Response: 1331927570
Conc: 107.54 ng/ml

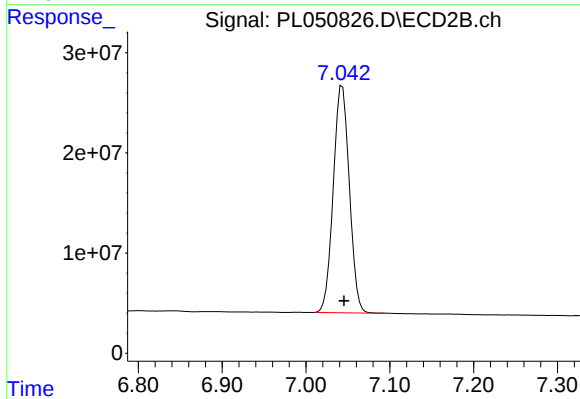

#17 4,4'-DDT


R.T.: 7.043 min
Delta R.T.: -0.002 min
Response: 302035673
Conc: 111.88 ng/ml

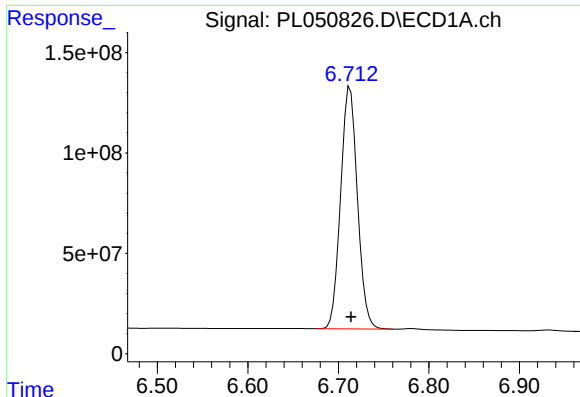

#20 Methoxychlor


R.T.: 6.713 min
Delta R.T.: -0.001 min
Response: 1557793473
Conc: 249.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
PEM

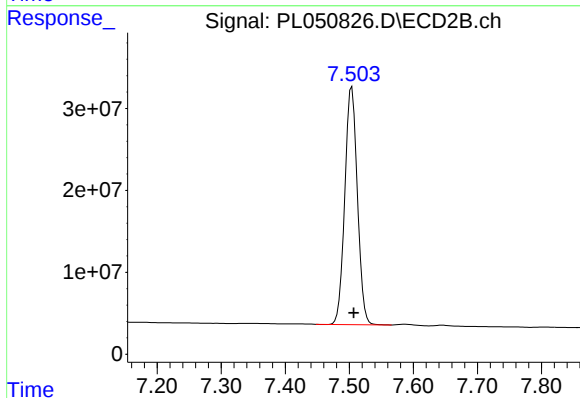


#20 Methoxychlor

R.T.: 7.504 min
Delta R.T.: -0.003 min
Response: 394320264
Conc: 268.74 ng/ml

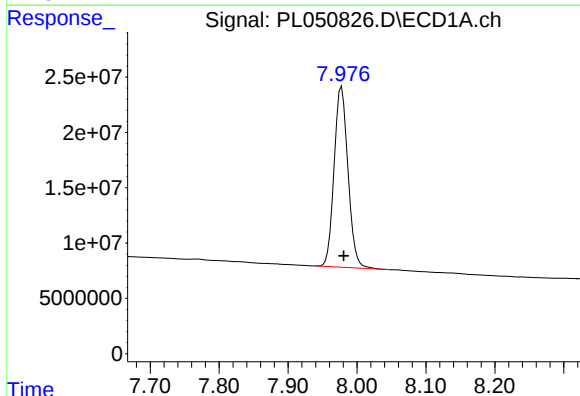

#28 Decachlorobiphenyl

R.T.: 7.978 min
Delta R.T.: -0.003 min
Response: 227661466
Conc: 22.48 ng/ml

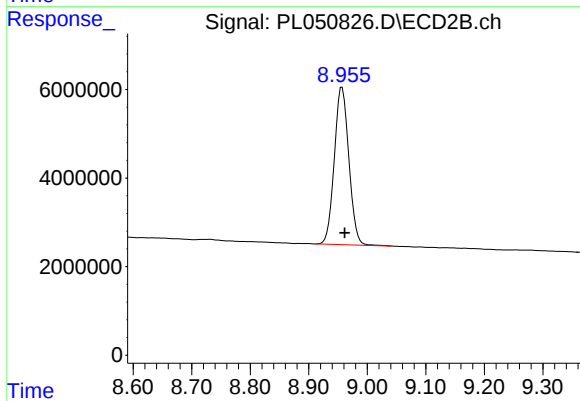

#28 Decachlorobiphenyl

R.T.: 8.957 min
Delta R.T.: -0.005 min
Response: 61342187
Conc: 21.69 ng/ml