

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072619\
 Data File : PL050837.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jul 2019 22:12
 Operator : SM\AJ
 Sample : K3961-04
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-10-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 22:55:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	3.928	197.8E6	50696101	19.687	17.768
28)	SA Decachlor...	7.977	8.957	210.3E6	57845733	20.773	20.455
Target Compounds							
5)	MB Aldrin	4.544	0.000	17219080	0	1.112	N.D. #
6)	B beta-BHC	0.000	4.804f	0	5813405	N.D.	3.363 #
8)	B Heptachlo...	4.976	5.805	13446514	5277419	0.910	1.380 #
9)	A Endosulfan I	5.315	0.000	20544351	0	1.413	N.D. #
10)	B gamma-Chl...	5.225f	0.000	50673040	0	3.211	N.D. #
13)	MA Dieldrin	5.570f	0.000	8177900	0	0.528	N.D. #
23)	Chlordane-1	4.152	0.000	5269353	0	14.321	N.D. #
25)	Chlordane-3	5.225f	0.000	50673040	0	36.201	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072619\
Data File : PL050837.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jul 2019 22:12
Operator : SM\AJ
Sample : K3961-04
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-10-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 22:55:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

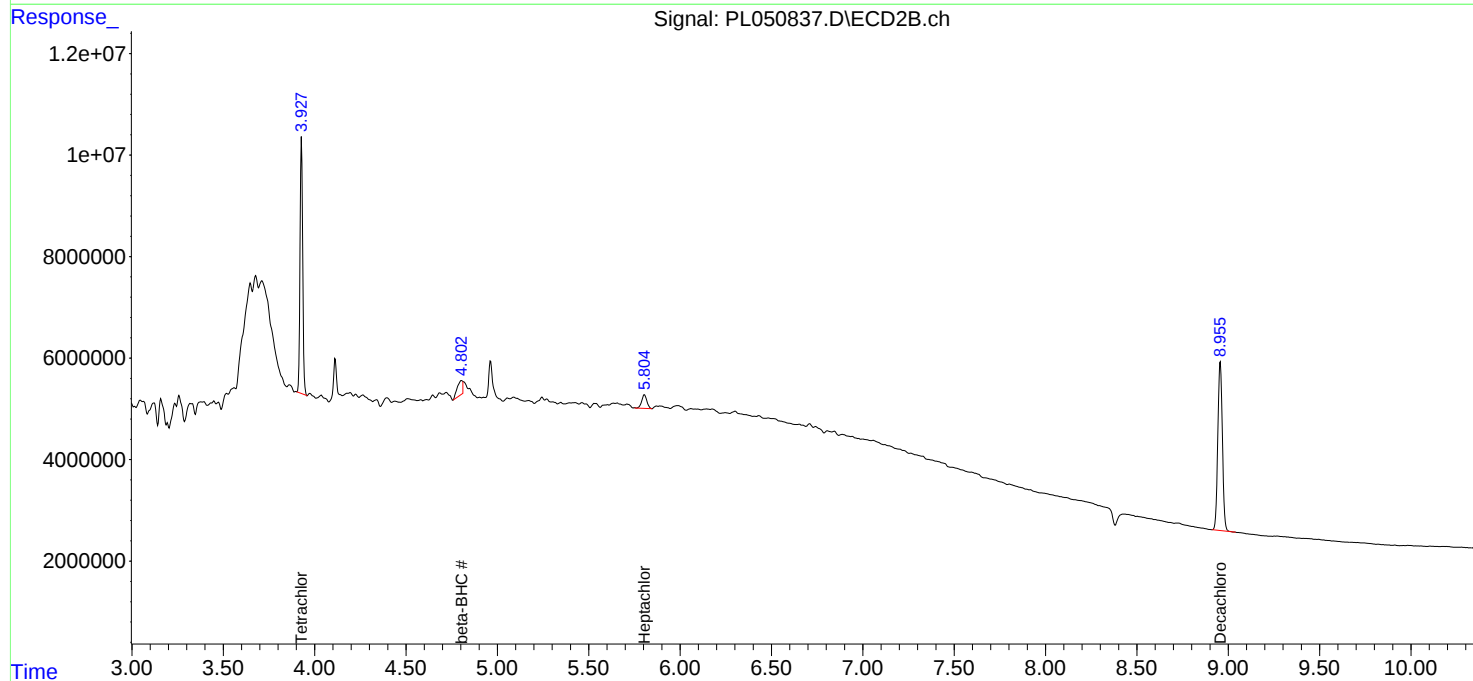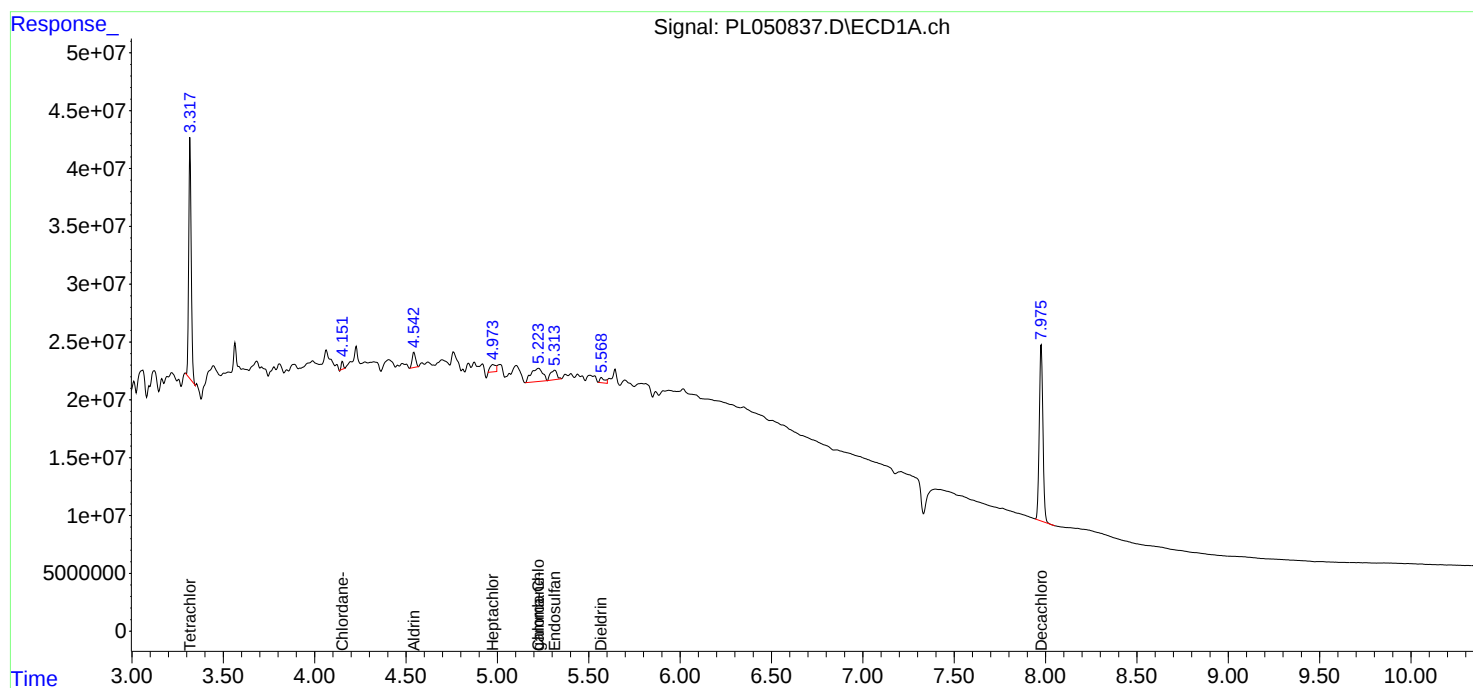


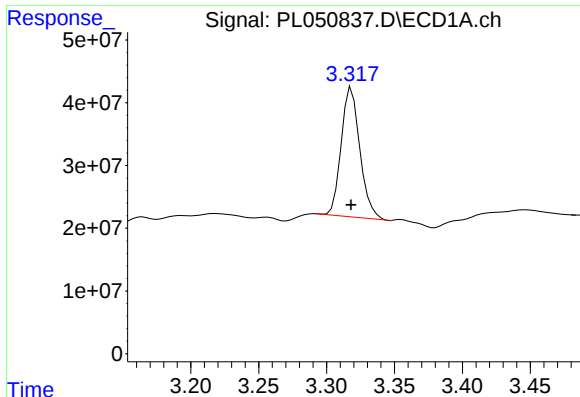

#1 Tetrachloro-m-xylene


R.T.: 3.318 min
Delta R.T.: 0.000 min
Response: 197806988
Conc: 19.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-10-A

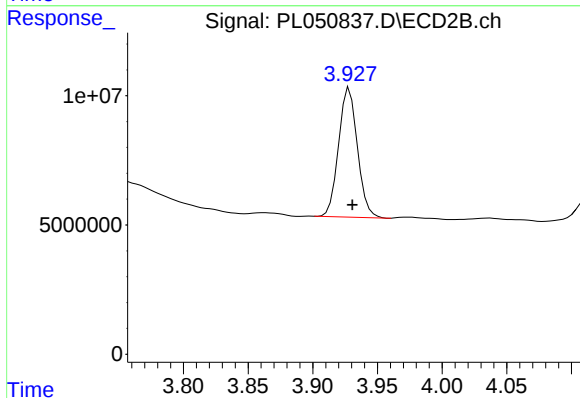


#1 Tetrachloro-m-xylene

R.T.: 3.928 min
Delta R.T.: -0.002 min
Response: 50696101
Conc: 17.77 ng/ml

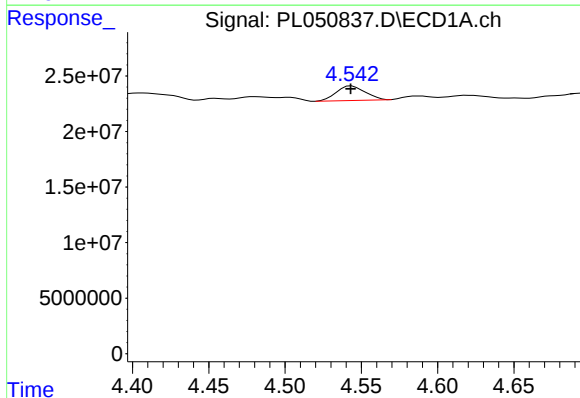


#5 Aldrin

R.T.: 4.544 min
Delta R.T.: 0.000 min
Response: 17219080
Conc: 1.11 ng/ml

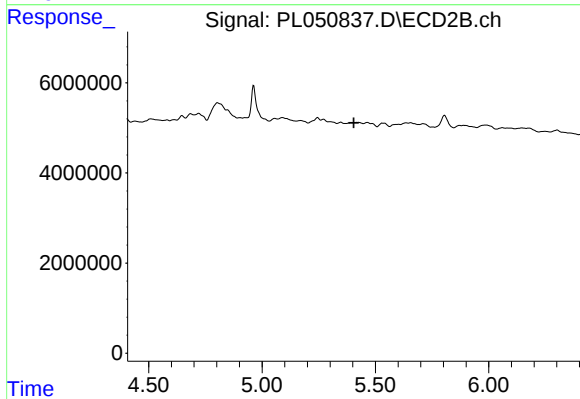

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.405 min
Response: 0
Conc: N.D.

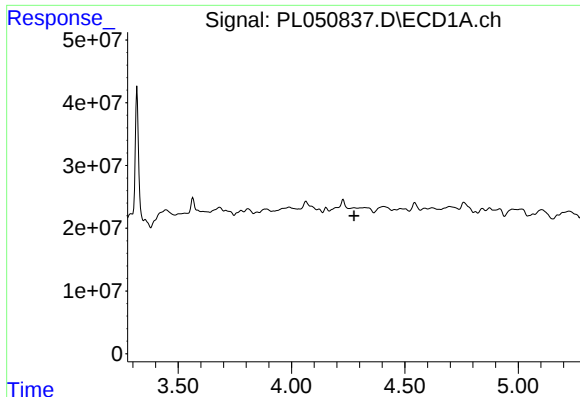

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.276 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-10-A

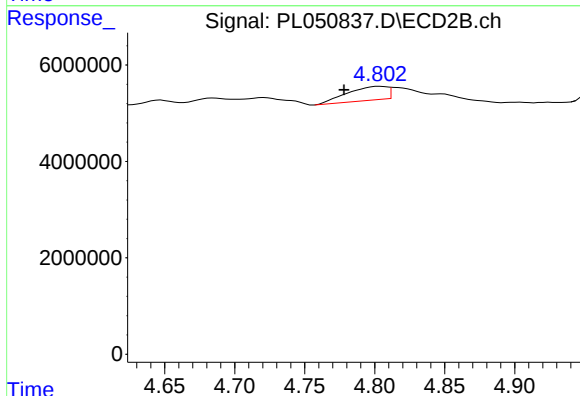


#6 beta-BHC

R.T.: 4.804 min
Delta R.T.: 0.026 min
Response: 5813405
Conc: 3.36 ng/ml

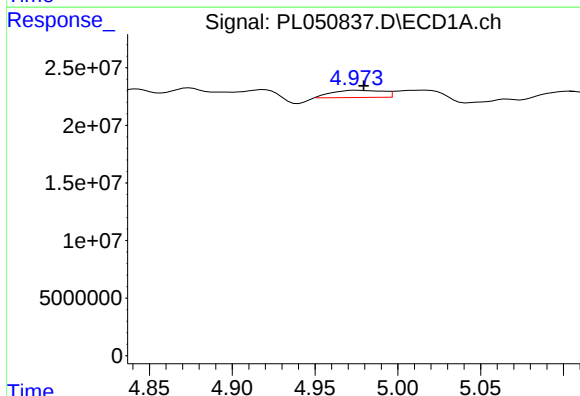


#8 Heptachlor epoxide

R.T.: 4.976 min
Delta R.T.: -0.004 min
Response: 13446514
Conc: 0.91 ng/ml

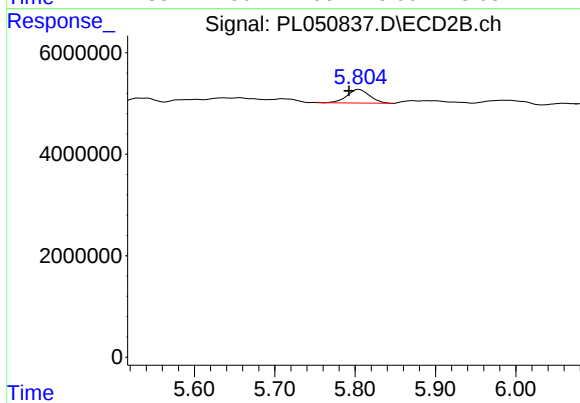

#8 Heptachlor epoxide


R.T.: 5.805 min
Delta R.T.: 0.012 min
Response: 5277419
Conc: 1.38 ng/ml

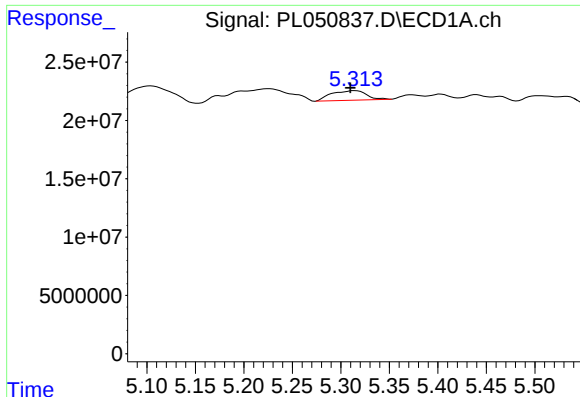

#9 Endosulfan I


R.T.: 5.315 min
Delta R.T.: 0.005 min
Response: 20544351
Conc: 1.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-10-A

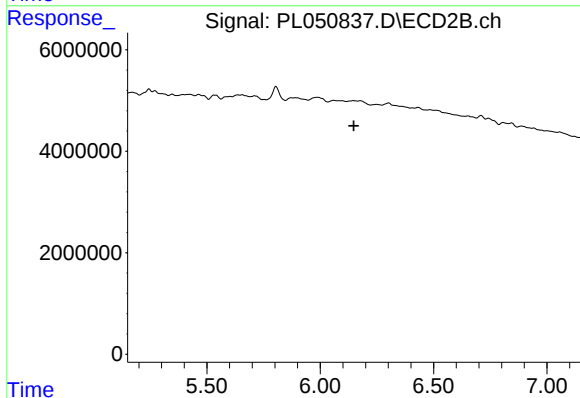


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.148 min
Response: 0
Conc: N.D.

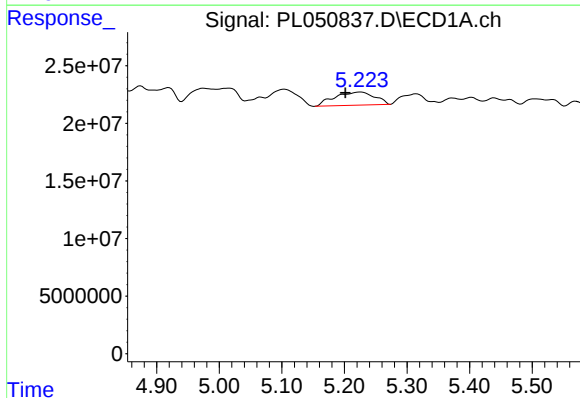


#10 gamma-Chlordane

R.T.: 5.225 min
Delta R.T.: 0.024 min
Response: 50673040
Conc: 3.21 ng/ml

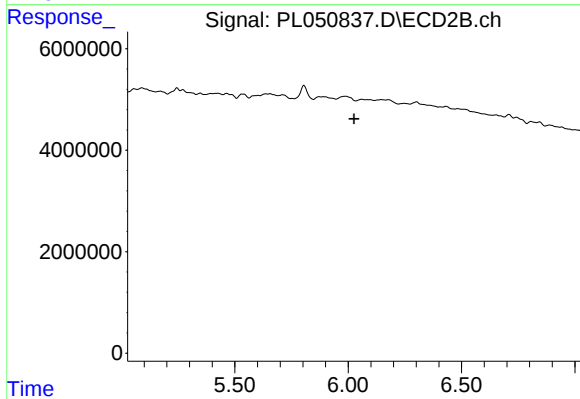

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.026 min
Response: 0
Conc: N.D.

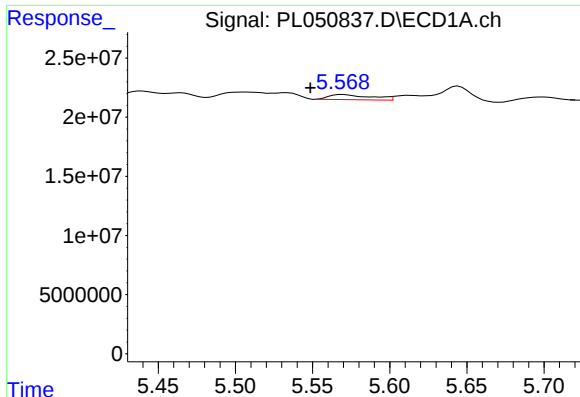

#13 Dieldrin


R.T.: 5.570 min
Delta R.T.: 0.021 min
Response: 8177900
Conc: 0.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-10-A

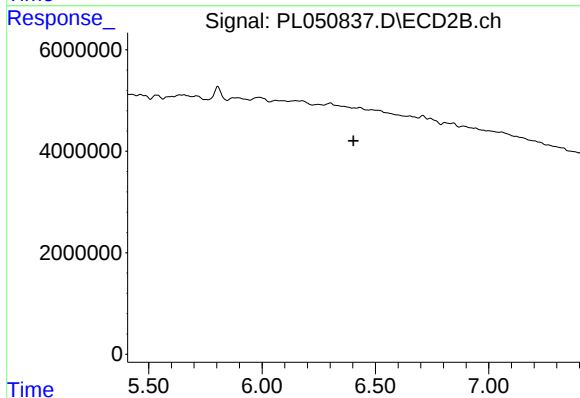


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.404 min
Response: 0
Conc: N.D.

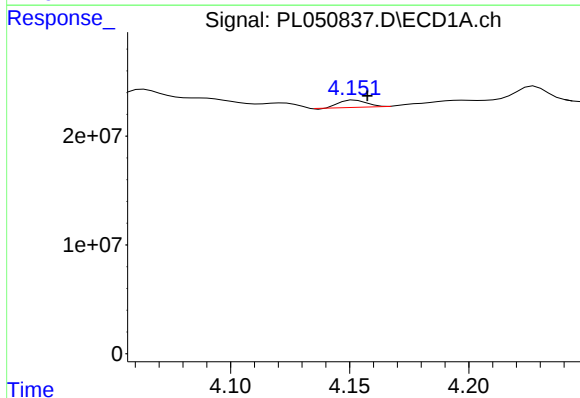


#23 Chlordane-1

R.T.: 4.152 min
Delta R.T.: -0.005 min
Response: 5269353
Conc: 14.32 ng/ml

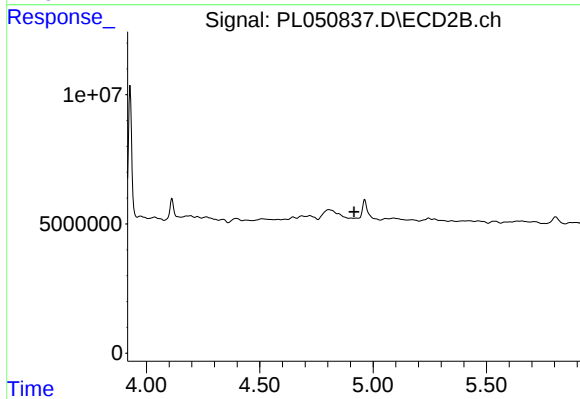

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.916 min
Response: 0
Conc: N.D.

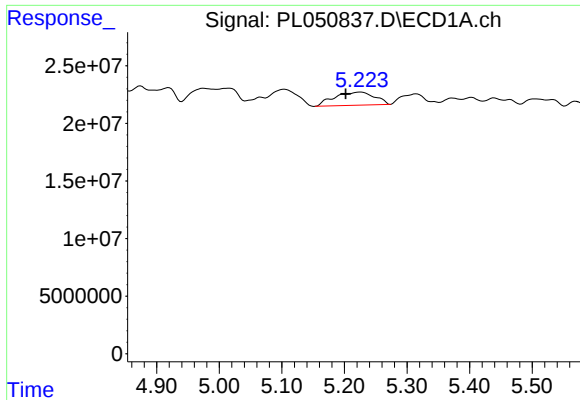

#25 Chlordane-3


R.T.: 5.225 min
Delta R.T.: 0.023 min
Response: 50673040
Conc: 36.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-10-A

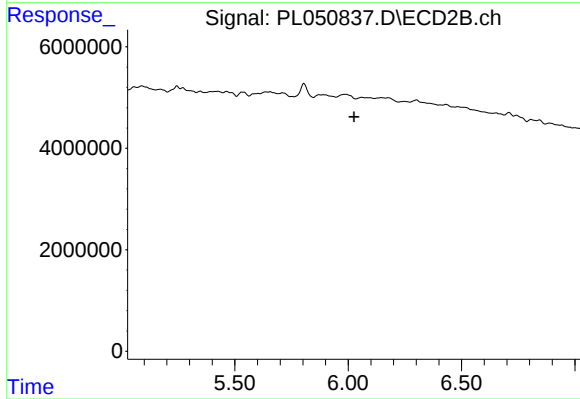


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 6.027 min
Response: 0
Conc: N.D.

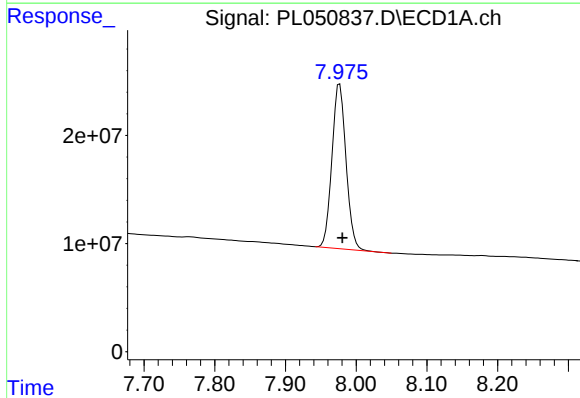

#28 Decachlorobiphenyl

R.T.: 7.977 min
Delta R.T.: -0.004 min
Response: 210333718
Conc: 20.77 ng/ml

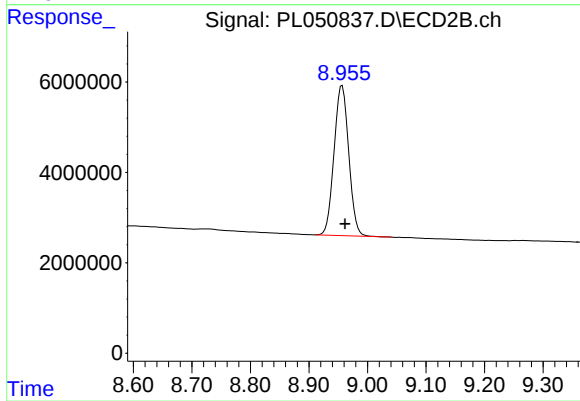

#28 Decachlorobiphenyl

R.T.: 8.957 min
Delta R.T.: -0.005 min
Response: 57845733
Conc: 20.46 ng/ml