

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072619\
 Data File : PL050812.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jul 2019 14:55
 Operator : SM\AJ
 Sample : K3620-15
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CL-02-072519-C

Manual Integrations
 APPROVED

Ankita
 7/27/2019 9:06:38 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 22:48:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	3.928	104.2E6	28331732	10.371	9.930
28)	SA Decachlor...	7.978	8.957	111.6E6	30908034	11.025	10.930
Target Compounds							
10)	B gamma-Chl...	5.200	6.023	42499253	8930997	2.693m	2.417
11)	B alpha-Chl...	5.256	6.095	131.0E6	37564303	8.588	10.249

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072619\
Data File : PL050812.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jul 2019 14:55
Operator : SM\AJ
Sample : K3620-15
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CL-02-072519-C


Manual Integrations
APPROVED

Ankita
7/27/2019 9:06:38 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 22:48:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

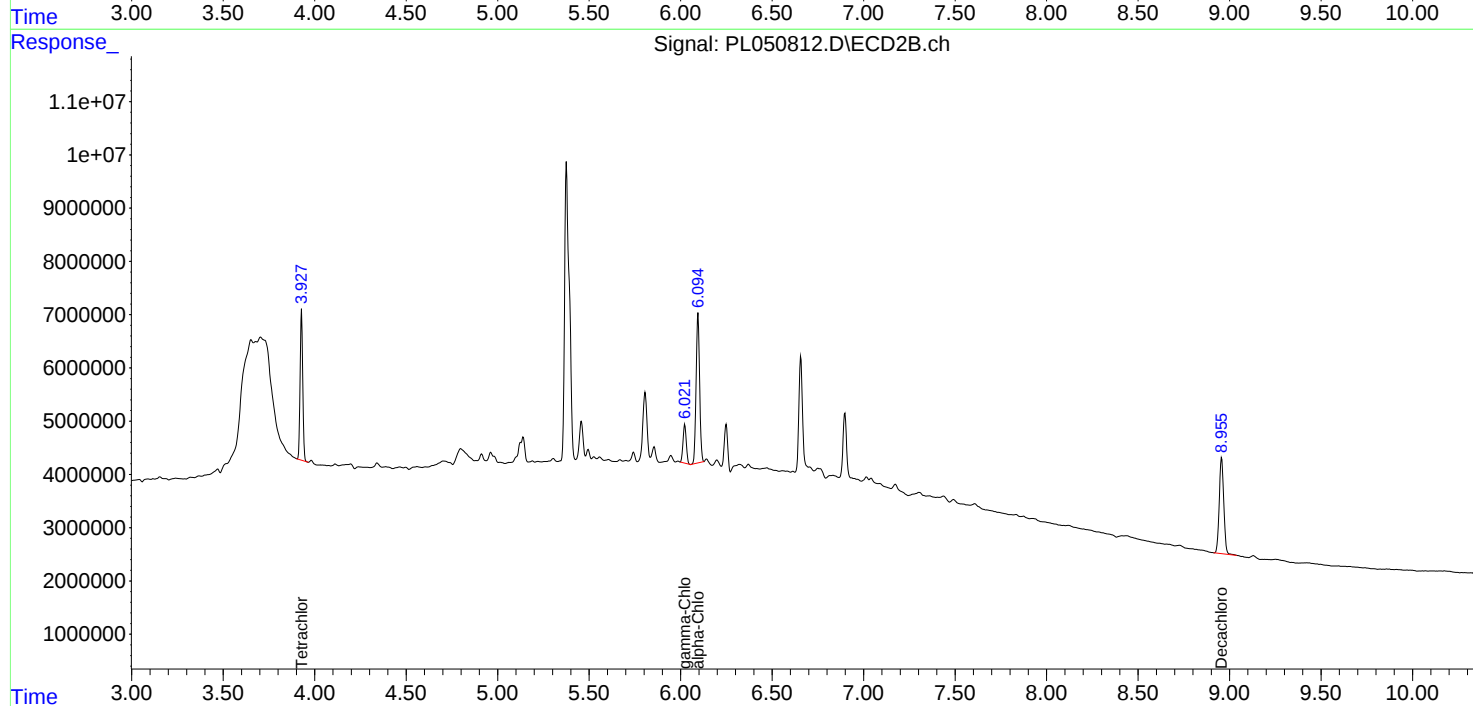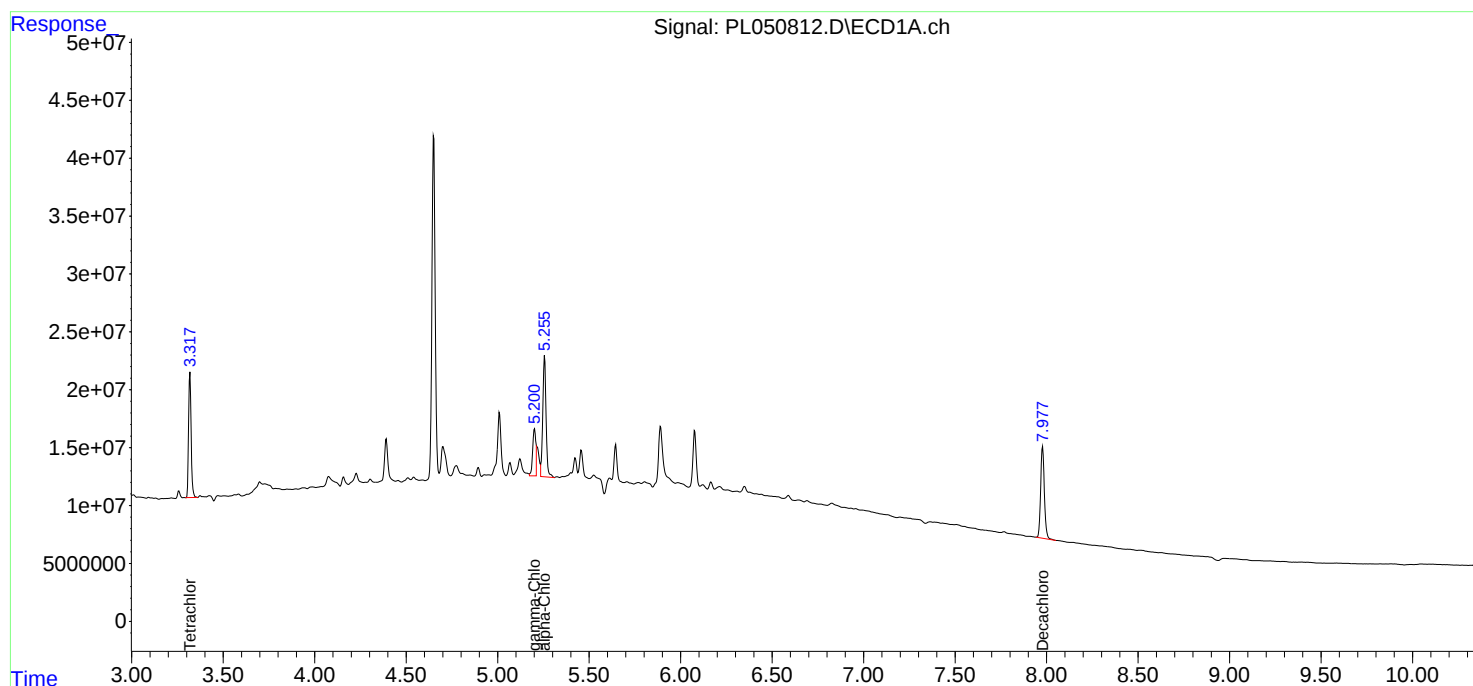

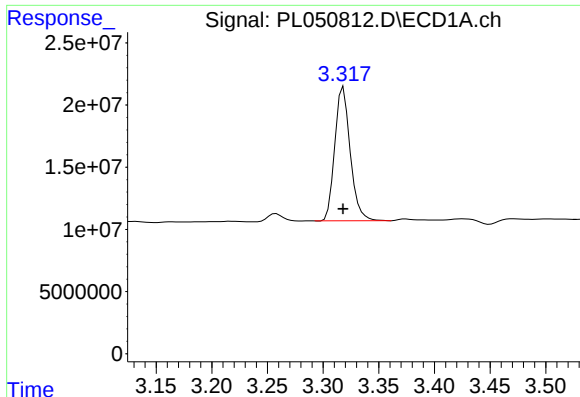


#1 Tetrachloro-m-xylene

R.T.: 3.318 min
Delta R.T.: 0.000 min
Response: 104210864
Conc: 10.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-072519-C


Manual Integrations
APPROVED

Ankita
7/27/2019 9:06:38 AM

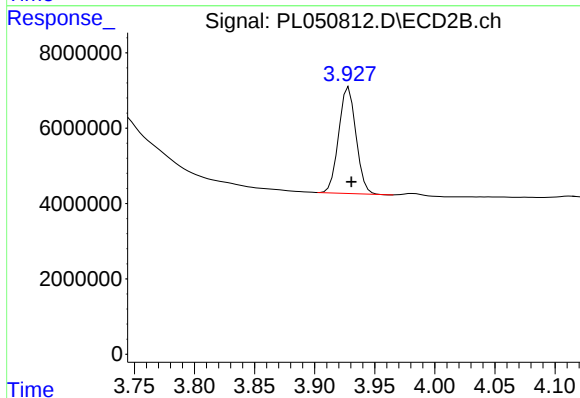


#1 Tetrachloro-m-xylene

R.T.: 3.928 min
Delta R.T.: -0.002 min
Response: 28331732
Conc: 9.93 ng/ml

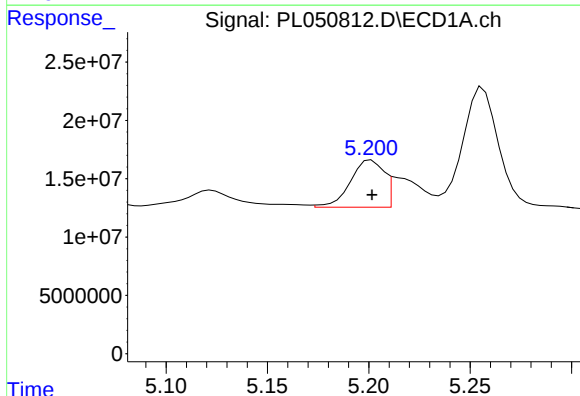


#10 gamma-Chlordane

R.T.: 5.200 min
Delta R.T.: -0.002 min
Response: 42499253
Conc: 2.69 ng/ml m

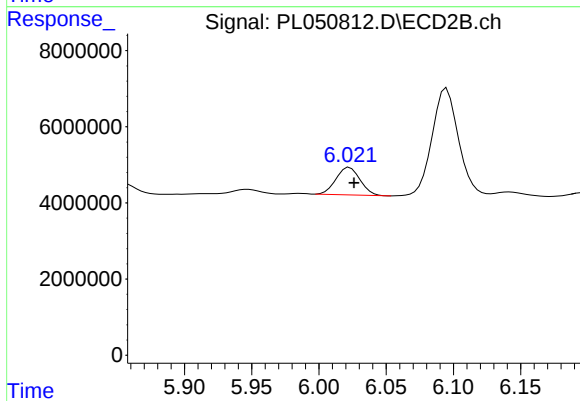

#10 gamma-Chlordane

R.T.: 6.023 min
Delta R.T.: -0.003 min
Response: 8930997
Conc: 2.42 ng/ml

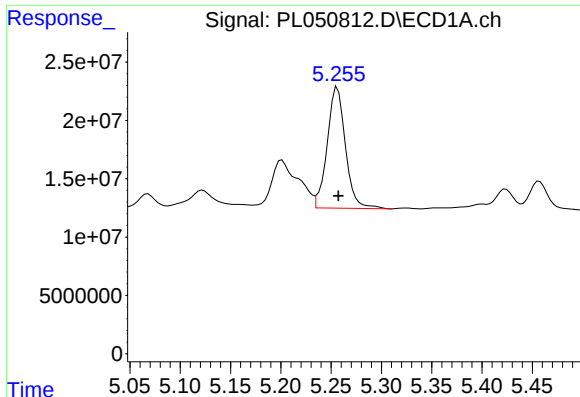


#11 alpha-Chlordane

R.T.: 5.256 min
Delta R.T.: -0.001 min
Response: 131023847
Conc: 8.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-072519-C


Manual Integrations
APPROVED

Ankita
7/27/2019 9:06:38 AM

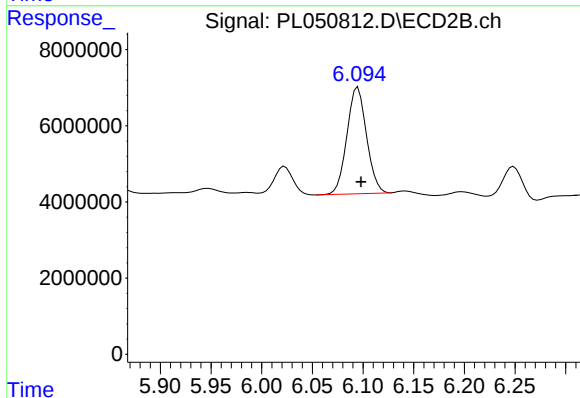


#11 alpha-Chlordane

R.T.: 6.095 min
Delta R.T.: -0.003 min
Response: 37564303
Conc: 10.25 ng/ml

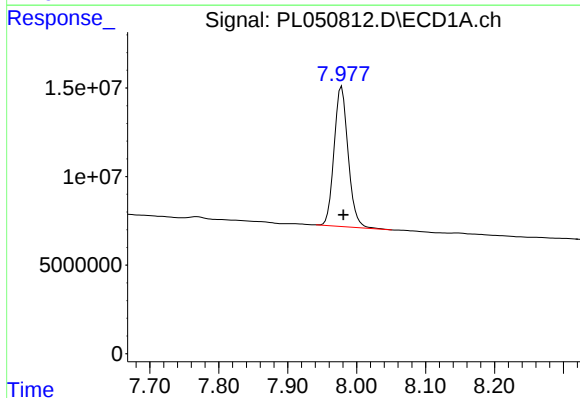

#28 Decachlorobiphenyl

R.T.: 7.978 min
Delta R.T.: -0.002 min
Response: 111628527
Conc: 11.02 ng/ml

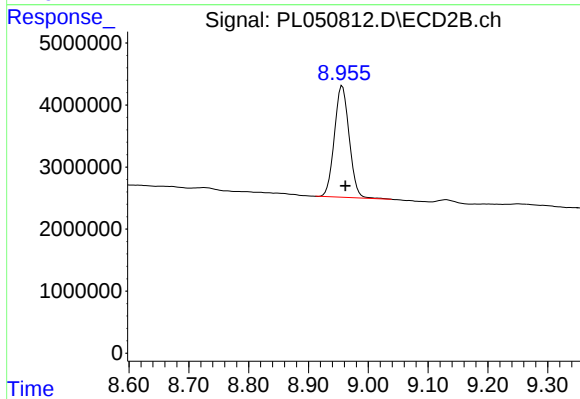

#28 Decachlorobiphenyl

R.T.: 8.957 min
Delta R.T.: -0.005 min
Response: 30908034
Conc: 10.93 ng/ml