

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072621\
 Data File : PL068449.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jul 2021 08:31
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 23:10:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:44:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

4) MA	Heptachlor	6.162f	0.000	2023070	0	3.319	N.D.	#
6) B	beta-BHC	6.162	0.000	2023070	0	6.914	N.D.	#
15) B	Endosulfa...	8.354f	0.000	583048	0	1.181	N.D.	#
17) MA	4,4'-DDT	8.504	0.000	413679	0	0.825	N.D.	#
23)	Chlordane-1	0.000	6.980f	0	903600	N.D.	22.306	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072621\
Data File : PL068449.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jul 2021 08:31
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 23:10:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:44:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

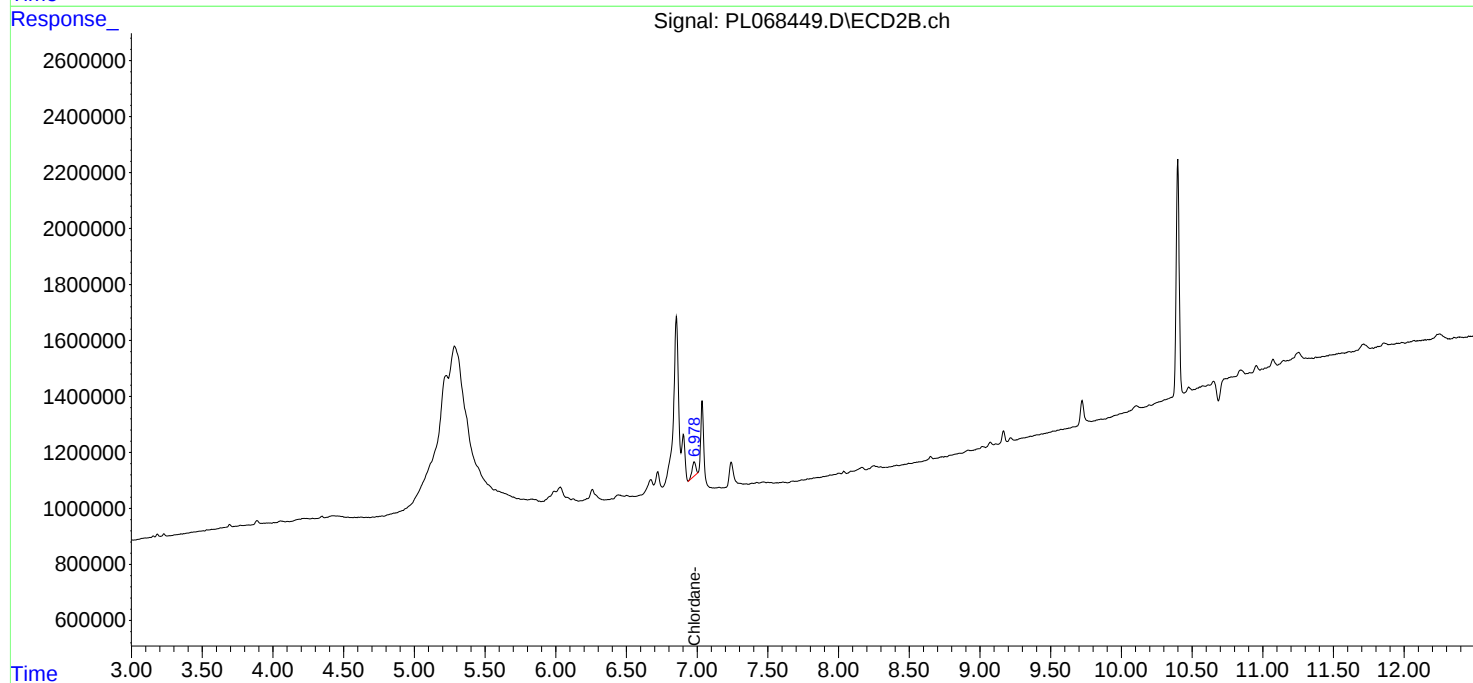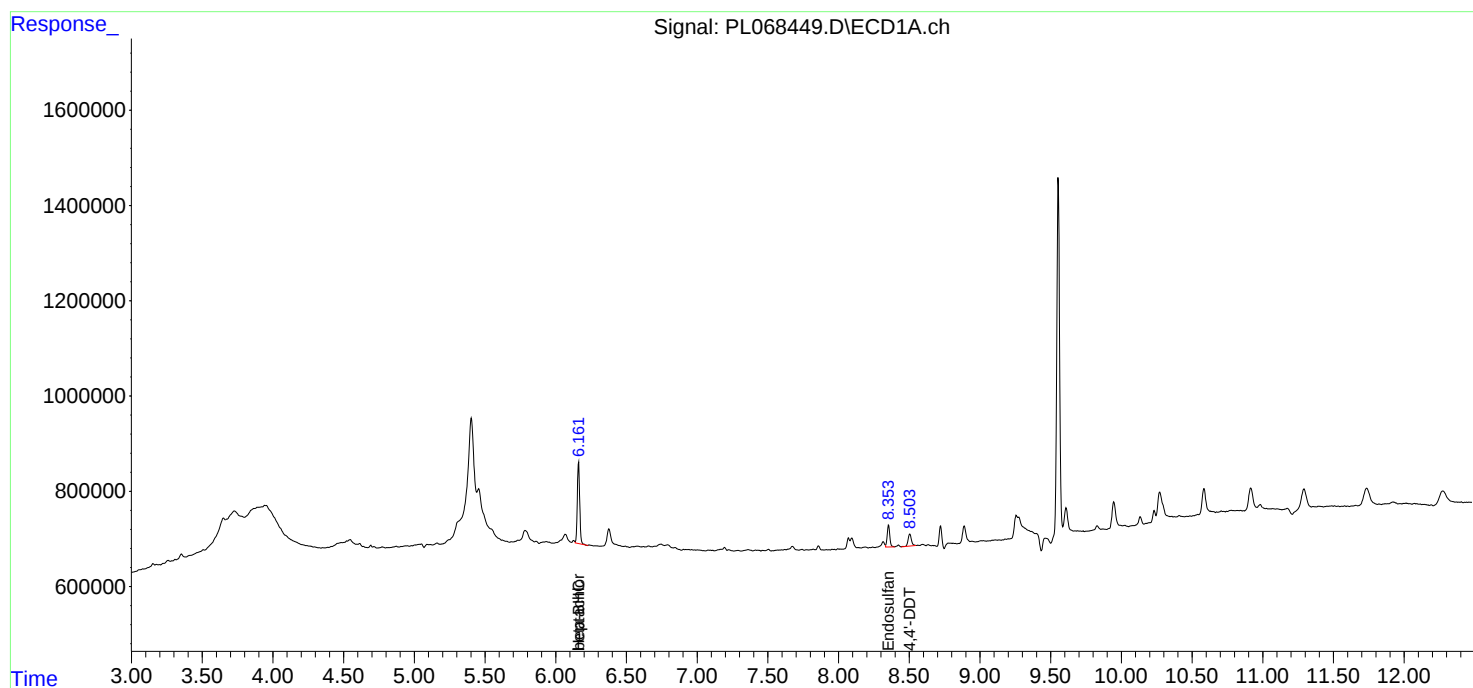


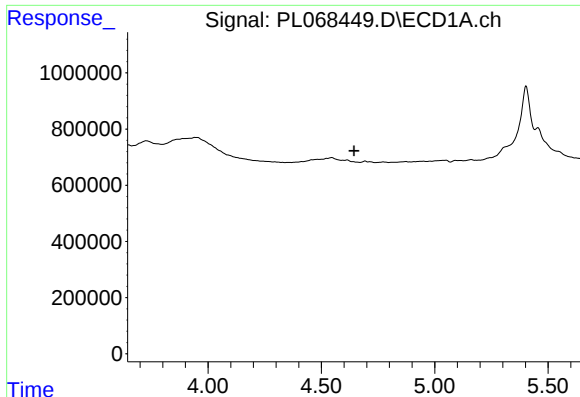

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.645 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

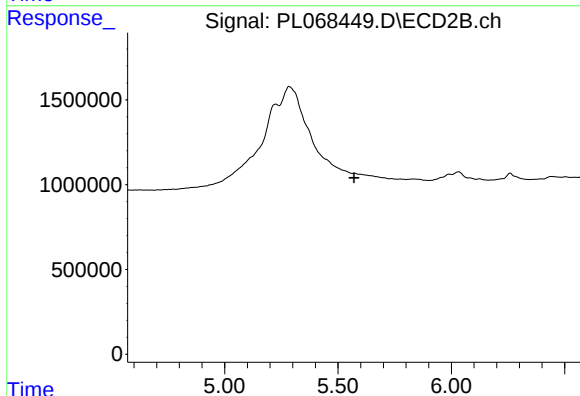


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 5.571 min
Response: 0
Conc: N.D.

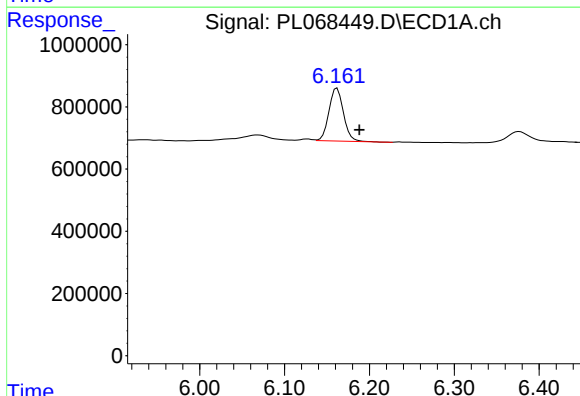


#4 Heptachlor

R.T.: 6.162 min
Delta R.T.: -0.026 min
Response: 2023070
Conc: 3.32 ng/ml

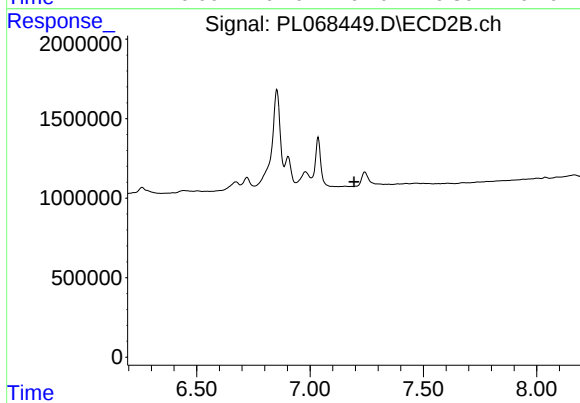

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 7.195 min
Response: 0
Conc: N.D.

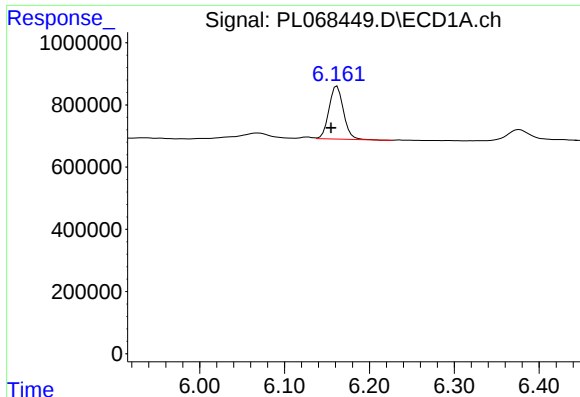

#6 beta-BHC


R.T.: 6.162 min
Delta R.T.: 0.007 min
Response: 2023070
Conc: 6.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

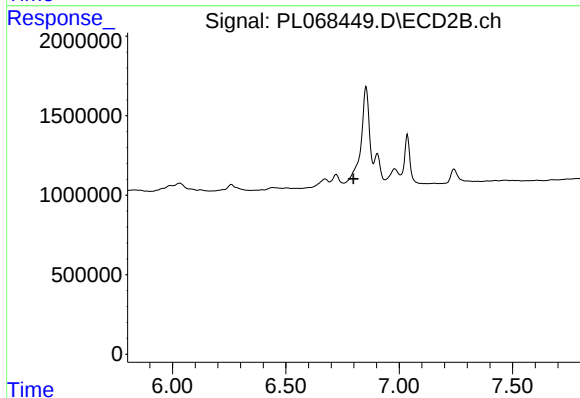


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.799 min
Response: 0
Conc: N.D.

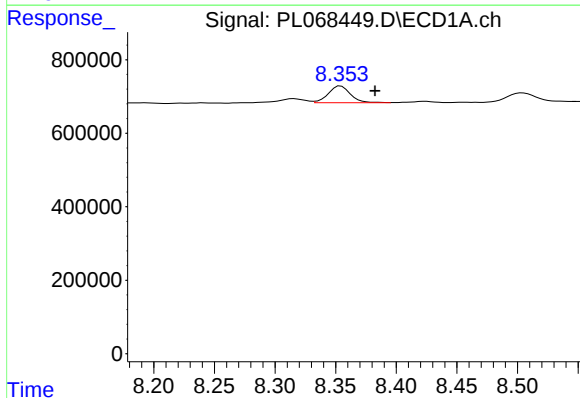


#15 Endosulfan II

R.T.: 8.354 min
Delta R.T.: -0.028 min
Response: 583048
Conc: 1.18 ng/ml

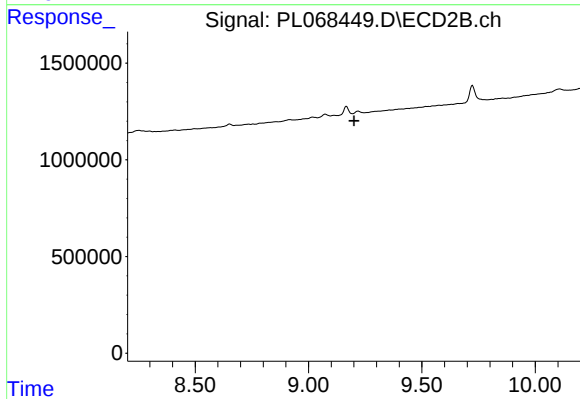

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 9.201 min
Response: 0
Conc: N.D.

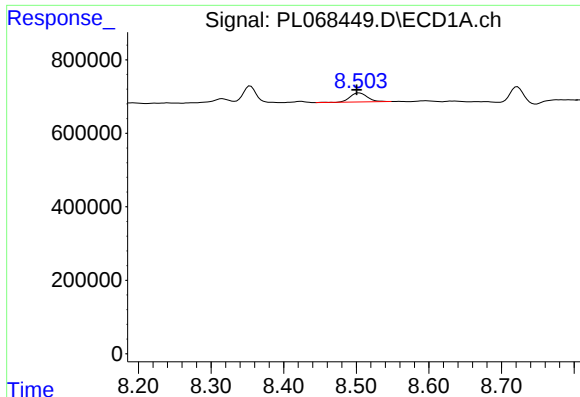

#17 4,4'-DDT


R.T.: 8.504 min
Delta R.T.: 0.004 min
Response: 413679
Conc: 0.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

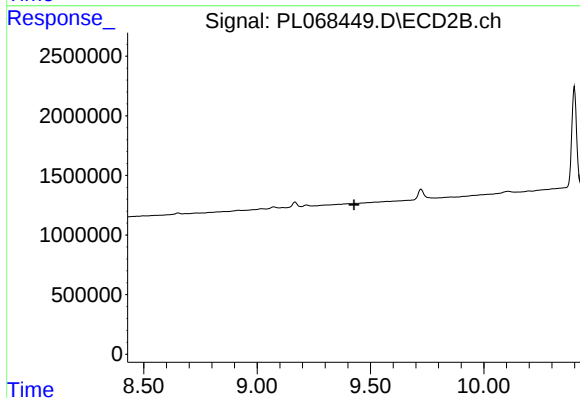


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 9.427 min
Response: 0
Conc: N.D.

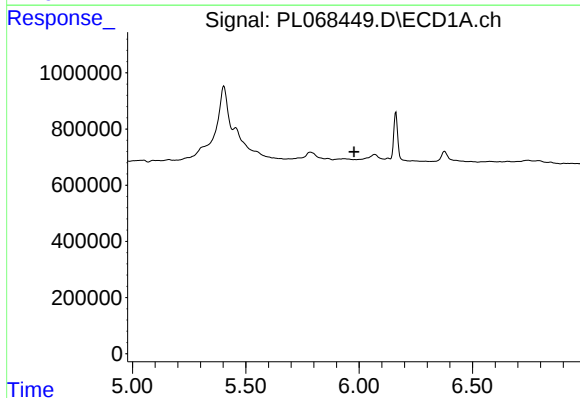


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.978 min
Response: 0
Conc: N.D.

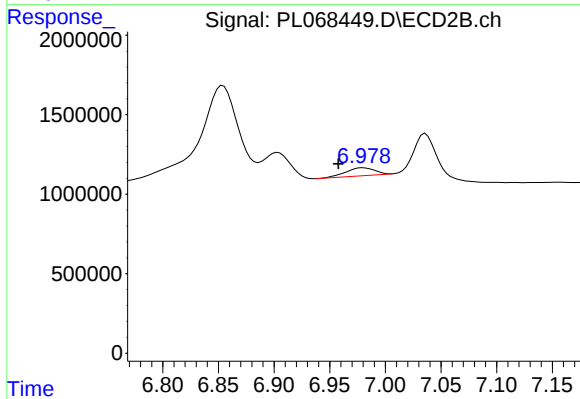

#23 Chlordane-1


R.T.: 6.980 min
Delta R.T.: 0.022 min
Response: 903600
Conc: 22.31 ng/ml

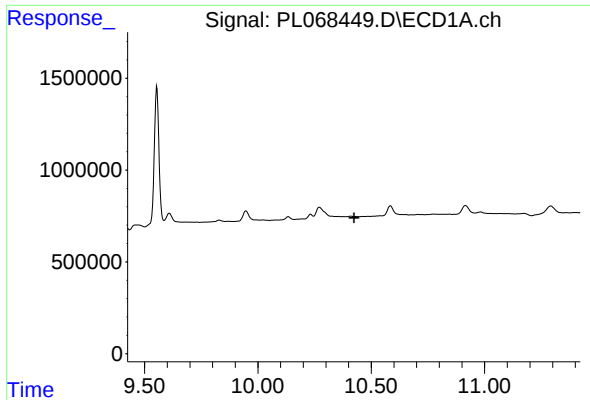

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.424 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

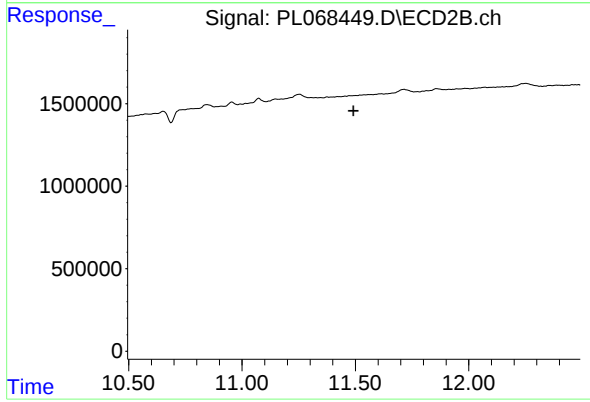

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 11.492 min
Response: 0
Conc: N.D.