

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072621\
 Data File : PL068473.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jul 2021 16:49
 Operator : AR\AJ
 Sample : M3159-14
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20210554-COM-27

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 23:16:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:44:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.642	5.570	5183887	11548250	12.079	11.317
28)	SA Decachlor...	10.418	11.492	5403363	8479282	9.607	9.506
Target Compounds							
3)	MA gamma-BHC...	5.775	0.000	750507	0	1.320	N.D. #
23)	Chlordane-1	0.000	6.972	0	1178563	N.D.	29.093 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072621\
Data File : PL068473.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jul 2021 16:49
Operator : AR\AJ
Sample : M3159-14
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
20210554-COM-27

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 23:16:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:44:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

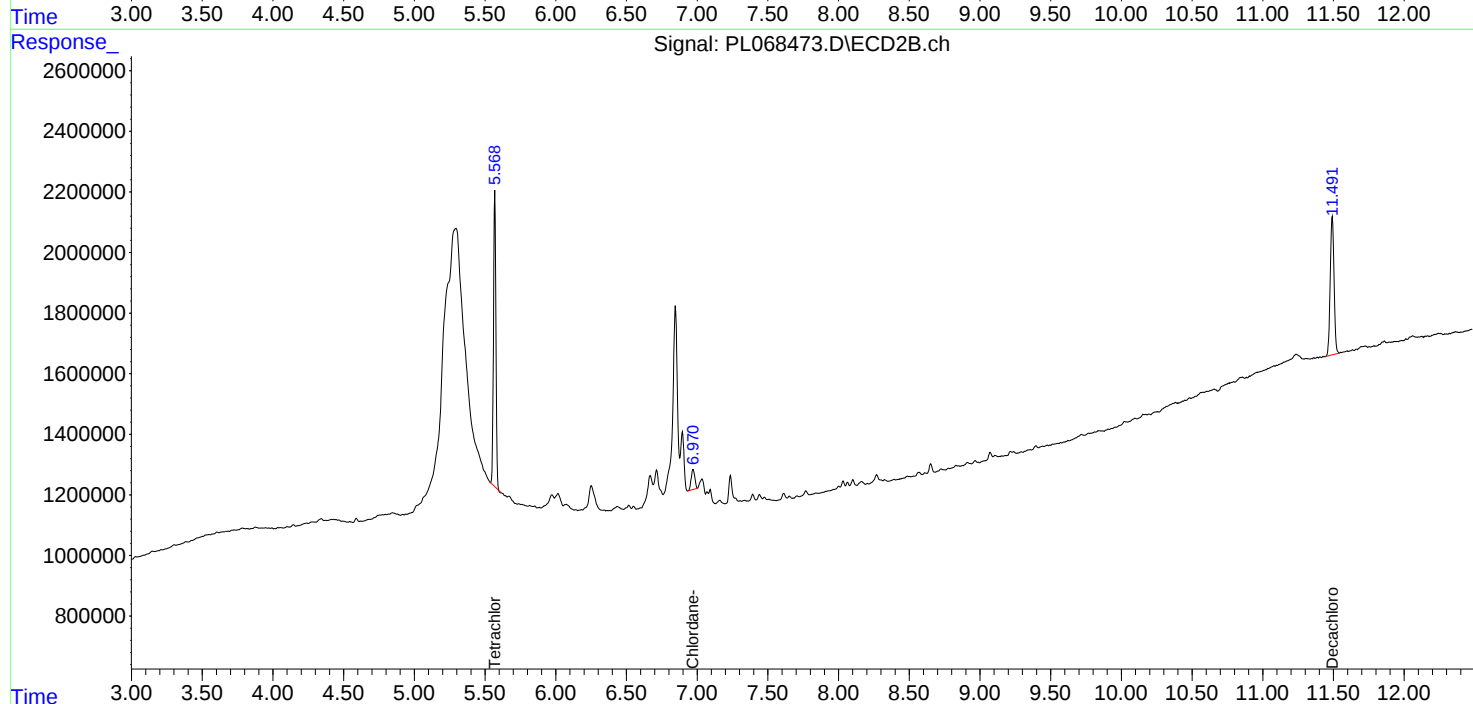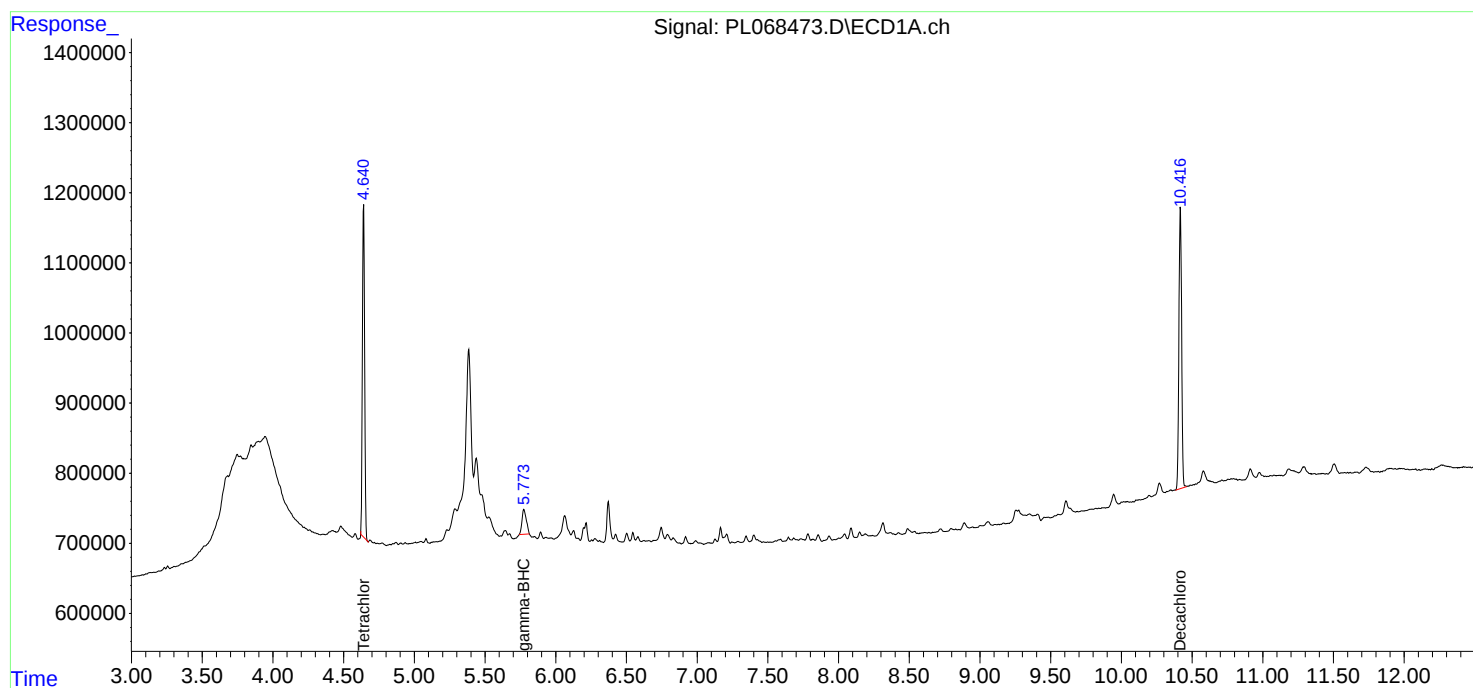


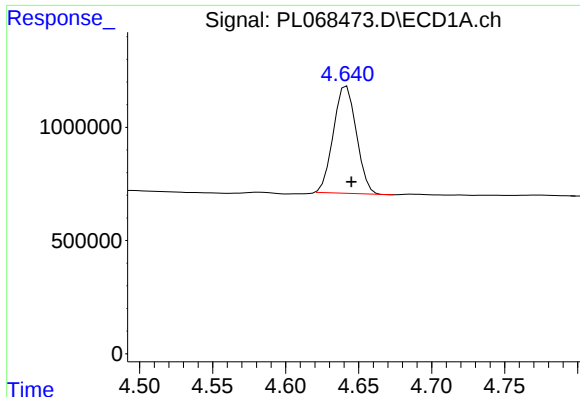

#1 Tetrachloro-m-xylene


R.T.: 4.642 min
Delta R.T.: -0.003 min
Response: 5183887
Conc: 12.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
20210554-COM-27

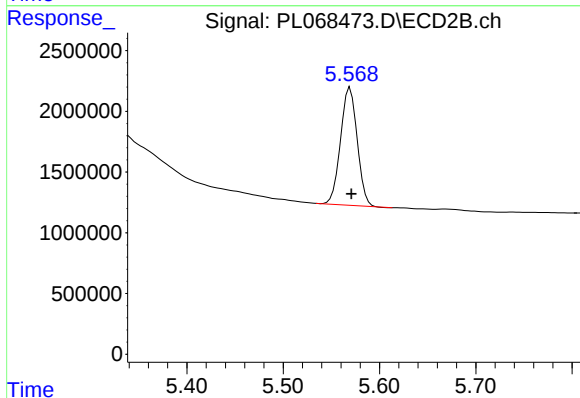


#1 Tetrachloro-m-xylene

R.T.: 5.570 min
Delta R.T.: -0.001 min
Response: 11548250
Conc: 11.32 ng/ml

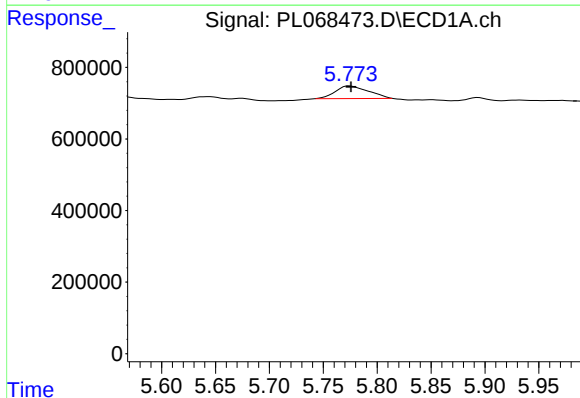


#3 gamma-BHC (Lindane)

R.T.: 5.775 min
Delta R.T.: -0.001 min
Response: 750507
Conc: 1.32 ng/ml

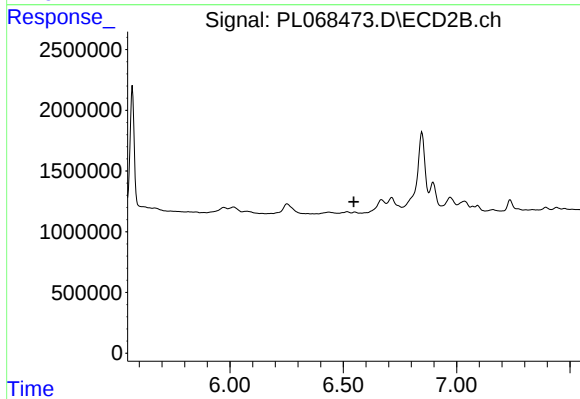

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 6.546 min
Response: 0
Conc: N.D.

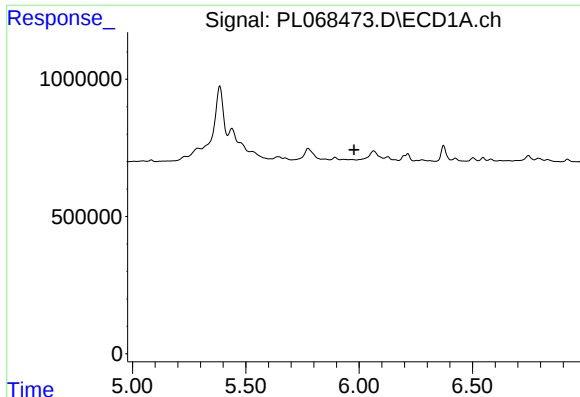

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.978 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20210554-COM-27

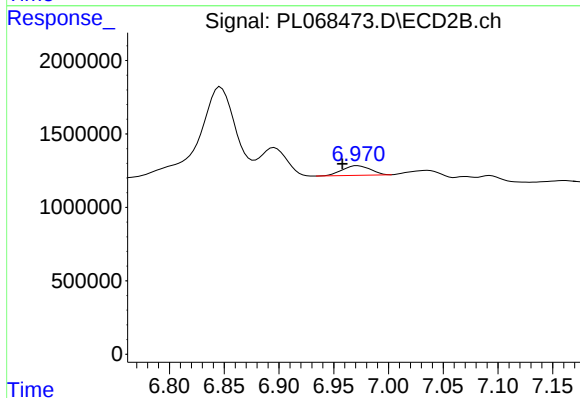


#23 Chlordane-1

R.T.: 6.972 min
Delta R.T.: 0.014 min
Response: 1178563
Conc: 29.09 ng/ml

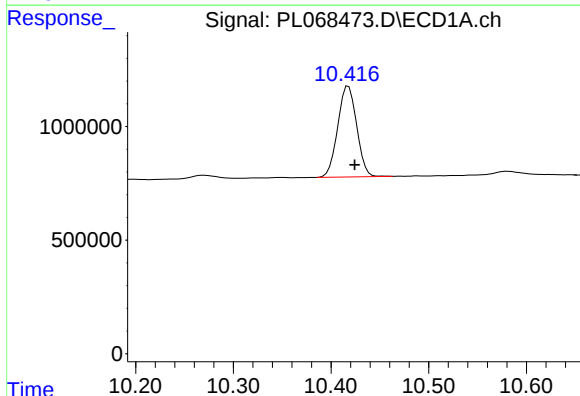

#28 Decachlorobiphenyl

R.T.: 10.418 min
Delta R.T.: -0.007 min
Response: 5403363
Conc: 9.61 ng/ml

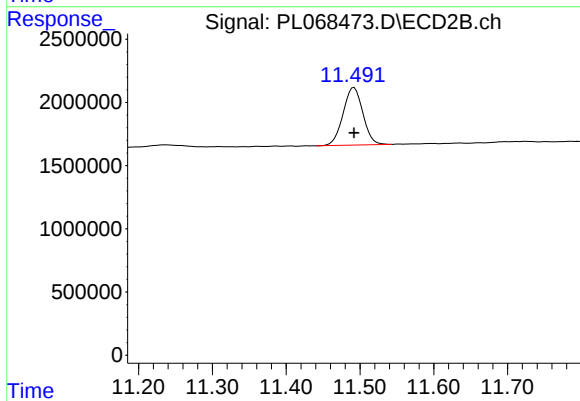

#28 Decachlorobiphenyl

R.T.: 11.492 min
Delta R.T.: 0.000 min
Response: 8479282
Conc: 9.51 ng/ml