

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072621\
 Data File : PL068474.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jul 2021 17:06
 Operator : AR\AJ
 Sample : M3159-15
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 23:16:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:44:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.642	5.569	7816208	17716727	18.212	17.362
28)	SA Decachlor...	10.417	11.492	8774834	13931859	15.602	15.619
Target Compounds							
10)	B gamma-Chl...	0.000	8.323f	0	518277	N.D.	0.460 #
15)	B Endosulfa...	0.000	9.217f	0	609766	N.D.	0.673 #
23)	Chlordane-1	0.000	6.977f	0	925897	N.D.	22.856 #
25)	Chlordane-3	0.000	8.323f	0	518277	N.D.	3.347 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072621\
Data File : PL068474.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jul 2021 17:06
Operator : AR\AJ
Sample : M3159-15
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 23:16:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:44:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

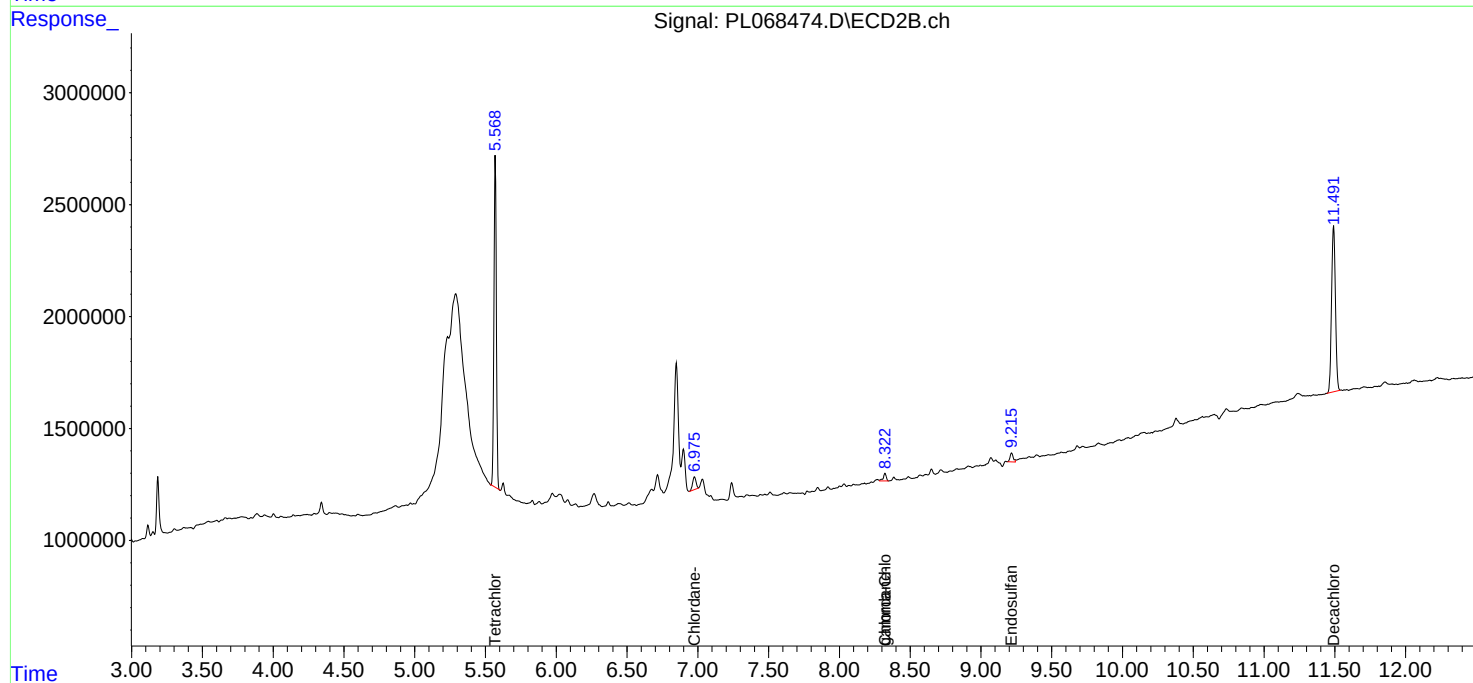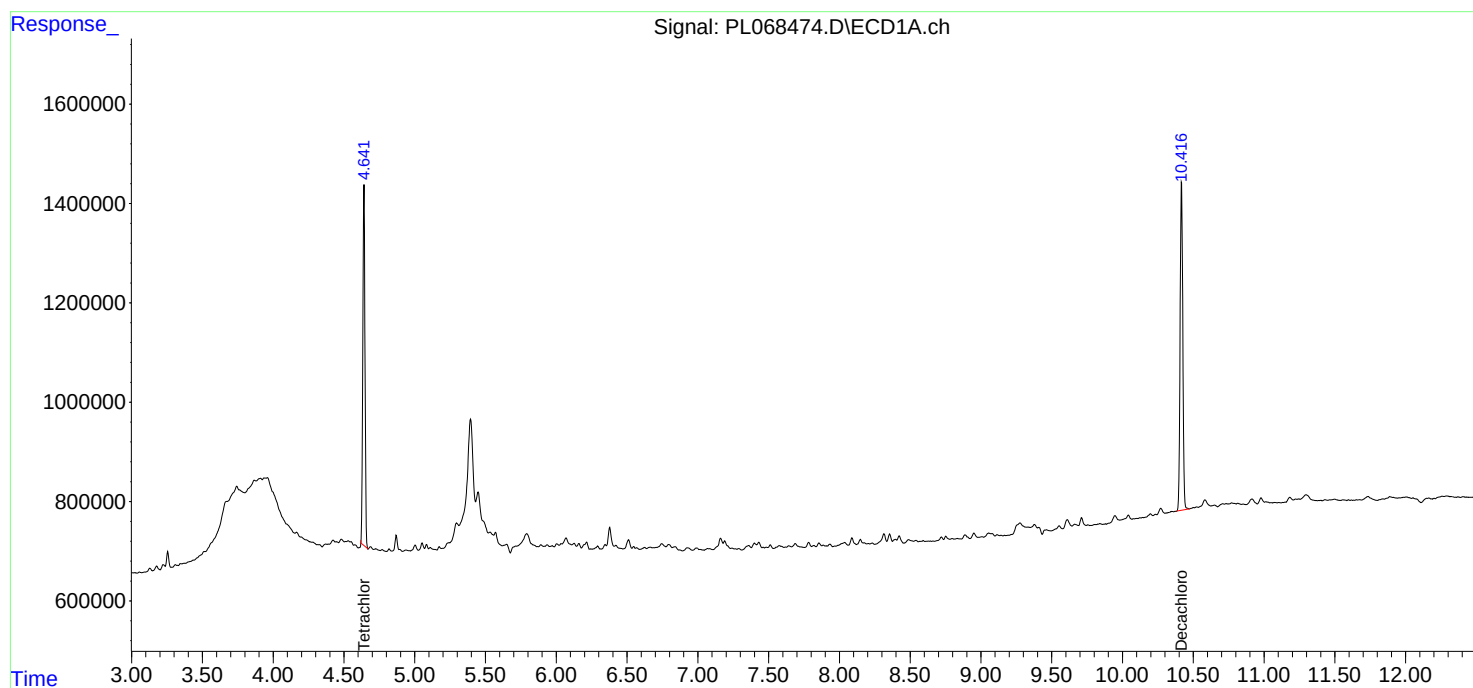


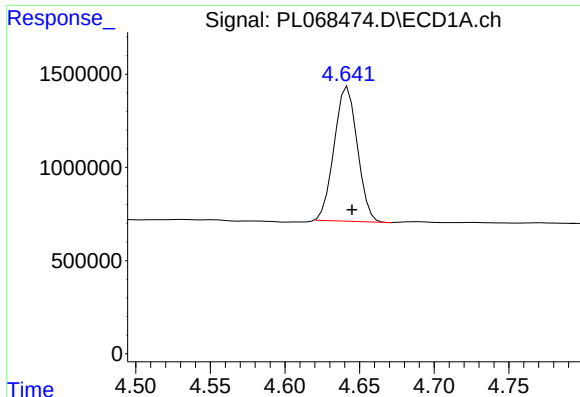

#1 Tetrachloro-m-xylene


R.T.: 4.642 min
Delta R.T.: -0.003 min
Response: 7816208
Conc: 18.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

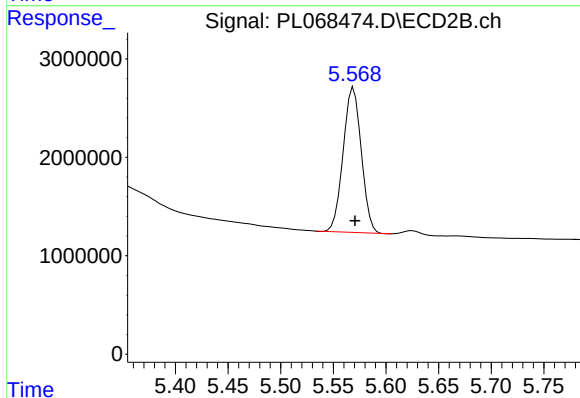


#1 Tetrachloro-m-xylene

R.T.: 5.569 min
Delta R.T.: -0.001 min
Response: 17716727
Conc: 17.36 ng/ml

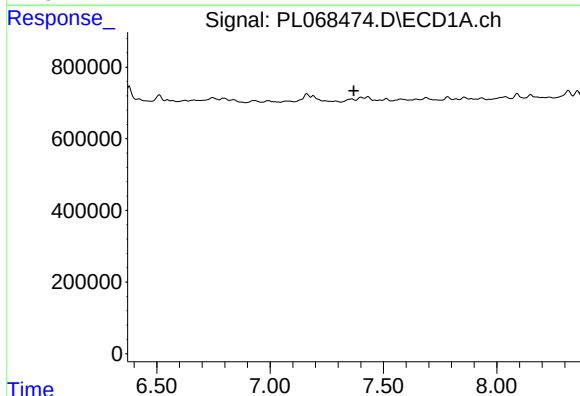


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.369 min
Response: 0
Conc: N.D.

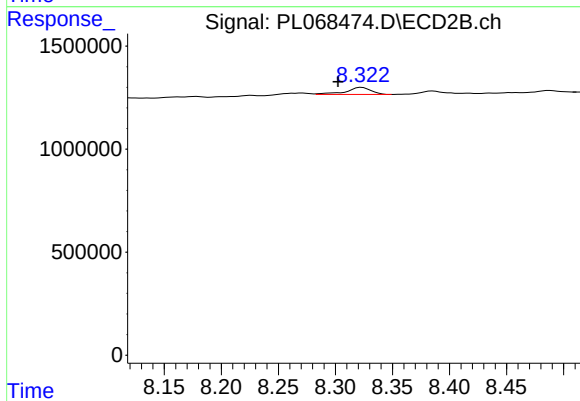

#10 gamma-Chlordane


R.T.: 8.323 min
Delta R.T.: 0.021 min
Response: 518277
Conc: 0.46 ng/ml

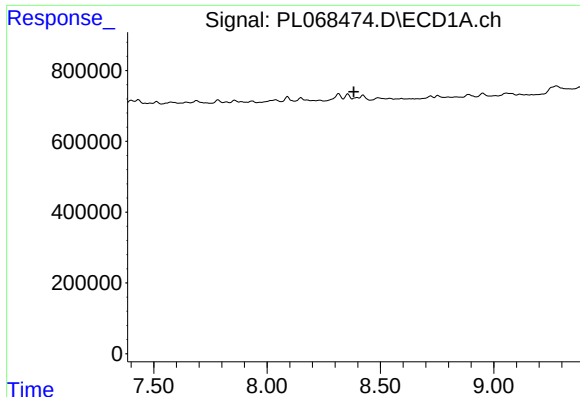

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

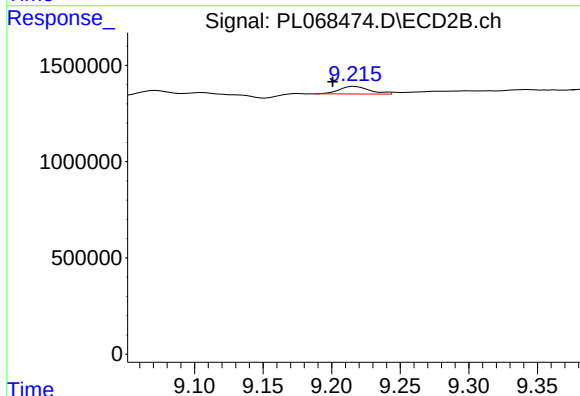


#15 Endosulfan II

R.T.: 9.217 min
Delta R.T.: 0.016 min
Response: 609766
Conc: 0.67 ng/ml

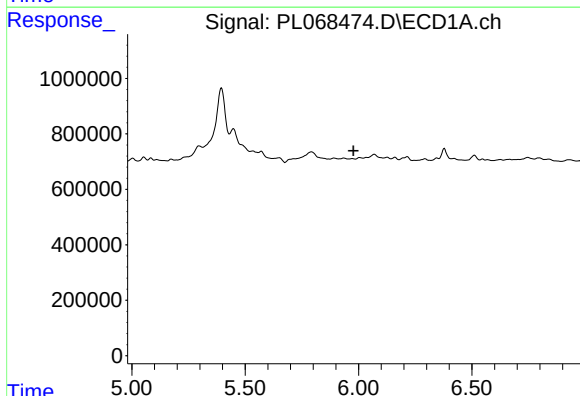


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.978 min
Response: 0
Conc: N.D.

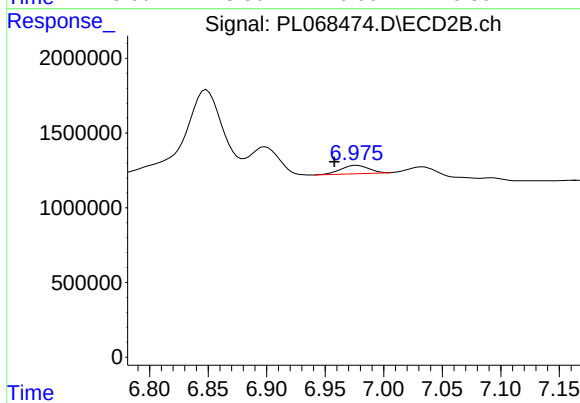

#23 Chlordane-1


R.T.: 6.977 min
Delta R.T.: 0.019 min
Response: 925897
Conc: 22.86 ng/ml

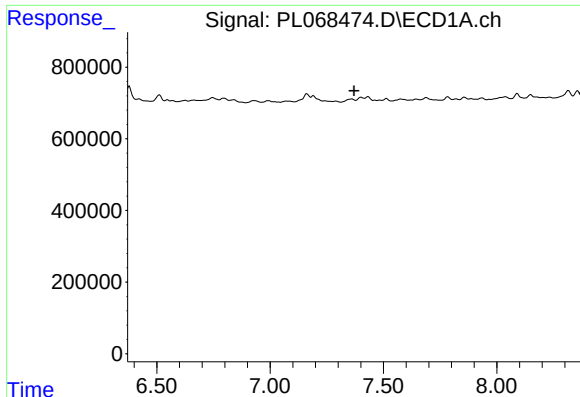

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.371 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

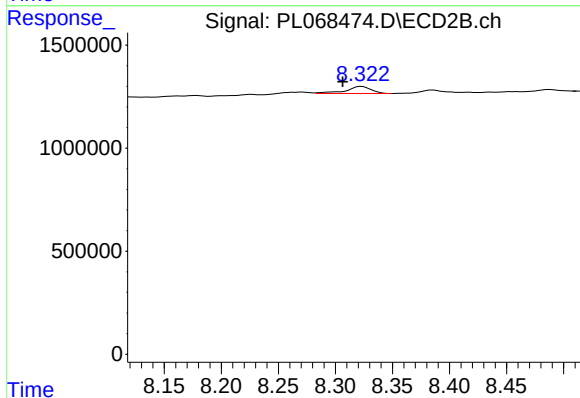


#25 Chlordane-3

R.T.: 8.323 min
Delta R.T.: 0.017 min
Response: 518277
Conc: 3.35 ng/ml

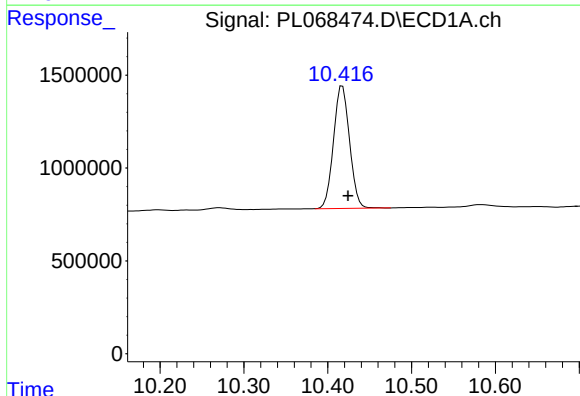

#28 Decachlorobiphenyl

R.T.: 10.417 min
Delta R.T.: -0.007 min
Response: 8774834
Conc: 15.60 ng/ml

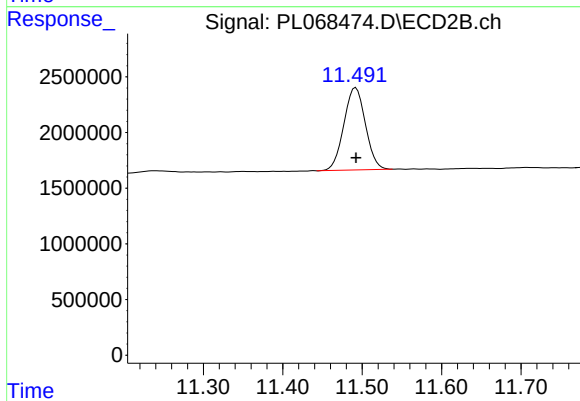

#28 Decachlorobiphenyl

R.T.: 11.492 min
Delta R.T.: 0.000 min
Response: 13931859
Conc: 15.62 ng/ml