

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072621\
 Data File : PL068475.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jul 2021 17:23
 Operator : AR\AJ
 Sample : M3165-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 23:16:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:44:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.642	5.569	6226403	14021268	14.508	13.741
28)	SA Decachlor...	10.418	11.491	7681835	12344456	13.659	13.839
Target Compounds							
3)	MA gamma-BHC...	5.774	0.000	761101	0	1.339	N.D. #
12)	B 4,4'-DDE	7.647	8.568	2676780	4042999	5.312	3.923 #
15)	B Endosulfa...	0.000	9.217f	0	830141	N.D.	0.916 #
16)	A 4,4'-DDD	0.000	9.107	0	376128	N.D.	0.442 #
17)	MA 4,4'-DDT	8.494	9.426	292581	605505	0.583	0.642
23)	Chlordane-1	0.000	6.973	0	1014405	N.D.	25.041 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072621\
Data File : PL068475.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jul 2021 17:23
Operator : AR\AJ
Sample : M3165-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
COMP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 23:16:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:44:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

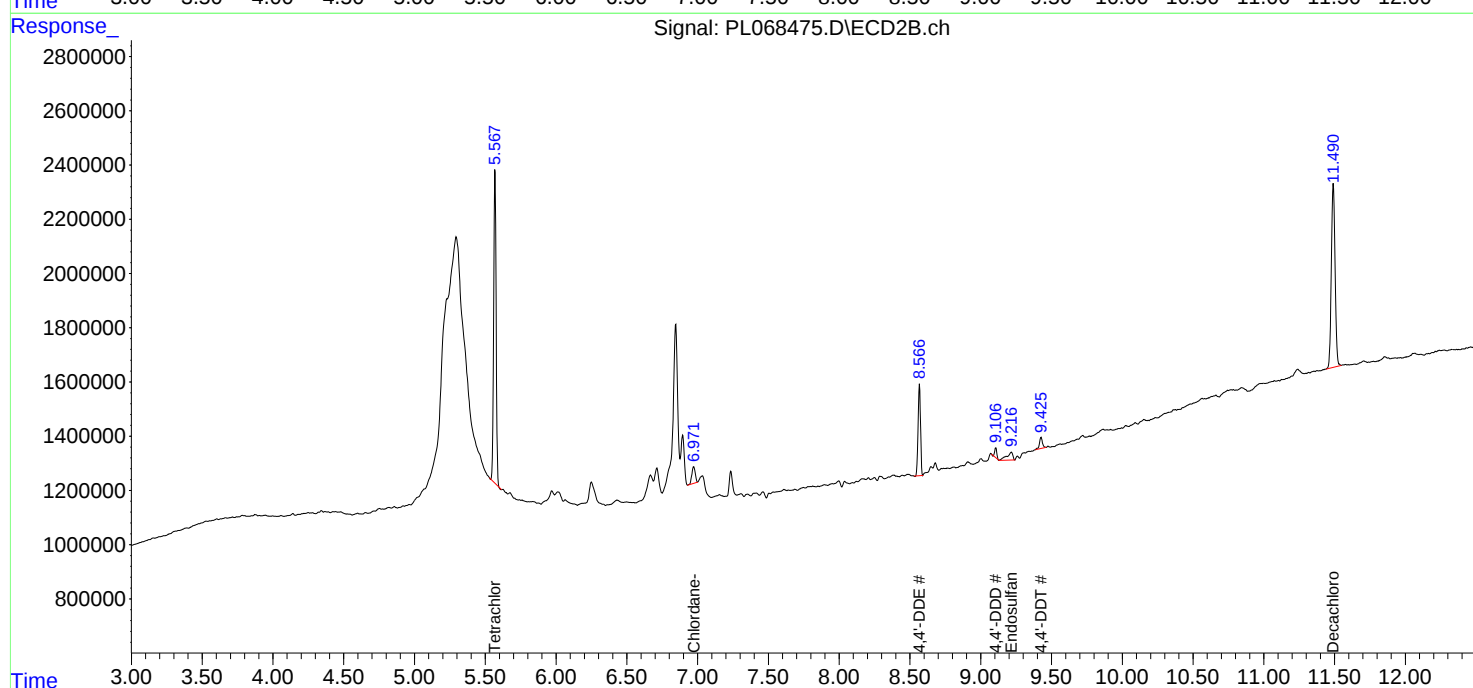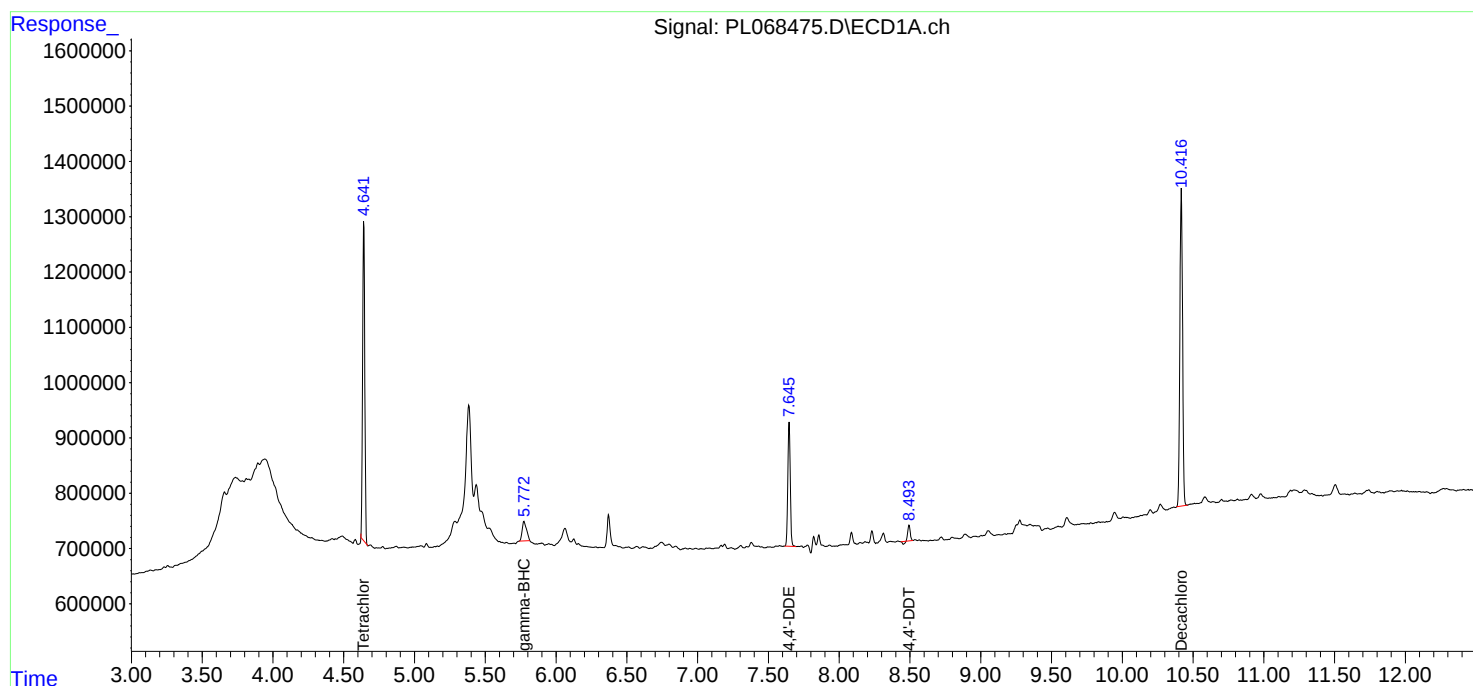


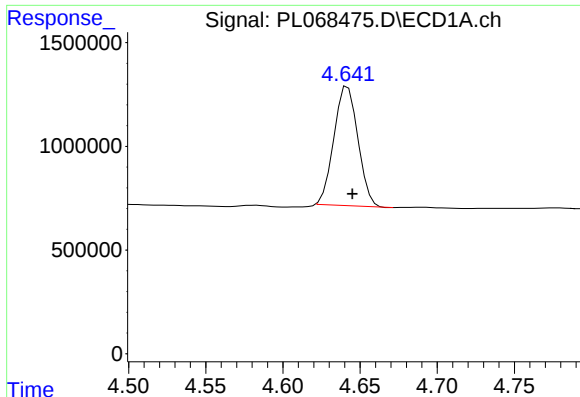

#1 Tetrachloro-m-xylene


R.T.: 4.642 min
Delta R.T.: -0.003 min
Response: 6226403
Conc: 14.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-1

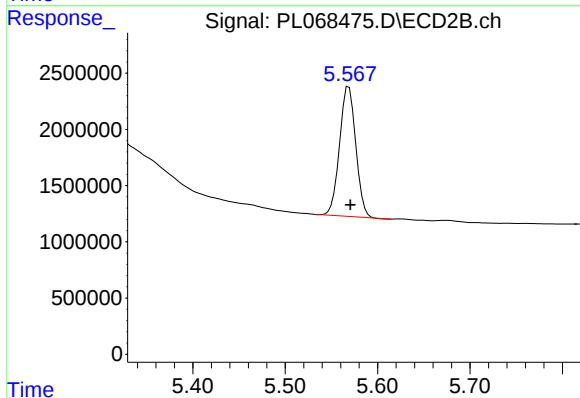


#1 Tetrachloro-m-xylene

R.T.: 5.569 min
Delta R.T.: -0.002 min
Response: 14021268
Conc: 13.74 ng/ml

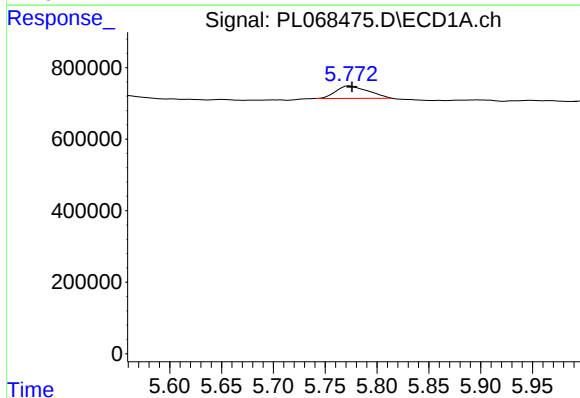


#3 gamma-BHC (Lindane)

R.T.: 5.774 min
Delta R.T.: -0.002 min
Response: 761101
Conc: 1.34 ng/ml

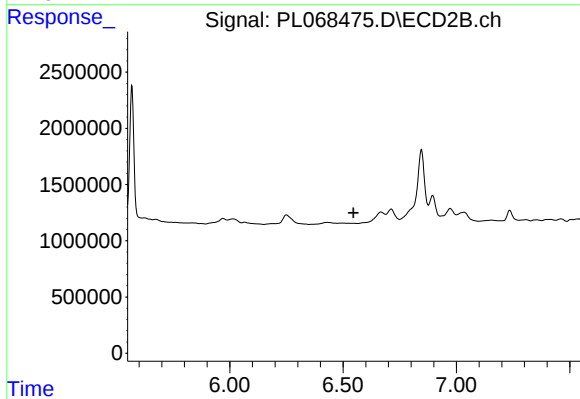

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 6.546 min
Response: 0
Conc: N.D.

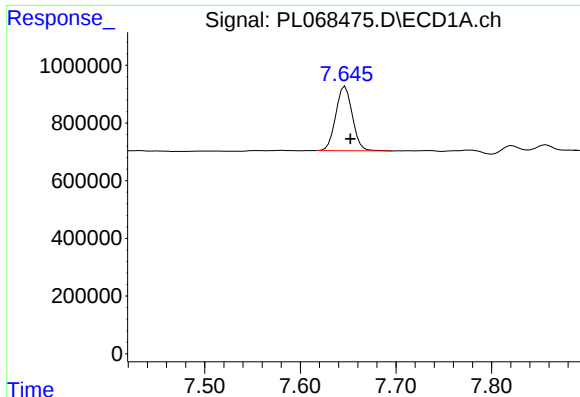

#12 4,4'-DDE


R.T.: 7.647 min
Delta R.T.: -0.006 min
Response: 2676780
Conc: 5.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-1

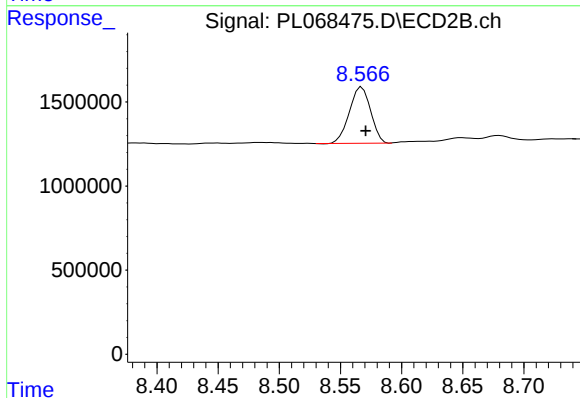


#12 4,4'-DDE

R.T.: 8.568 min
Delta R.T.: -0.003 min
Response: 4042999
Conc: 3.92 ng/ml

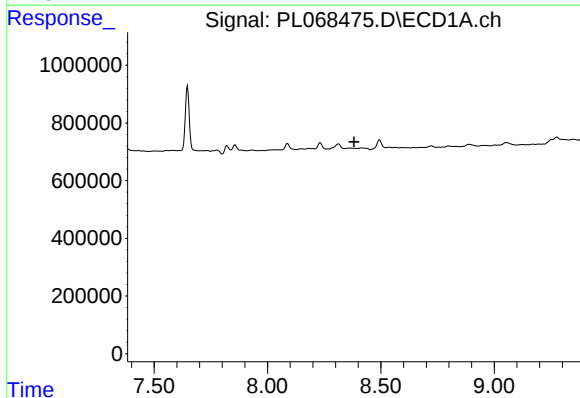


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.382 min
Response: 0
Conc: N.D.

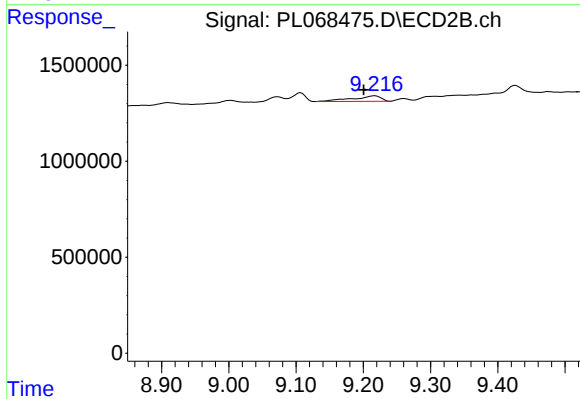

#15 Endosulfan II


R.T.: 9.217 min
Delta R.T.: 0.016 min
Response: 830141
Conc: 0.92 ng/ml

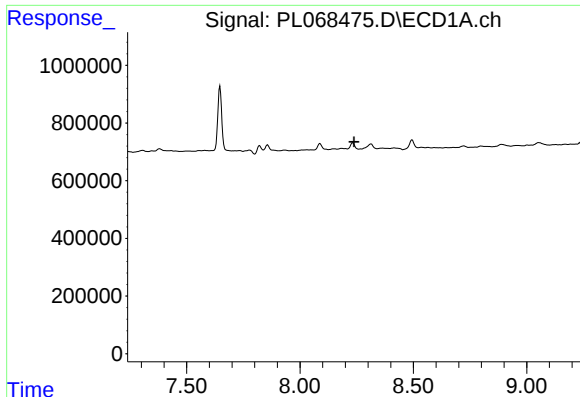

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.238 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-1

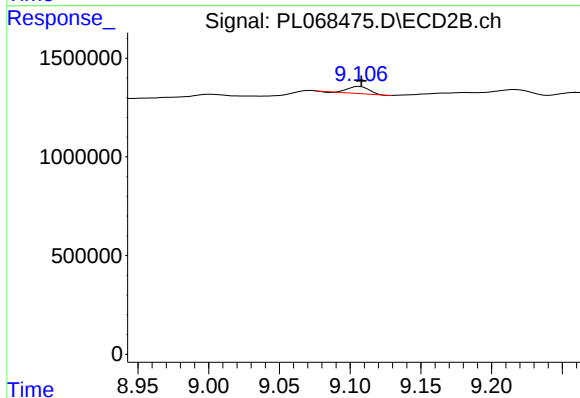


#16 4,4'-DDD

R.T.: 9.107 min
Delta R.T.: -0.001 min
Response: 376128
Conc: 0.44 ng/ml

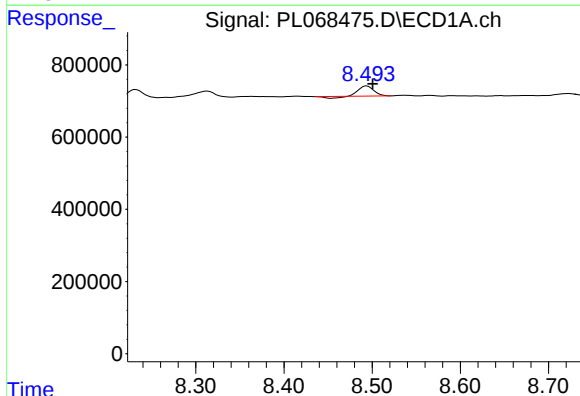


#17 4,4'-DDT

R.T.: 8.494 min
Delta R.T.: -0.006 min
Response: 292581
Conc: 0.58 ng/ml

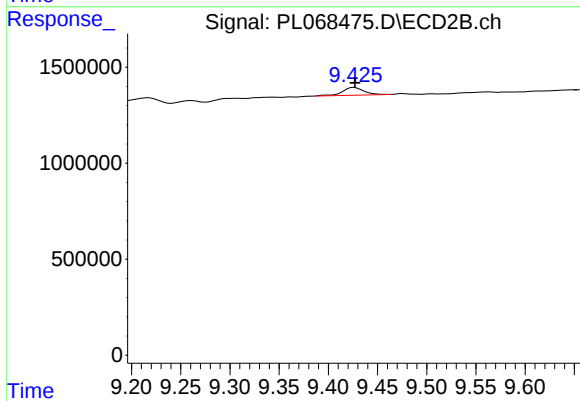

#17 4,4'-DDT


R.T.: 9.426 min
Delta R.T.: 0.000 min
Response: 605505
Conc: 0.64 ng/ml

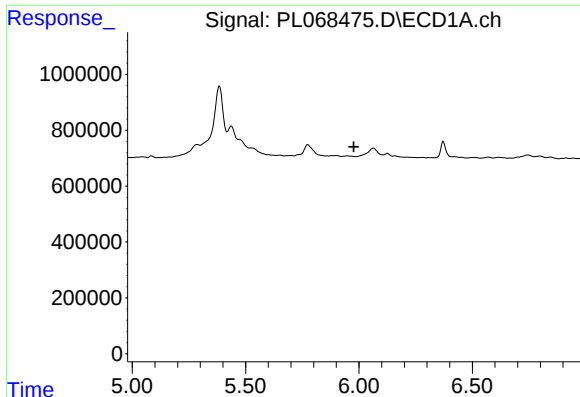

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.978 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-1

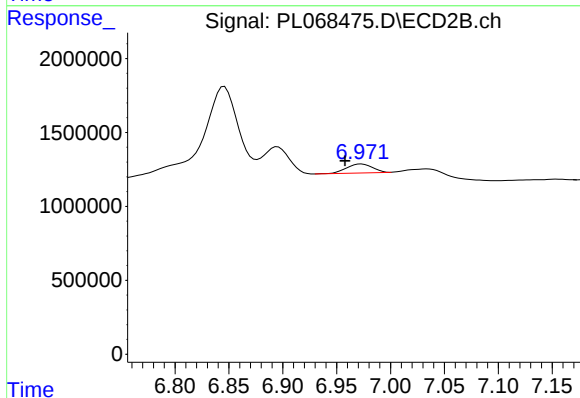


#23 Chlordane-1

R.T.: 6.973 min
Delta R.T.: 0.015 min
Response: 1014405
Conc: 25.04 ng/ml

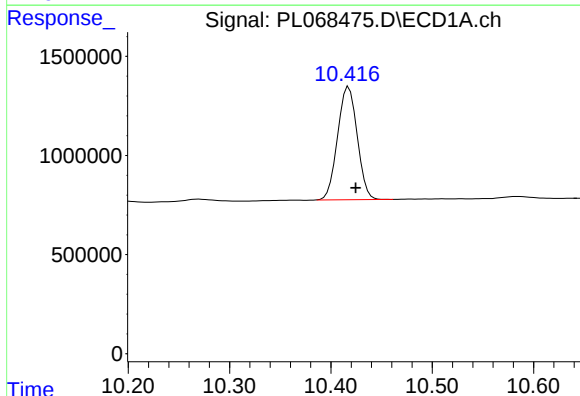

#28 Decachlorobiphenyl

R.T.: 10.418 min
Delta R.T.: -0.007 min
Response: 7681835
Conc: 13.66 ng/ml

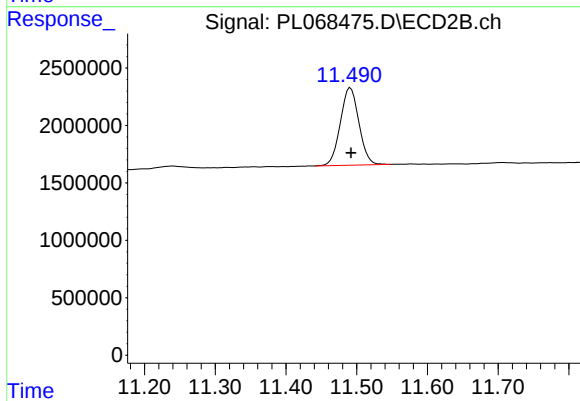

#28 Decachlorobiphenyl

R.T.: 11.491 min
Delta R.T.: 0.000 min
Response: 12344456
Conc: 13.84 ng/ml