

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072621\
 Data File : PL068477.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jul 2021 17:56
 Operator : AR\AJ
 Sample : M3165-03
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 23:16:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:44:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.642	5.569	7565730	17324364	17.628	16.978
28)	SA Decachlor...	10.416	11.491	9868495	16142195	17.546	18.097
Target Compounds							
9)	A Endosulfan I	7.512f	0.000	414270	0	0.784	N.D. #
12)	B 4,4'-DDE	0.000	8.565	0	275337	N.D.	0.267 #
13)	MA Dieldrin	7.783	0.000	435674	0	0.809	N.D. #
14)	MA Endrin	0.000	8.963	0	423880	N.D.	0.474 #
16)	A 4,4'-DDD	0.000	9.109	0	448408	N.D.	0.527 #
17)	MA 4,4'-DDT	8.489	0.000	799604	0	1.594	N.D. #
20)	A Methoxychlor	9.112f	0.000	154568	0	0.494	N.D. #
23)	Chlordane-1	0.000	6.979f	0	526803	N.D.	13.004 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072621\
Data File : PL068477.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jul 2021 17:56
Operator : AR\AJ
Sample : M3165-03
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
COMP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 23:16:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:44:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

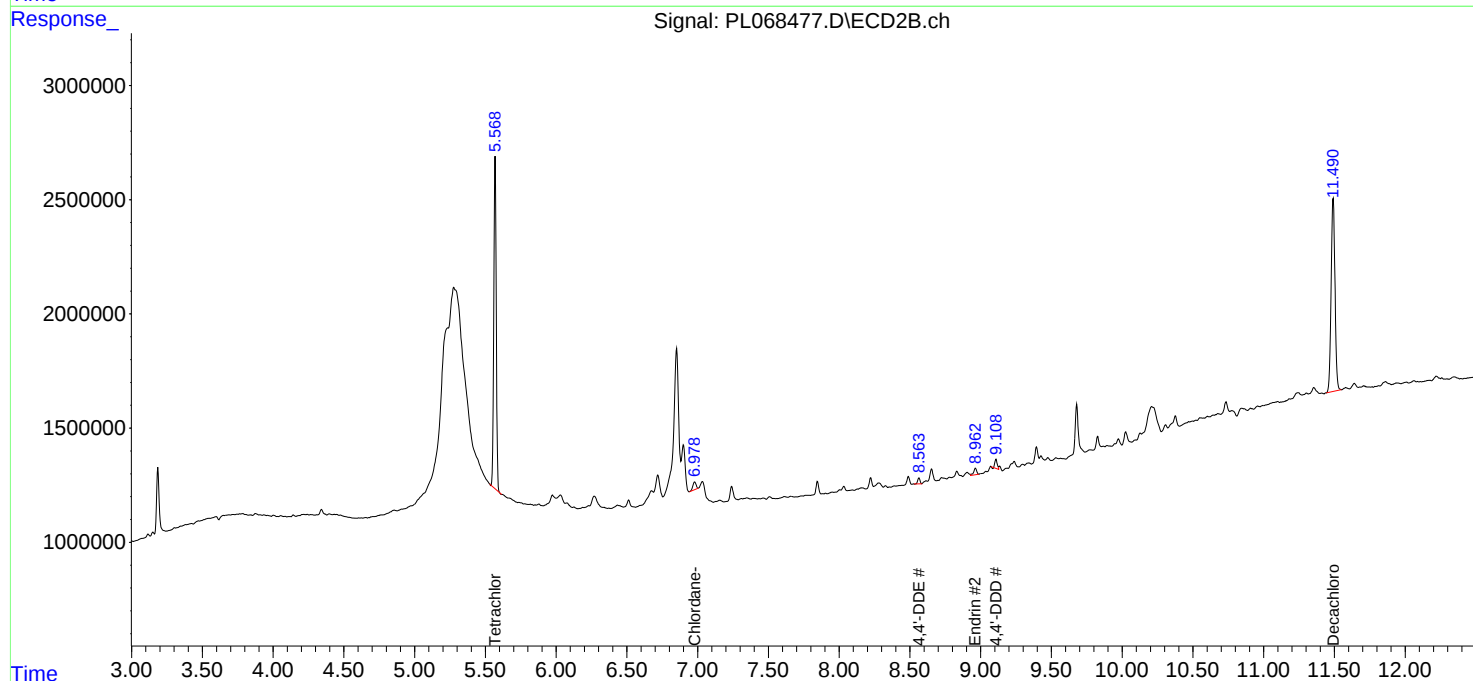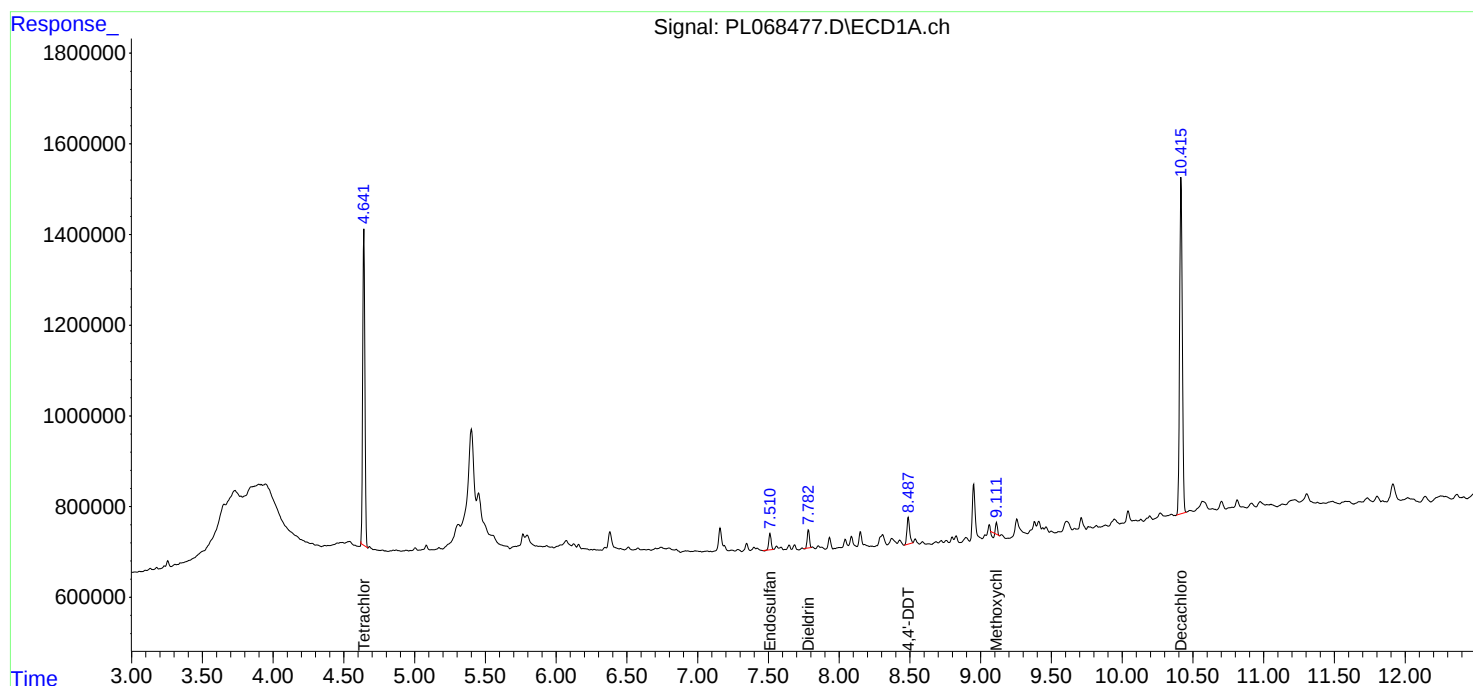


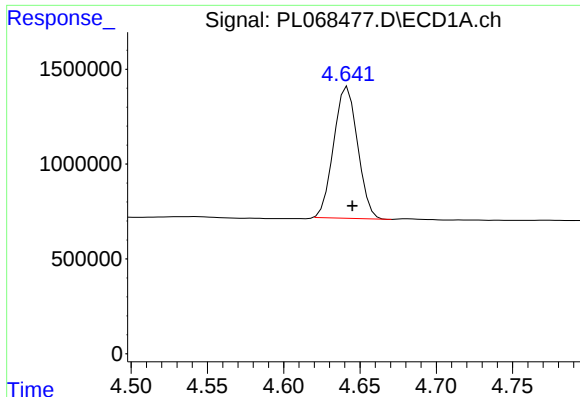

#1 Tetrachloro-m-xylene


R.T.: 4.642 min
Delta R.T.: -0.003 min
Response: 7565730
Conc: 17.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-3

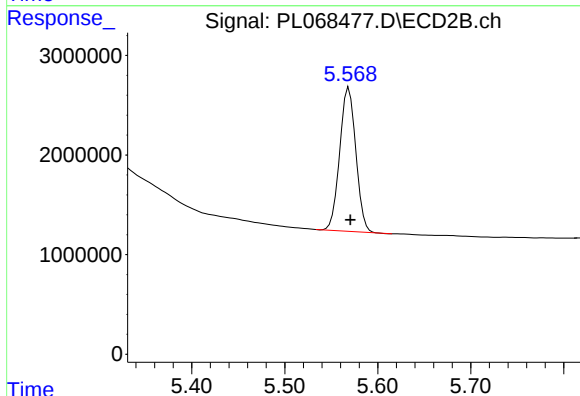


#1 Tetrachloro-m-xylene

R.T.: 5.569 min
Delta R.T.: -0.002 min
Response: 17324364
Conc: 16.98 ng/ml

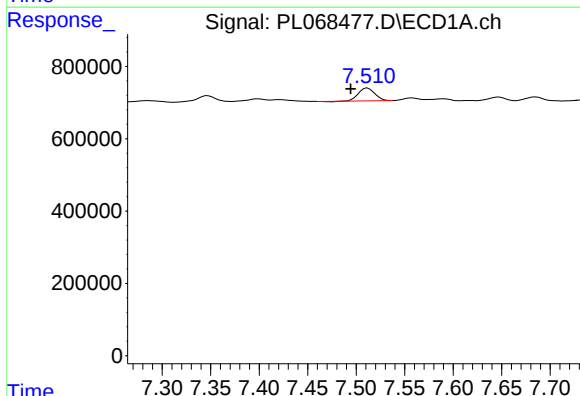


#9 Endosulfan I

R.T.: 7.512 min
Delta R.T.: 0.017 min
Response: 414270
Conc: 0.78 ng/ml

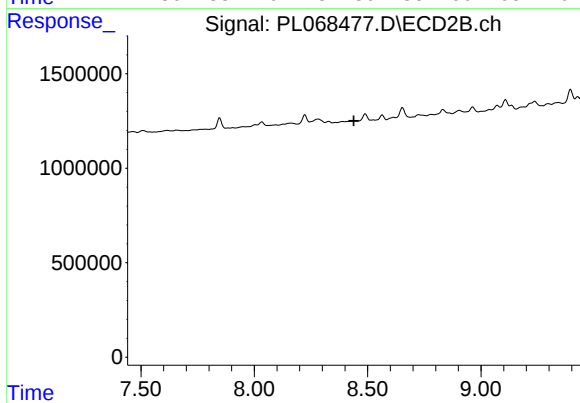

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 8.439 min
Response: 0
Conc: N.D.

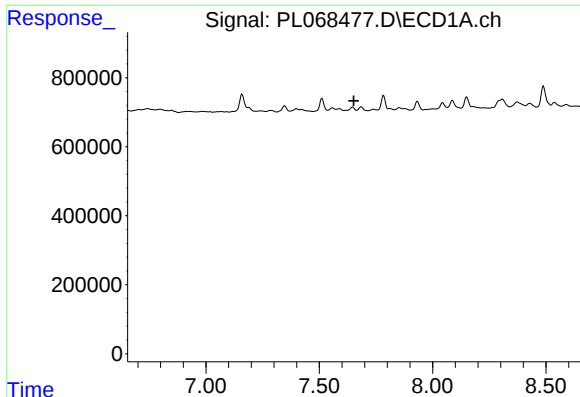

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 7.653 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-3

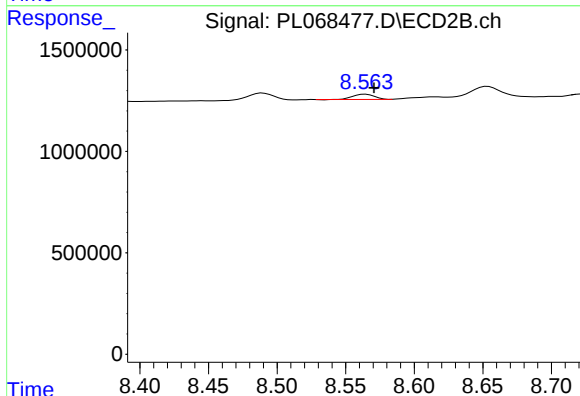


#12 4,4'-DDE

R.T.: 8.565 min
Delta R.T.: -0.006 min
Response: 275337
Conc: 0.27 ng/ml

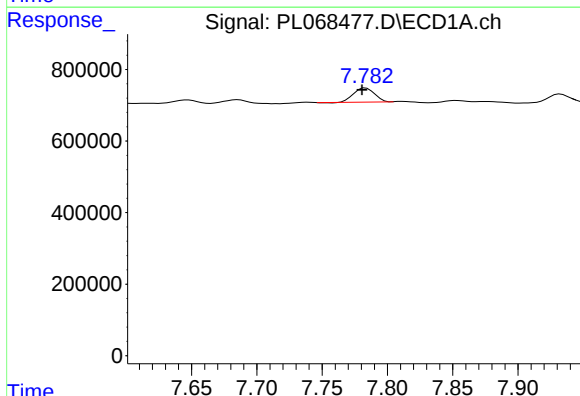


#13 Dieldrin

R.T.: 7.783 min
Delta R.T.: 0.003 min
Response: 435674
Conc: 0.81 ng/ml

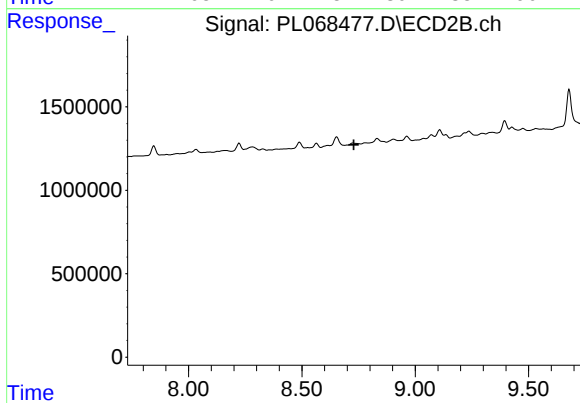

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 8.728 min
Response: 0
Conc: N.D.

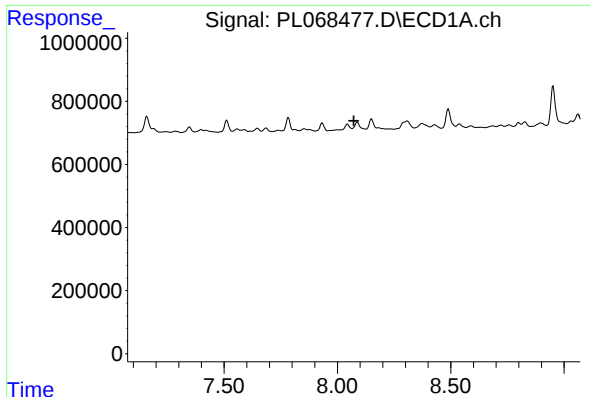

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 8.072 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-3

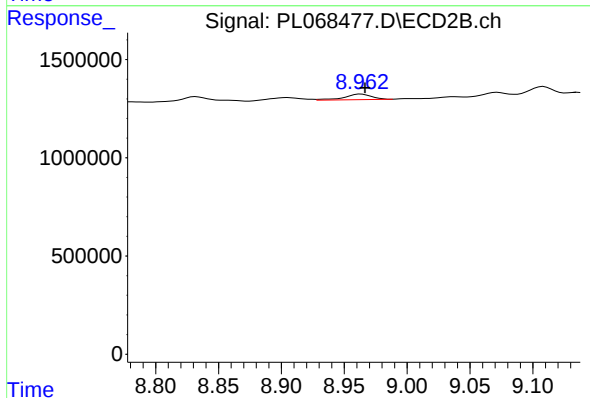


#14 Endrin

R.T.: 8.963 min
Delta R.T.: -0.003 min
Response: 423880
Conc: 0.47 ng/ml

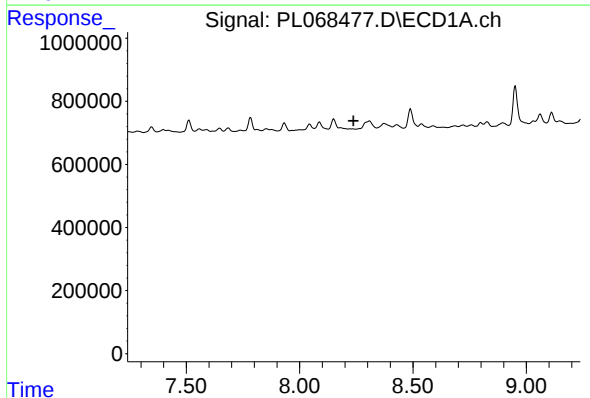


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.238 min
Response: 0
Conc: N.D.

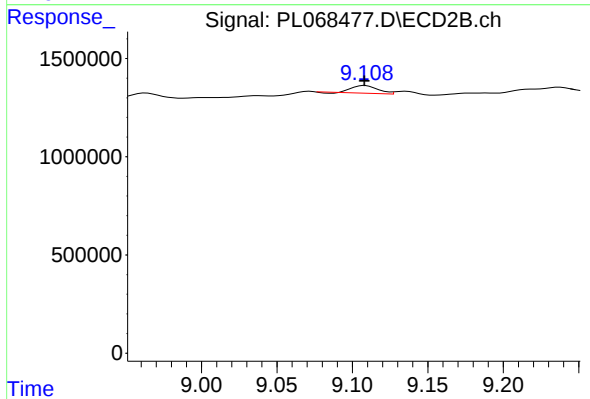

#16 4,4'-DDD


R.T.: 9.109 min
Delta R.T.: 0.000 min
Response: 448408
Conc: 0.53 ng/ml

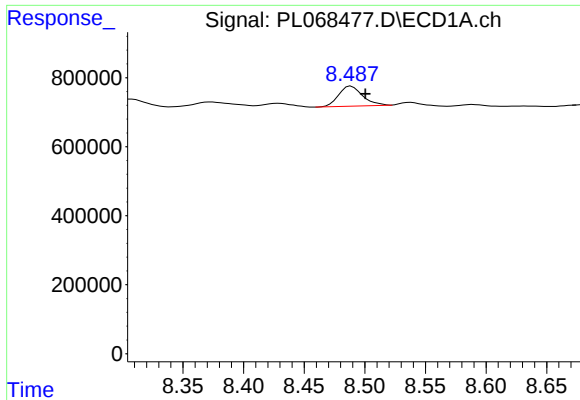

#17 4,4'-DDT


R.T.: 8.489 min
Delta R.T.: -0.012 min
Response: 799604
Conc: 1.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-3

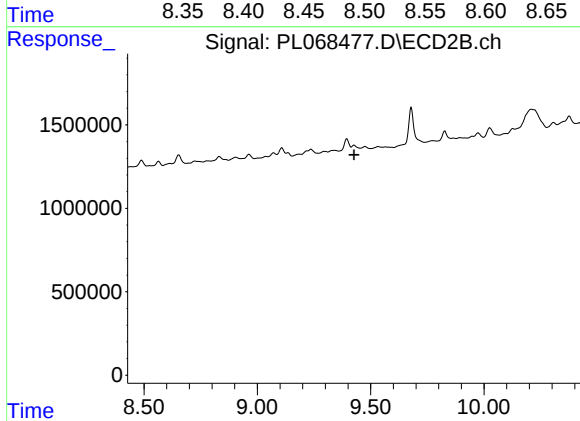


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 9.427 min
Response: 0
Conc: N.D.

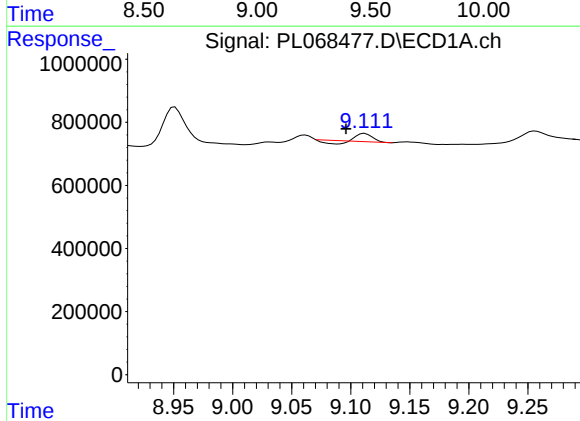


#20 Methoxychlor

R.T.: 9.112 min
Delta R.T.: 0.016 min
Response: 154568
Conc: 0.49 ng/ml

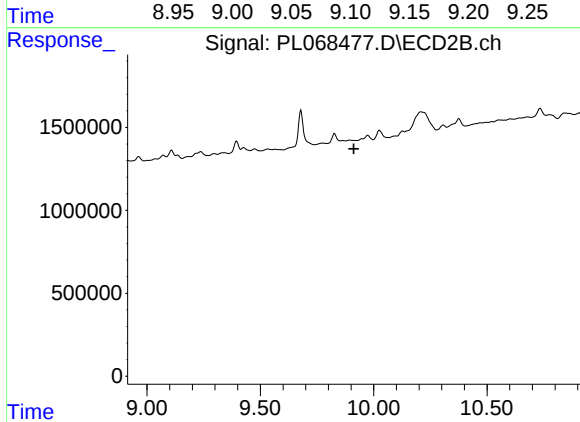

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 9.913 min
Response: 0
Conc: N.D.

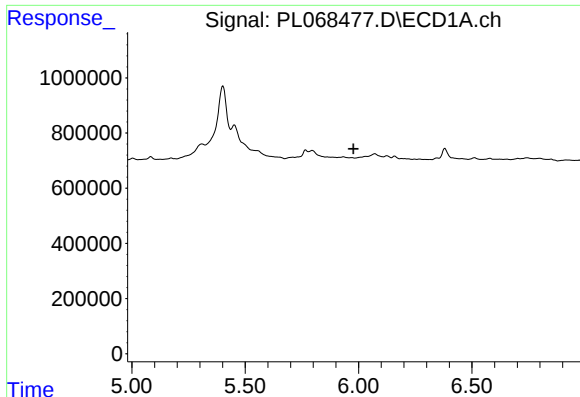

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.978 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-3

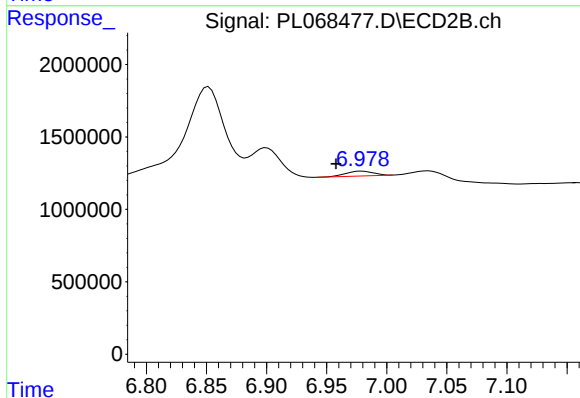


#23 Chlordane-1

R.T.: 6.979 min
Delta R.T.: 0.021 min
Response: 526803
Conc: 13.00 ng/ml

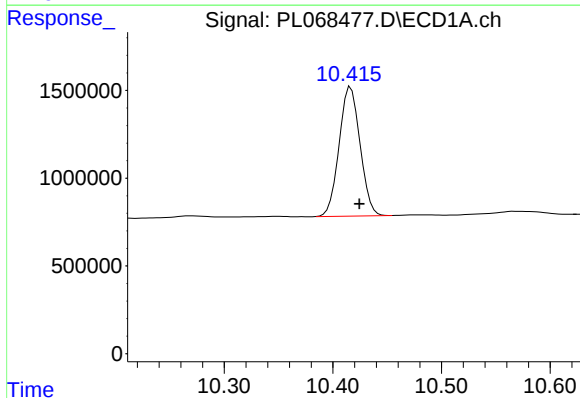

#28 Decachlorobiphenyl

R.T.: 10.416 min
Delta R.T.: -0.008 min
Response: 9868495
Conc: 17.55 ng/ml

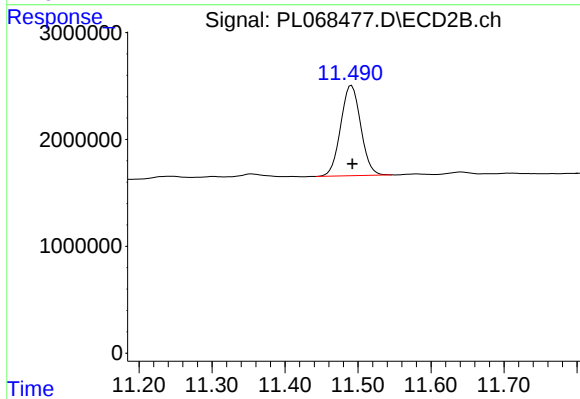

#28 Decachlorobiphenyl

R.T.: 11.491 min
Delta R.T.: -0.001 min
Response: 16142195
Conc: 18.10 ng/ml