

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072621\
 Data File : PL068481.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jul 2021 19:03
 Operator : AR\AJ
 Sample : M3175-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-BPM-03-025-ABCD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 23:17:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:44:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.641	5.569	8810708	20638114	20.529	20.225
28)	SA Decachlor...	10.416	11.491	11187132	18842949	19.891	21.125
Target Compounds							
3)	MA gamma-BHC...	5.786	0.000	482416	0	0.849	N.D. #
23)	Chlordane-1	0.000	6.976f	0	753882	N.D.	18.610 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072621\
Data File : PL068481.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jul 2021 19:03
Operator : AR\AJ
Sample : M3175-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
FK-BPM-03-025-ABCD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 23:17:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:44:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

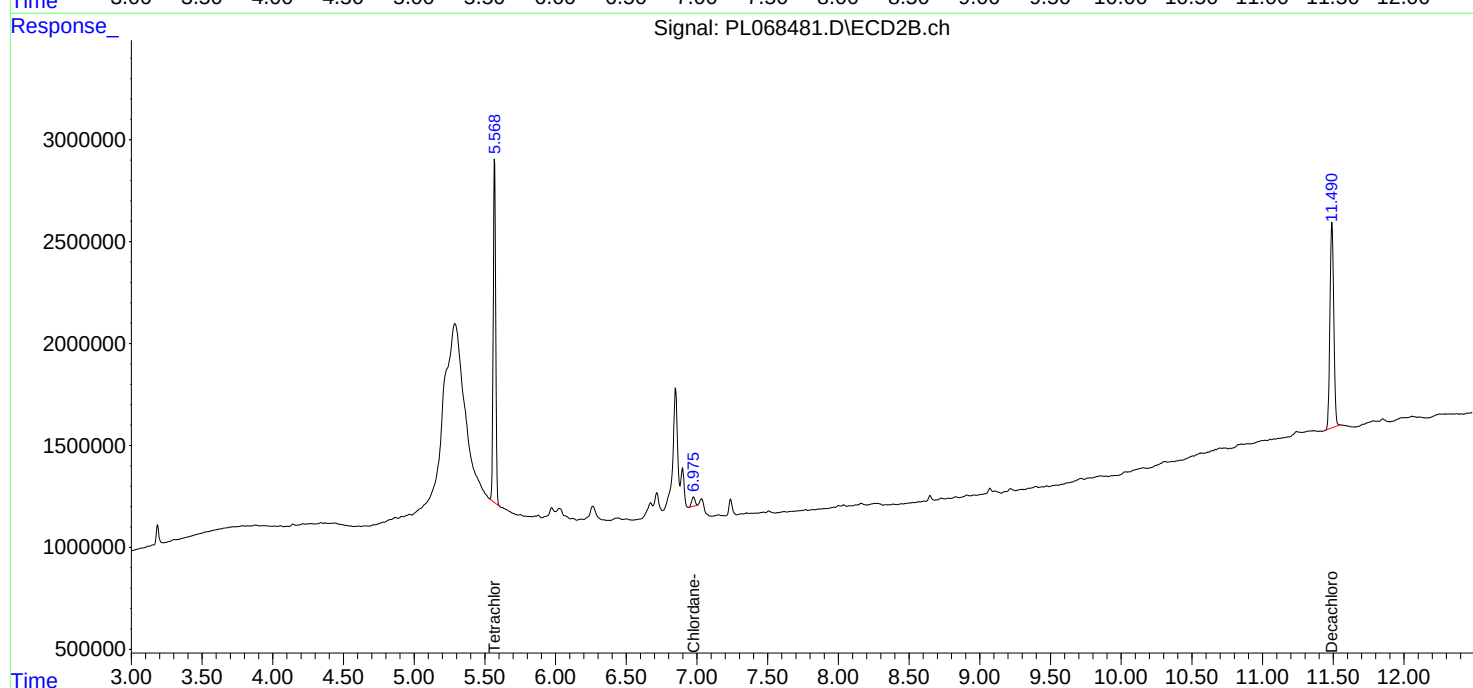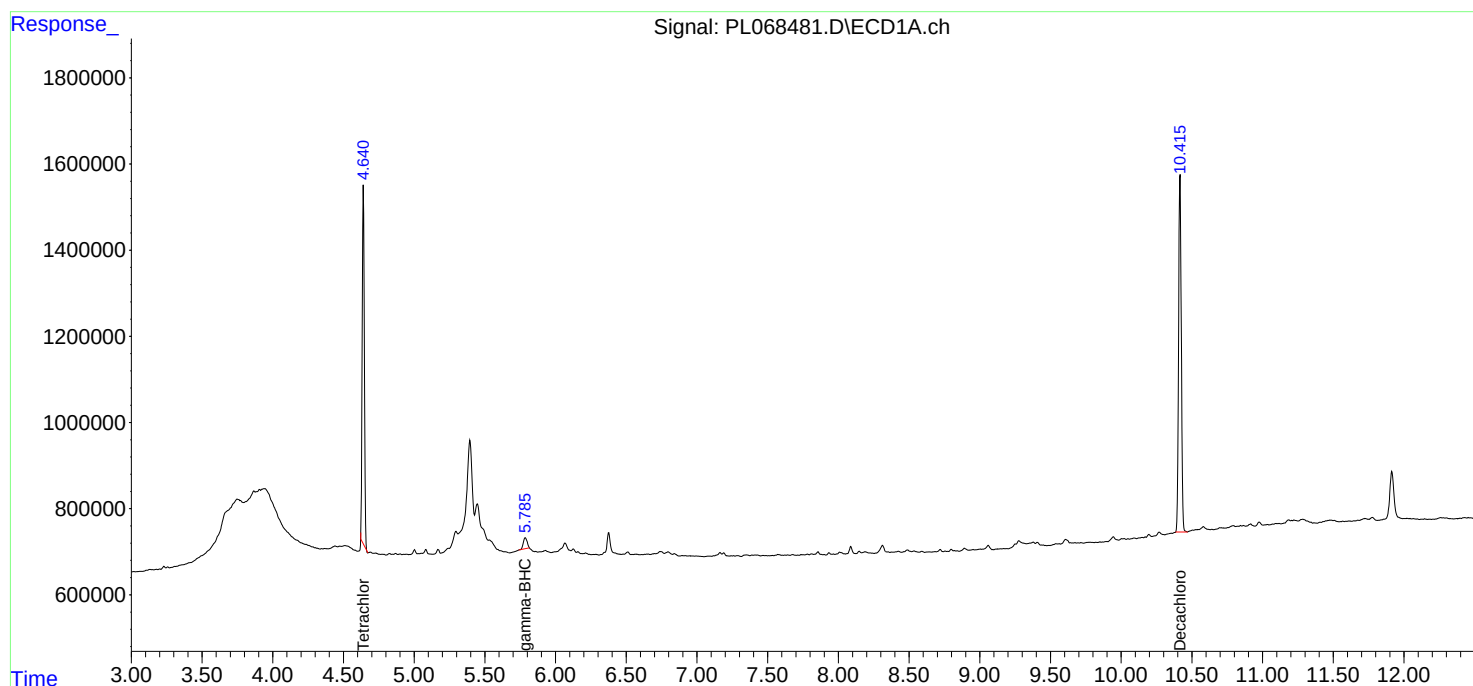


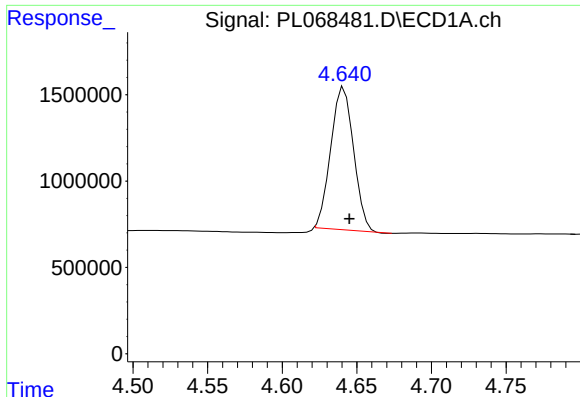

#1 Tetrachloro-m-xylene


R.T.: 4.641 min
Delta R.T.: -0.003 min
Response: 8810708
Conc: 20.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-BPM-03-025-ABCD

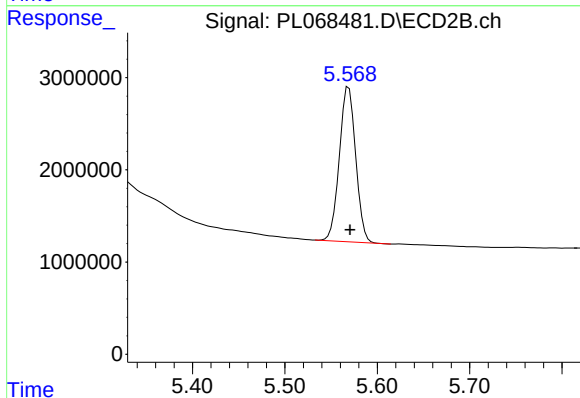


#1 Tetrachloro-m-xylene

R.T.: 5.569 min
Delta R.T.: -0.002 min
Response: 20638114
Conc: 20.22 ng/ml

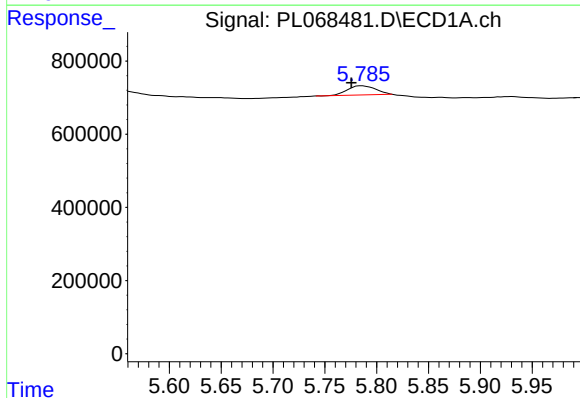


#3 gamma-BHC (Lindane)

R.T.: 5.786 min
Delta R.T.: 0.010 min
Response: 482416
Conc: 0.85 ng/ml

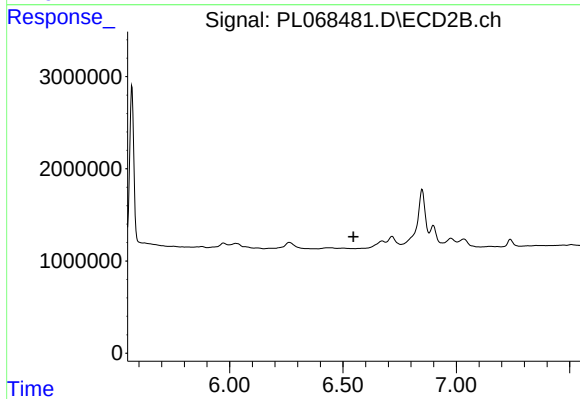

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 6.546 min
Response: 0
Conc: N.D.

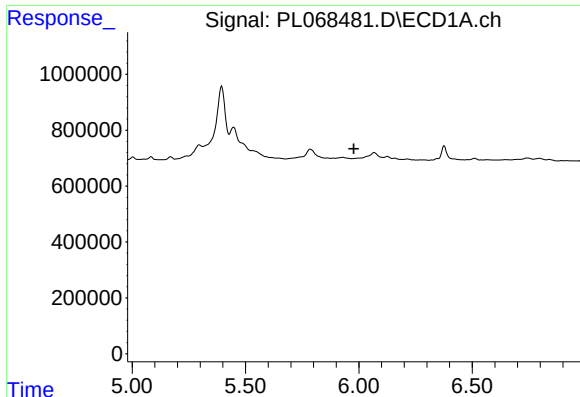

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.978 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
FK-BPM-03-025-ABCD

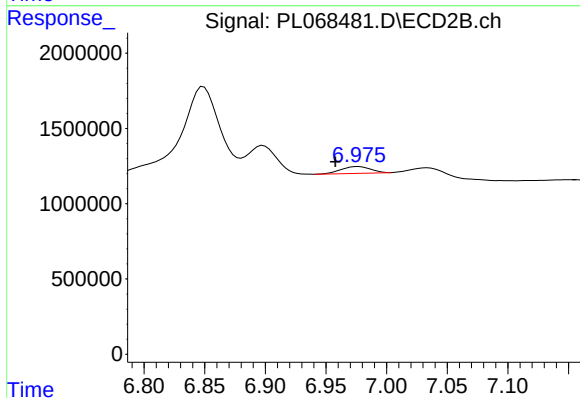


#23 Chlordane-1

R.T.: 6.976 min
Delta R.T.: 0.019 min
Response: 753882
Conc: 18.61 ng/ml

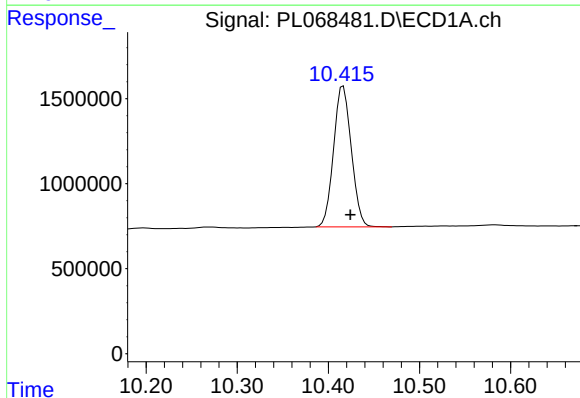

#28 Decachlorobiphenyl

R.T.: 10.416 min
Delta R.T.: -0.008 min
Response: 11187132
Conc: 19.89 ng/ml

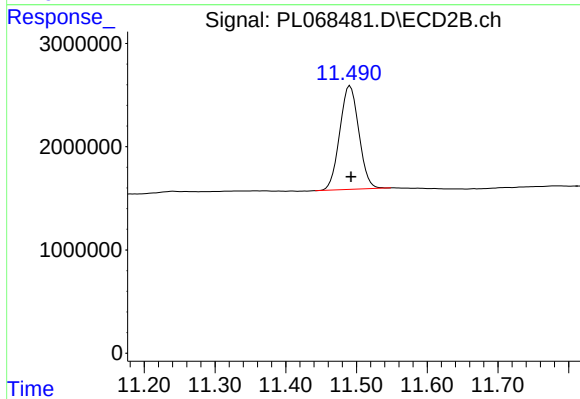

#28 Decachlorobiphenyl

R.T.: 11.491 min
Delta R.T.: -0.001 min
Response: 18842949
Conc: 21.12 ng/ml