

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072621\
 Data File : PL068479.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jul 2021 18:29
 Operator : AR\AJ
 Sample : M3171-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-PS-01-078

Manual Integrations
 APPROVED

Ankita
 7/27/2021 4:52:29 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 27 08:46:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:44:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.642	5.570	5136326	11232612	11.968	11.008
28) SA Decachlor...	10.417	11.491	5510205	8446997	9.797	9.470
Target Compounds						
10) B gamma-Chl...	7.364	8.301	332201	701540	0.579	0.623
11) B alpha-Chl...	7.433	8.384	551841	1395089	0.961	1.240 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072621\
Data File : PL068479.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jul 2021 18:29
Operator : AR\AJ
Sample : M3171-01
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
FK-PS-01-078


Manual Integrations
APPROVED

Ankita
7/27/2021 4:52:29 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 27 08:46:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:44:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

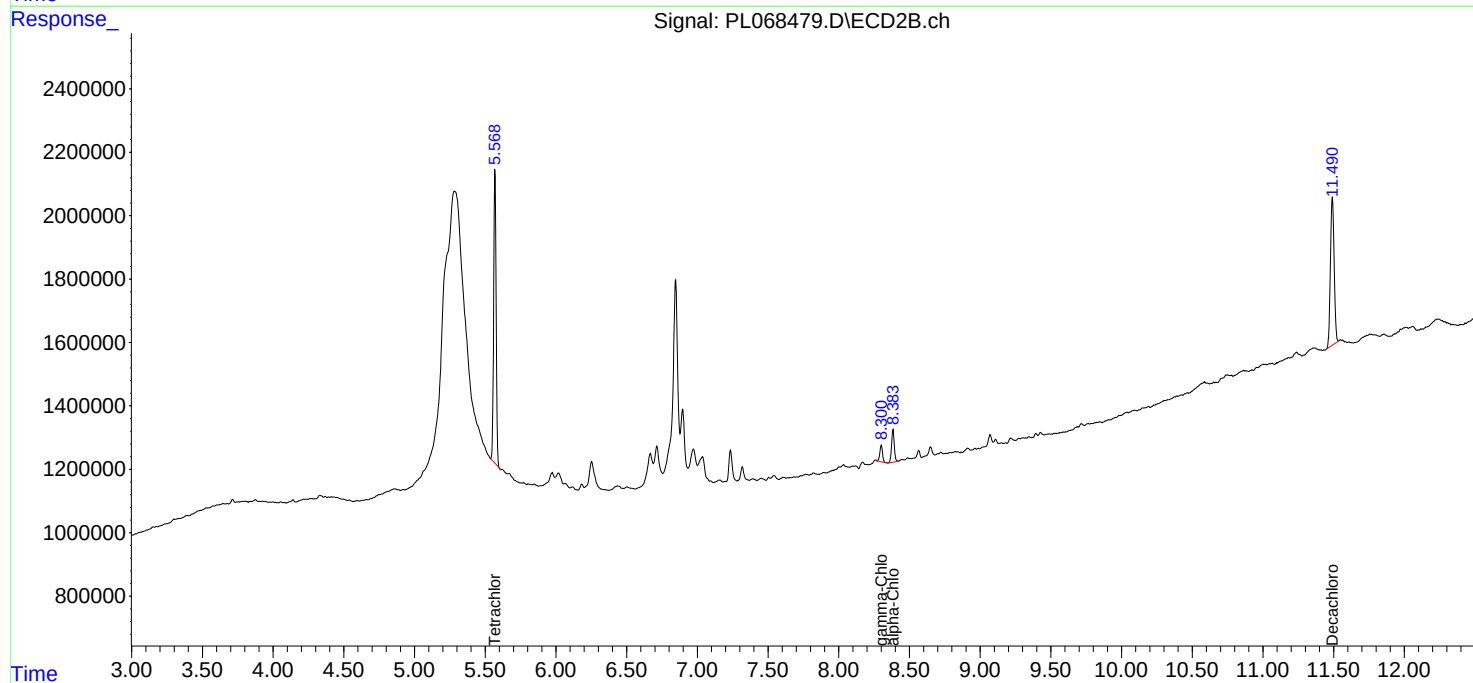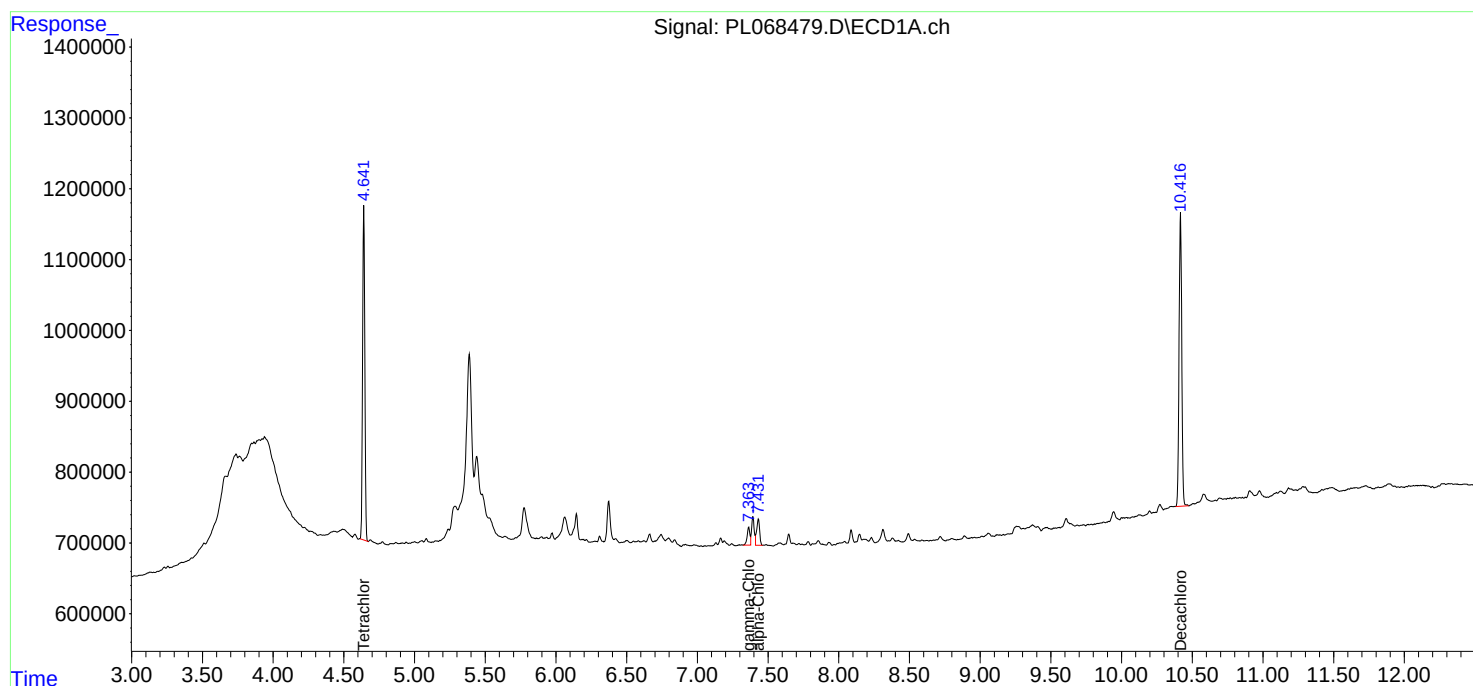

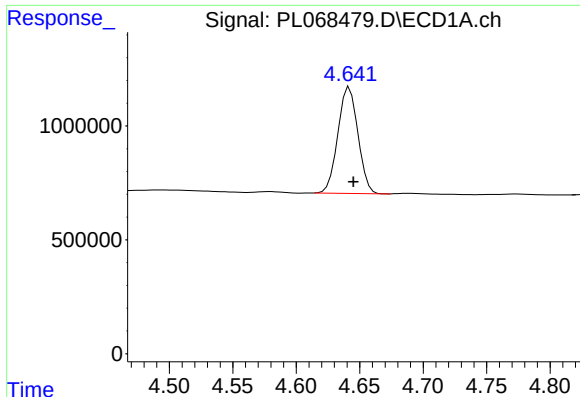


#1 Tetrachloro-m-xylene

R.T.: 4.642 min
Delta R.T.: -0.003 min
Response: 5136326
Conc: 11.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-078


Manual Integrations
APPROVED

Ankita
7/27/2021 4:52:29 PM

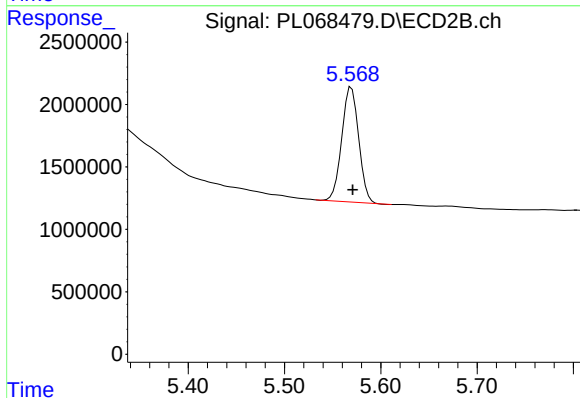


#1 Tetrachloro-m-xylene

R.T.: 5.570 min
Delta R.T.: -0.001 min
Response: 11232612
Conc: 11.01 ng/ml

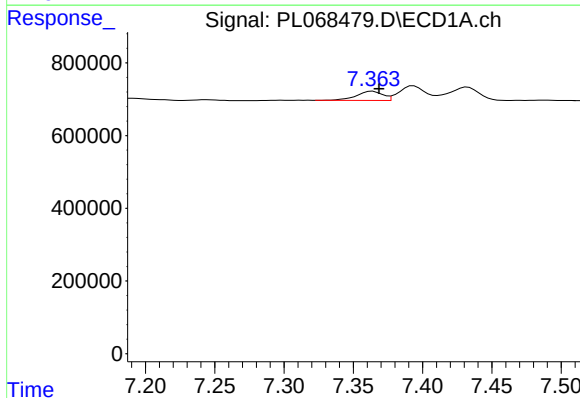


#10 gamma-Chlordane

R.T.: 7.364 min
Delta R.T.: -0.005 min
Response: 332201
Conc: 0.58 ng/ml

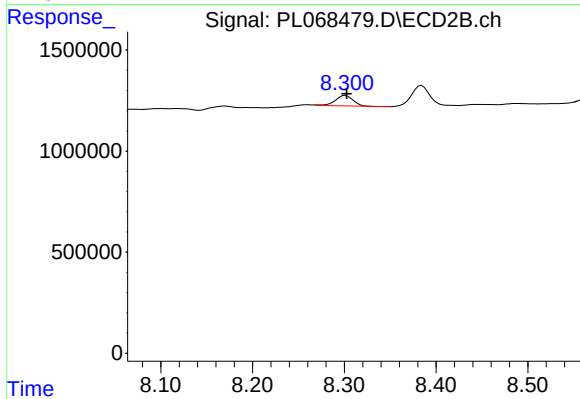

#10 gamma-Chlordane

R.T.: 8.301 min
Delta R.T.: -0.001 min
Response: 701540
Conc: 0.62 ng/ml

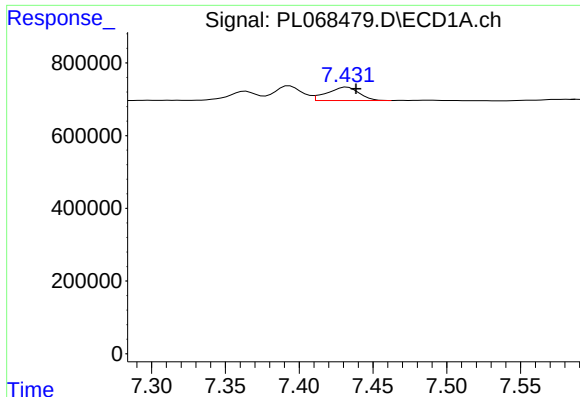


#11 alpha-Chlordane

R.T.: 7.433 min
Delta R.T.: -0.006 min
Response: 551841
Conc: 0.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-078


Manual Integrations
APPROVED

Ankita
7/27/2021 4:52:29 PM

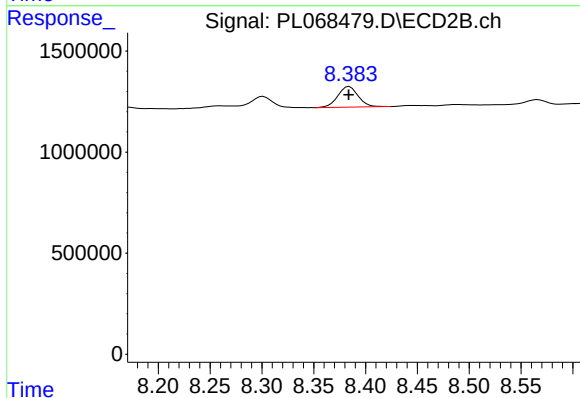


#11 alpha-Chlordane

R.T.: 8.384 min
Delta R.T.: 0.000 min
Response: 1395089
Conc: 1.24 ng/ml

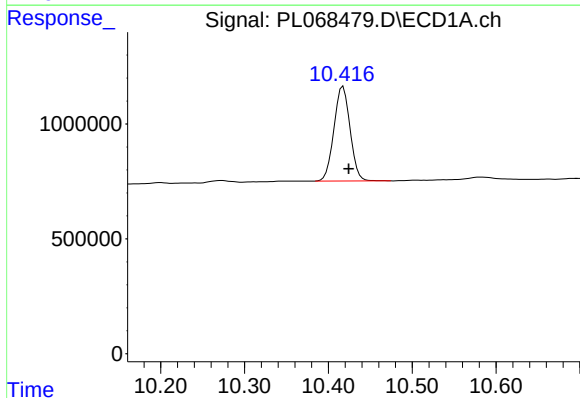

#28 Decachlorobiphenyl

R.T.: 10.417 min
Delta R.T.: -0.007 min
Response: 5510205
Conc: 9.80 ng/ml

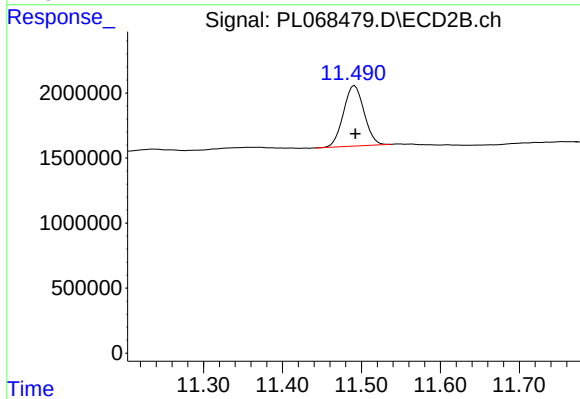

#28 Decachlorobiphenyl

R.T.: 11.491 min
Delta R.T.: 0.000 min
Response: 8446997
Conc: 9.47 ng/ml