

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072622\
 Data File : PL076626.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jul 2022 03:37
 Operator : AR\AJ
 Sample : PB141146BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 07:34:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 26 05:22:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.420	2.641	17258532	47651718	16.723	16.065
28)	SA Decachlor...	8.909	7.748	16311057	45766648	18.494	17.830
Target Compounds							
2)	A alpha-BHC	0.000	3.133	0	371361	N.D.	0.089 #
3)	MA gamma-BHC...	4.223	3.458	173038	135891	0.128	0.036 #
10)	B gamma-Chl...	0.000	4.817	0	201837	N.D.	0.063 #
13)	MA Dieldrin	0.000	5.194	0	743069	N.D.	0.239 #
14)	MA Endrin	0.000	5.494f	0	233558	N.D.	0.093 #
15)	B Endosulfa...	6.708f	0.000	236577	0	0.264	N.D. #
21)	B Endrin ke...	7.571f	0.000	625935	0	0.612	N.D. #
25)	Chlordane-3	0.000	4.817	0	201837	N.D.	0.713 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072622\
Data File : PL076626.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jul 2022 03:37
Operator : AR\AJ
Sample : PB141146BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 07:34:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072622.M
Quant Title : GC Extractables
QLast Update : Tue Jul 26 05:22:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

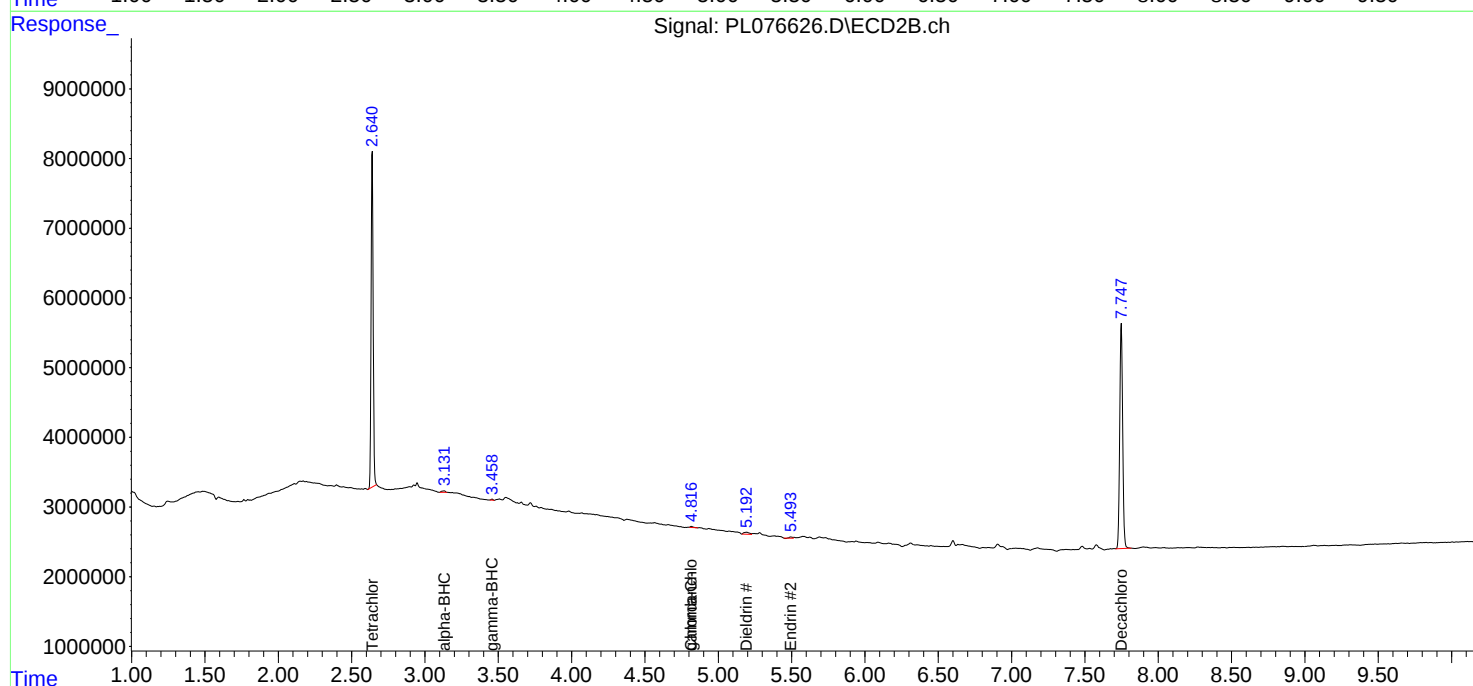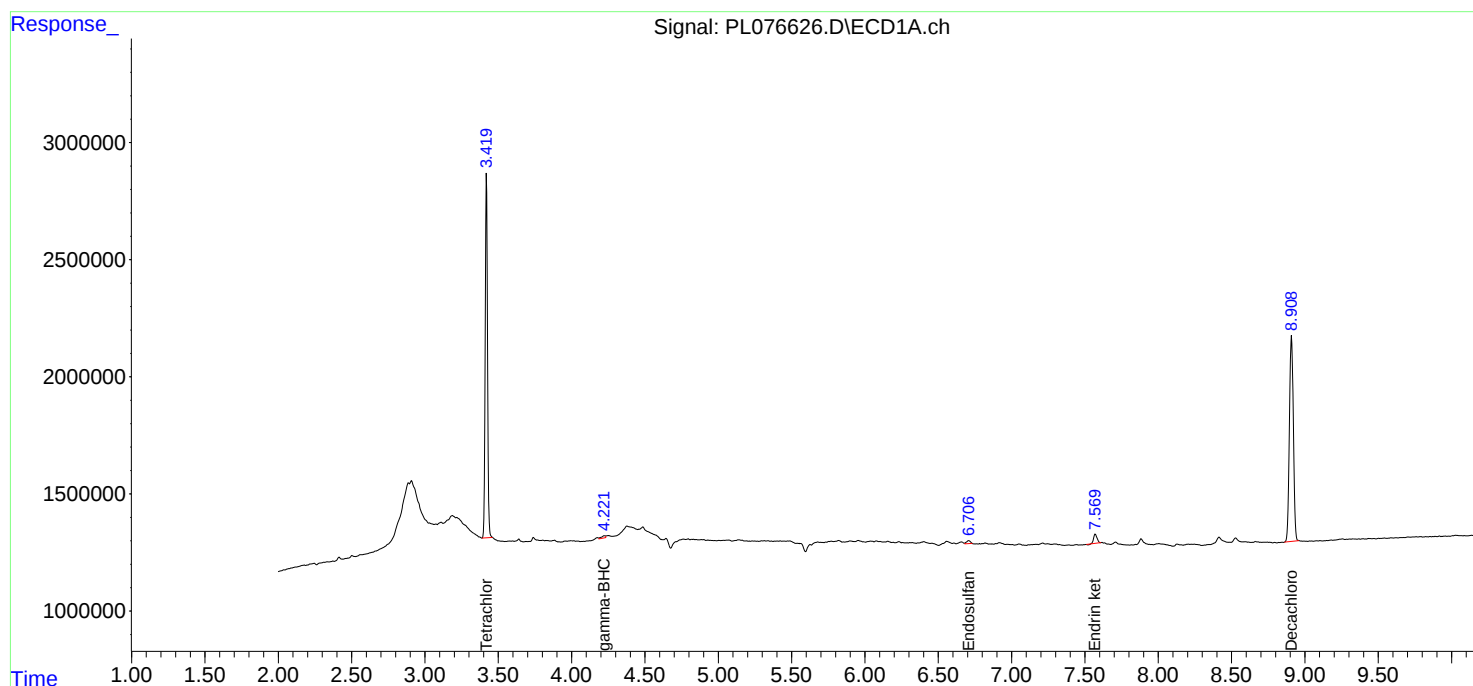


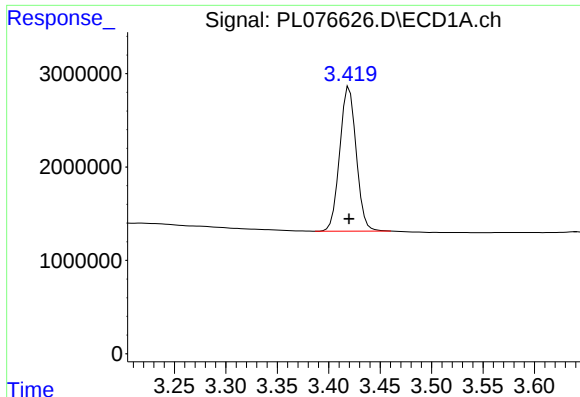

#1 Tetrachloro-m-xylene


R.T.: 3.420 min
Delta R.T.: 0.000 min
Response: 17258532
Conc: 16.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

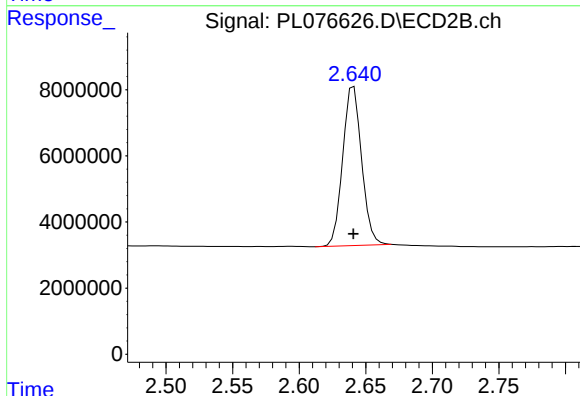


#1 Tetrachloro-m-xylene

R.T.: 2.641 min
Delta R.T.: 0.000 min
Response: 47651718
Conc: 16.06 ng/ml

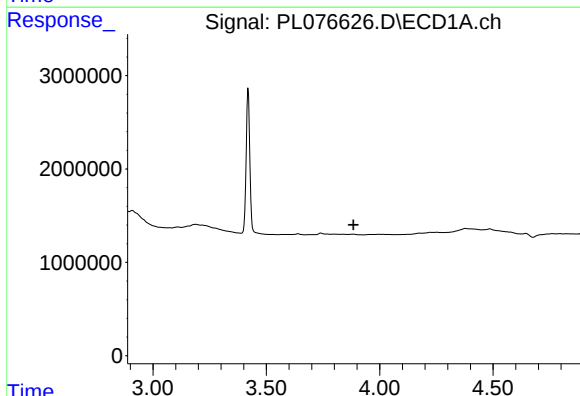


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.885 min
Response: 0
Conc: N.D.

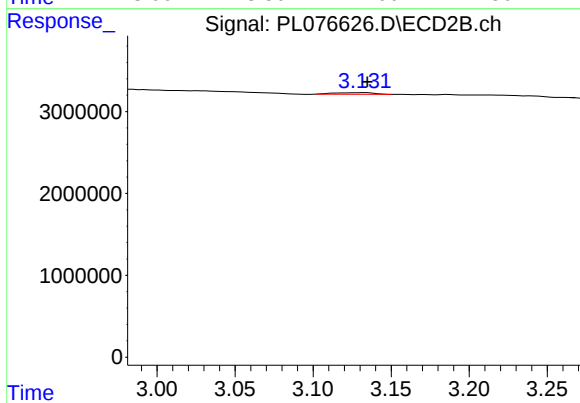

#2 alpha-BHC


R.T.: 3.133 min
Delta R.T.: -0.002 min
Response: 371361
Conc: 0.09 ng/ml

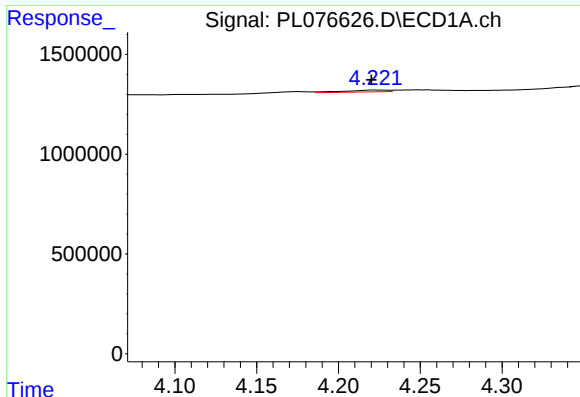

#3 gamma-BHC (Lindane)


R.T.: 4.223 min
Delta R.T.: 0.002 min
Response: 173038
Conc: 0.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

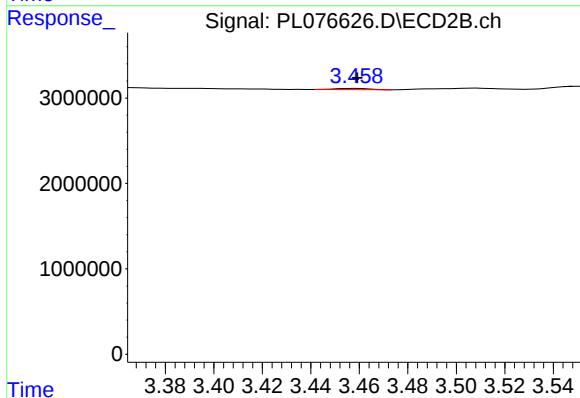


#3 gamma-BHC (Lindane)

R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 135891
Conc: 0.04 ng/ml

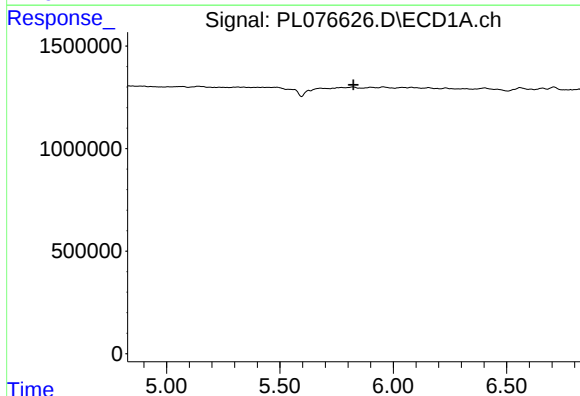


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.825 min
Response: 0
Conc: N.D.

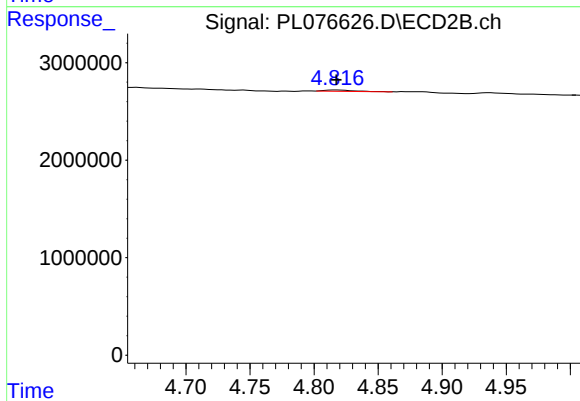

#10 gamma-Chlordane


R.T.: 4.817 min
Delta R.T.: 0.000 min
Response: 201837
Conc: 0.06 ng/ml

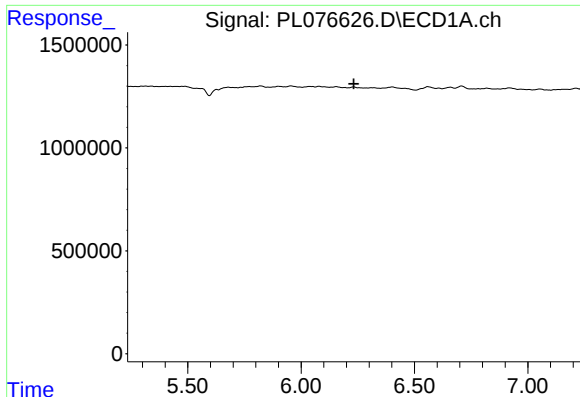

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.233 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

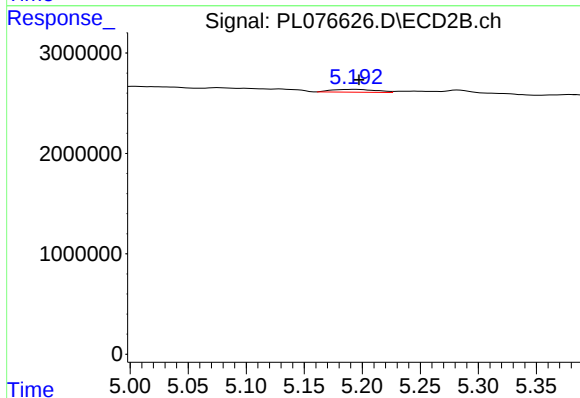


#13 Dieldrin

R.T.: 5.194 min
Delta R.T.: -0.003 min
Response: 743069
Conc: 0.24 ng/ml

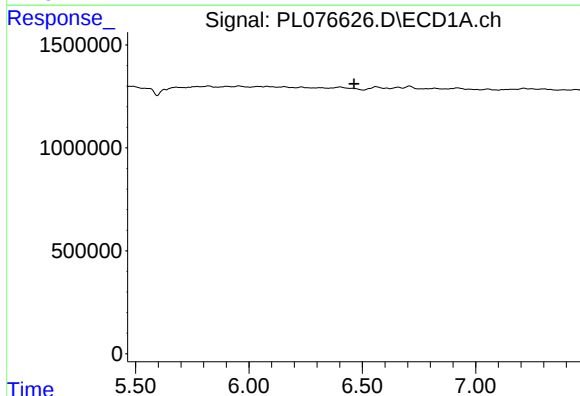


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.464 min
Response: 0
Conc: N.D.

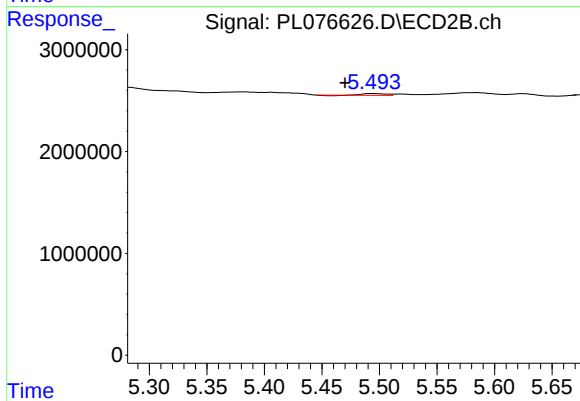

#14 Endrin


R.T.: 5.494 min
Delta R.T.: 0.024 min
Response: 233558
Conc: 0.09 ng/ml

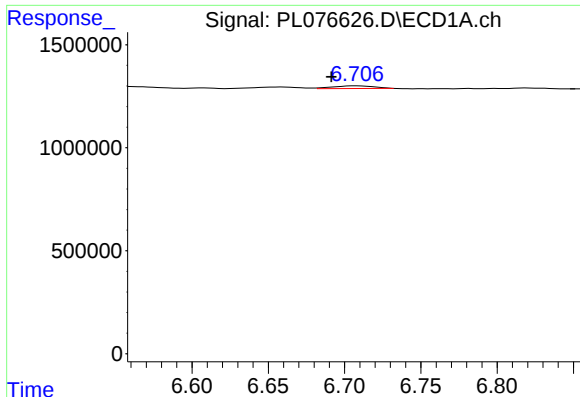

#15 Endosulfan II


R.T.: 6.708 min
Delta R.T.: 0.016 min
Response: 236577
Conc: 0.26 ng/ml

Instrument :
ECD_L
ClientSampleId :

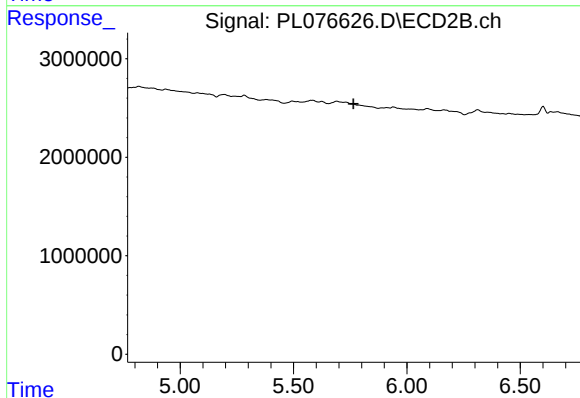


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.765 min
Response: 0
Conc: N.D.

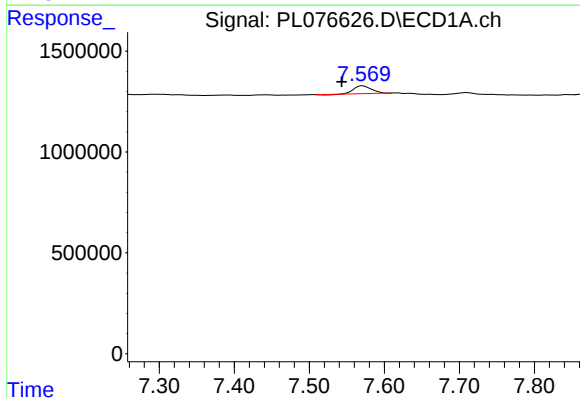


#21 Endrin ketone

R.T.: 7.571 min
Delta R.T.: 0.027 min
Response: 625935
Conc: 0.61 ng/ml

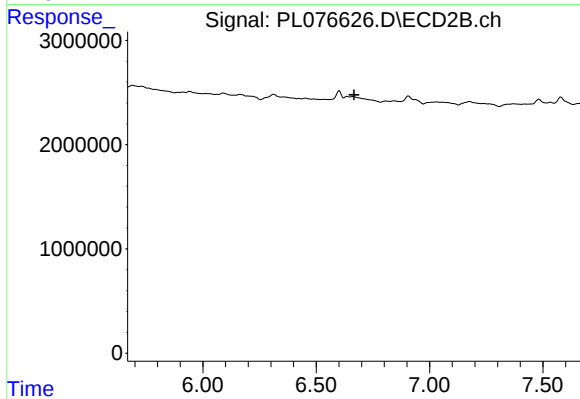

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 6.667 min
Response: 0
Conc: N.D.

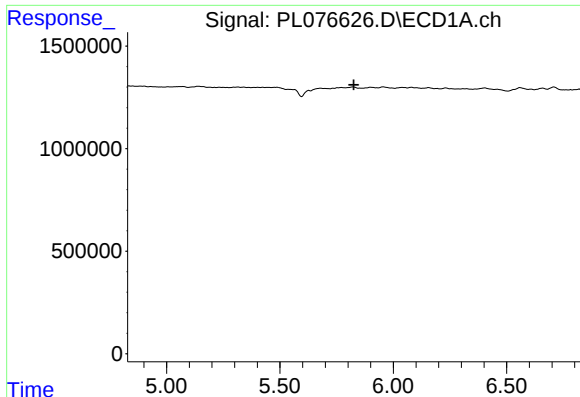

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.825 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

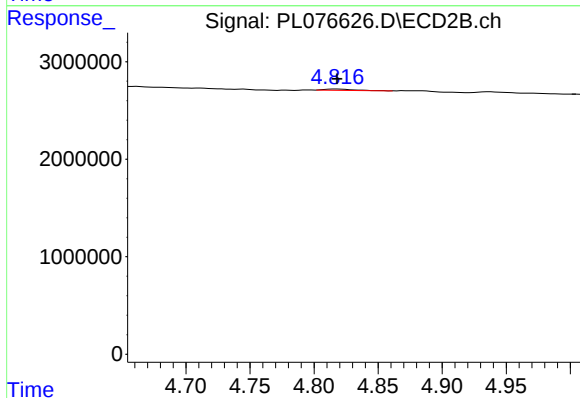


#25 Chlordane-3

R.T.: 4.817 min
Delta R.T.: 0.000 min
Response: 201837
Conc: 0.71 ng/ml

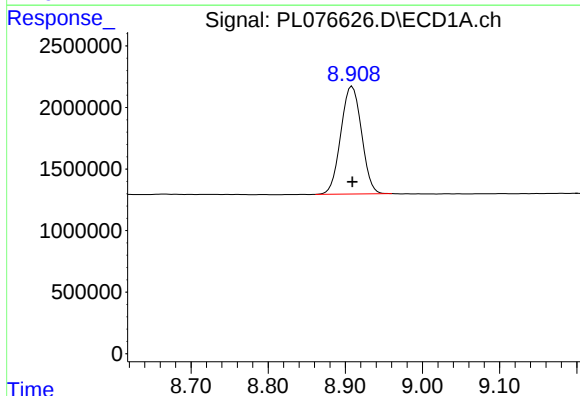

#28 Decachlorobiphenyl

R.T.: 8.909 min
Delta R.T.: 0.000 min
Response: 16311057
Conc: 18.49 ng/ml

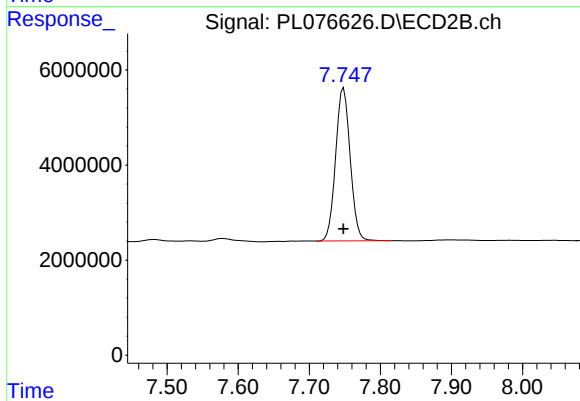

#28 Decachlorobiphenyl

R.T.: 7.748 min
Delta R.T.: 0.000 min
Response: 45766648
Conc: 17.83 ng/ml