

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072622\
 Data File : PL076610.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jul 2022 23:41
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 02:02:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 26 02:01:57 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.420	2.641	95450879	314.2E6	98.808	97.900
28)	SA Decachlor...	8.908	7.748	73325166	217.9E6	94.925	95.096
Target Compounds							
23)	Chlordane-1	4.580	3.622	34287504	84323611	976.688	970.637
24)	Chlordane-2	5.113	4.193	35299265	98887445	954.758	959.611
25)	Chlordane-3	5.825	4.818	140.8E6	280.8E6	990.977	976.981
26)	Chlordane-4	5.903	4.879	171.0E6	291.2E6	982.182	981.045
27)	Chlordane-5	6.761	5.544	30269070	81005106	972.900	983.782



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072622\
Data File : PL076610.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jul 2022 23:41
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 02:02:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072622.M
Quant Title : GC Extractables
QLast Update : Tue Jul 26 02:01:57 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

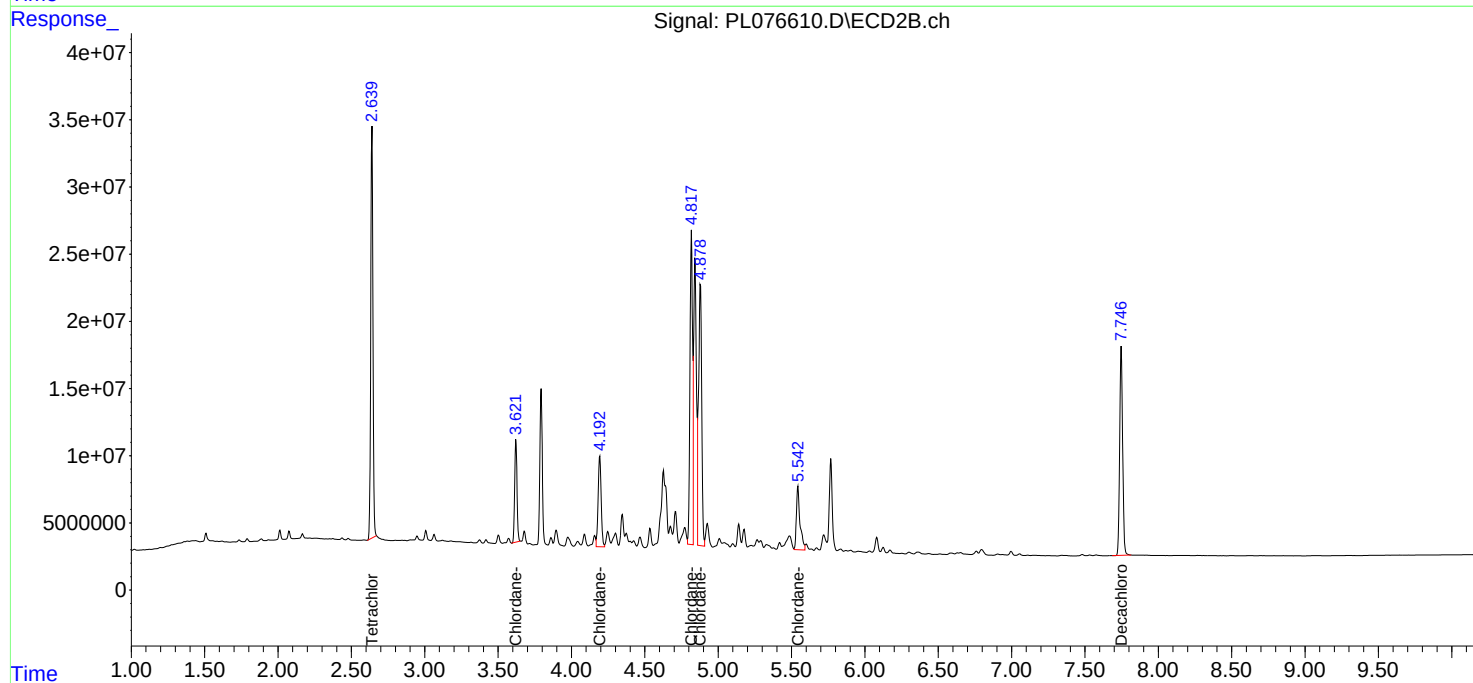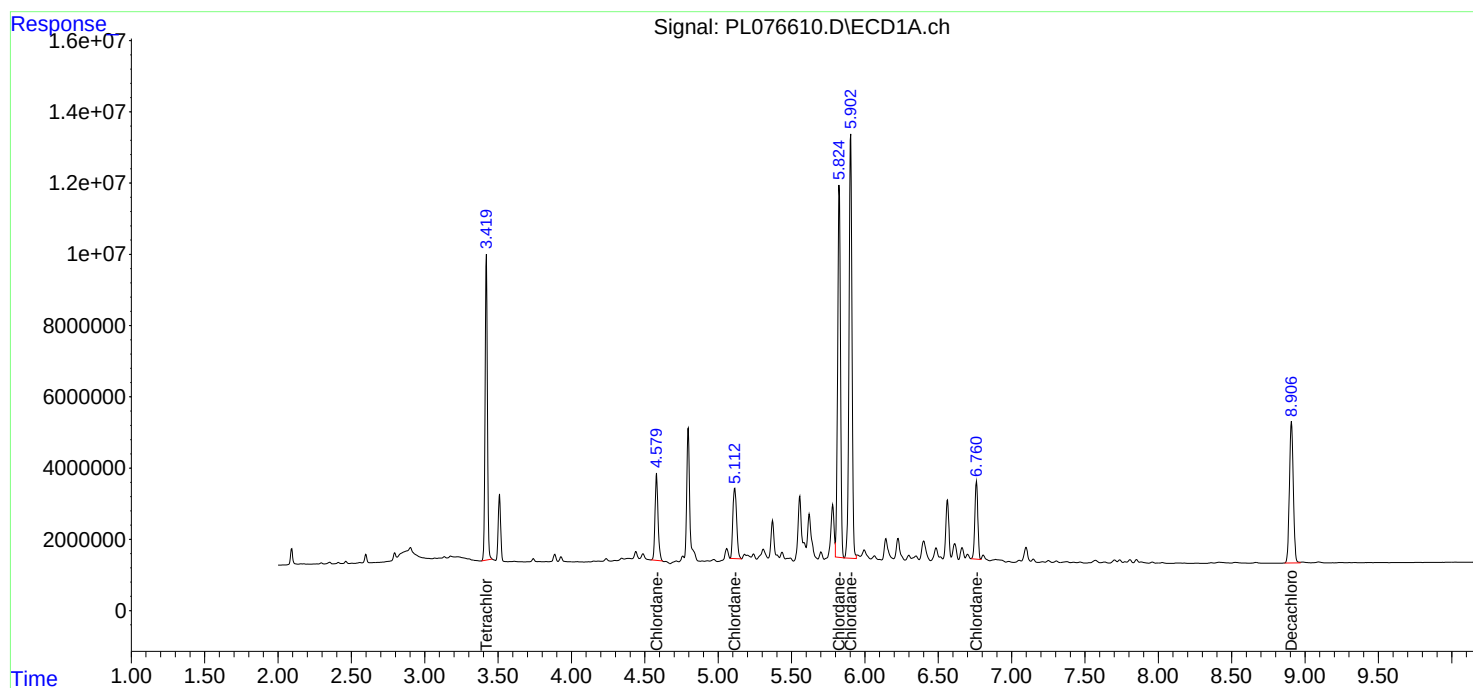


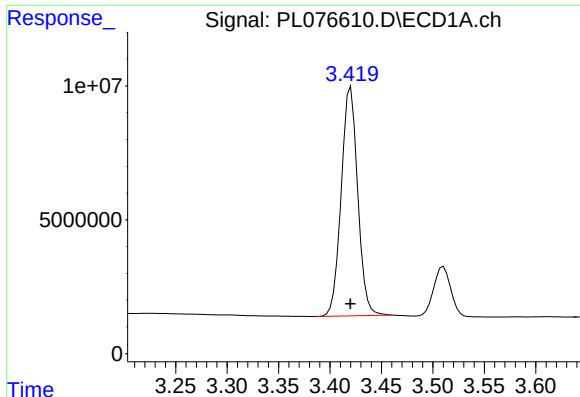

#1 Tetrachloro-m-xylene


R.T.: 3.420 min
Delta R.T.: 0.000 min
Response: 95450879
Conc: 98.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

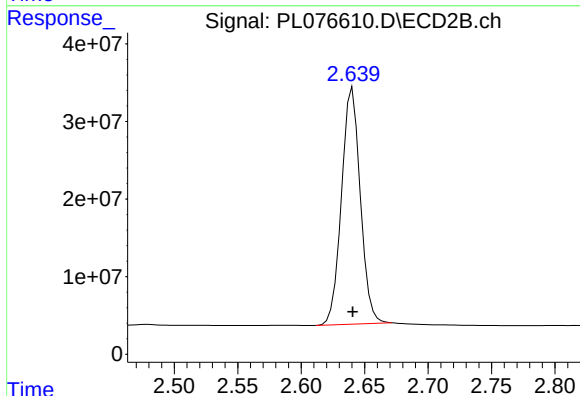


#1 Tetrachloro-m-xylene

R.T.: 2.641 min
Delta R.T.: 0.000 min
Response: 314180053
Conc: 97.90 ng/ml

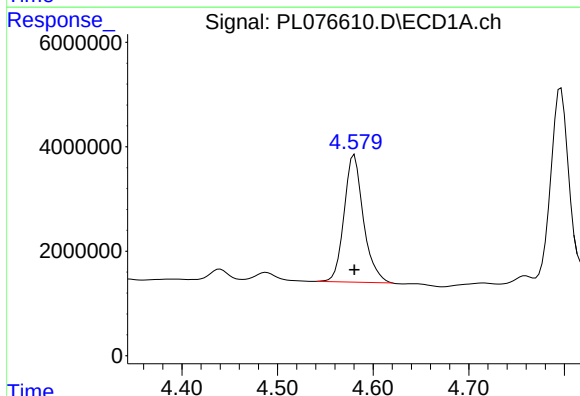


#23 Chlordane-1

R.T.: 4.580 min
Delta R.T.: 0.000 min
Response: 34287504
Conc: 976.69 ng/ml

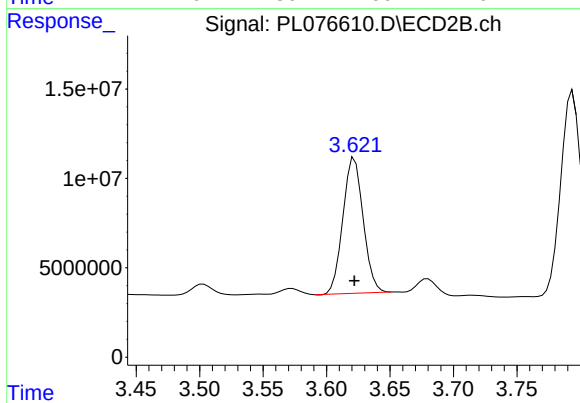

#23 Chlordane-1


R.T.: 3.622 min
Delta R.T.: 0.000 min
Response: 84323611
Conc: 970.64 ng/ml

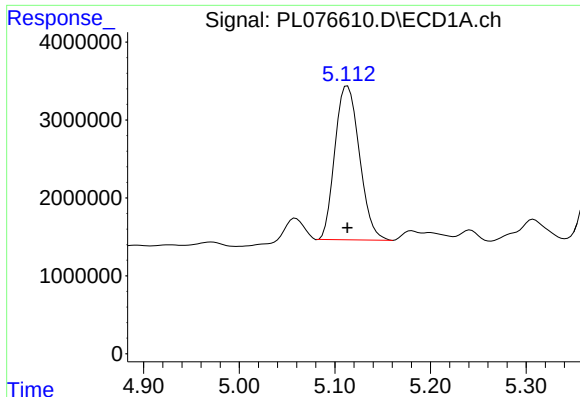

#24 Chlordane-2


R.T.: 5.113 min
Delta R.T.: 0.000 min
Response: 35299265
Conc: 954.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

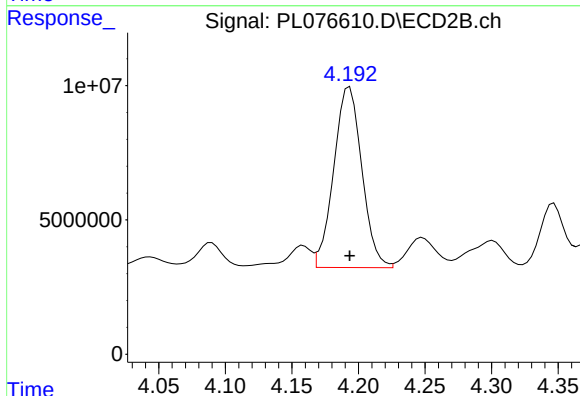


#24 Chlordane-2

R.T.: 4.193 min
Delta R.T.: 0.000 min
Response: 98887445
Conc: 959.61 ng/ml

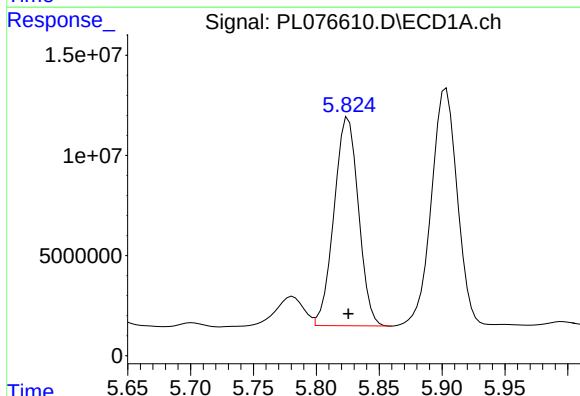


#25 Chlordane-3

R.T.: 5.825 min
Delta R.T.: 0.000 min
Response: 140813427
Conc: 990.98 ng/ml

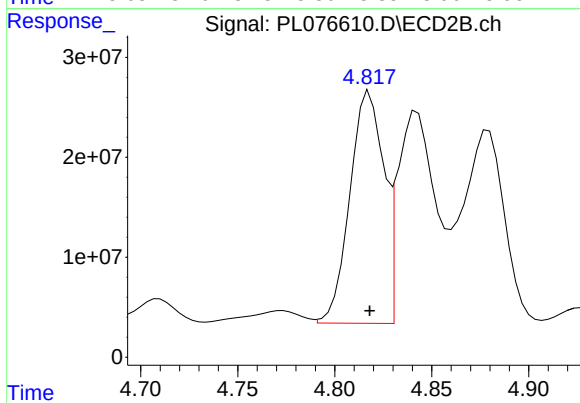

#25 Chlordane-3


R.T.: 4.818 min
Delta R.T.: 0.000 min
Response: 280775812
Conc: 976.98 ng/ml

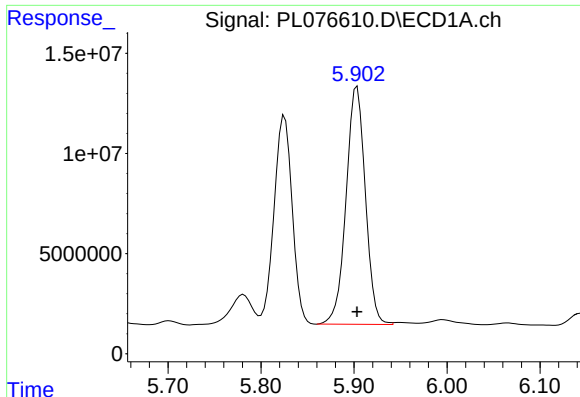

#26 Chlordane-4


R.T.: 5.903 min
Delta R.T.: 0.000 min
Response: 170954591
Conc: 982.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

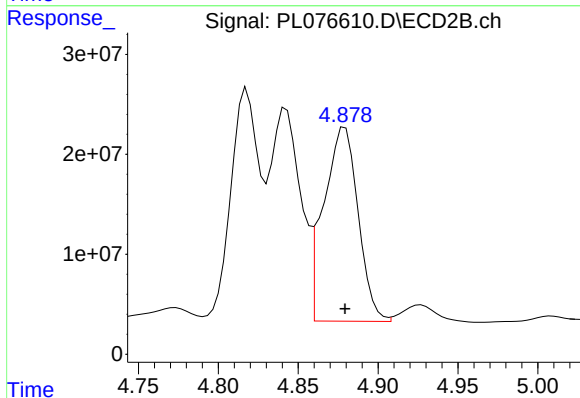


#26 Chlordane-4

R.T.: 4.879 min
Delta R.T.: 0.000 min
Response: 291182174
Conc: 981.05 ng/ml

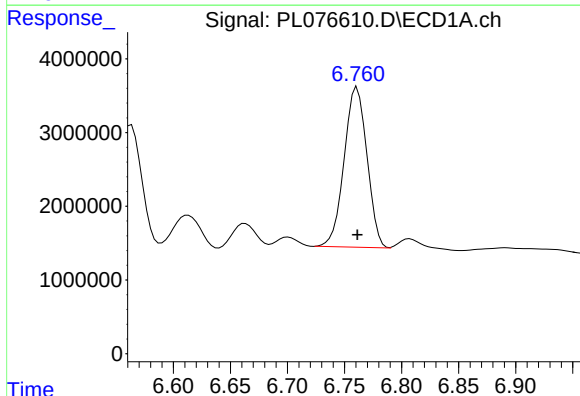


#27 Chlordane-5

R.T.: 6.761 min
Delta R.T.: 0.000 min
Response: 30269070
Conc: 972.90 ng/ml

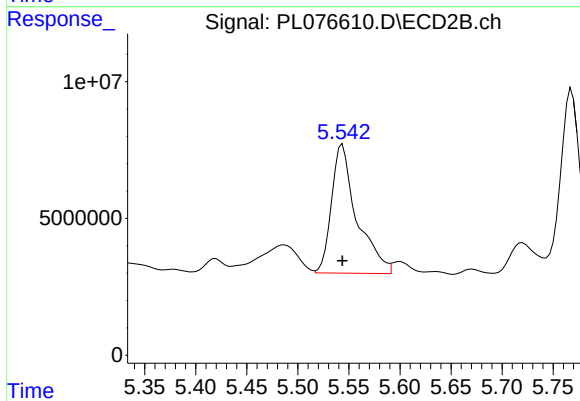

#27 Chlordane-5


R.T.: 5.544 min
Delta R.T.: 0.000 min
Response: 81005106
Conc: 983.78 ng/ml

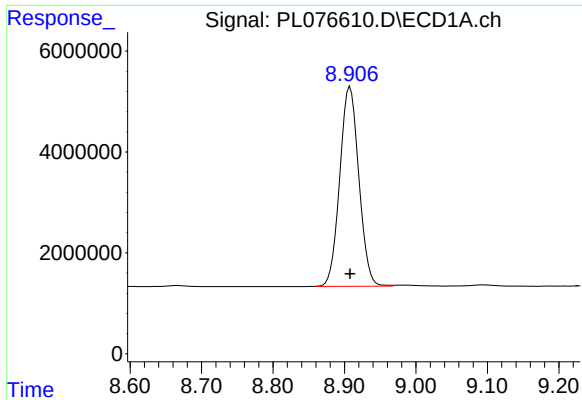

#28 Decachlorobiphenyl

R.T.: 8.908 min
Delta R.T.: 0.000 min
Response: 73325166
Conc: 94.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

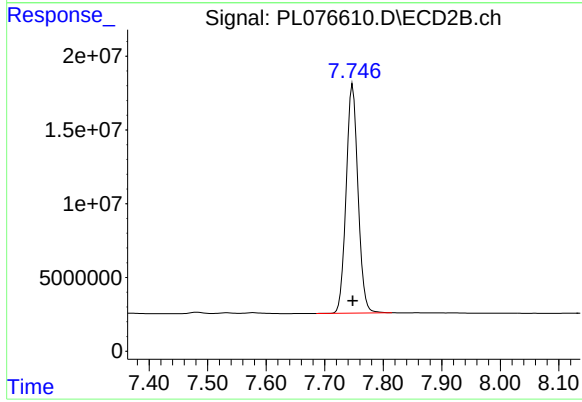

#28 Decachlorobiphenyl

R.T.: 7.748 min
Delta R.T.: 0.000 min
Response: 217937354
Conc: 95.10 ng/ml