

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072622\
 Data File : PL076611.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jul 2022 23:55
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 02:03:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 26 02:03:28 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.420	2.640	71476816	236.8E6	74.324	74.188
28)	SA Decachlor...	8.908	7.748	56763479	168.1E6	73.983	73.891
Target Compounds							
23)	Chlordane-1	4.580	3.622	25653382	64249176	737.051	743.009
24)	Chlordane-2	5.113	4.193	27189412	75836142	740.208	740.554
25)	Chlordane-3	5.825	4.818	105.2E6	211.5E6	743.473	740.528
26)	Chlordane-4	5.903	4.879	128.8E6	219.4E6	743.175	742.837
27)	Chlordane-5	6.761	5.543	22960895	59241958	741.959	729.370



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072622\
Data File : PL076611.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jul 2022 23:55
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 02:03:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072622.M
Quant Title : GC Extractables
QLast Update : Tue Jul 26 02:03:28 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

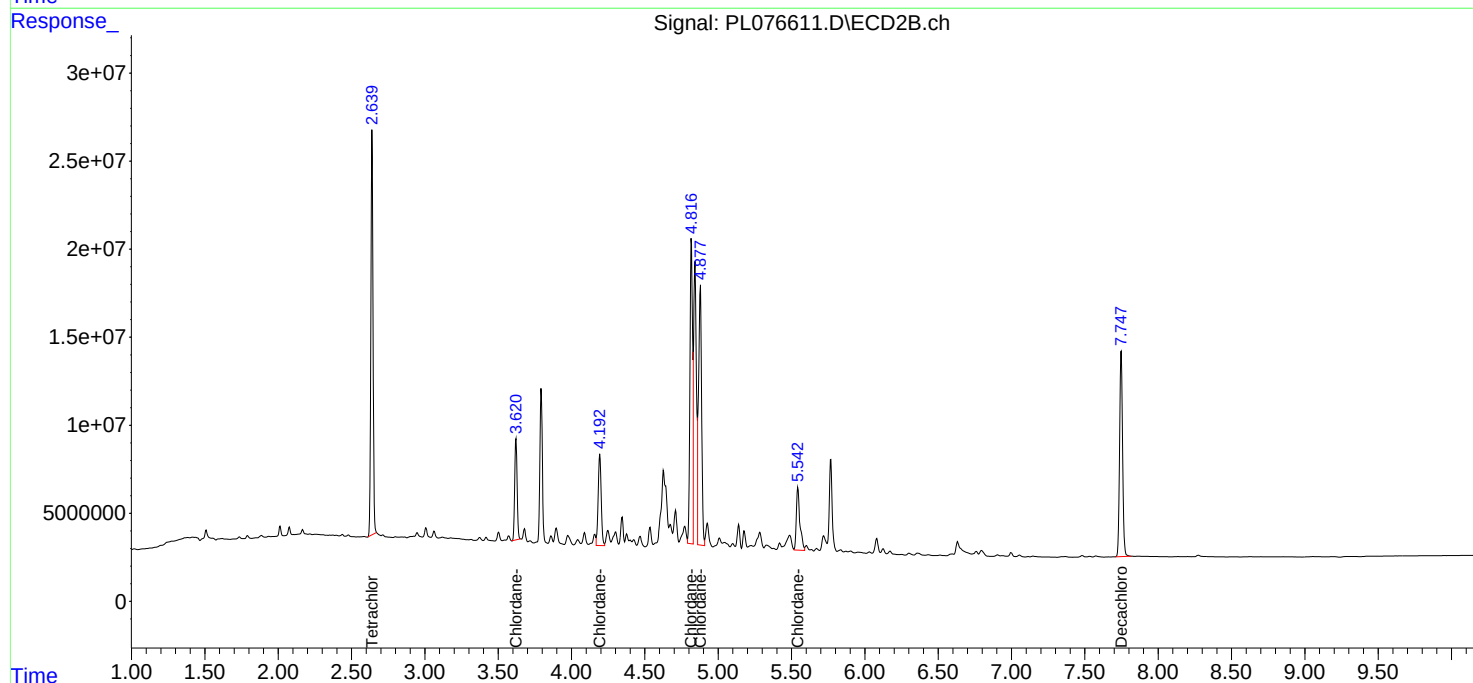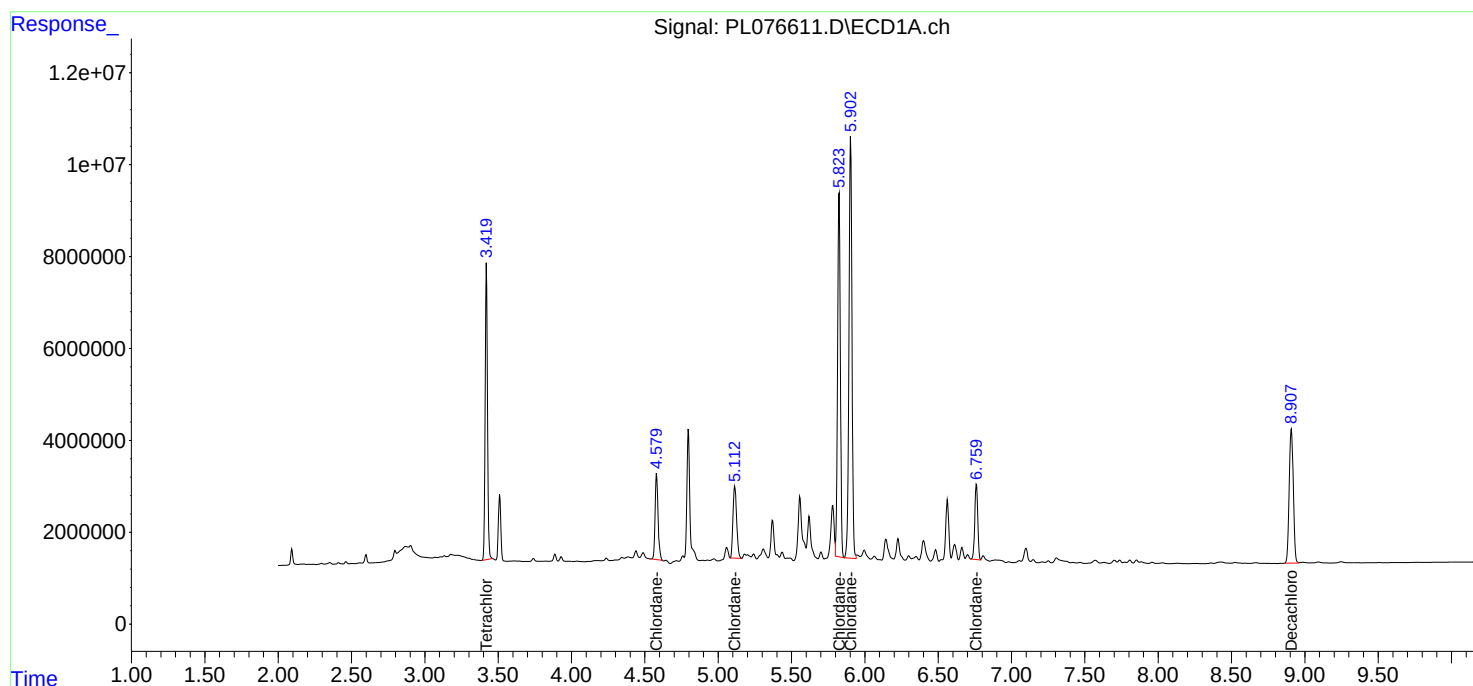


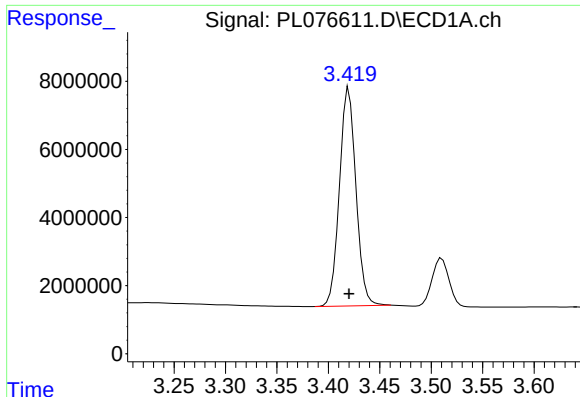

#1 Tetrachloro-m-xylene


R.T.: 3.420 min
Delta R.T.: 0.000 min
Response: 71476816
Conc: 74.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

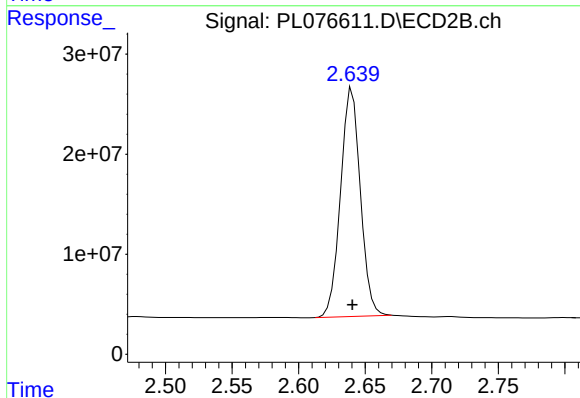


#1 Tetrachloro-m-xylene

R.T.: 2.640 min
Delta R.T.: 0.000 min
Response: 236803148
Conc: 74.19 ng/ml

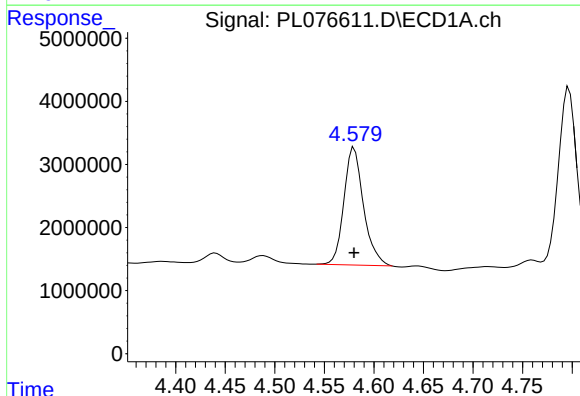


#23 Chlordane-1

R.T.: 4.580 min
Delta R.T.: 0.000 min
Response: 25653382
Conc: 737.05 ng/ml

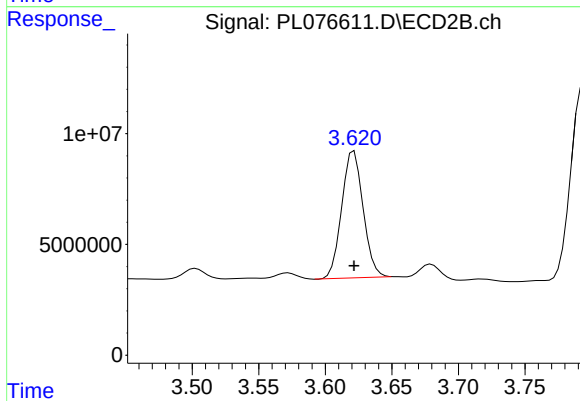

#23 Chlordane-1


R.T.: 3.622 min
Delta R.T.: 0.000 min
Response: 64249176
Conc: 743.01 ng/ml

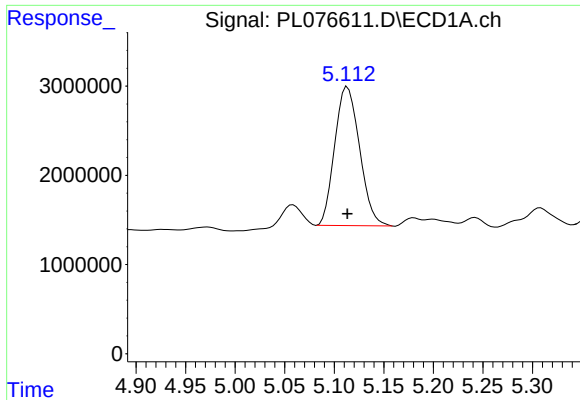

#24 Chlordane-2


R.T.: 5.113 min
Delta R.T.: 0.000 min
Response: 27189412
Conc: 740.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

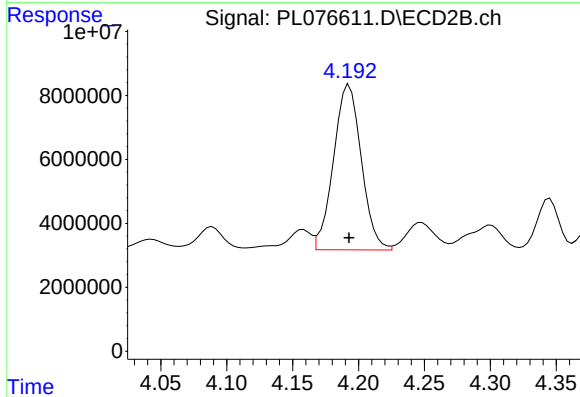


#24 Chlordane-2

R.T.: 4.193 min
Delta R.T.: 0.000 min
Response: 75836142
Conc: 740.55 ng/ml

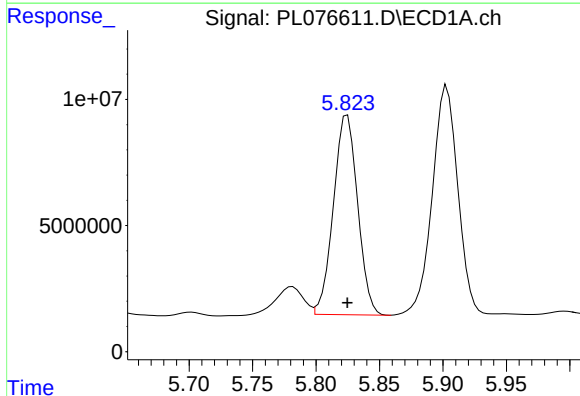


#25 Chlordane-3

R.T.: 5.825 min
Delta R.T.: 0.000 min
Response: 105186449
Conc: 743.47 ng/ml

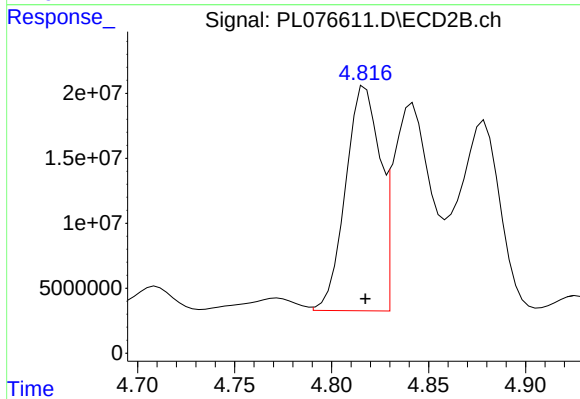

#25 Chlordane-3


R.T.: 4.818 min
Delta R.T.: 0.000 min
Response: 211485563
Conc: 740.53 ng/ml

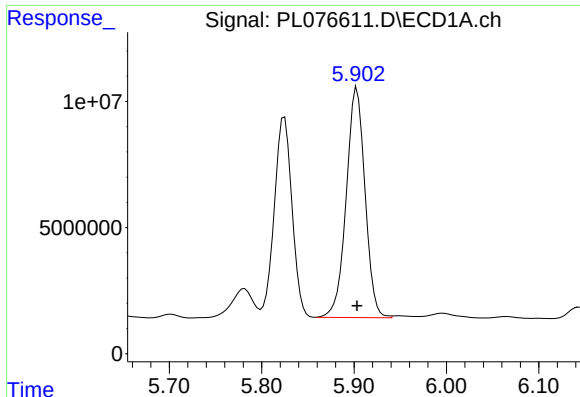

#26 Chlordane-4


R.T.: 5.903 min
Delta R.T.: 0.000 min
Response: 128768098
Conc: 743.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

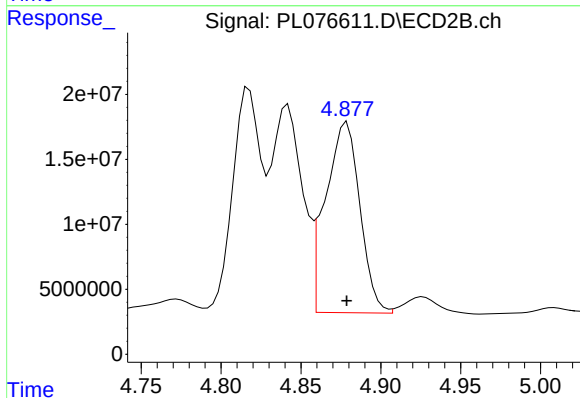


#26 Chlordane-4

R.T.: 4.879 min
Delta R.T.: 0.000 min
Response: 219432015
Conc: 742.84 ng/ml

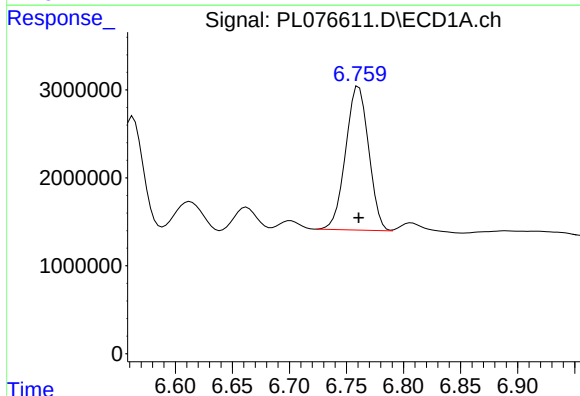


#27 Chlordane-5

R.T.: 6.761 min
Delta R.T.: 0.000 min
Response: 22960895
Conc: 741.96 ng/ml

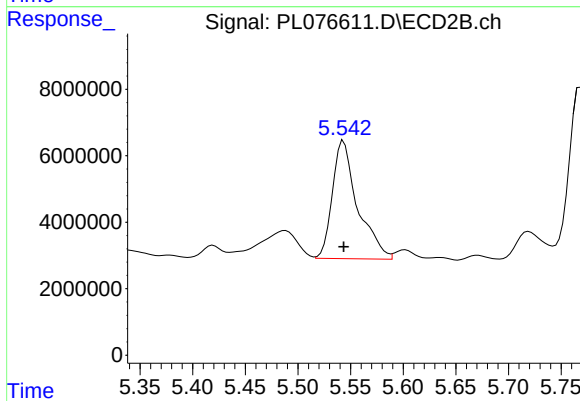

#27 Chlordane-5


R.T.: 5.543 min
Delta R.T.: 0.000 min
Response: 59241958
Conc: 729.37 ng/ml

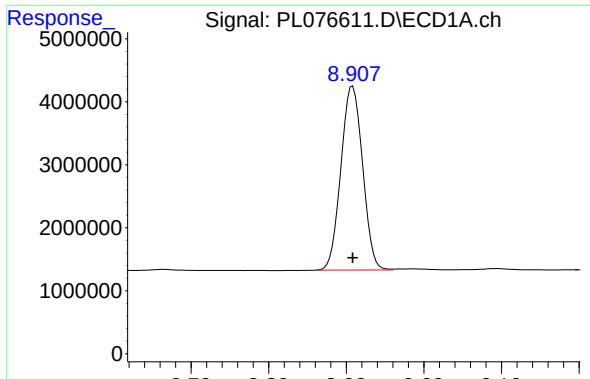

#28 Decachlorobiphenyl

R.T.: 8.908 min
Delta R.T.: 0.000 min
Response: 56763479
Conc: 73.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

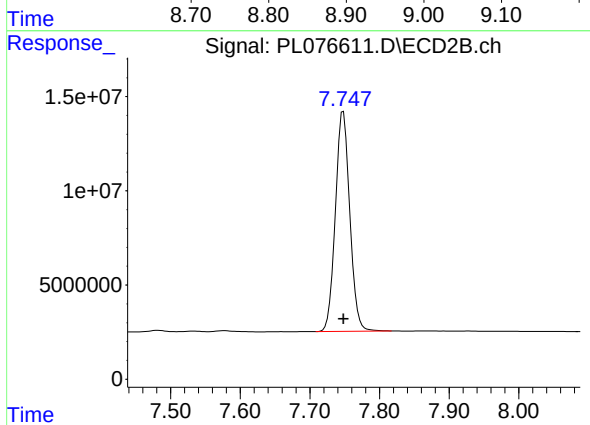

#28 Decachlorobiphenyl

R.T.: 7.748 min
Delta R.T.: 0.000 min
Response: 168098378
Conc: 73.89 ng/ml